

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010837.D
 Acq On : 25 Jun 2022 20:41
 Operator : CG/JU
 Sample : PB145745BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK745

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010837.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	31	rVB	162421	217366	2.53%	0.195%
2	3.611	86	89	111	rBV	2007639	2915573	33.96%	2.622%
3	3.934	140	144	150	rVB	38182	56752	0.66%	0.051%
4	6.899	640	648	664	rVB	2165859	3359137	39.13%	3.021%
5	7.058	669	675	687	rVB	1865430	2826655	32.93%	2.542%
6	7.252	698	708	718	rBV	2320521	3519569	41.00%	3.165%
7	7.716	779	787	796	rBV	2077997	3201473	37.30%	2.879%
8	8.434	902	909	919	rBV	2775558	4230527	49.28%	3.805%
9	8.875	975	984	994	rBV	1996234	3265324	38.04%	2.937%
10	9.599	1097	1107	1115	rBV	1510256	2418744	28.18%	2.175%
11	10.140	1190	1199	1209	rBV	2365967	3933627	45.82%	3.538%
12	10.510	1254	1262	1273	rBV	2780882	4615277	53.77%	4.151%
13	10.657	1279	1287	1302	rBV	2681947	4373402	50.95%	3.933%
14	12.110	1527	1534	1539	rBV	47948	79239	0.92%	0.071%
15	12.322	1561	1570	1576	rVB	6303	16632	0.19%	0.015%
16	13.098	1697	1702	1708	rBV6	6729	11238	0.13%	0.010%
17	13.334	1738	1742	1747	rBV4	6842	11311	0.13%	0.010%
18	13.792	1813	1820	1828	rBV	4197203	5634421	65.64%	5.067%
19	14.063	1857	1866	1875	rBV	4846056	6846521	79.76%	6.157%
20	14.375	1912	1919	1926	rBV	3791434	5547748	64.63%	4.989%
21	14.587	1949	1955	1974	rBV	1588564	2312085	26.93%	2.079%
22	14.739	1977	1981	1986	rVV7	10840	21654	0.25%	0.019%
23	14.804	1986	1992	1997	rVB10	8489	15972	0.19%	0.014%
24	15.369	2081	2088	2098	rBV	5618574	8338733	97.14%	7.499%
25	15.492	2102	2109	2123	rVV	929223	1346572	15.69%	1.211%
26	15.610	2124	2129	2135	rVB	72461	105220	1.23%	0.095%
27	16.157	2217	2222	2230	rBV4	22735	37316	0.43%	0.034%
28	16.810	2329	2333	2337	rVB6	11176	17511	0.20%	0.016%
29	16.922	2346	2352	2356	rBV4	11491	20845	0.24%	0.019%
30	17.133	2382	2388	2398	rBV	4147987	5689649	66.28%	5.117%
31	17.233	2398	2405	2420	rBV2	5717310	8193111	95.45%	7.368%
32	17.392	2429	2432	2437	rVB6	10541	14133	0.16%	0.013%
33	17.822	2503	2505	2509	rVB4	11041	10541	0.12%	0.009%
34	19.063	2712	2716	2720	rVB	64649	82169	0.96%	0.074%
35	19.127	2723	2727	2731	rBV	66013	83095	0.97%	0.075%
36	19.486	2782	2788	2795	rBV	6395141	8450682	98.45%	7.600%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010837.D
Acq On : 25 Jun 2022 20:41
Operator : CG/JU
Sample : PB145745BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK745

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION

37	21.245	3082	3087	3093	rBV	4328461	5239929	61.04%	4.712%
38	23.463	3457	3464	3474	rVB2	4417791	8584054	100.00%	7.720%
39	23.615	3483	3490	3500	rVB2	2778625	5551788	64.68%	4.993%




Sum of corrected areas: 111195595

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010837.D
Acq On : 25 Jun 2022 20:41
Operator : CG/JU
Sample : PB145745BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK745

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

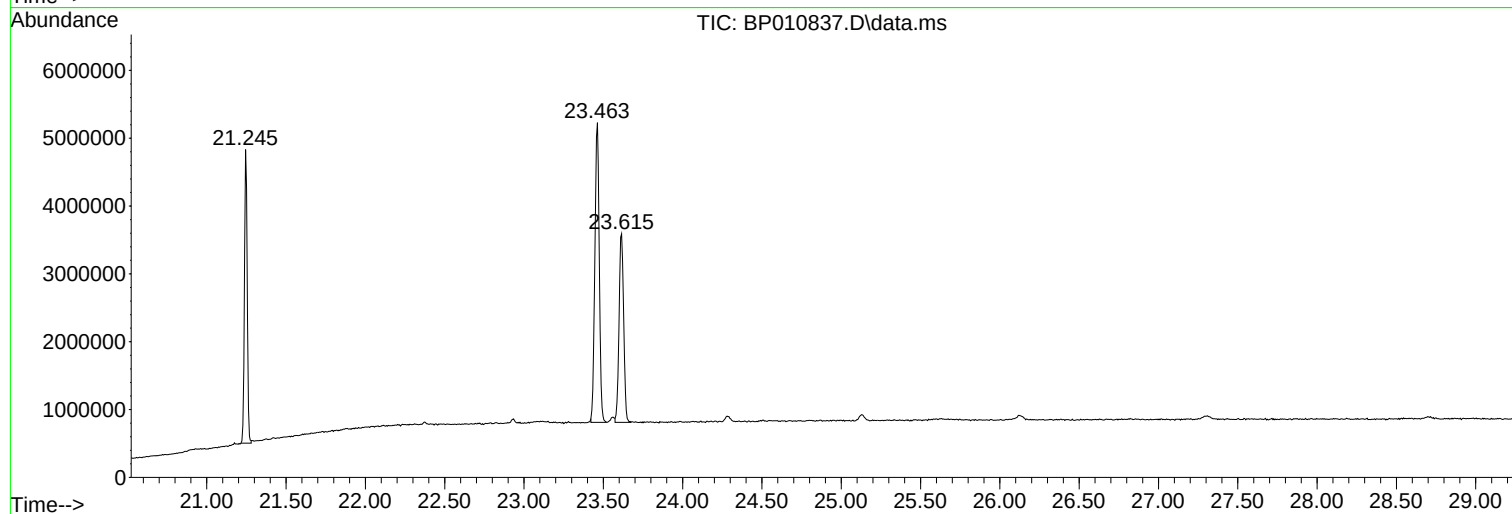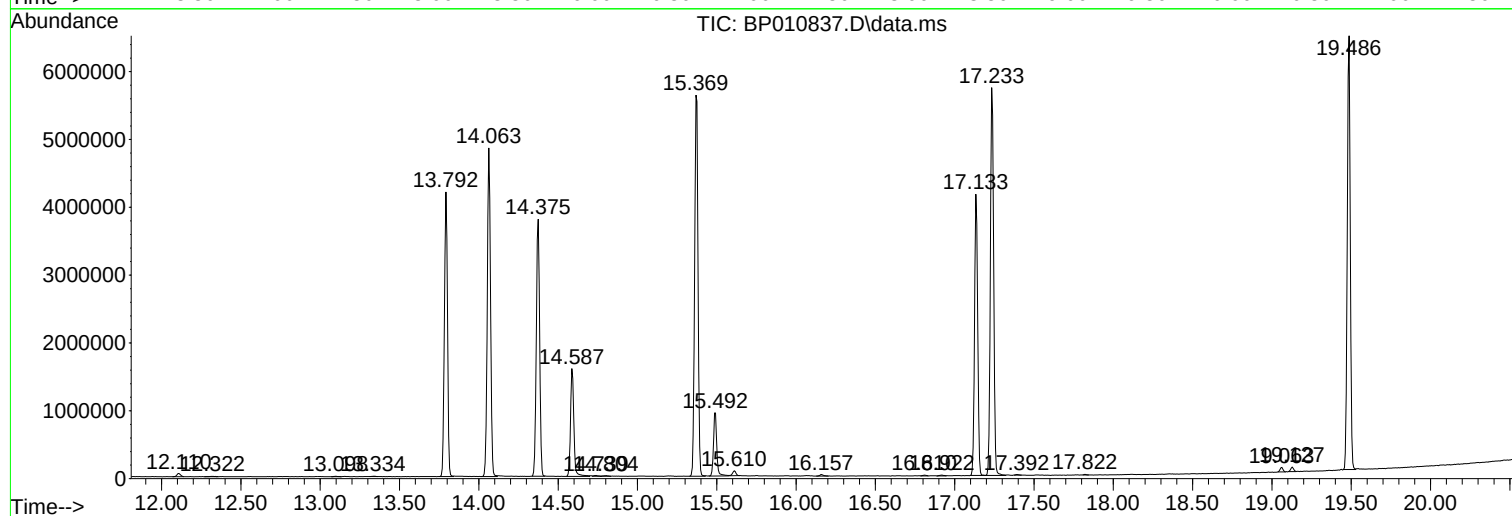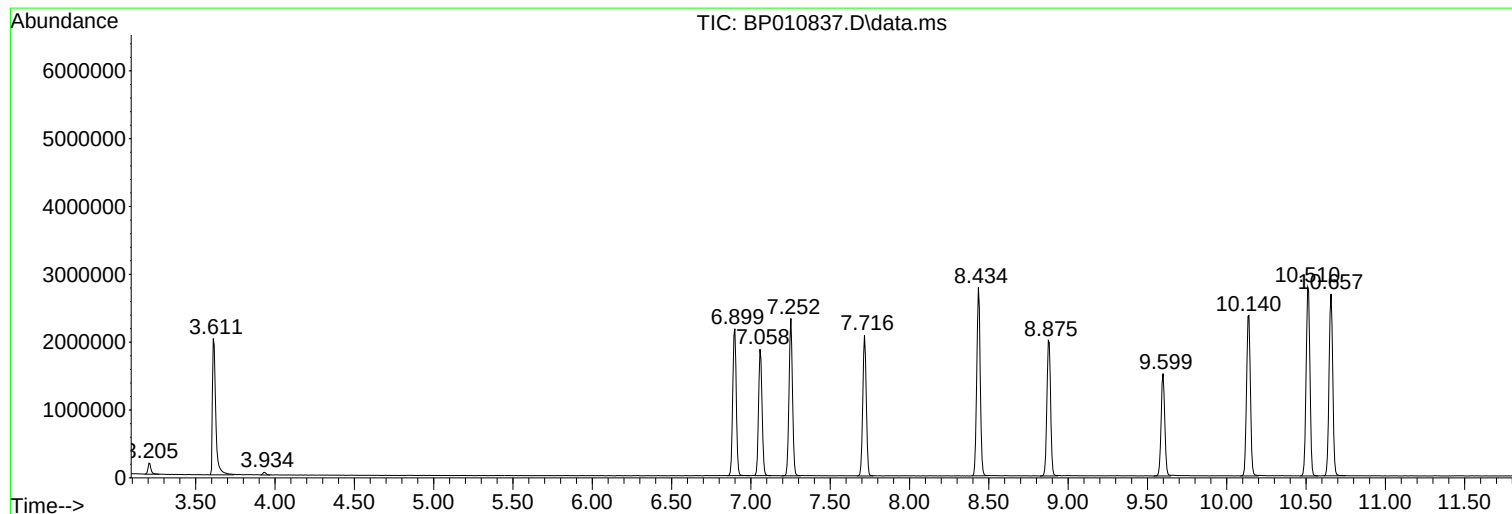

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010837.D
Acq On : 25 Jun 2022 20:41
Operator : CG/JU
Sample : PB145745BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK745

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010837.D
Acq On : 25 Jun 2022 20:41
Operator : CG/JU
Sample : PB145745BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK745

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
