

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010838.D
 Acq On : 25 Jun 2022 21:15
 Operator : CG/JU
 Sample : PB145746BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK746

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010838.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	16	20	31	rVB	156861	215187	2.47%	0.225%
2	3.610	86	89	114	rBV	1869273	2757471	31.60%	2.884%
3	3.934	140	144	151	rVB	33813	48012	0.55%	0.050%
4	6.898	640	648	657	rBV	2034523	3121051	35.76%	3.264%
5	7.057	669	675	686	rVB	1725508	2648041	30.34%	2.769%
6	7.251	700	708	717	rBV	2188720	3310788	37.94%	3.462%
7	7.716	778	787	795	rVB	1557351	2393512	27.43%	2.503%
8	8.434	900	909	918	rBV	2489777	3837372	43.97%	4.013%
9	8.881	977	985	995	rBV	1828119	2951029	33.81%	3.086%
10	9.598	1100	1107	1120	rBV	1366375	2159573	24.75%	2.258%
11	10.134	1190	1198	1208	rBV	2127485	3515037	40.28%	3.676%
12	10.510	1254	1262	1272	rVB	1981912	3316113	38.00%	3.468%
13	10.657	1279	1287	1300	rBV	2305477	3836578	43.96%	4.012%
14	12.110	1528	1534	1542	rBV2	44445	74984	0.86%	0.078%
15	13.339	1741	1743	1750	rVB8	7293	10210	0.12%	0.011%
16	13.792	1813	1820	1830	rBV	3500388	4690010	53.74%	4.905%
17	14.063	1858	1866	1880	rBV	4018165	5822748	66.72%	6.089%
18	14.374	1911	1919	1928	rBV	2547844	3764221	43.13%	3.936%
19	14.586	1948	1955	1970	rBV	1506880	2141718	24.54%	2.240%
20	14.733	1976	1980	1986	rVB9	5614	12416	0.14%	0.013%
21	14.798	1989	1991	1998	rVB7	6083	9136	0.10%	0.010%
22	15.374	2082	2089	2102	rBV	4863431	6987680	80.07%	7.307%
23	15.492	2102	2109	2123	rVV	858733	1219111	13.97%	1.275%
24	15.610	2125	2129	2135	rVB	59568	92094	1.06%	0.096%
25	15.945	2179	2186	2191	rBV	6146	10721	0.12%	0.011%
26	16.163	2218	2223	2228	rBV3	18925	27952	0.32%	0.029%
27	16.810	2328	2333	2338	rBV9	12683	20855	0.24%	0.022%
28	16.916	2347	2351	2354	rBV5	9438	15907	0.18%	0.017%
29	17.133	2382	2388	2396	rBV	2756777	3909290	44.79%	4.088%
30	17.233	2399	2405	2423	rVV2	5014846	7040008	80.67%	7.362%
31	17.398	2427	2433	2438	rVV8	13252	25576	0.29%	0.027%
32	19.057	2711	2715	2721	rBV	57796	82741	0.95%	0.087%
33	19.127	2723	2727	2731	rBV	62896	79287	0.91%	0.083%
34	19.486	2782	2788	2794	rBV	6138058	7851393	89.97%	8.211%
35	21.245	3082	3087	3094	rBV	3554638	4340129	49.73%	4.539%
36	23.462	3457	3464	3475	rVB2	4551477	8727113	100.00%	9.126%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010838.D
Acq On : 25 Jun 2022 21:15
Operator : CG/JU
Sample : PB145746BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK746

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION

37 23.609 3483 3489 3503 rVB2 2412531 4560239 52.25% 4.769%




Sum of corrected areas: 95625303

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010838.D
Acq On : 25 Jun 2022 21:15
Operator : CG/JU
Sample : PB145746BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK746

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

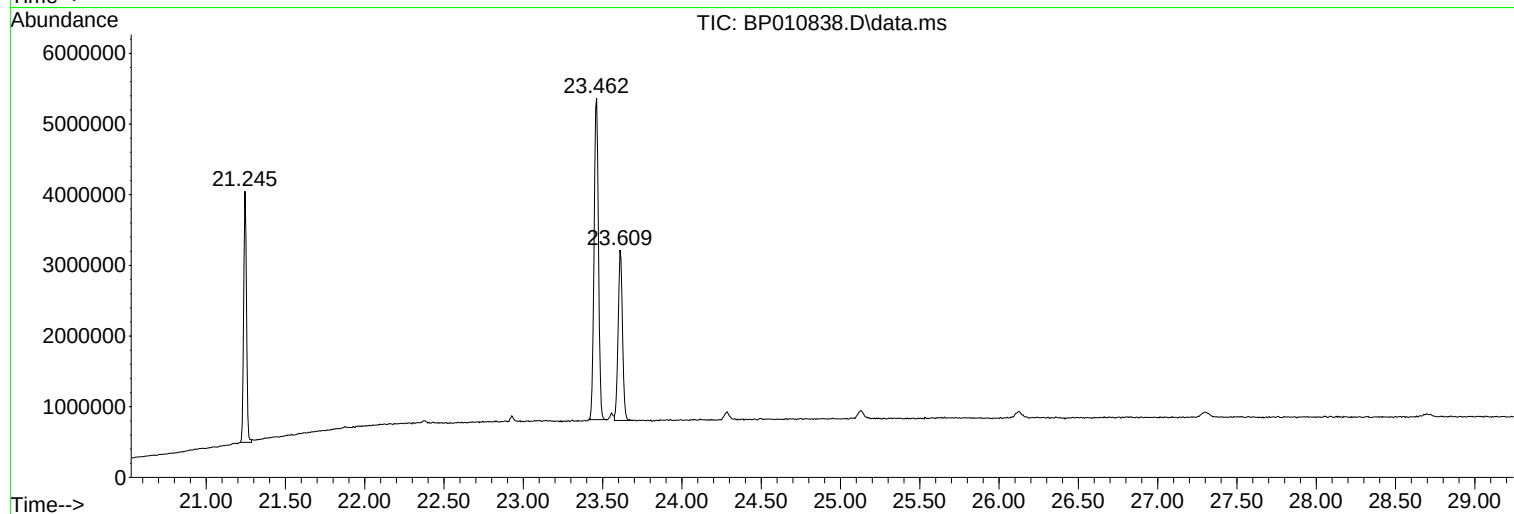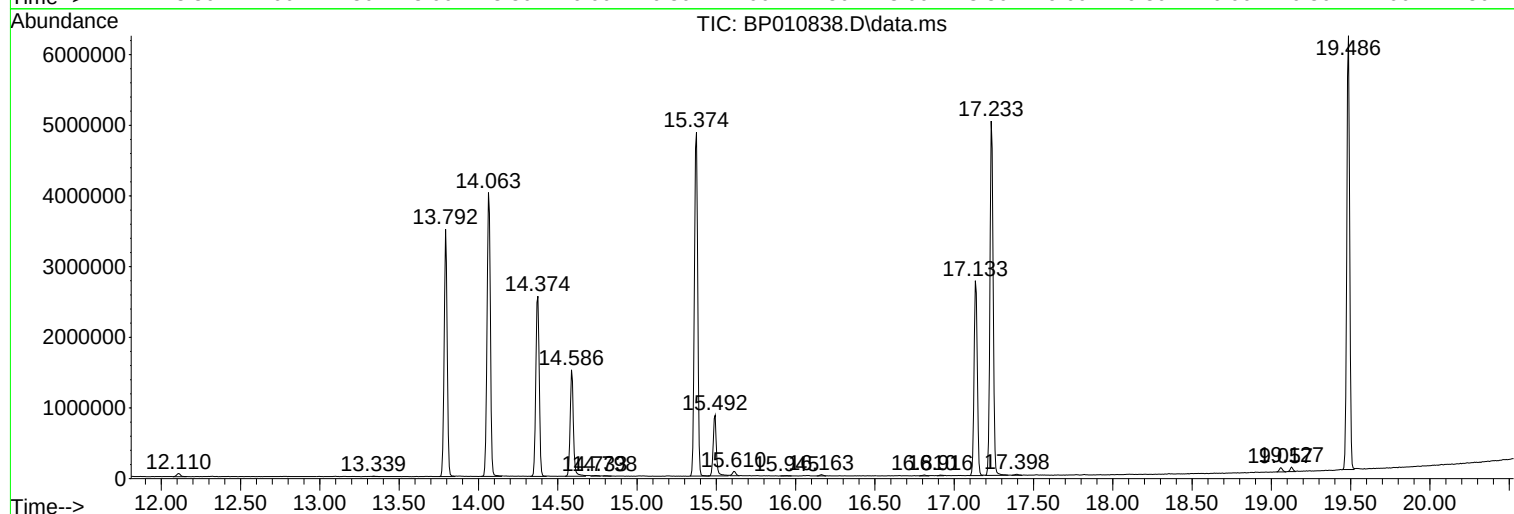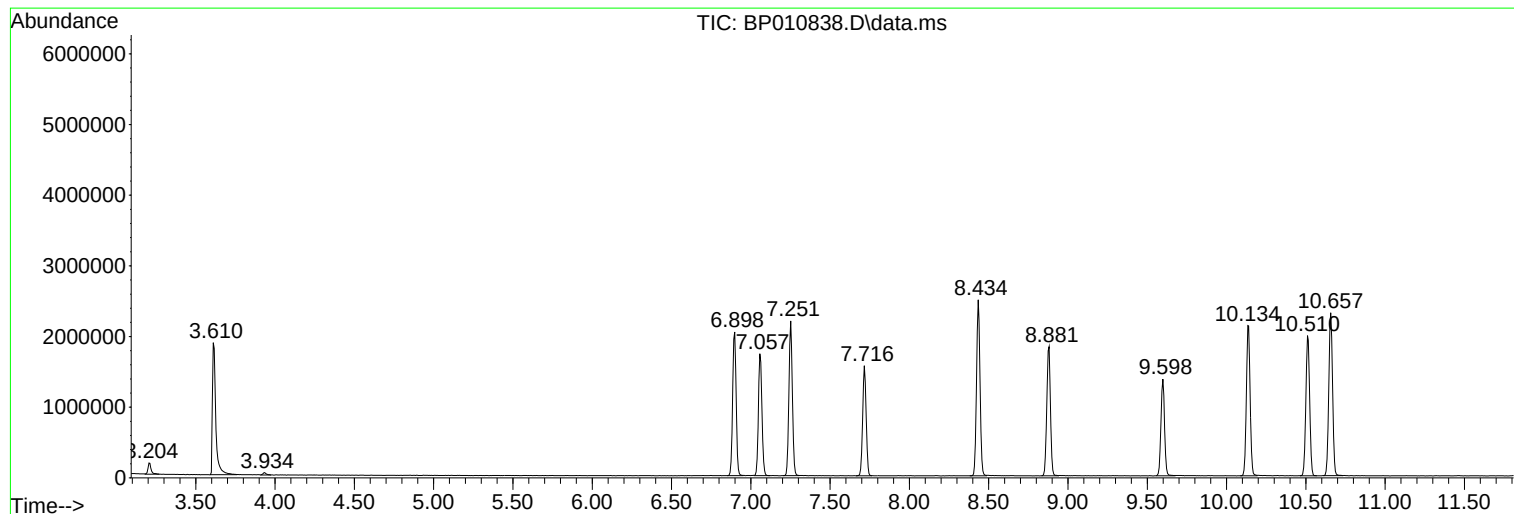

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010838.D
Acq On : 25 Jun 2022 21:15
Operator : CG/JU
Sample : PB145746BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK746

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010838.D
Acq On : 25 Jun 2022 21:15
Operator : CG/JU
Sample : PB145746BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK746

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc