

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010844.D
 Acq On : 26 Jun 2022 00:38
 Operator : CG/JU
 Sample : N3392-03 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010844.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	23	rBV	60744	77907	0.83%	0.080%
2	3.246	23	27	38	rVB	530076	614303	6.51%	0.628%
3	3.487	65	68	74	rVB	20984	28224	0.30%	0.029%
4	3.546	74	78	83	rVB	34834	46145	0.49%	0.047%
5	3.616	87	90	96	rBV	671756	871869	9.24%	0.891%
6	3.663	96	98	107	rVB	144405	176883	1.87%	0.181%
7	3.840	121	128	133	rVV2	53066	87462	0.93%	0.089%
8	3.916	135	141	151	rVB2	88943	178519	1.89%	0.182%
9	4.075	165	168	175	rBV2	22884	32480	0.34%	0.033%
10	4.193	184	188	196	rVB	182987	239817	2.54%	0.245%
11	4.263	196	200	203	rVV2	27800	31986	0.34%	0.033%
12	4.299	204	206	212	rVB7	8567	12489	0.13%	0.013%
13	4.375	214	219	225	rVB	241163	306369	3.25%	0.313%
14	4.434	225	229	234	rBV	96771	120162	1.27%	0.123%
15	4.651	262	266	270	rBV4	8087	11788	0.12%	0.012%
16	4.722	275	278	281	rVB4	8743	11220	0.12%	0.011%
17	4.822	287	295	303	rBV	481702	656166	6.95%	0.670%
18	5.222	360	363	369	rVB6	5729	9833	0.10%	0.010%
19	5.316	374	379	384	rVB2	13607	21719	0.23%	0.022%
20	5.440	394	400	404	rBV	13926	21442	0.23%	0.022%
21	5.681	436	441	446	rBV	34406	49141	0.52%	0.050%
22	5.816	461	464	472	rVB7	6513	11450	0.12%	0.012%
23	6.722	613	618	622	rBV5	7124	10500	0.11%	0.011%
24	6.892	638	647	659	rVB	434172	680651	7.21%	0.695%
25	7.057	668	675	683	rBV	1916666	2853253	30.24%	2.915%
26	7.128	683	687	693	rVB	33866	50613	0.54%	0.052%
27	7.251	698	708	719	rBV	1693713	2625043	27.82%	2.682%
28	7.345	720	724	732	rVB5	10147	21447	0.23%	0.022%
29	7.716	779	787	795	rBV	1903184	2932657	31.08%	2.996%
30	7.787	795	799	810	rVB	31252	54935	0.58%	0.056%
31	8.434	901	909	917	rBV	1263591	1970139	20.88%	2.013%
32	8.539	921	927	934	rVB	76458	125778	1.33%	0.129%
33	8.875	977	984	992	rBV	2049278	3214712	34.07%	3.285%
34	9.004	1001	1006	1010	rBV2	12137	19375	0.21%	0.020%
35	9.045	1010	1013	1020	rVB8	9030	12213	0.13%	0.012%
36	9.304	1052	1057	1063	rVB	32148	51421	0.54%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010844.D
 Acq On : 26 Jun 2022 00:38
 Operator : CG/JU
 Sample : N3392-03 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	9.381	1063	1070	1073	rVV5	19358	37226	0.39%	0.038%
38	9.439	1076	1080	1088	rVB7	25524	53407	0.57%	0.055%
39	9.598	1099	1107	1122	rBV	1356473	2242065	23.76%	2.291%
40	9.904	1154	1159	1162	rBV6	5377	10565	0.11%	0.011%
41	10.051	1175	1184	1189	rBV6	10172	21506	0.23%	0.022%
42	10.134	1190	1198	1206	rBV	2091242	3319872	35.19%	3.392%
43	10.198	1206	1209	1214	rVB7	15549	25072	0.27%	0.026%
44	10.310	1222	1228	1232	rVB9	5727	10525	0.11%	0.011%
45	10.439	1245	1250	1254	rVB4	14531	24010	0.25%	0.025%
46	10.510	1254	1262	1277	rVB	2511609	4092530	43.37%	4.182%
47	10.657	1277	1287	1298	rBV	2077119	3422233	36.27%	3.497%
48	10.728	1298	1299	1307	rVB8	8999	14861	0.16%	0.015%
49	11.063	1352	1356	1361	rVB	21515	33817	0.36%	0.035%
50	11.128	1361	1367	1371	rBV	23668	41641	0.44%	0.043%
51	12.022	1513	1519	1523	rBV7	10644	19969	0.21%	0.020%
52	12.104	1528	1533	1540	rVB2	44373	72180	0.76%	0.074%
53	12.310	1560	1568	1575	rVB2	5205	13382	0.14%	0.014%
54	12.980	1680	1682	1687	rVB6	6858	9661	0.10%	0.010%
55	13.204	1716	1720	1725	rVB3	18780	26080	0.28%	0.027%
56	13.286	1725	1734	1738	rBV10	9212	17121	0.18%	0.017%
57	13.333	1738	1742	1750	rVB8	8082	16447	0.17%	0.017%
58	13.792	1813	1820	1826	rBV	3639954	4965482	52.63%	5.074%
59	13.833	1826	1827	1831	rVB2	14384	14701	0.16%	0.015%
60	14.063	1857	1866	1873	rBV	4228180	6212296	65.84%	6.347%
61	14.280	1900	1903	1908	rVB6	10207	12927	0.14%	0.013%
62	14.369	1912	1918	1932	rBV	3190954	4610023	48.86%	4.710%
63	14.586	1949	1955	1967	rBV	231052	356917	3.78%	0.365%
64	14.739	1975	1981	1985	rVV8	6183	10677	0.11%	0.011%
65	14.798	1988	1991	1997	rVB8	9212	15289	0.16%	0.016%
66	15.157	2046	2052	2055	rBV	59070	82828	0.88%	0.085%
67	15.369	2081	2088	2099	rBV	5608424	7675395	81.35%	7.842%
68	15.486	2102	2108	2123	rVV	854866	1174597	12.45%	1.200%
69	15.610	2124	2129	2136	rVB	64897	102807	1.09%	0.105%
70	15.939	2180	2185	2190	rBV9	9365	15578	0.17%	0.016%
71	16.157	2219	2222	2228	rVB4	18888	28854	0.31%	0.029%
72	16.280	2239	2243	2249	rBV9	7372	18268	0.19%	0.019%
73	16.804	2330	2332	2338	rVB6	10151	14836	0.16%	0.015%
74	16.910	2347	2350	2355	rBV5	11868	16969	0.18%	0.017%
75	17.133	2381	2388	2398	rBV	3350844	4565214	48.38%	4.665%
76	17.233	2398	2405	2422	rBV2	5563831	7835981	83.05%	8.006%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010844.D
 Acq On : 26 Jun 2022 00:38
 Operator : CG/JU
 Sample : N3392-03 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

77	17.386	2427	2431	2438	rBV8	11926	22600	0.24%	0.023%
78	17.439	2438	2440	2446	rVB7	5859	9798	0.10%	0.010%
79	17.515	2449	2453	2455	rBV5	10219	16028	0.17%	0.016%
80	17.827	2502	2506	2511	rBV	213320	255890	2.71%	0.261%
81	18.968	2696	2700	2704	rBV	124446	134183	1.42%	0.137%
82	19.057	2711	2715	2719	rBV	67191	93008	0.99%	0.095%
83	19.127	2724	2727	2730	rVB	59747	70618	0.75%	0.072%
84	19.480	2782	2787	2796	rBV	6378256	8407579	89.11%	8.590%
85	20.974	3038	3041	3044	rBV	96184	109982	1.17%	0.112%
86	21.245	3082	3087	3091	rBV	3808137	4702349	49.84%	4.805%
87	23.456	3456	3463	3474	rVB2	4925745	9435360	100.00%	9.641%
88	23.609	3483	3489	3500	rVB2	2604004	5119347	54.26%	5.231%




Sum of corrected areas: 97870662

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010844.D
Acq On : 26 Jun 2022 00:38
Operator : CG/JU
Sample : N3392-03 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

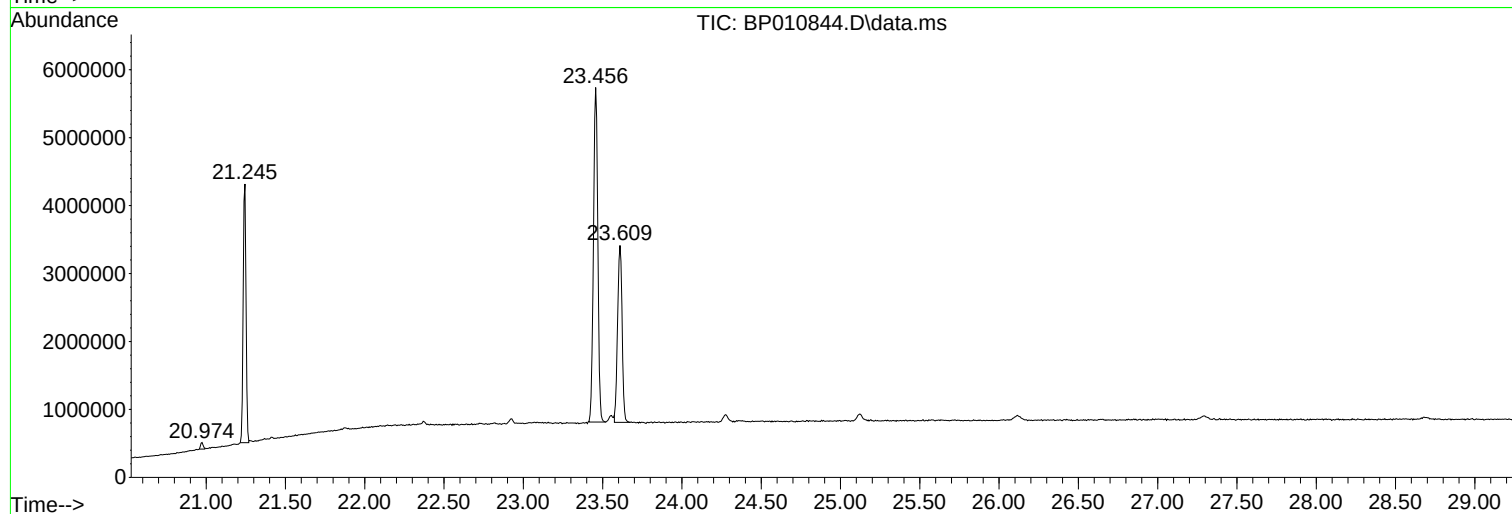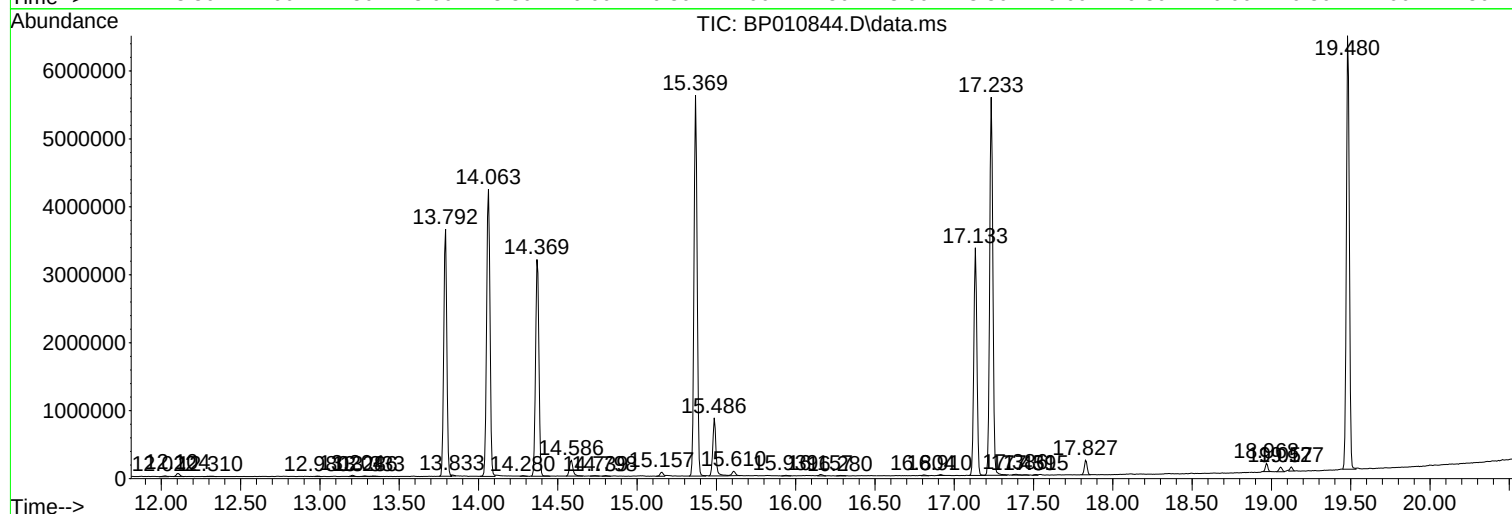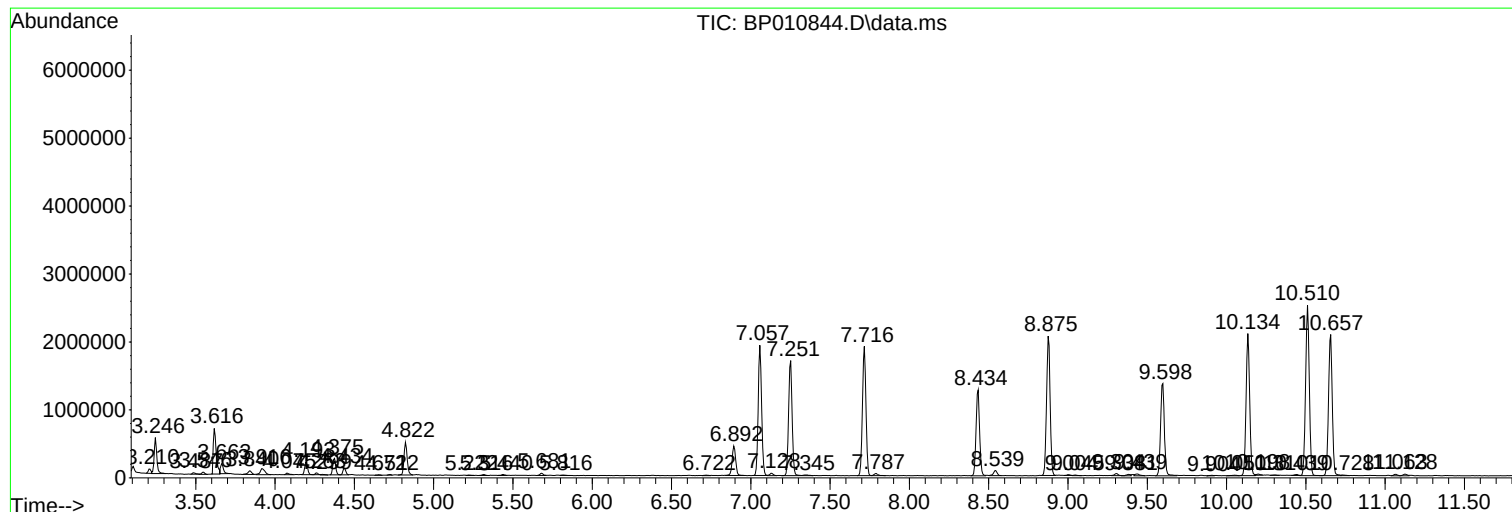

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010844.D
Acq On : 26 Jun 2022 00:38
Operator : CG/JU
Sample : N3392-03 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propanoic acid, propyl ester Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.375	2.09 ng/ul	306369	1,4-Dichlorobenzene-d4	7.716

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	83		
2	Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78		
3	Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	72		
4	Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	64		
5	Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	56		

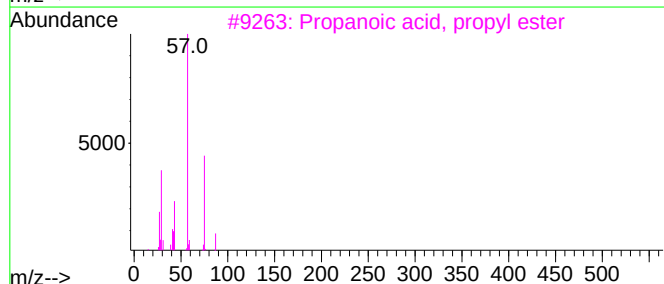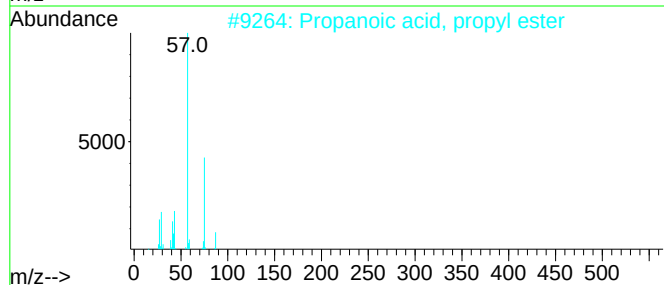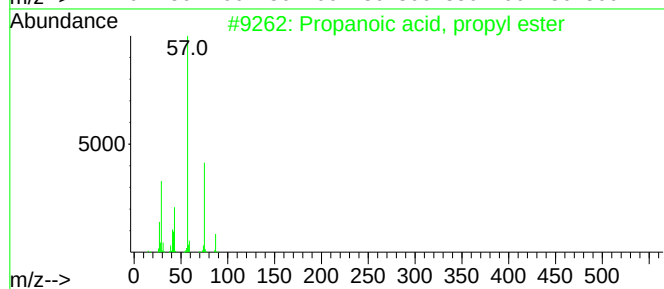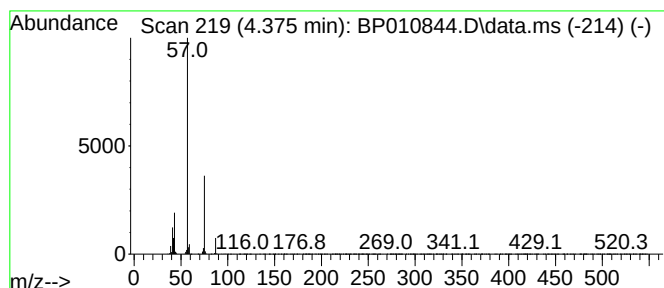

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010844.D
Acq On : 26 Jun 2022 00:38
Operator : CG/JU
Sample : N3392-03 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl butyrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.822	4.47 ng/ul	656166	1,4-Dichlorobenzene-d4	7.716

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl butyrate	130	C7H14O2	000638-11-9	94
2			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
3			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
4			Propanoic acid, 2-methyl-, 1-met...	130	C7H14O2	000617-50-5	72
5			Propanoic acid, 2-methyl-, 1-met...	130	C7H14O2	000617-50-5	72

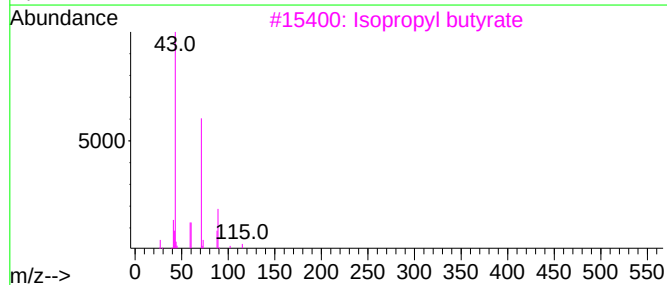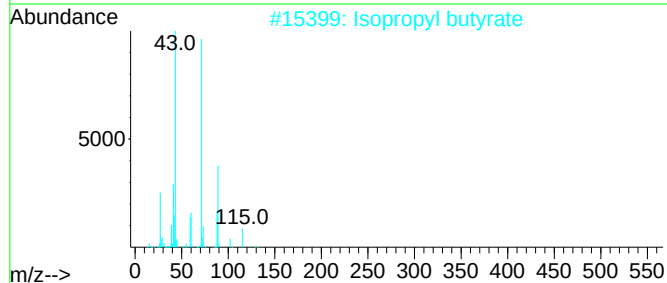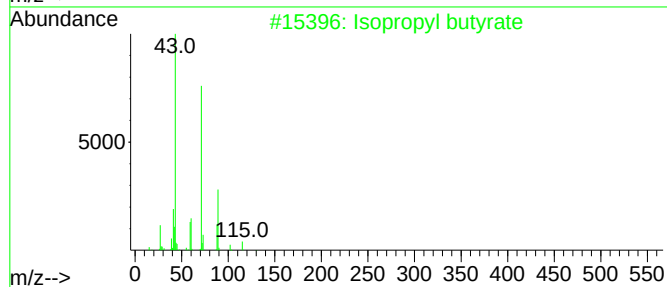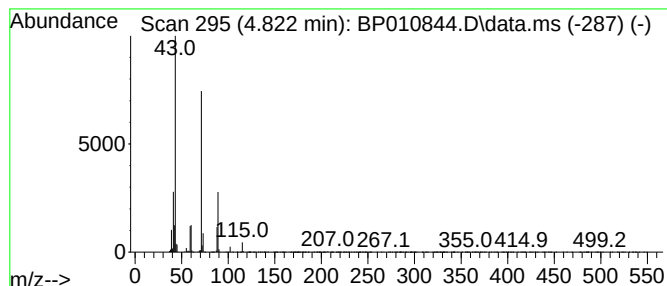

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010844.D
Acq On : 26 Jun 2022 00:38
Operator : CG/JU
Sample : N3392-03 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propanoic acid,...	4.375	2.1	ng/ul	306369	1	7.716	2932660	20.0
Isopropyl butyrate	4.822	4.5	ng/ul	656166	1	7.716	2932660	20.0