

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010846.D
 Acq On : 26 Jun 2022 01:45
 Operator : CG/JU
 Sample : N3392-09 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	17	21	23	rBV	70574	88636	0.82%	0.083%
2	3.246	23	27	38	rVB	1176110	1334689	12.32%	1.248%
3	3.546	75	78	83	rVB	31948	38127	0.35%	0.036%
4	3.617	87	90	95	rBV	543648	687345	6.34%	0.643%
5	3.664	95	98	107	rVB	155543	207938	1.92%	0.194%
6	3.840	121	128	133	rVV2	59695	100187	0.92%	0.094%
7	3.899	133	138	139	rVV3	11746	15858	0.15%	0.015%
8	3.934	139	144	149	rVB2	48502	75970	0.70%	0.071%
9	4.193	184	188	195	rVB	40828	53613	0.49%	0.050%
10	4.264	195	200	204	rBV	92469	118337	1.09%	0.111%
11	4.369	213	218	226	rBV	1227859	1615617	14.91%	1.510%
12	4.434	226	229	235	rVV	145273	186346	1.72%	0.174%
13	4.481	235	237	242	rVB3	9052	13776	0.13%	0.013%
14	4.652	261	266	274	rVB3	7578	12287	0.11%	0.011%
15	4.716	274	277	281	rBV3	10510	15733	0.15%	0.015%
16	4.822	289	295	304	rBV	708217	931946	8.60%	0.871%
17	5.081	335	339	346	rVB3	8586	11921	0.11%	0.011%
18	5.316	375	379	383	rVB2	8553	12376	0.11%	0.012%
19	5.440	396	400	406	rVB2	11490	19444	0.18%	0.018%
20	5.681	436	441	446	rBV2	29960	43987	0.41%	0.041%
21	6.693	608	613	617	rBV	13288	22547	0.21%	0.021%
22	6.728	617	619	624	rVV6	7231	11635	0.11%	0.011%
23	6.810	627	633	635	rVV6	7192	13524	0.12%	0.013%
24	6.893	638	647	661	rVB	498964	772342	7.13%	0.722%
25	7.058	664	675	684	rBV	2037029	3079575	28.43%	2.879%
26	7.134	684	688	693	rVB	11150	16194	0.15%	0.015%
27	7.252	700	708	716	rBV	1847059	2870490	26.50%	2.684%
28	7.346	719	724	732	rVB10	14077	36890	0.34%	0.034%
29	7.716	778	787	795	rBV	1831197	2810226	25.94%	2.627%
30	7.787	795	799	807	rVB	30091	45716	0.42%	0.043%
31	8.081	842	849	855	rVB4	11225	22120	0.20%	0.021%
32	8.428	901	908	918	rBV	1369288	2181404	20.14%	2.039%
33	8.540	921	927	934	rVB	83776	137291	1.27%	0.128%
34	8.646	941	945	953	rVB7	7421	14304	0.13%	0.013%
35	8.822	970	975	977	rBV5	7786	12065	0.11%	0.011%
36	8.875	977	984	993	rVV	2211691	3465091	31.99%	3.239%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010846.D
 Acq On : 26 Jun 2022 01:45
 Operator : CG/JU
 Sample : N3392-09 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	9.004	1002	1006	1011	rBV5	7174	11548	0.11%	0.011%
38	9.116	1020	1025	1032	rVB2	16257	29793	0.28%	0.028%
39	9.304	1052	1057	1061	rVB3	7601	13234	0.12%	0.012%
40	9.381	1065	1070	1073	rBV4	17923	33699	0.31%	0.032%
41	9.434	1076	1079	1084	rVB4	25896	40839	0.38%	0.038%
42	9.593	1098	1106	1123	rBV	1469376	2476019	22.86%	2.315%
43	9.910	1156	1160	1165	rVV7	8333	12828	0.12%	0.012%
44	10.046	1175	1183	1188	rBV10	9842	22939	0.21%	0.021%
45	10.134	1191	1198	1206	rBV	2353146	3708822	34.24%	3.467%
46	10.199	1206	1209	1216	rVB8	12194	24664	0.23%	0.023%
47	10.440	1244	1250	1254	rVB4	14763	23687	0.22%	0.022%
48	10.510	1254	1262	1268	rVV	2401369	3906162	36.06%	3.652%
49	10.557	1268	1270	1276	rVB	43030	60497	0.56%	0.057%
50	10.651	1276	1286	1298	rBV	2168798	3604018	33.27%	3.369%
51	10.734	1298	1300	1308	rVB9	14090	23953	0.22%	0.022%
52	11.063	1352	1356	1362	rBV	18104	27114	0.25%	0.025%
53	11.128	1362	1367	1373	rVV2	22096	36436	0.34%	0.034%
54	11.316	1393	1399	1404	rBV10	5539	11261	0.10%	0.011%
55	12.104	1526	1533	1541	rVV	50433	86661	0.80%	0.081%
56	12.181	1541	1546	1554	rVB2	26049	46974	0.43%	0.044%
57	12.310	1559	1568	1575	rBV10	7229	21921	0.20%	0.020%
58	12.398	1577	1583	1589	rVV	19517	32008	0.30%	0.030%
59	13.198	1714	1719	1726	rVB7	10765	18851	0.17%	0.018%
60	13.281	1726	1733	1737	rBV7	10564	20715	0.19%	0.019%
61	13.698	1799	1804	1807	rVB6	8986	15743	0.15%	0.015%
62	13.792	1813	1820	1826	rBV	4025419	5529730	51.04%	5.170%
63	13.834	1826	1827	1832	rVB	20993	22030	0.20%	0.021%
64	14.063	1857	1866	1881	rBV	4795349	6974094	64.38%	6.520%
65	14.287	1899	1904	1909	rVB2	21250	29574	0.27%	0.028%
66	14.369	1911	1918	1926	rVV	3079665	4394552	40.57%	4.108%
67	14.434	1927	1929	1938	rVB9	11046	20672	0.19%	0.019%
68	14.581	1949	1954	1966	rBV	275922	439853	4.06%	0.411%
69	14.734	1975	1980	1984	rBV7	12515	19403	0.18%	0.018%
70	14.792	1984	1990	1996	rVB7	9211	22906	0.21%	0.021%
71	15.157	2046	2052	2056	rBV	72762	115852	1.07%	0.108%
72	15.369	2081	2088	2095	rBV	5957242	8405880	77.59%	7.858%
73	15.487	2102	2108	2116	rBV	1005216	1331433	12.29%	1.245%
74	15.610	2124	2129	2135	rVB2	72560	102364	0.94%	0.096%
75	15.881	2172	2175	2180	rVB4	9601	17224	0.16%	0.016%
76	15.939	2180	2185	2188	rBV7	7241	13845	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010846.D
 Acq On : 26 Jun 2022 01:45
 Operator : CG/JU
 Sample : N3392-09 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

77	16.081	2204	2209	2218	rVB	160158	226099	2.09%	0.211%
78	16.157	2218	2222	2226	rVB3	22358	29342	0.27%	0.027%
79	16.810	2329	2333	2338	rVB7	10055	16393	0.15%	0.015%
80	16.916	2345	2351	2356	rBV8	13464	28156	0.26%	0.026%
81	17.133	2381	2388	2398	rBV	3150331	4431398	40.91%	4.143%
82	17.233	2398	2405	2421	rVV2	6076544	8468080	78.17%	7.916%
83	17.386	2427	2431	2439	rVB7	12834	24239	0.22%	0.023%
84	17.516	2448	2453	2455	rBV6	9490	15039	0.14%	0.014%
85	17.822	2501	2505	2510	rBV8	14669	26861	0.25%	0.025%
86	19.057	2711	2715	2721	rBV2	77502	104103	0.96%	0.097%
87	19.127	2723	2727	2731	rVV	66160	88916	0.82%	0.083%
88	19.480	2781	2787	2794	rBV	6957355	9431188	87.06%	8.817%
89	19.533	2794	2796	2802	rVB2	39631	54316	0.50%	0.051%
90	20.974	3038	3041	3045	rBV2	133340	148796	1.37%	0.139%
91	21.245	3082	3087	3092	rBV	3913075	4880251	45.05%	4.562%
92	23.457	3456	3463	3474	rVB2	5765552	10833234	100.00%	10.128%
93	23.610	3482	3489	3498	rVB2	2716960	5316117	49.07%	4.970%


Sum of corrected areas: 106967873

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010846.D
Acq On : 26 Jun 2022 01:45
Operator : CG/JU
Sample : N3392-09 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

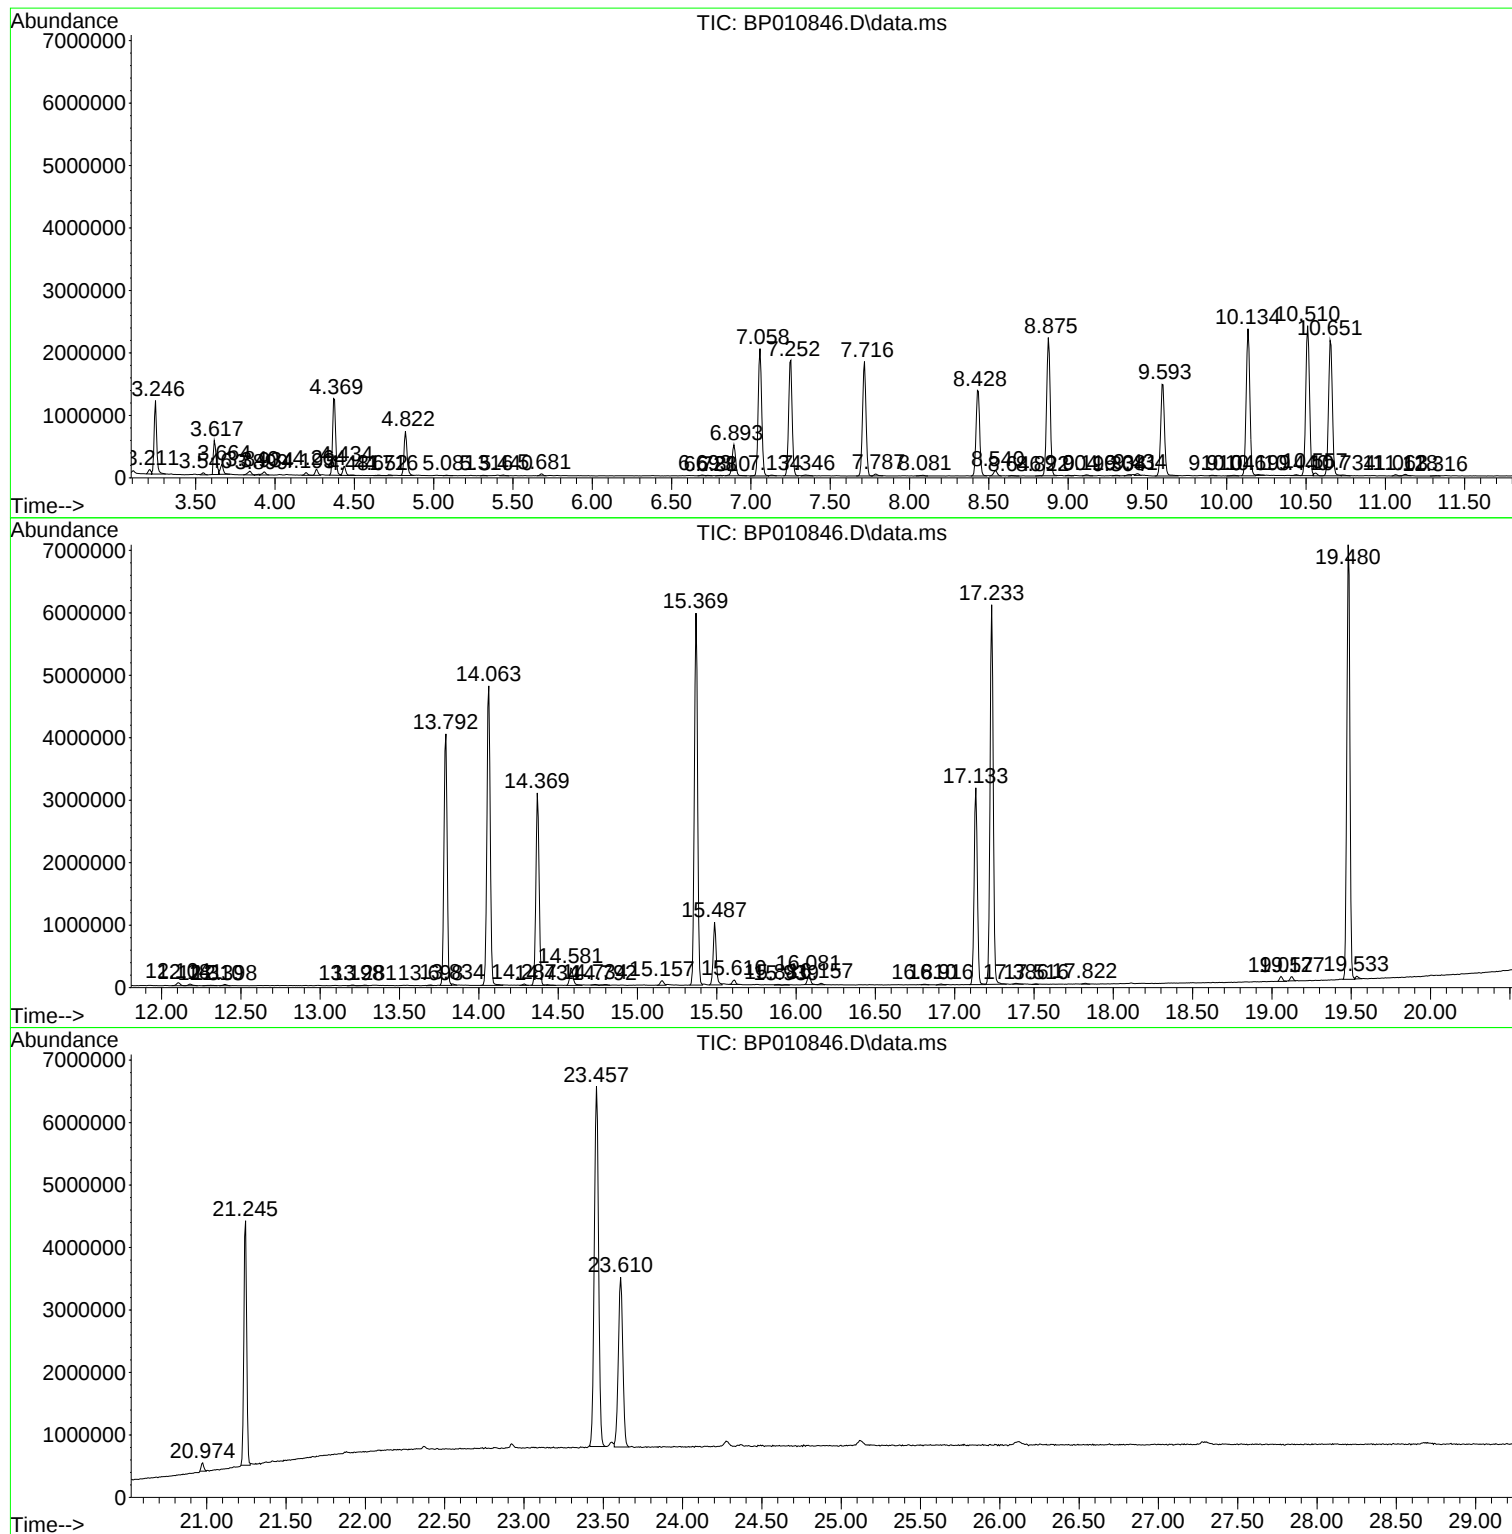

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010846.D
Acq On : 26 Jun 2022 01:45
Operator : CG/JU
Sample : N3392-09 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propanoic acid, propyl ester Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.369	11.50 ng/ul	1615620	1,4-Dichlorobenzene-d4	7.716

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	83
2			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	83
3			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
4			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
5			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	64

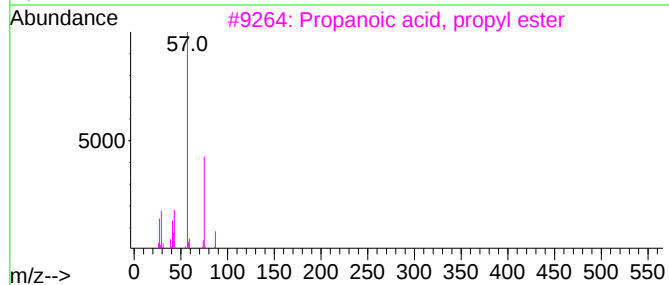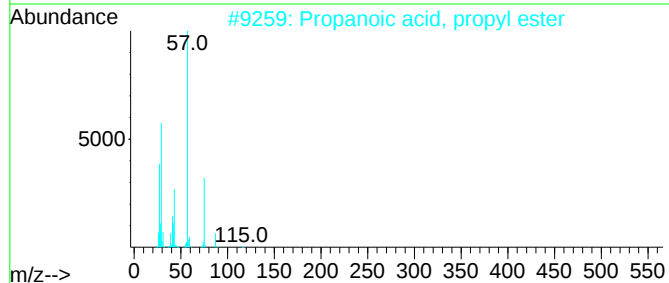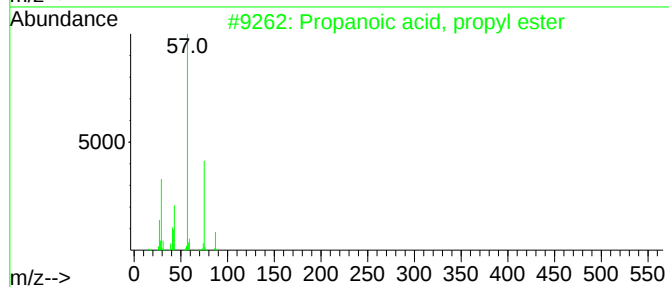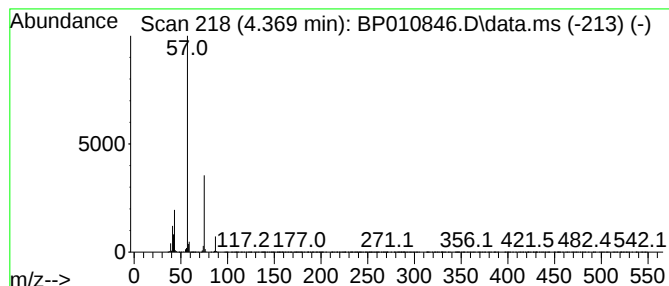

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010846.D
Acq On : 26 Jun 2022 01:45
Operator : CG/JU
Sample : N3392-09 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl butyrate Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.822	6.63 ng/ul	931946	1,4-Dichlorobenzene-d4	7.716

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl butyrate	130	C7H14O2	000638-11-9	94
2			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
3			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
4			Ethylene glycol Formate Isobutyrate	160	C7H12O4	1000458-48-0	64
5			Butanoic acid, butyl ester	144	C8H16O2	000109-21-7	64

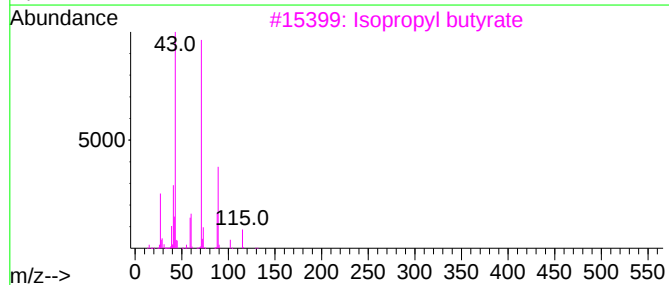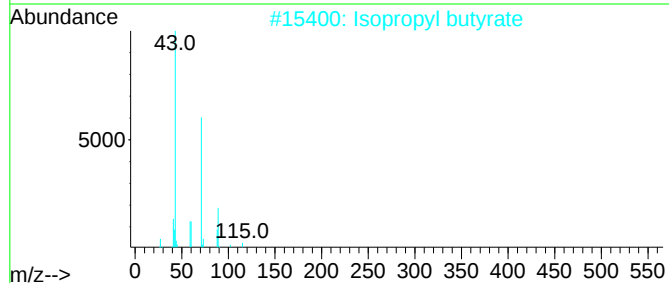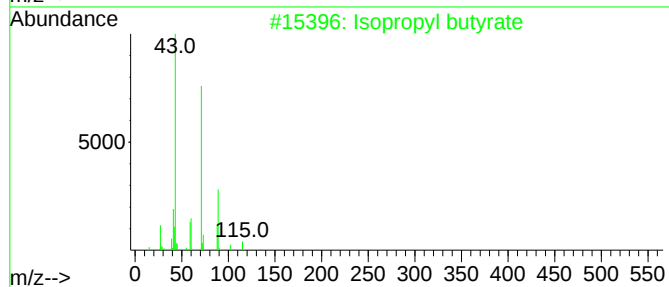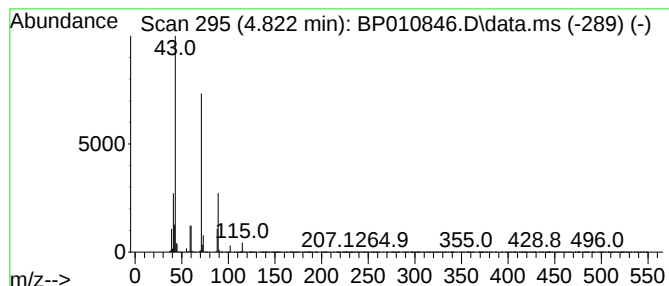

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010846.D
Acq On : 26 Jun 2022 01:45
Operator : CG/JU
Sample : N3392-09 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propanoic acid,...	4.369	11.5	ng/ul	1615620	1	7.716	2810230	20.0
Isopropyl butyrate	4.822	6.6	ng/ul	931946	1	7.716	2810230	20.0