

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010853.D
 Acq On : 26 Jun 2022 06:15
 Operator : CG/JU
 Sample : PB145766BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK766

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	27	rVB	168793	203821	2.11%	0.190%
2	3.611	86	89	113	rBV	1951192	2766351	28.58%	2.572%
3	3.934	140	144	151	rVB	45309	66356	0.69%	0.062%
4	6.893	639	647	657	rBV	2081197	3162314	32.67%	2.941%
5	7.058	668	675	684	rVB	1729136	2636171	27.23%	2.451%
6	7.146	686	690	697	rVB4	7365	12415	0.13%	0.012%
7	7.246	700	707	720	rBV	2176494	3339266	34.50%	3.105%
8	7.710	779	786	796	rBV	1868897	2939288	30.37%	2.733%
9	8.163	856	863	869	rBV8	9537	15457	0.16%	0.014%
10	8.428	900	908	917	rBV	2550789	3925630	40.56%	3.650%
11	8.493	917	919	924	rVV5	13315	22388	0.23%	0.021%
12	8.540	924	927	934	rVB6	12244	20188	0.21%	0.019%
13	8.875	975	984	996	rBV	1898107	2989649	30.89%	2.780%
14	9.452	1072	1082	1087	rBV4	7752	15980	0.17%	0.015%
15	9.593	1097	1106	1115	rBV	1408397	2221989	22.96%	2.066%
16	9.693	1120	1123	1128	rVB7	10726	17173	0.18%	0.016%
17	9.934	1160	1164	1169	rVB6	7458	14001	0.14%	0.013%
18	10.134	1190	1198	1213	rBV	2240145	3647843	37.69%	3.392%
19	10.510	1254	1262	1269	rBV	2541023	4109586	42.46%	3.821%
20	10.557	1269	1270	1276	rVB3	12358	11590	0.12%	0.011%
21	10.652	1278	1286	1300	rVV	2401030	3932135	40.62%	3.656%
22	10.846	1313	1319	1325	rVB	7399	13965	0.14%	0.013%
23	11.810	1477	1483	1488	rBV8	10577	17756	0.18%	0.017%
24	12.104	1527	1533	1540	rBV	46753	77069	0.80%	0.072%
25	12.181	1542	1546	1551	rVB2	12345	20633	0.21%	0.019%
26	12.316	1559	1569	1572	rBV2	7855	20465	0.21%	0.019%
27	12.398	1579	1583	1589	rVB2	13416	22038	0.23%	0.020%
28	12.546	1601	1608	1613	rVB6	13267	25442	0.26%	0.024%
29	12.787	1645	1649	1656	rVB10	9346	17431	0.18%	0.016%
30	12.863	1656	1662	1670	rBV8	11606	21996	0.23%	0.020%
31	13.093	1695	1701	1705	rBV9	5495	9978	0.10%	0.009%
32	13.157	1705	1712	1716	rVV6	13065	22516	0.23%	0.021%
33	13.198	1716	1719	1723	rVV	16857	25264	0.26%	0.023%
34	13.240	1723	1726	1730	rVB2	11717	16733	0.17%	0.016%
35	13.334	1738	1742	1751	rVB8	6856	9757	0.10%	0.009%
36	13.787	1809	1819	1825	rBV	3506070	4797466	49.56%	4.461%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010853.D
 Acq On : 26 Jun 2022 06:15
 Operator : CG/JU
 Sample : PB145766BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK766

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	13.951	1842	1847	1851	rBV8	5967	10559	0.11%	0.010%
38	14.057	1858	1865	1877	rBV	4166311	5992061	61.90%	5.572%
39	14.369	1911	1918	1925	rBV	3353228	4796587	49.55%	4.460%
40	14.434	1925	1929	1934	rVB3	19823	31443	0.32%	0.029%
41	14.581	1947	1954	1968	rBV	1740636	2465291	25.47%	2.292%
42	14.687	1968	1972	1976	rVV5	17405	31760	0.33%	0.030%
43	14.734	1976	1980	1983	rVV6	10725	17660	0.18%	0.016%
44	14.769	1983	1986	1990	rVB2	14388	19091	0.20%	0.018%
45	15.010	2020	2027	2029	rBV7	9785	19403	0.20%	0.018%
46	15.034	2029	2031	2037	rVB7	7794	12799	0.13%	0.012%
47	15.204	2055	2060	2066	rBV2	16866	28381	0.29%	0.026%
48	15.369	2081	2088	2094	rBV	5123007	7273812	75.14%	6.764%
49	15.422	2094	2097	2102	rVV3	44015	70412	0.73%	0.065%
50	15.487	2102	2108	2123	rVV	994029	1378628	14.24%	1.282%
51	15.610	2124	2129	2132	rVV	62650	100638	1.04%	0.094%
52	15.639	2132	2134	2141	rVB2	22015	27750	0.29%	0.026%
53	16.157	2218	2222	2227	rVB3	18657	25435	0.26%	0.024%
54	16.322	2246	2250	2256	rVB7	16113	22880	0.24%	0.021%
55	16.428	2263	2268	2272	rVB7	13924	19981	0.21%	0.019%
56	16.604	2294	2298	2301	rBV5	8318	12258	0.13%	0.011%
57	16.775	2324	2327	2330	rBV5	10135	13868	0.14%	0.013%
58	16.804	2330	2332	2338	rVB6	10065	15710	0.16%	0.015%
59	16.916	2347	2351	2354	rBV3	11468	14782	0.15%	0.014%
60	17.134	2381	2388	2394	rBV	3671731	5251237	54.25%	4.883%
61	17.175	2394	2395	2398	rVV	30507	23587	0.24%	0.022%
62	17.234	2398	2405	2420	rVV	5471648	7693061	79.48%	7.154%
63	17.386	2427	2431	2436	rBV8	11675	19220	0.20%	0.018%
64	17.545	2454	2458	2464	rVB	19073	30285	0.31%	0.028%
65	18.116	2552	2555	2558	rVB	17239	21789	0.23%	0.020%
66	19.057	2711	2715	2720	rBV	69313	88120	0.91%	0.082%
67	19.122	2723	2726	2730	rBV2	60044	81922	0.85%	0.076%
68	19.480	2781	2787	2795	rBV	6887134	8909320	92.04%	8.285%
69	21.245	3081	3087	3092	rBV	4601247	5986390	61.84%	5.567%
70	23.457	3456	3463	3474	rVB2	5082130	9679756	100.00%	9.001%
71	23.610	3482	3489	3501	rVB2	3135872	6164733	63.69%	5.733%




Sum of corrected areas: 107538709

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010853.D
Acq On : 26 Jun 2022 06:15
Operator : CG/JU
Sample : PB145766BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK766

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

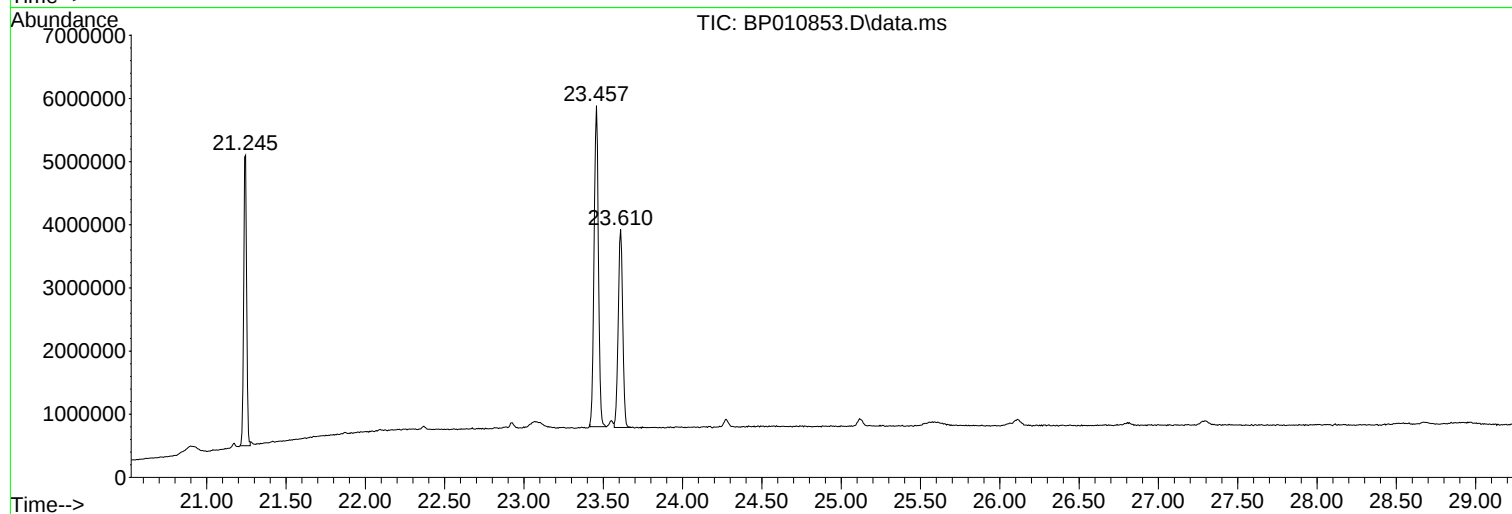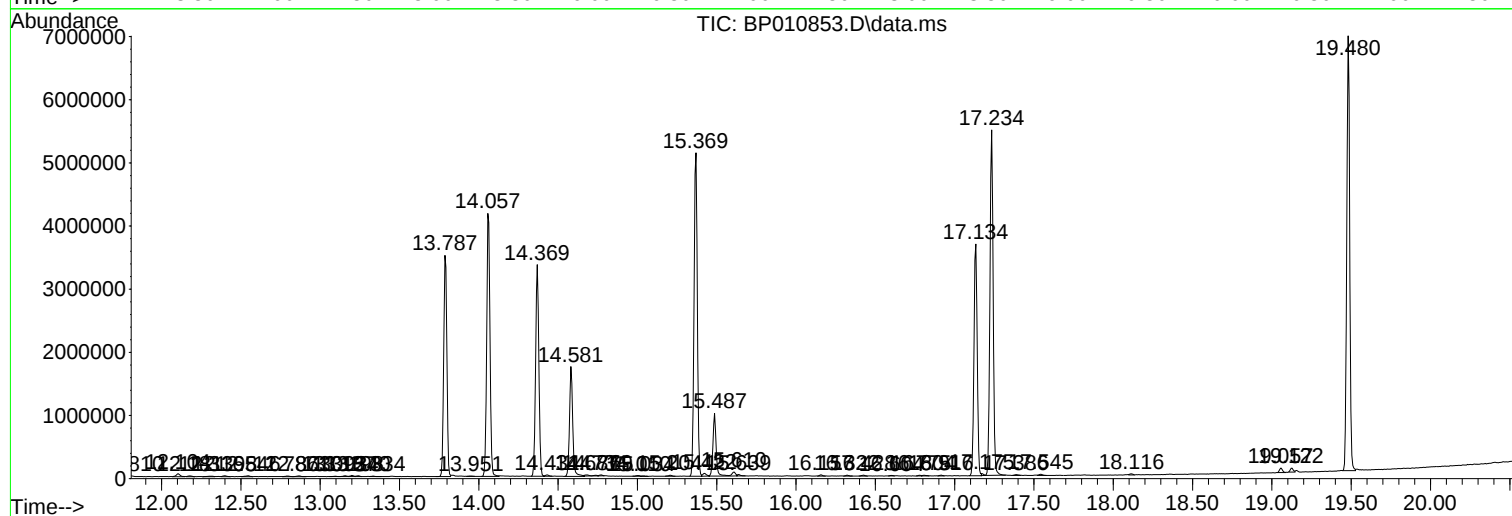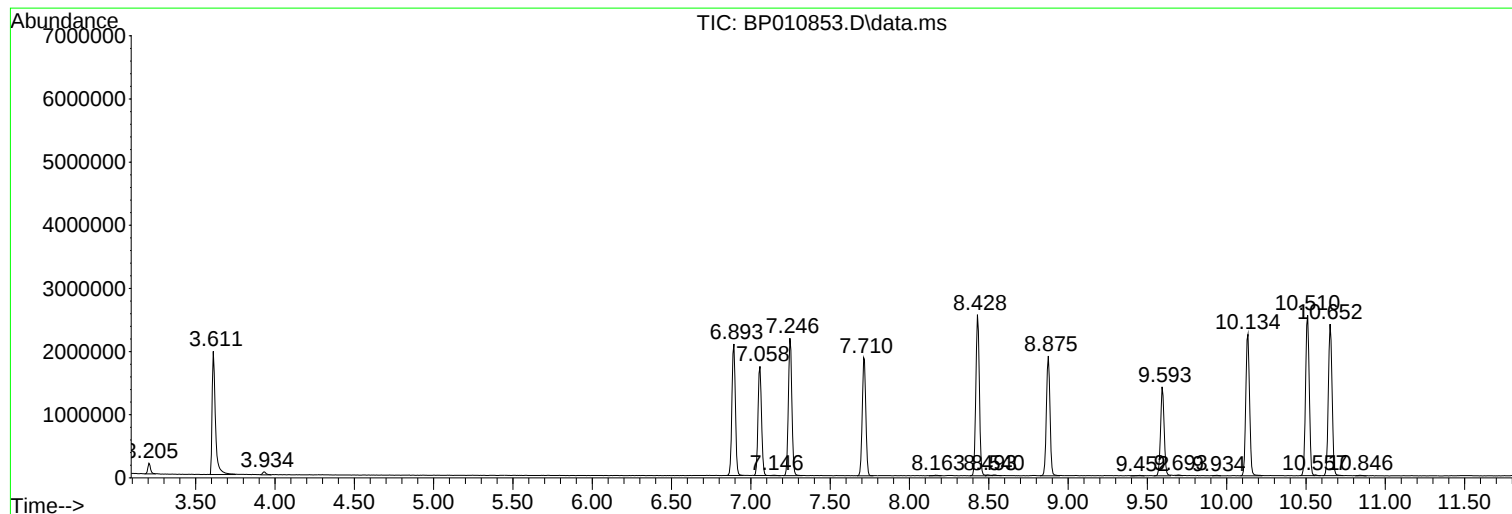

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010853.D
Acq On : 26 Jun 2022 06:15
Operator : CG/JU
Sample : PB145766BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK766

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010853.D
Acq On : 26 Jun 2022 06:15
Operator : CG/JU
Sample : PB145766BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK766

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------