

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010855.D
 Acq On : 26 Jun 2022 07:22
 Operator : CG/JU
 Sample : N3392-07 10X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	17	21	23	rBV2	55648	74322	0.75%	0.079%
2	3.246	23	27	37	rVB	1010510	1172556	11.87%	1.243%
3	3.546	73	78	84	rVB	30947	45435	0.46%	0.048%
4	3.617	87	90	95	rBV	280916	371769	3.76%	0.394%
5	3.664	95	98	106	rVB	164354	203660	2.06%	0.216%
6	3.840	122	128	134	rVV	61322	91206	0.92%	0.097%
7	3.917	134	141	150	rVB2	161281	263341	2.67%	0.279%
8	4.075	164	168	172	rBV	25019	33131	0.34%	0.035%
9	4.193	183	188	194	rVV	193446	240324	2.43%	0.255%
10	4.258	196	199	203	rVV	40999	53223	0.54%	0.056%
11	4.299	204	206	211	rVV6	9439	13528	0.14%	0.014%
12	4.370	213	218	224	rVV	470843	595657	6.03%	0.631%
13	4.434	224	229	235	rVV	208124	269381	2.73%	0.285%
14	4.481	235	237	243	rVB4	9853	15865	0.16%	0.017%
15	4.658	263	267	271	rVB4	6542	10693	0.11%	0.011%
16	4.722	274	278	281	rBV3	10238	14678	0.15%	0.016%
17	4.822	288	295	304	rVB	506002	689016	6.97%	0.730%
18	5.317	374	379	384	rBV3	13327	19537	0.20%	0.021%
19	5.369	384	388	396	rVB10	5188	10773	0.11%	0.011%
20	5.440	396	400	403	rBV	9689	14177	0.14%	0.015%
21	5.517	411	413	419	rVB7	6434	11988	0.12%	0.013%
22	5.675	435	440	445	rBV2	39617	59140	0.60%	0.063%
23	6.399	555	563	569	rVB	24809	42881	0.43%	0.045%
24	6.887	638	646	659	rVB	411333	663689	6.72%	0.703%
25	7.052	667	674	684	rBV	1677662	2640714	26.73%	2.798%
26	7.128	684	687	692	rVB	13270	19225	0.19%	0.020%
27	7.246	699	707	719	rBV	1629502	2477384	25.07%	2.625%
28	7.340	719	723	726	rBV6	9512	15568	0.16%	0.016%
29	7.711	779	786	794	rBV	1614993	2518359	25.49%	2.669%
30	7.787	794	799	805	rVV	25601	37206	0.38%	0.039%
31	8.428	900	908	917	rBV	1197066	1834805	18.57%	1.944%
32	8.540	920	927	933	rVB	74719	124857	1.26%	0.132%
33	8.875	976	984	993	rBV	1876527	2953363	29.89%	3.130%
34	9.305	1052	1057	1061	rVB3	17380	27010	0.27%	0.029%
35	9.381	1061	1070	1071	rBV5	15529	24723	0.25%	0.026%
36	9.434	1076	1079	1089	rVB7	25246	47558	0.48%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010855.D
 Acq On : 26 Jun 2022 07:22
 Operator : CG/JU
 Sample : N3392-07 10X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	9.593	1099	1106	1123	rBV	1281565	2059394	20.84%	2.182%
38	9.910	1157	1160	1167	rVB9	8501	12624	0.13%	0.013%
39	10.040	1174	1182	1188	rBV10	9858	26036	0.26%	0.028%
40	10.134	1190	1198	1206	rBV	1923239	3138070	31.76%	3.326%
41	10.199	1207	1209	1215	rVB6	15488	22875	0.23%	0.024%
42	10.434	1245	1249	1255	rBV5	12900	20598	0.21%	0.022%
43	10.510	1255	1262	1268	rBV	2139318	3501511	35.44%	3.711%
44	10.557	1268	1270	1276	rVB	17798	23675	0.24%	0.025%
45	10.652	1278	1286	1298	rBV	1858287	3032903	30.70%	3.214%
46	11.063	1352	1356	1361	rBV2	16008	27820	0.28%	0.029%
47	11.122	1361	1366	1371	rVV	20012	37066	0.38%	0.039%
48	11.157	1371	1372	1378	rVB5	8930	12033	0.12%	0.013%
49	11.316	1395	1399	1406	rVB10	6023	11842	0.12%	0.013%
50	12.104	1528	1533	1541	rVB	41462	67670	0.68%	0.072%
51	12.181	1541	1546	1553	rVB3	15083	24933	0.25%	0.026%
52	12.398	1577	1583	1588	rBV3	9393	15567	0.16%	0.016%
53	13.093	1695	1701	1704	rBV8	5682	11080	0.11%	0.012%
54	13.204	1715	1720	1725	rVB4	12963	19615	0.20%	0.021%
55	13.281	1728	1733	1736	rBV7	8798	15403	0.16%	0.016%
56	13.387	1749	1751	1756	rVB6	7358	10084	0.10%	0.011%
57	13.687	1798	1802	1807	rVB8	7596	11725	0.12%	0.012%
58	13.787	1813	1819	1825	rBV	3497634	4632177	46.88%	4.909%
59	13.834	1825	1827	1833	rVB	24139	33349	0.34%	0.035%
60	14.057	1856	1865	1879	rBV	4040228	5841346	59.12%	6.190%
61	14.369	1911	1918	1925	rBV	2757801	3990380	40.39%	4.229%
62	14.428	1925	1928	1938	rVB	26672	47253	0.48%	0.050%
63	14.581	1948	1954	1968	rBV	259784	417185	4.22%	0.442%
64	14.692	1970	1973	1977	rVB2	9216	12989	0.13%	0.014%
65	14.769	1983	1986	1990	rVV	12358	16233	0.16%	0.017%
66	15.004	2017	2026	2027	rBV9	5184	12140	0.12%	0.013%
67	15.151	2045	2051	2056	rBV	58101	92760	0.94%	0.098%
68	15.369	2081	2088	2094	rBV	5049357	7126463	72.13%	7.552%
69	15.422	2094	2097	2102	rVB2	23668	35181	0.36%	0.037%
70	15.487	2102	2108	2117	rBV	818039	1129641	11.43%	1.197%
71	15.610	2123	2129	2135	rVB	62249	89282	0.90%	0.095%
72	15.934	2179	2184	2191	rVB10	6774	18384	0.19%	0.019%
73	16.157	2217	2222	2228	rBV2	17764	25793	0.26%	0.027%
74	16.804	2325	2332	2337	rBV9	15730	34496	0.35%	0.037%
75	16.910	2345	2350	2354	rBV4	13864	23629	0.24%	0.025%
76	17.134	2381	2388	2394	rBV	3070453	4331376	43.84%	4.590%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010855.D
 Acq On : 26 Jun 2022 07:22
 Operator : CG/JU
 Sample : N3392-07 10X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

77	17.234	2398	2405	2421	rVB	5576621	7616778	77.09%	8.072%
78	17.386	2428	2431	2436	rBV5	10813	14670	0.15%	0.016%
79	17.516	2449	2453	2455	rBV4	8391	11007	0.11%	0.012%
80	17.816	2500	2504	2510	rVB8	22936	37203	0.38%	0.039%
81	18.639	2641	2644	2646	rBV3	7639	10416	0.11%	0.011%
82	19.057	2711	2715	2720	rBV	72656	94736	0.96%	0.100%
83	19.128	2723	2727	2730	rBV	63967	79716	0.81%	0.084%
84	19.480	2782	2787	2794	rBV	6653764	8739237	88.45%	9.261%
85	19.539	2794	2797	2803	rVB	51107	64844	0.66%	0.069%
86	21.245	3082	3087	3092	rBV	4015102	4924674	49.85%	5.219%
87	23.457	3456	3463	3474	rVB2	5192344	9879926	100.00%	10.470%
88	23.610	3483	3489	3500	rVB2	2661222	5175456	52.38%	5.485%




Sum of corrected areas: 94361986

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010855.D
Acq On : 26 Jun 2022 07:22
Operator : CG/JU
Sample : N3392-07 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

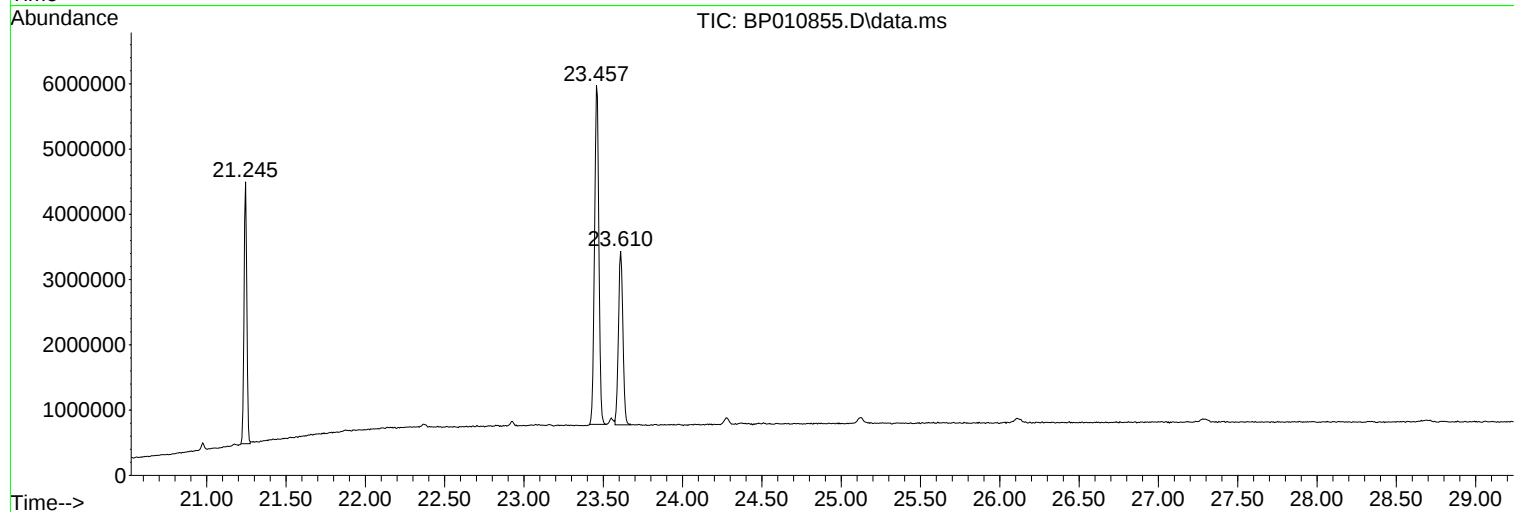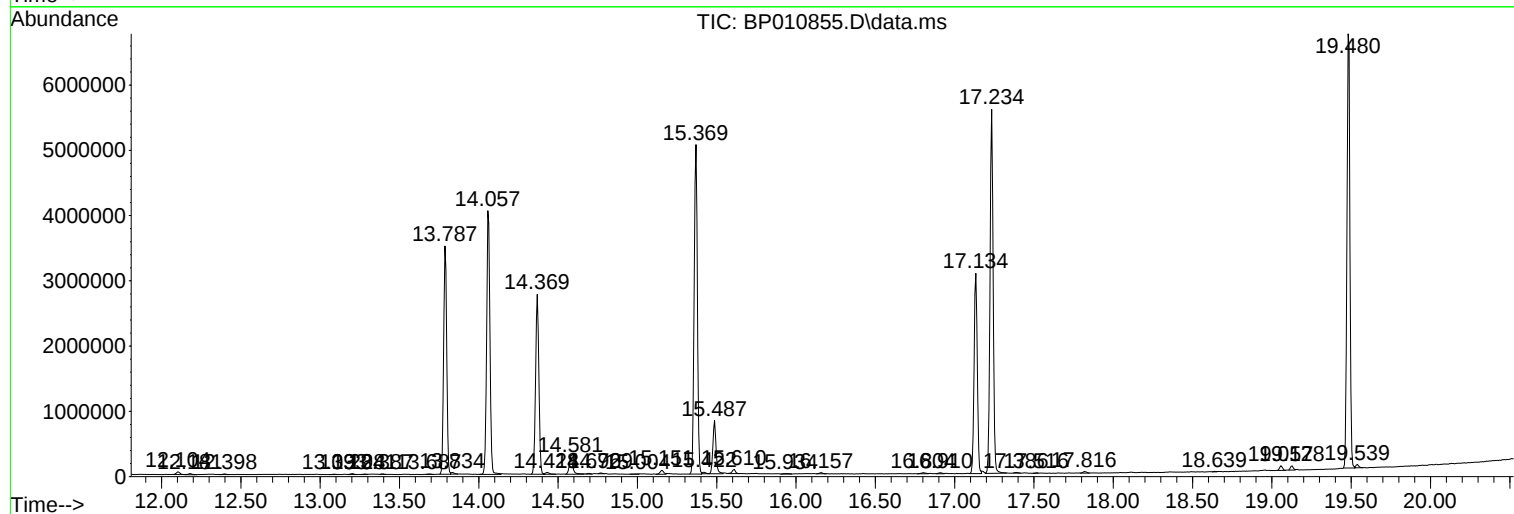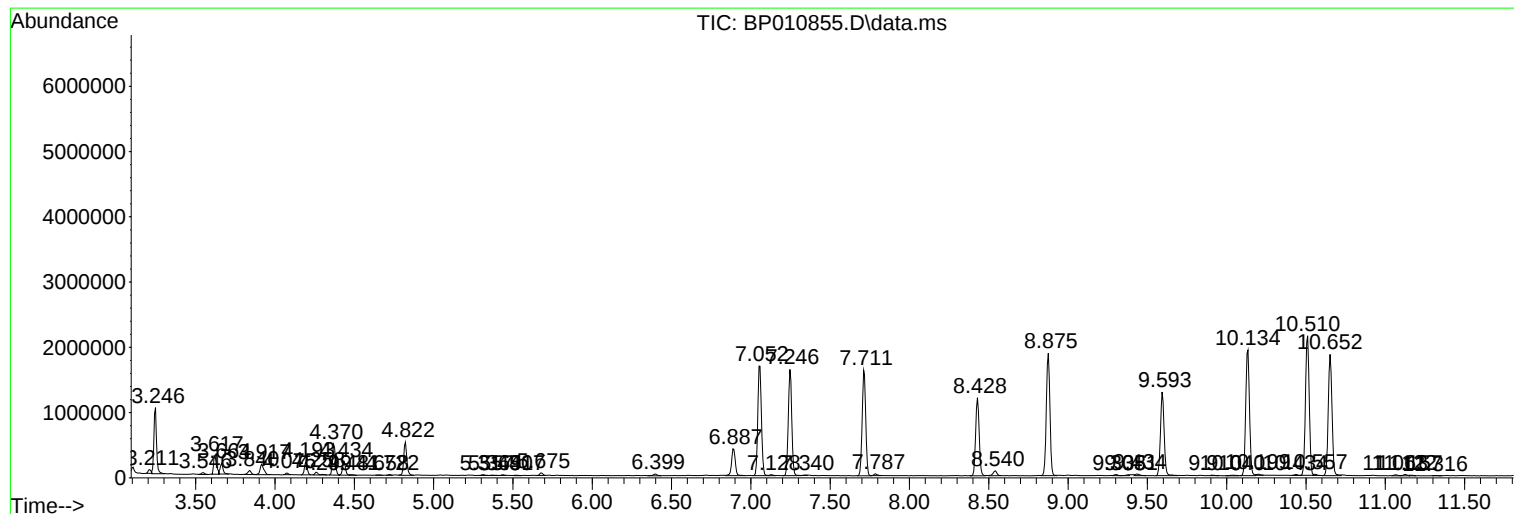

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010855.D
Acq On : 26 Jun 2022 07:22
Operator : CG/JU
Sample : N3392-07 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isobutyl acetate Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.917	2.09 ng/ul	263341	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isobutyl acetate	116	C6H12O2	000110-19-0	64
2			Isobutyl acetate	116	C6H12O2	000110-19-0	64
3			Isobutyl acetate	116	C6H12O2	000110-19-0	50
4			Isobutyl acetate	116	C6H12O2	000110-19-0	50
5			Isobutyl acetate	116	C6H12O2	000110-19-0	50

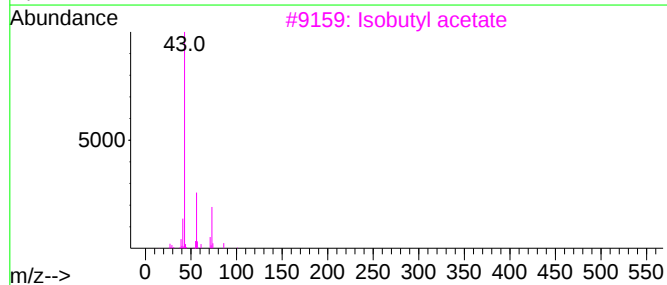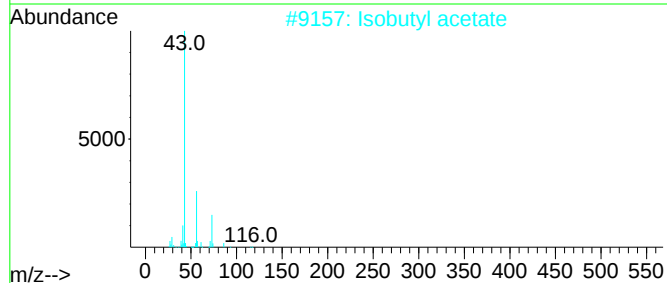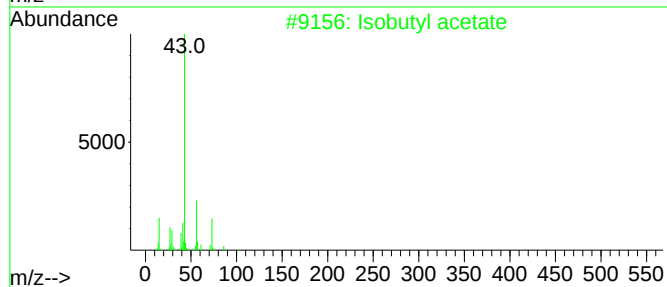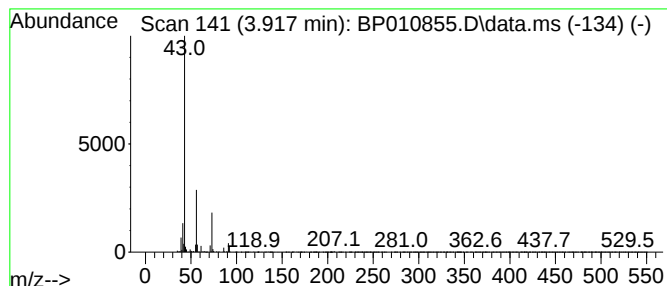

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010855.D
Acq On : 26 Jun 2022 07:22
Operator : CG/JU
Sample : N3392-07 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Propanoic acid, propyl ester Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.370	4.73 ng/ul	595657	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	83
2			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
3			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
4			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	64
5			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	40

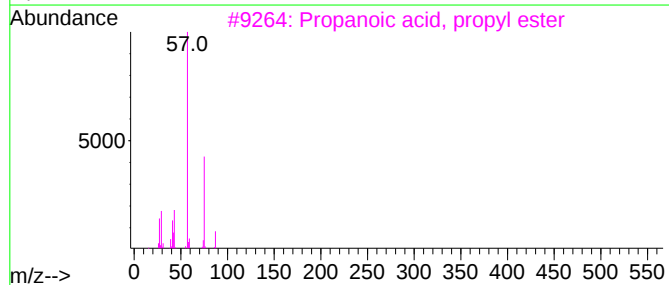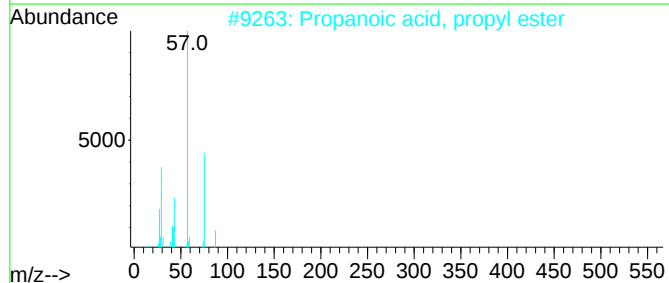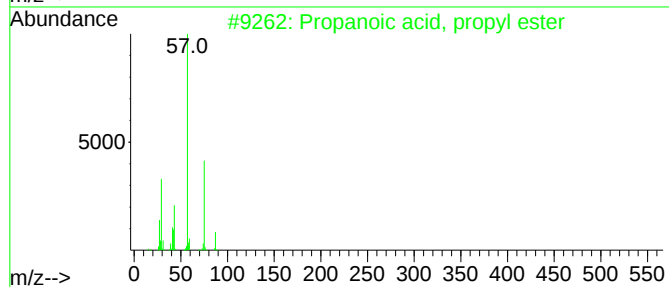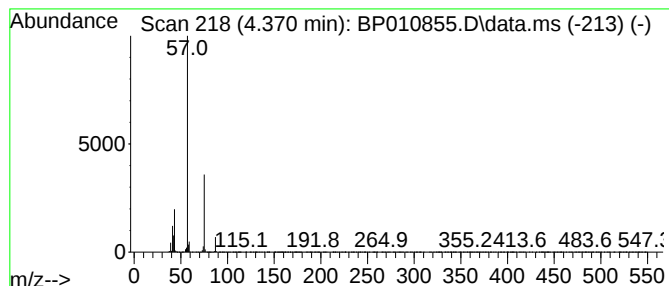

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010855.D
Acq On : 26 Jun 2022 07:22
Operator : CG/JU
Sample : N3392-07 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Acetic acid, butyl ester Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.434	2.14 ng/ul	269381	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Acetic acid, butyl ester	116	C6H12O2	000123-86-4	78		
2	Acetic acid, butyl ester	116	C6H12O2	000123-86-4	78		
3	Acetic acid, butyl ester	116	C6H12O2	000123-86-4	64		
4	Acetic acid, butyl ester	116	C6H12O2	000123-86-4	42		
5	Di-n-propyl ether	102	C6H14O	000111-43-3	12		

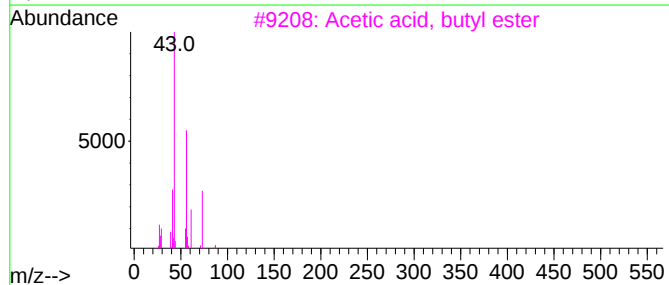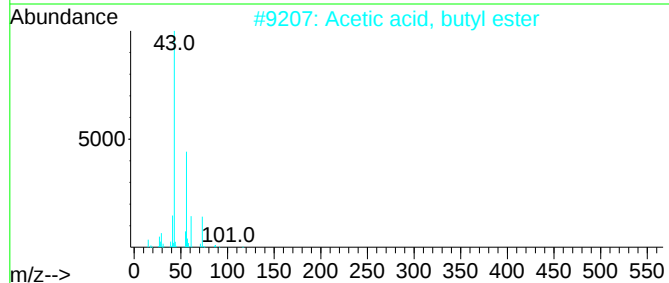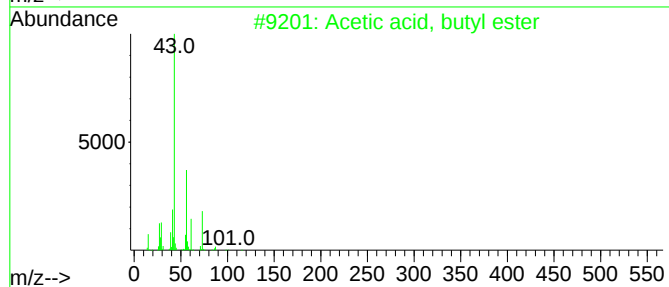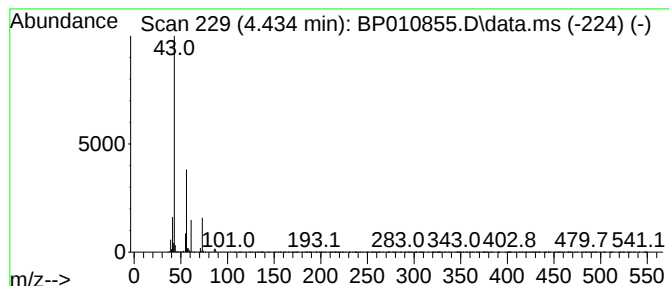

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010855.D
Acq On : 26 Jun 2022 07:22
Operator : CG/JU
Sample : N3392-07 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Isopropyl butyrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.822	5.47 ng/ul	689016	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl butyrate	130	C7H14O2	000638-11-9	94
2			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
3			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
4			Propanoic acid, 2-methyl-, propy...	130	C7H14O2	000644-49-5	64
5			Ethylene glycol Formate Isobutyrate	160	C7H12O4	1000458-48-0	64

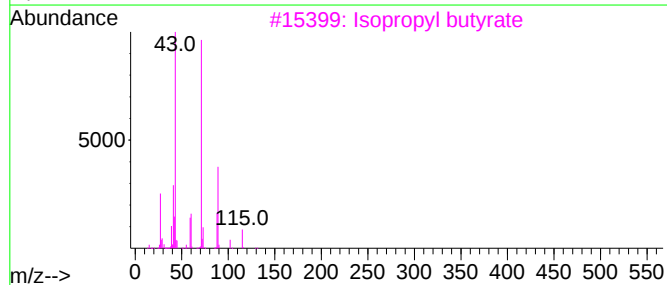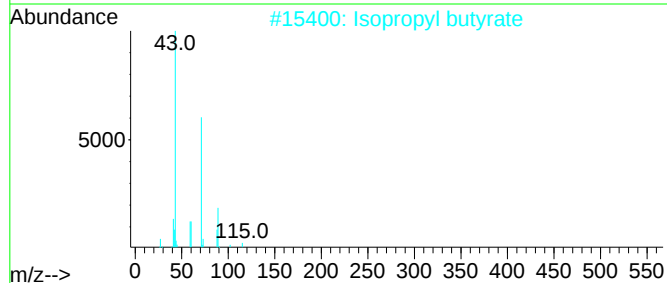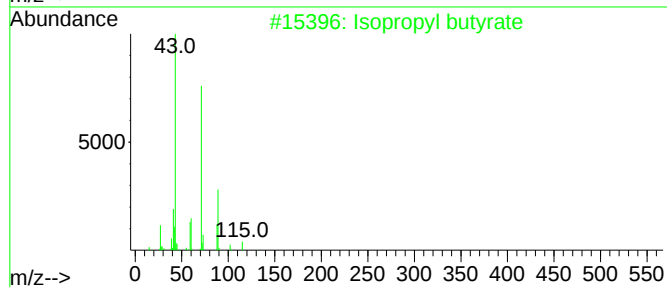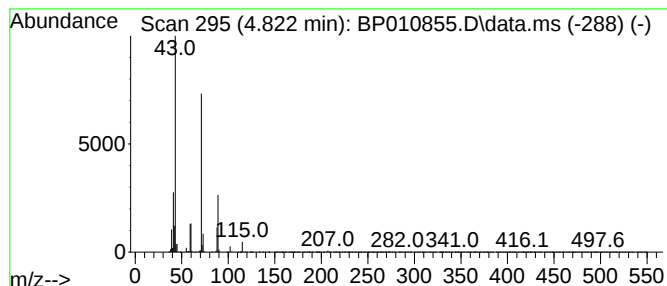

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010855.D
Acq On : 26 Jun 2022 07:22
Operator : CG/JU
Sample : N3392-07 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isobutyl acetate	3.917	2.1	ng/ul	263341	1	7.710	2518360	20.0
Propanoic acid,...	4.370	4.7	ng/ul	595657	1	7.710	2518360	20.0
Acetic acid, bu...	4.434	2.1	ng/ul	269381	1	7.710	2518360	20.0
Isopropyl butyrate	4.822	5.5	ng/ul	689016	1	7.710	2518360	20.0