

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010857.D
 Acq On : 26 Jun 2022 08:30
 Operator : CG/JU
 Sample : N3392-14 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	17	21	23	rBV2	65735	89108	0.71%	0.078%
2	3.246	23	27	37	rVB	920996	1088856	8.63%	0.954%
3	3.546	74	78	84	rVB	23022	30213	0.24%	0.026%
4	3.617	86	90	95	rVV	738071	997599	7.90%	0.874%
5	3.664	95	98	114	rVB	174991	282221	2.24%	0.247%
6	3.840	123	128	133	rVV	58830	87138	0.69%	0.076%
7	3.916	136	141	151	rVB2	173376	283511	2.25%	0.248%
8	4.075	164	168	176	rVB2	26754	41577	0.33%	0.036%
9	4.193	183	188	196	rBV	204846	258311	2.05%	0.226%
10	4.258	196	199	204	rVV	28421	35899	0.28%	0.031%
11	4.299	204	206	213	rVB8	10518	15686	0.12%	0.014%
12	4.369	213	218	224	rBV	310189	397780	3.15%	0.348%
13	4.434	224	229	235	rVV	209793	258038	2.04%	0.226%
14	4.822	288	295	305	rVB	450572	638023	5.05%	0.559%
15	5.316	374	379	382	rVB4	12227	17490	0.14%	0.015%
16	5.434	395	399	404	rBV	10219	15074	0.12%	0.013%
17	5.681	436	441	446	rBV	41569	58611	0.46%	0.051%
18	5.775	453	457	465	rVB7	6858	13552	0.11%	0.012%
19	6.887	636	646	653	rBV	498997	789920	6.26%	0.692%
20	7.057	665	675	688	rVB	1914315	3004382	23.80%	2.631%
21	7.246	700	707	719	rBV	1895723	2917455	23.11%	2.555%
22	7.340	719	723	732	rVB6	10257	27244	0.22%	0.024%
23	7.710	778	786	794	rBV	1803775	2838553	22.49%	2.486%
24	7.787	794	799	804	rBV	17680	28911	0.23%	0.025%
25	8.428	899	908	919	rBV	1465845	2227407	17.64%	1.951%
26	8.540	919	927	933	rVB	70310	120025	0.95%	0.105%
27	8.875	977	984	992	rVV	2146779	3382483	26.79%	2.962%
28	9.381	1065	1070	1071	rBV3	14400	19492	0.15%	0.017%
29	9.434	1076	1079	1089	rVB7	20761	43161	0.34%	0.038%
30	9.593	1099	1106	1114	rBV	1491282	2365376	18.74%	2.071%
31	10.134	1189	1198	1206	rBV	2261514	3714633	29.43%	3.253%
32	10.199	1206	1209	1215	rVB7	16265	26056	0.21%	0.023%
33	10.434	1245	1249	1254	rVB3	10820	18962	0.15%	0.017%
34	10.510	1254	1262	1269	rBV	2385737	3947947	31.27%	3.457%
35	10.651	1278	1286	1297	rBV	2374906	3806406	30.15%	3.333%
36	11.063	1351	1356	1361	rBV	14566	20082	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010857.D
 Acq On : 26 Jun 2022 08:30
 Operator : CG/JU
 Sample : N3392-14 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	11.122	1361	1366	1371	rVV2	18158	30754	0.24%	0.027%
38	12.104	1528	1533	1539	rVB	51039	79052	0.63%	0.069%
39	12.181	1542	1546	1554	rVB4	9965	16490	0.13%	0.014%
40	12.316	1560	1569	1575	rBV4	7878	19216	0.15%	0.017%
41	13.092	1696	1701	1706	rBV8	5689	12820	0.10%	0.011%
42	13.275	1723	1732	1737	rBV7	11086	22342	0.18%	0.020%
43	13.687	1795	1802	1807	rBV7	6316	12842	0.10%	0.011%
44	13.787	1813	1819	1825	rBV	4134702	5743033	45.49%	5.029%
45	13.834	1825	1827	1832	rVB	37555	45336	0.36%	0.040%
46	14.057	1857	1865	1875	rBV	4680375	6841861	54.20%	5.992%
47	14.369	1910	1918	1925	rBV	3199035	4592564	36.38%	4.022%
48	14.434	1925	1929	1932	rVB	14169	21837	0.17%	0.019%
49	14.581	1946	1954	1964	rBV	389498	600613	4.76%	0.526%
50	15.151	2046	2051	2057	rBV	92499	141495	1.12%	0.124%
51	15.369	2080	2088	2095	rBV	6426211	8938878	70.81%	7.828%
52	15.416	2095	2096	2102	rVV4	21007	28059	0.22%	0.025%
53	15.486	2102	2108	2122	rVV	1226730	1651993	13.09%	1.447%
54	15.604	2123	2128	2135	rVB	73969	118898	0.94%	0.104%
55	16.157	2217	2222	2226	rBV3	24101	33453	0.26%	0.029%
56	16.810	2329	2333	2338	rVB6	13610	18980	0.15%	0.017%
57	16.910	2345	2350	2355	rBV6	11629	23065	0.18%	0.020%
58	17.133	2381	2388	2394	rBV	3650836	5107802	40.46%	4.473%
59	17.233	2398	2405	2418	rVV	7480736	10121134	80.17%	8.863%
60	17.386	2427	2431	2439	rBV5	16618	27418	0.22%	0.024%
61	17.816	2501	2504	2511	rVB8	13051	16521	0.13%	0.014%
62	19.057	2711	2715	2720	rBV	92759	121784	0.96%	0.107%
63	19.122	2722	2726	2730	rVV	80324	103110	0.82%	0.090%
64	19.480	2781	2787	2795	rBV	8671685	11547219	91.47%	10.112%
65	21.245	3082	3087	3092	rBV	4589880	5666651	44.89%	4.962%
66	23.457	3456	3463	3474	rVB2	6640794	12623985	100.00%	11.055%
67	23.610	3482	3489	3501	rVB2	3100190	5954251	47.17%	5.214%




Sum of corrected areas: 114190638

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010857.D
Acq On : 26 Jun 2022 08:30
Operator : CG/JU
Sample : N3392-14 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

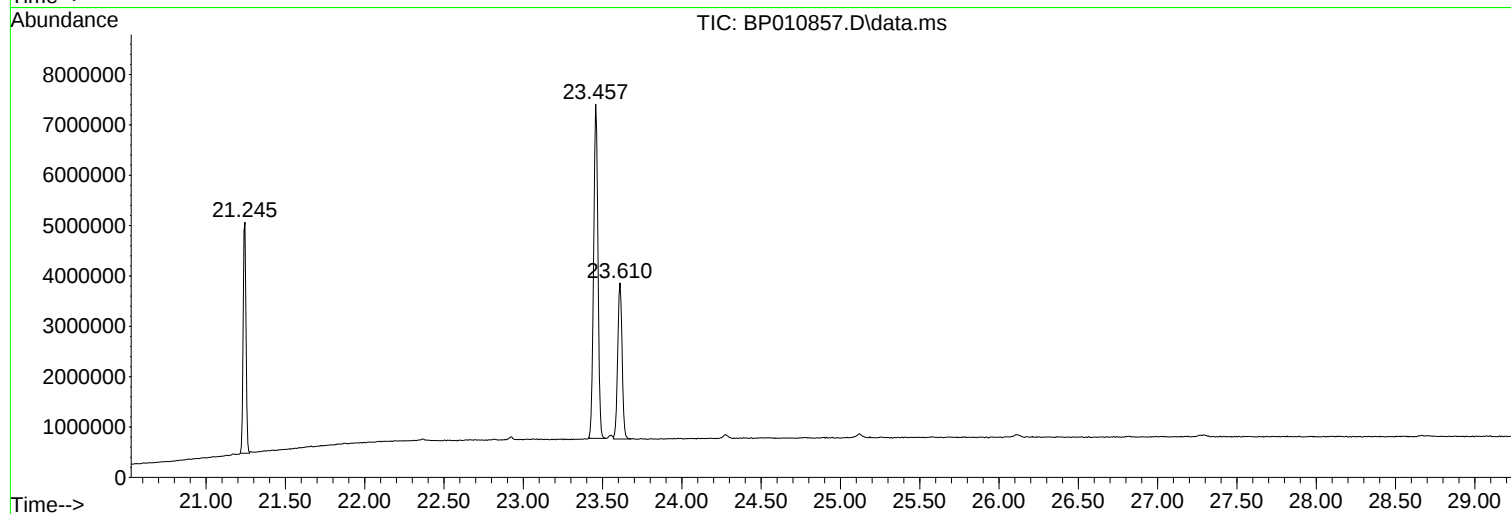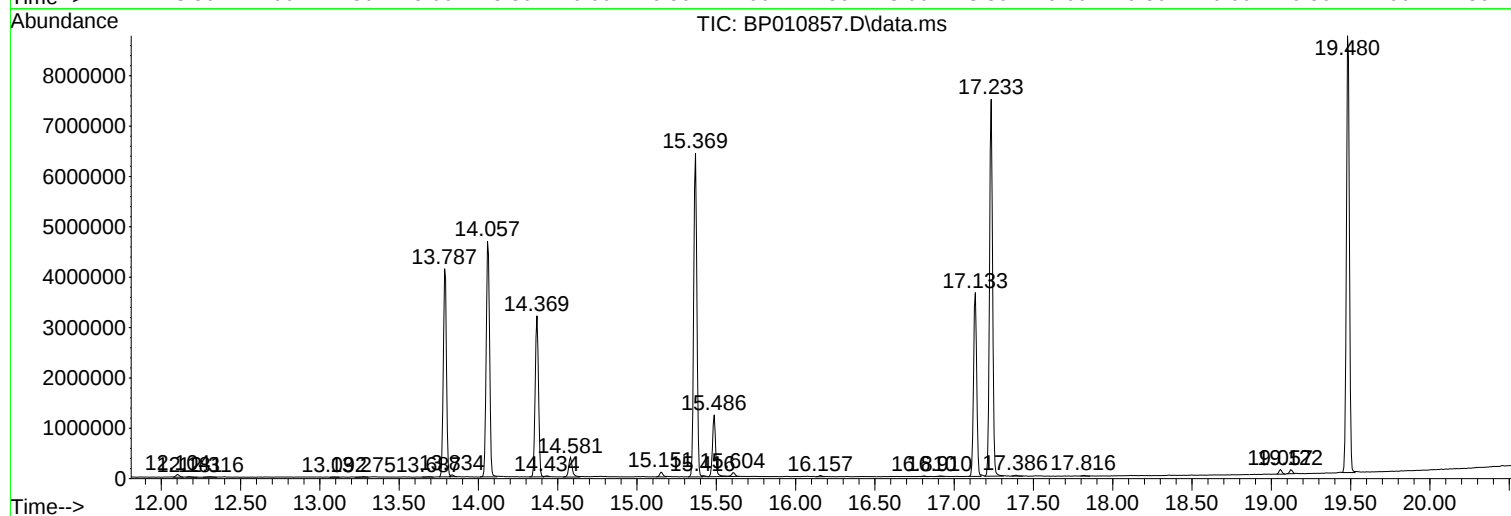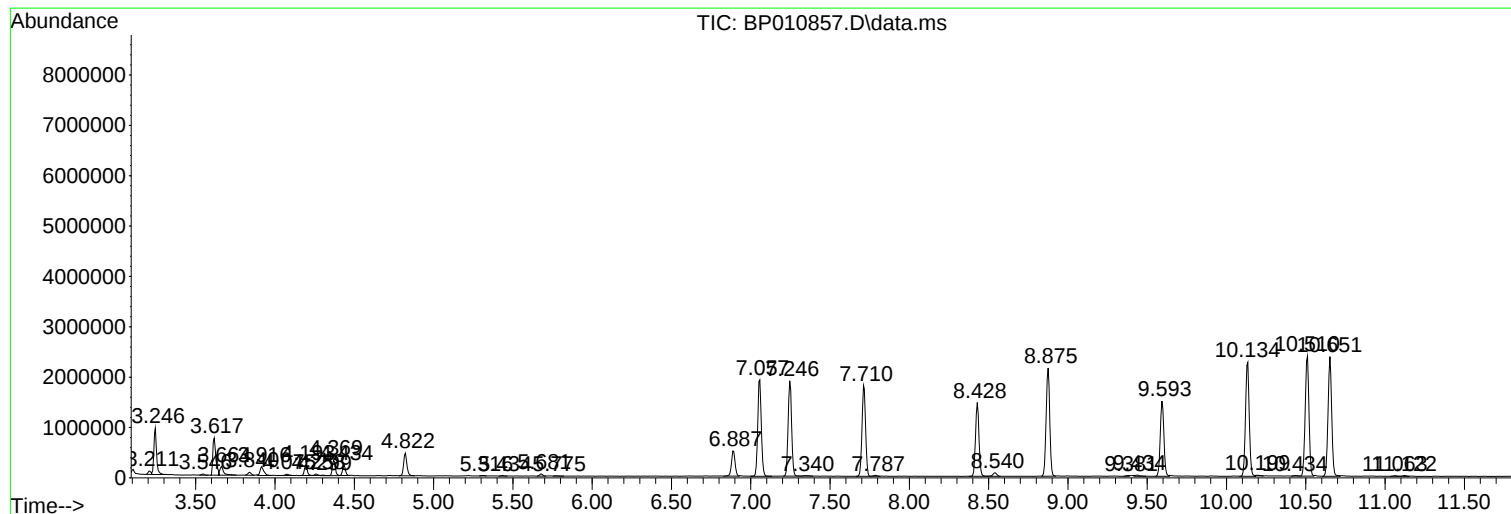

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010857.D
Acq On : 26 Jun 2022 08:30
Operator : CG/JU
Sample : N3392-14 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propanoic acid, propyl ester Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.369	2.80 ng/ul	397780	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	83
2			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	83
3			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
4			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
5			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	72

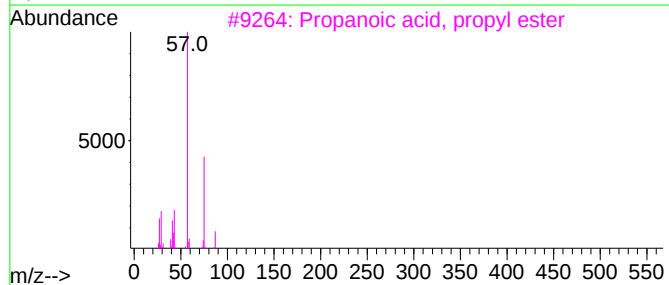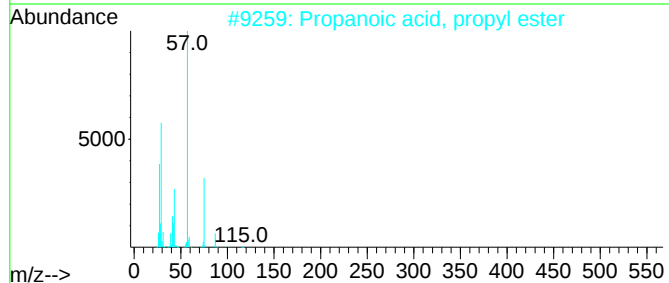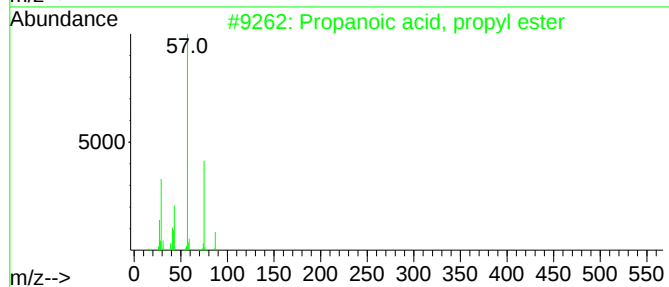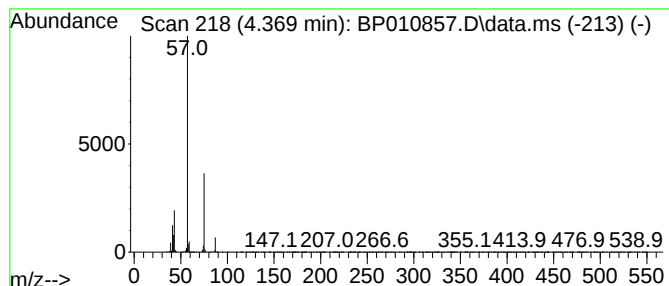

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010857.D
Acq On : 26 Jun 2022 08:30
Operator : CG/JU
Sample : N3392-14 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl butyrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.822	4.50 ng/ul	638023	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl butyrate	130	C7H14O2	000638-11-9	97
2			Isopropyl butyrate	130	C7H14O2	000638-11-9	86
3			Isopropyl butyrate	130	C7H14O2	000638-11-9	86
4			Isopropyl butyrate	130	C7H14O2	000638-11-9	78
5			Propanoic acid, 2-methyl-, 1-met...	130	C7H14O2	000617-50-5	64

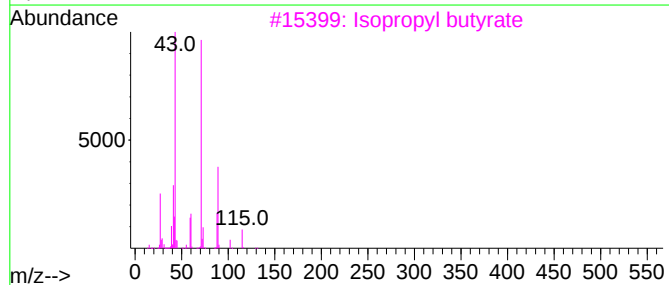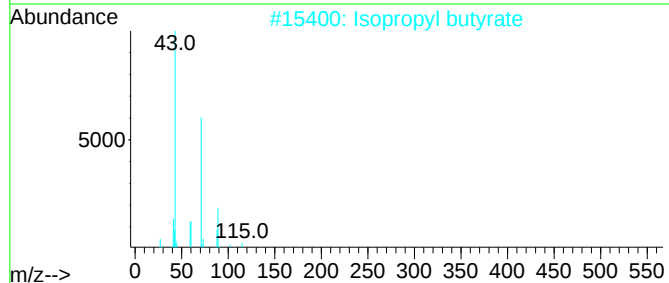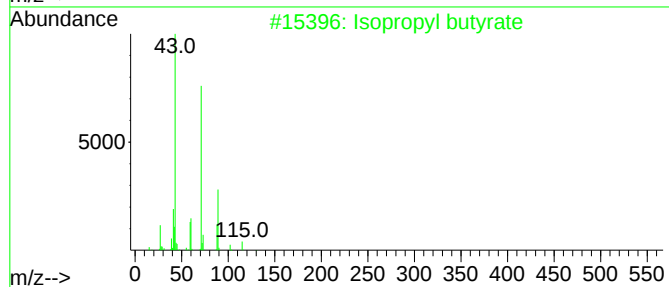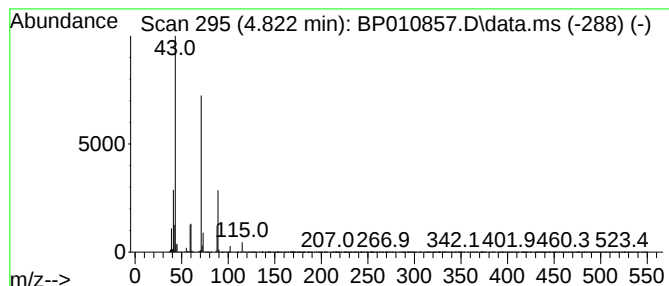

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010857.D
Acq On : 26 Jun 2022 08:30
Operator : CG/JU
Sample : N3392-14 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propanoic acid,...	4.369	2.8	ng/ul	397780	1	7.710	2838550	20.0
Isopropyl butyrate	4.822	4.5	ng/ul	638023	1	7.710	2838550	20.0