

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010859.D
 Acq On : 26 Jun 2022 09:38
 Operator : CG/JU
 Sample : N3392-02 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	23	rBV2	64971	85160	0.80%	0.084%
2	3.240	23	26	38	rVB	982240	1174754	11.01%	1.164%
3	3.546	74	78	83	rVB	29946	36815	0.35%	0.036%
4	3.617	87	90	95	rBV	610121	814395	7.64%	0.807%
5	3.664	95	98	104	rVB	157717	199284	1.87%	0.198%
6	3.840	123	128	133	rVB	63939	96804	0.91%	0.096%
7	3.917	135	141	150	rVB2	152611	262316	2.46%	0.260%
8	4.075	164	168	171	rBV	23163	28796	0.27%	0.029%
9	4.193	184	188	195	rVB	190497	235203	2.21%	0.233%
10	4.258	195	199	204	rBV	38476	50555	0.47%	0.050%
11	4.369	213	218	224	rBV	463684	571081	5.35%	0.566%
12	4.434	224	229	235	rVV	199853	250762	2.35%	0.249%
13	4.481	235	237	242	rVB3	8557	11289	0.11%	0.011%
14	4.652	263	266	271	rVB3	8711	11932	0.11%	0.012%
15	4.722	273	278	281	rBV3	10735	14273	0.13%	0.014%
16	4.822	287	295	304	rVV	477271	668491	6.27%	0.663%
17	4.899	304	308	314	rVB6	5601	11817	0.11%	0.012%
18	5.311	374	378	383	rVB5	14619	20760	0.19%	0.021%
19	5.434	393	399	404	rBV2	11325	21642	0.20%	0.021%
20	5.675	436	440	445	rBV	40418	57449	0.54%	0.057%
21	6.887	636	646	654	rBV	417423	651704	6.11%	0.646%
22	7.052	668	674	683	rBV	1778073	2729043	25.59%	2.705%
23	7.128	683	687	692	rVB	14937	23338	0.22%	0.023%
24	7.246	698	707	718	rBV	1688583	2572668	24.12%	2.550%
25	7.340	718	723	731	rVB9	10018	20494	0.19%	0.020%
26	7.710	778	786	794	rBV	1669541	2563256	24.03%	2.540%
27	7.787	794	799	811	rVB	43691	74433	0.70%	0.074%
28	8.022	834	839	843	rBV8	6967	11056	0.10%	0.011%
29	8.428	900	908	917	rBV	1237685	1913259	17.94%	1.896%
30	8.540	920	927	937	rVB	73153	127947	1.20%	0.127%
31	8.875	976	984	992	rBV	1969845	3070165	28.78%	3.043%
32	8.940	992	995	1000	rVB7	6771	12560	0.12%	0.012%
33	8.999	1000	1005	1009	rBV3	17636	31283	0.29%	0.031%
34	9.040	1009	1012	1016	rVB6	7949	12737	0.12%	0.013%
35	9.299	1052	1056	1061	rVB3	13964	21462	0.20%	0.021%
36	9.381	1064	1070	1072	rBV4	15373	28084	0.26%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010859.D
 Acq On : 26 Jun 2022 09:38
 Operator : CG/JU
 Sample : N3392-02 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	9.434	1076	1079	1086	rVB7	21649	41636	0.39%	0.041%
38	9.593	1097	1106	1115	rBV	1329418	2133708	20.00%	2.115%
39	10.128	1190	1197	1206	rBV	1991980	3312956	31.06%	3.283%
40	10.199	1206	1209	1216	rVB8	14904	25265	0.24%	0.025%
41	10.434	1246	1249	1254	rVB6	14423	20959	0.20%	0.021%
42	10.510	1254	1262	1274	rVB	2116424	3577823	33.54%	3.546%
43	10.651	1278	1286	1297	rBV	2027042	3277864	30.73%	3.249%
44	10.922	1328	1332	1338	rVB9	5542	12707	0.12%	0.013%
45	11.063	1352	1356	1360	rBV	16417	24420	0.23%	0.024%
46	11.122	1362	1366	1370	rBV	22258	33227	0.31%	0.033%
47	11.863	1487	1492	1498	rBV8	6104	10807	0.10%	0.011%
48	12.104	1524	1533	1541	rVB2	47091	83483	0.78%	0.083%
49	12.304	1561	1567	1576	rVB2	6992	21241	0.20%	0.021%
50	13.198	1714	1719	1725	rBV5	11286	18713	0.18%	0.019%
51	13.287	1728	1734	1738	rBV7	9597	19476	0.18%	0.019%
52	13.787	1812	1819	1825	rBV	3848437	5143811	48.23%	5.098%
53	13.834	1825	1827	1835	rVB	29961	40165	0.38%	0.040%
54	14.057	1856	1865	1873	rBV	4224588	6286900	58.94%	6.231%
55	14.281	1899	1903	1908	rVB8	7262	10742	0.10%	0.011%
56	14.369	1911	1918	1926	rBV	2829654	4089698	38.34%	4.053%
57	14.581	1948	1954	1963	rBV	284673	434076	4.07%	0.430%
58	14.804	1988	1992	1997	rVB7	12280	18530	0.17%	0.018%
59	14.963	2015	2019	2023	rBV7	7541	11472	0.11%	0.011%
60	15.151	2045	2051	2056	rBV	73082	112498	1.05%	0.111%
61	15.187	2056	2057	2064	rVB5	9489	14206	0.13%	0.014%
62	15.369	2081	2088	2102	rBV	5647633	8084718	75.80%	8.013%
63	15.486	2102	2108	2123	rVV	1015416	1395362	13.08%	1.383%
64	15.610	2123	2129	2135	rVB	65376	105074	0.99%	0.104%
65	15.928	2181	2183	2189	rBV7	6423	13114	0.12%	0.013%
66	16.069	2201	2207	2212	rBV10	5297	12628	0.12%	0.013%
67	16.157	2218	2222	2226	rBV3	19930	26580	0.25%	0.026%
68	16.810	2328	2333	2338	rBV8	11841	20588	0.19%	0.020%
69	16.910	2346	2350	2355	rBV6	11454	18503	0.17%	0.018%
70	17.133	2381	2388	2398	rBV	3260031	4405194	41.30%	4.366%
71	17.233	2398	2405	2418	rVV	6175416	8645111	81.05%	8.568%
72	17.510	2449	2452	2455	rBV4	8032	11153	0.10%	0.011%
73	17.663	2472	2478	2484	rBV3	25975	46196	0.43%	0.046%
74	17.828	2501	2506	2512	rBV	68101	89563	0.84%	0.089%
75	18.969	2697	2700	2705	rVB5	28077	32147	0.30%	0.032%
76	19.057	2711	2715	2719	rBV2	80106	111618	1.05%	0.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010859.D
Acq On : 26 Jun 2022 09:38
Operator : CG/JU
Sample : N3392-02 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION

77	19.127	2722	2727	2731	rVV	68490	98316	0.92%	0.097%
78	19.480	2781	2787	2795	rBV	7495827	9811247	91.99%	9.724%
79	20.974	3038	3041	3045	rBV	146346	168196	1.58%	0.167%
80	21.245	3082	3087	3092	rBV	3978014	4849438	45.47%	4.806%
81	23.457	3456	3463	3474	rVB2	5704313	10666099	100.00%	10.571%
82	23.610	3483	3489	3499	rVB2	2588987	5025248	47.11%	4.980%




Sum of corrected areas: 100899543

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010859.D
Acq On : 26 Jun 2022 09:38
Operator : CG/JU
Sample : N3392-02 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

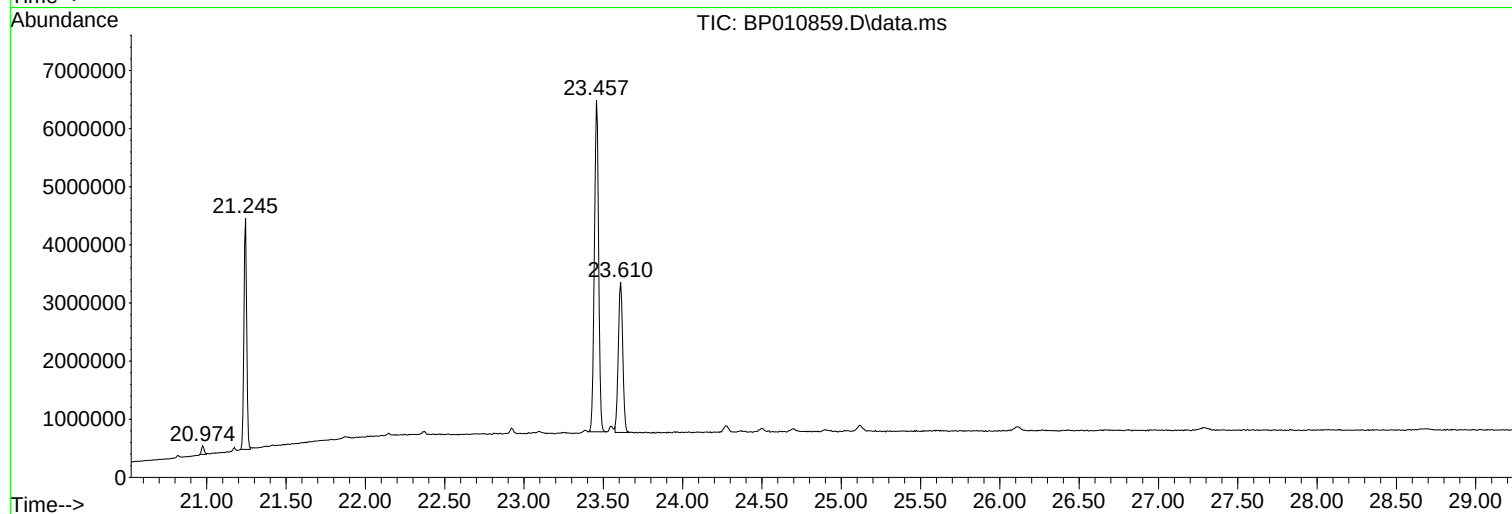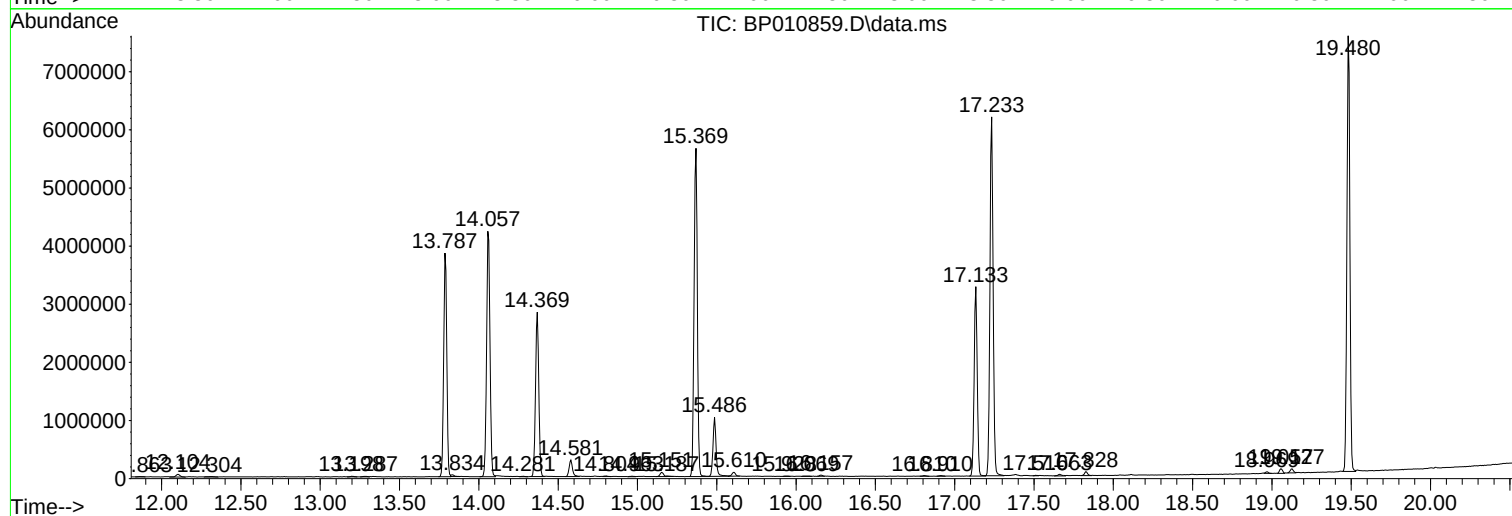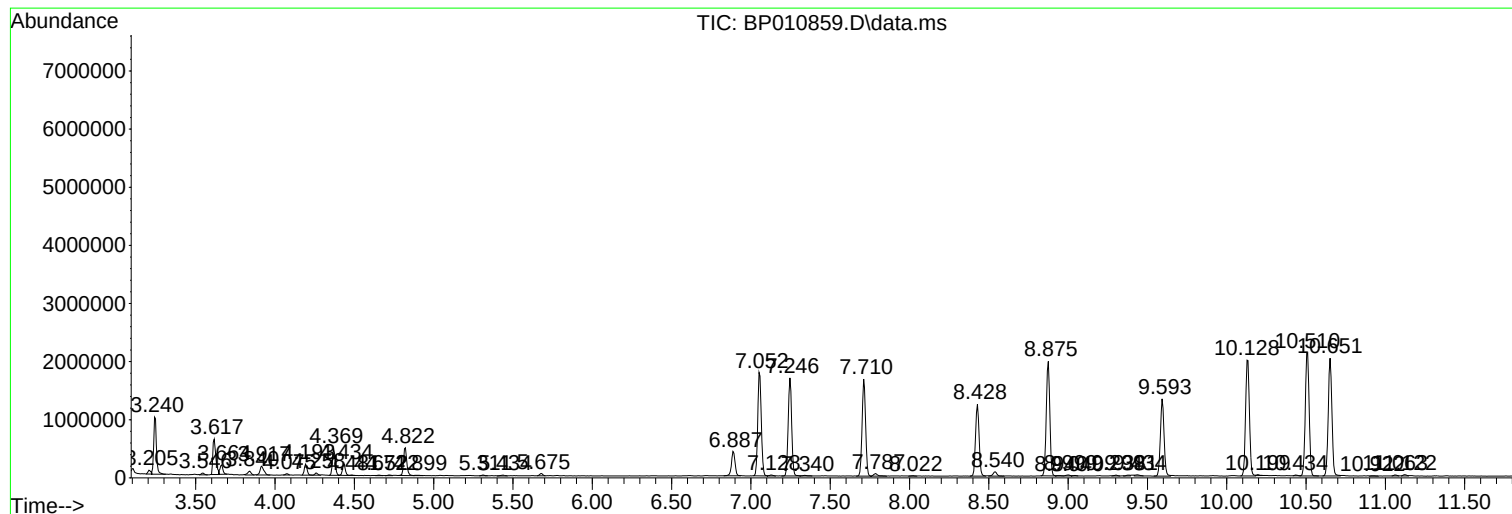

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010859.D
Acq On : 26 Jun 2022 09:38
Operator : CG/JU
Sample : N3392-02 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isobutyl acetate Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.917	2.05 ng/ul	262316	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isobutyl acetate	116	C6H12O2	000110-19-0	64
2			Isobutyl acetate	116	C6H12O2	000110-19-0	64
3			Isobutyl acetate	116	C6H12O2	000110-19-0	43
4			Isobutyl acetate	116	C6H12O2	000110-19-0	42
5			Isobutyl acetate	116	C6H12O2	000110-19-0	42

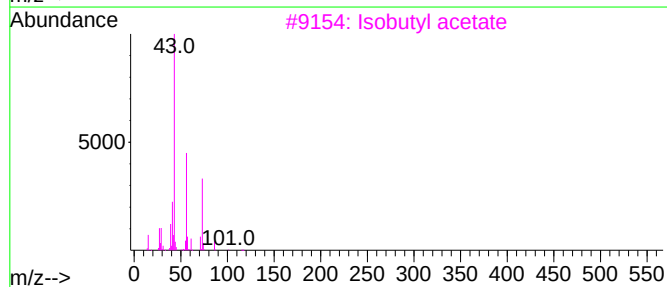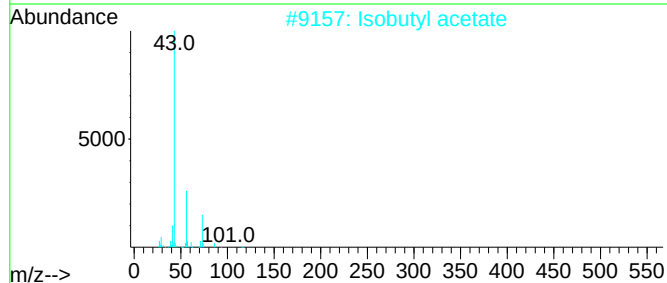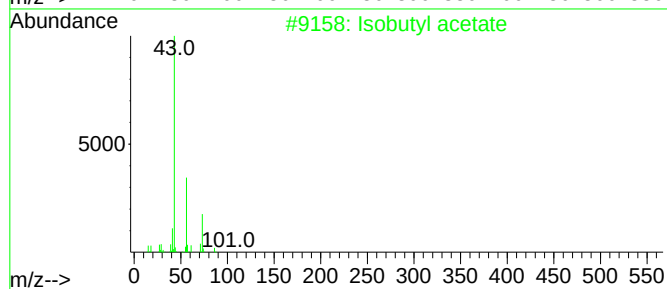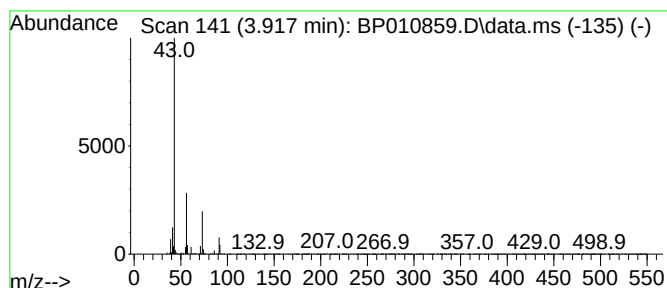

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010859.D
Acq On : 26 Jun 2022 09:38
Operator : CG/JU
Sample : N3392-02 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Propanoic acid, propyl ester Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.369	4.46 ng/ul	571081	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	83
2			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
3			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
4			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
5			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	64

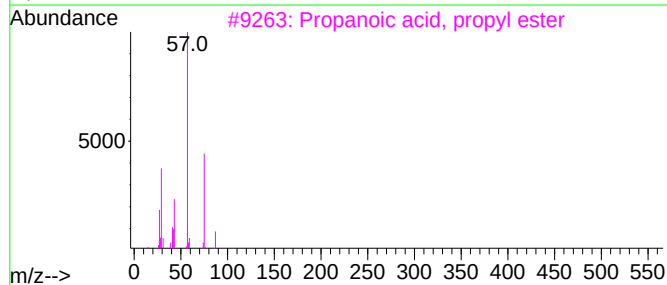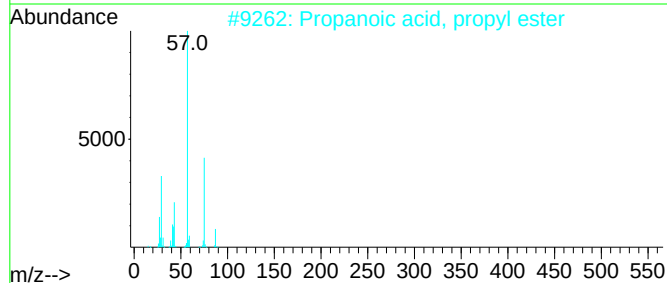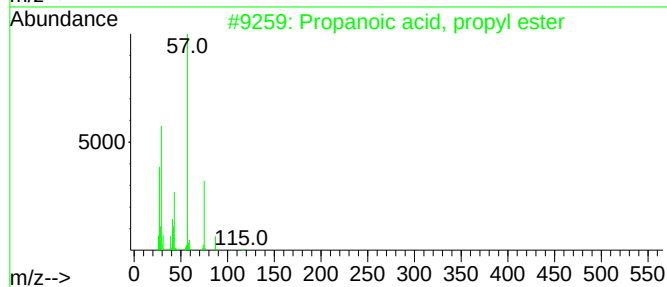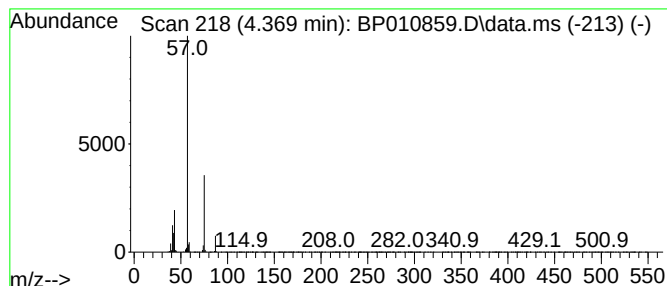

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010859.D
Acq On : 26 Jun 2022 09:38
Operator : CG/JU
Sample : N3392-02 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Isopropyl butyrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.822	5.22 ng/ul	668491	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl butyrate	130	C7H14O2	000638-11-9	94
2			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
3			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
4			Propanoic acid, 2-methyl-, 1-met...	130	C7H14O2	000617-50-5	72
5			Propanoic acid, 2-methyl-, propy...	130	C7H14O2	000644-49-5	64

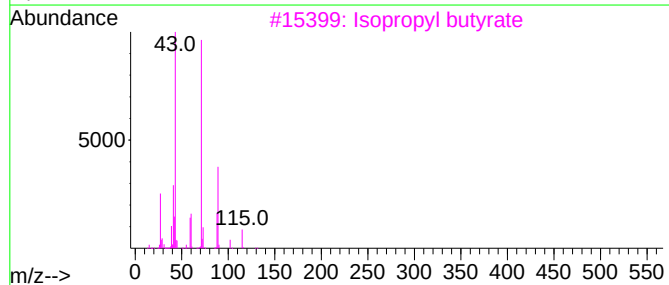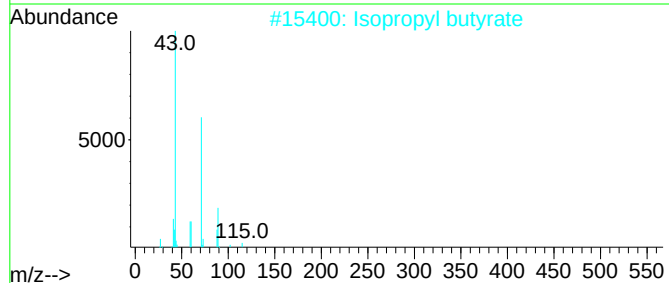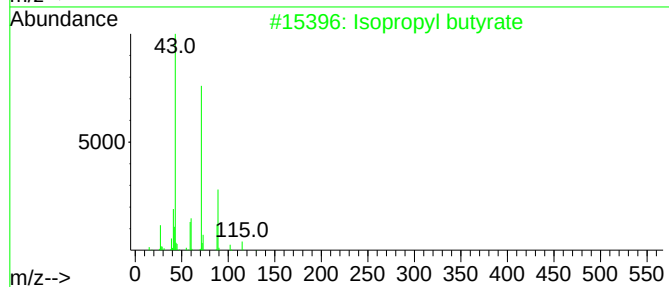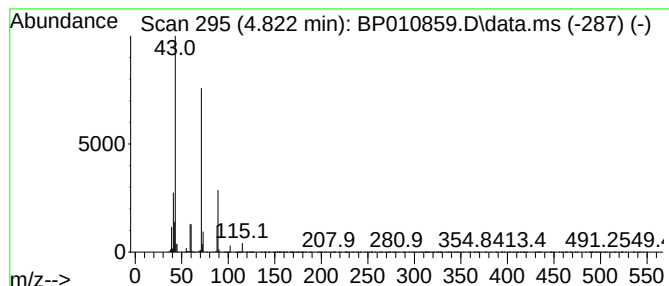

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010859.D
Acq On : 26 Jun 2022 09:38
Operator : CG/JU
Sample : N3392-02 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isobutyl acetate	3.917	2.0	ng/ul	262316	1	7.710	2563260	20.0
Propanoic acid,...	4.369	4.5	ng/ul	571081	1	7.710	2563260	20.0
Isopropyl butyrate	4.822	5.2	ng/ul	668491	1	7.710	2563260	20.0