

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010866.D
 Acq On : 26 Jun 2022 13:34
 Operator : CG/JU
 Sample : N3392-05 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	23	rBV2	77925	101331	0.93%	0.091%
2	3.240	23	26	41	rVV	1189312	1426000	13.11%	1.281%
3	3.546	74	78	85	rVB	32688	39014	0.36%	0.035%
4	3.617	86	90	95	rBV	712783	971774	8.94%	0.873%
5	3.664	95	98	104	rVB	180279	231653	2.13%	0.208%
6	3.840	122	128	133	rVB	62035	97520	0.90%	0.088%
7	3.917	133	141	149	rVB2	191307	318168	2.93%	0.286%
8	4.075	163	168	176	rBV2	28987	43386	0.40%	0.039%
9	4.152	178	181	184	rVV3	11938	14157	0.13%	0.013%
10	4.193	184	188	194	rVB	227412	282035	2.59%	0.253%
11	4.258	194	199	203	rBV	47893	58537	0.54%	0.053%
12	4.370	213	218	224	rBV	577720	698990	6.43%	0.628%
13	4.434	224	229	235	rVV	265240	331698	3.05%	0.298%
14	4.481	235	237	243	rVB	13086	15699	0.14%	0.014%
15	4.658	260	267	270	rVB2	7037	12769	0.12%	0.011%
16	4.722	274	278	281	rBV4	10174	14337	0.13%	0.013%
17	4.817	287	294	303	rVV	577590	813026	7.48%	0.731%
18	5.040	328	332	336	rBV2	16705	22036	0.20%	0.020%
19	5.217	357	362	369	rVB5	10222	18792	0.17%	0.017%
20	5.311	374	378	383	rVB4	16761	22922	0.21%	0.021%
21	5.434	395	399	403	rVB2	13065	17735	0.16%	0.016%
22	5.675	435	440	447	rVB	46885	63081	0.58%	0.057%
23	6.393	554	562	571	rVB	35828	62498	0.57%	0.056%
24	6.887	637	646	657	rVB	521621	805704	7.41%	0.724%
25	7.052	667	674	683	rBV	2119323	3188959	29.32%	2.866%
26	7.134	684	688	693	rVB	10290	16153	0.15%	0.015%
27	7.246	700	707	716	rBV	1991647	3021637	27.78%	2.715%
28	7.334	719	722	727	rVV3	8613	11044	0.10%	0.010%
29	7.711	779	786	794	rBV	1916306	2953131	27.15%	2.654%
30	7.781	794	798	807	rVB	25066	45960	0.42%	0.041%
31	8.428	901	908	918	rBV	1447116	2282677	20.99%	2.051%
32	8.540	918	927	933	rVB	80459	137632	1.27%	0.124%
33	8.875	976	984	991	rBV	2271507	3619254	33.28%	3.252%
34	8.999	1000	1005	1009	rVV2	10313	16669	0.15%	0.015%
35	9.299	1052	1056	1063	rVB3	15544	24757	0.23%	0.022%
36	9.381	1063	1070	1073	rVV7	18381	40386	0.37%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010866.D
 Acq On : 26 Jun 2022 13:34
 Operator : CG/JU
 Sample : N3392-05 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	9.434	1076	1079	1090	rVB4	24602	50049	0.46%	0.045%
38	9.593	1098	1106	1120	rBV	1608018	2582210	23.74%	2.320%
39	9.916	1155	1161	1168	rBV	6119	16015	0.15%	0.014%
40	10.040	1177	1182	1187	rBV9	6171	13222	0.12%	0.012%
41	10.128	1189	1197	1205	rBV	2418816	3879300	35.67%	3.486%
42	10.199	1206	1209	1216	rVB8	15721	26824	0.25%	0.024%
43	10.434	1244	1249	1254	rBV4	14947	26565	0.24%	0.024%
44	10.505	1254	1261	1269	rBV	2474563	4123136	37.91%	3.705%
45	10.652	1276	1286	1296	rBV	2348286	3797242	34.92%	3.412%
46	11.063	1351	1356	1360	rBV	18911	29122	0.27%	0.026%
47	11.122	1362	1366	1371	rBV	26182	40017	0.37%	0.036%
48	12.104	1527	1533	1539	rVB2	51582	85591	0.79%	0.077%
49	13.081	1691	1699	1706	rBV2	5260	12272	0.11%	0.011%
50	13.199	1715	1719	1725	rVB5	10534	16703	0.15%	0.015%
51	13.275	1725	1732	1738	rBV5	18392	34496	0.32%	0.031%
52	13.334	1738	1742	1748	rBV7	8478	17281	0.16%	0.016%
53	13.787	1812	1819	1825	rBV	4309000	5814335	53.46%	5.225%
54	13.834	1825	1827	1834	rVB2	22641	32066	0.29%	0.029%
55	14.057	1856	1865	1874	rBV	4786290	7164975	65.88%	6.438%
56	14.281	1899	1903	1910	rVB8	6786	11428	0.11%	0.010%
57	14.369	1910	1918	1927	rBV	3304484	4761924	43.79%	4.279%
58	14.581	1947	1954	1967	rBV	292244	467819	4.30%	0.420%
59	14.728	1975	1979	1983	rVV6	8673	12982	0.12%	0.012%
60	14.798	1987	1991	1995	rVB6	8094	12188	0.11%	0.011%
61	15.028	2024	2030	2034	rVB9	8071	16012	0.15%	0.014%
62	15.151	2045	2051	2057	rBV	84370	130962	1.20%	0.118%
63	15.240	2063	2066	2071	rVB3	10733	13634	0.13%	0.012%
64	15.369	2081	2088	2099	rBV	6186966	8782790	80.76%	7.892%
65	15.487	2101	2108	2119	rVV	1049357	1450666	13.34%	1.304%
66	15.610	2123	2129	2133	rVB2	69062	103691	0.95%	0.093%
67	16.063	2200	2206	2207	rBV6	7052	11056	0.10%	0.010%
68	16.104	2210	2213	2217	rVV2	18434	26958	0.25%	0.024%
69	16.157	2218	2222	2227	rVB3	22932	34745	0.32%	0.031%
70	16.281	2238	2243	2247	rBV8	5535	11235	0.10%	0.010%
71	16.810	2330	2333	2338	rVB6	12946	13950	0.13%	0.013%
72	16.910	2344	2350	2354	rBV2	32881	47911	0.44%	0.043%
73	17.134	2381	2388	2398	rBV	3374557	4824084	44.36%	4.335%
74	17.234	2398	2405	2419	rVV	6347502	9013739	82.88%	8.100%
75	17.445	2439	2441	2448	rVB8	8764	12050	0.11%	0.011%
76	17.539	2454	2457	2465	rVB9	19593	31687	0.29%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010866.D
 Acq On : 26 Jun 2022 13:34
 Operator : CG/JU
 Sample : N3392-05 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

77	17.657	2473	2477	2480	rBV5	22532	29088	0.27%	0.026%
78	17.828	2501	2506	2511	rBV	128887	154706	1.42%	0.139%
79	18.969	2696	2700	2704	rBV	207320	216403	1.99%	0.194%
80	19.057	2711	2715	2719	rBV2	82157	106112	0.98%	0.095%
81	19.098	2719	2722	2724	rVV	56520	65416	0.60%	0.059%
82	19.122	2724	2726	2730	rVB	72348	81764	0.75%	0.073%
83	19.481	2781	2787	2794	rBV	7588548	9777529	89.91%	8.786%
84	20.975	3038	3041	3046	rBV2	133579	156506	1.44%	0.141%
85	21.245	3082	3087	3092	rBV	4068838	4997538	45.95%	4.491%
86	23.457	3456	3463	3473	rVB2	5620737	10875356	100.00%	9.773%
87	23.610	3482	3489	3502	rVB2	2830248	5430006	49.93%	4.879%




Sum of corrected areas: 111284477

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010866.D
Acq On : 26 Jun 2022 13:34
Operator : CG/JU
Sample : N3392-05 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

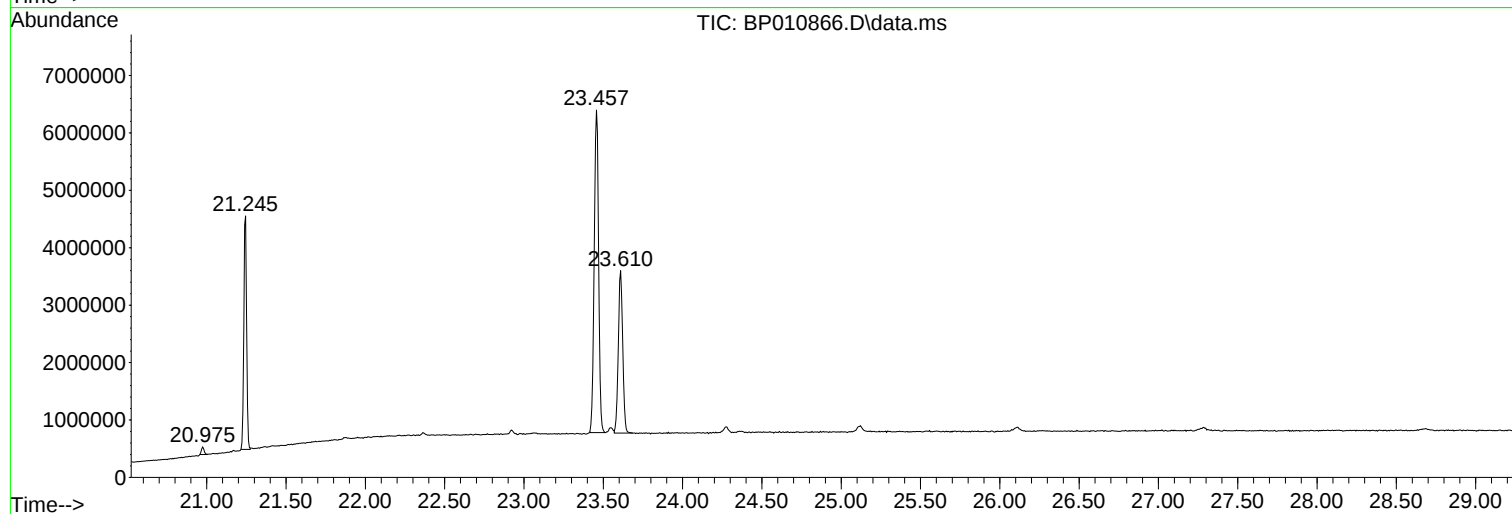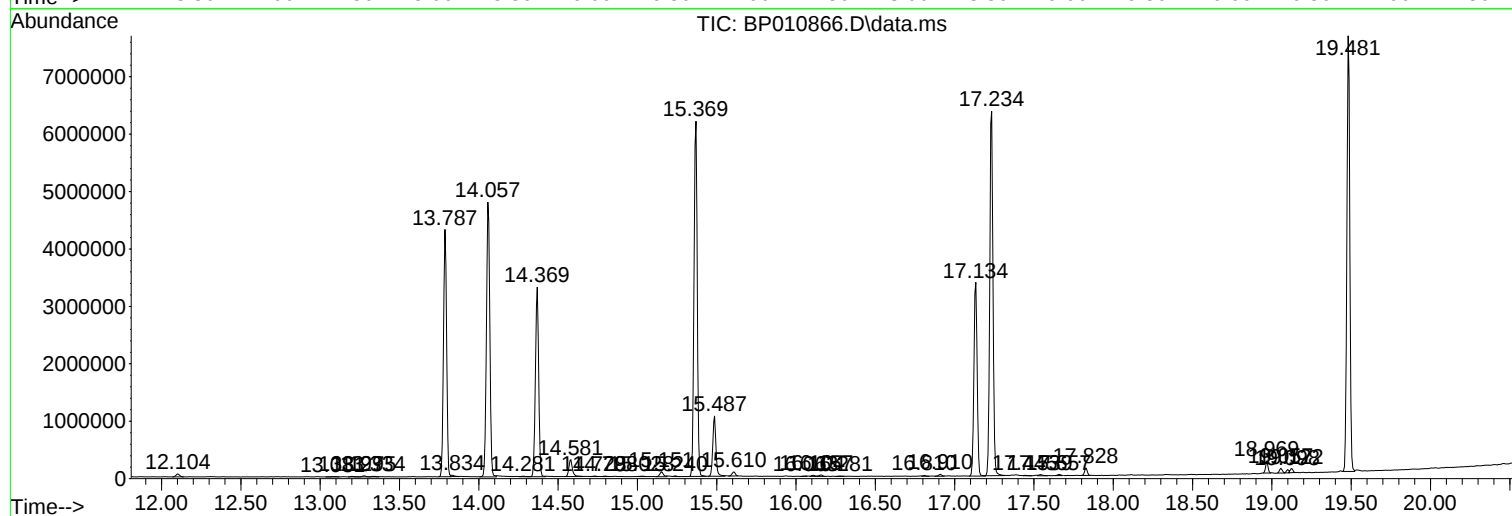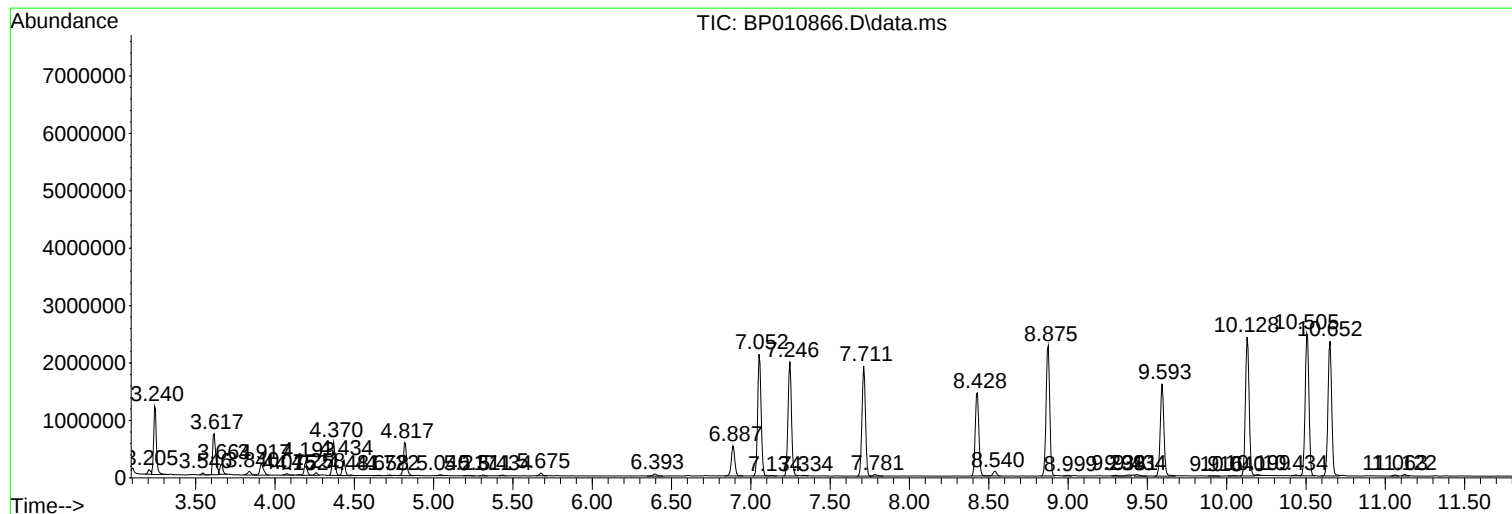

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010866.D
Acq On : 26 Jun 2022 13:34
Operator : CG/JU
Sample : N3392-05 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isobutyl acetate Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.917	2.15 ng/ul	318168	1,4-Dichlorobenzene-d4	7.711

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isobutyl acetate	116	C6H12O2	000110-19-0	72
2			Isobutyl acetate	116	C6H12O2	000110-19-0	72
3			Isobutyl acetate	116	C6H12O2	000110-19-0	64
4			Isobutyl acetate	116	C6H12O2	000110-19-0	59
5			Isobutyl acetate	116	C6H12O2	000110-19-0	50

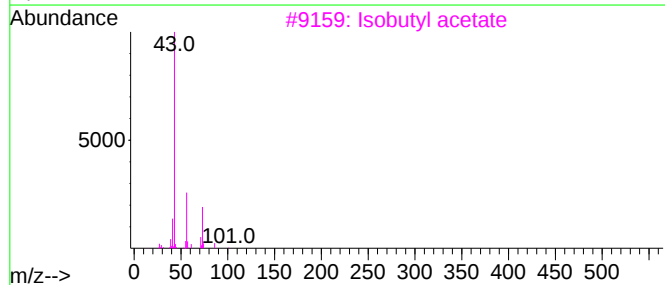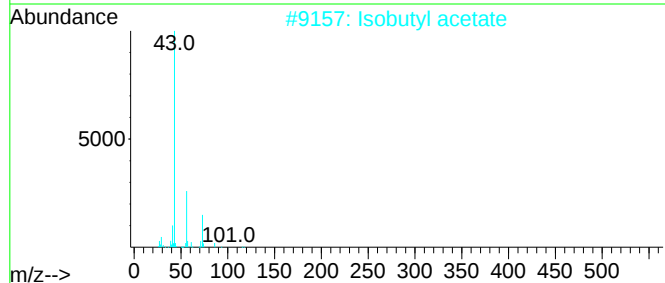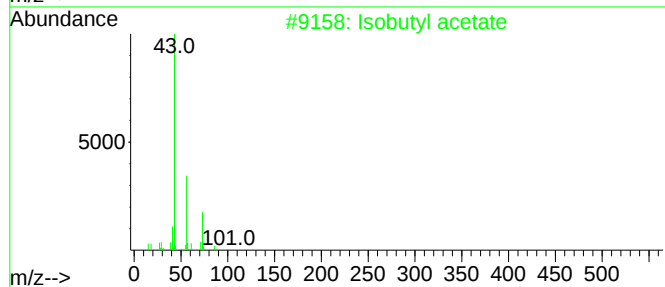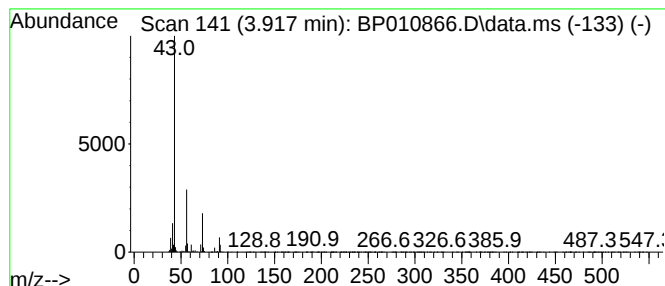

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010866.D
Acq On : 26 Jun 2022 13:34
Operator : CG/JU
Sample : N3392-05 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Propanoic acid, propyl ester Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.370	4.73 ng/ul	698990	1,4-Dichlorobenzene-d4	7.711

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	83
2			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	83
3			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
4			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
5			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	64

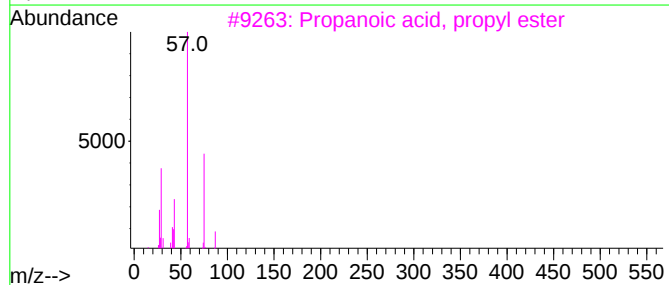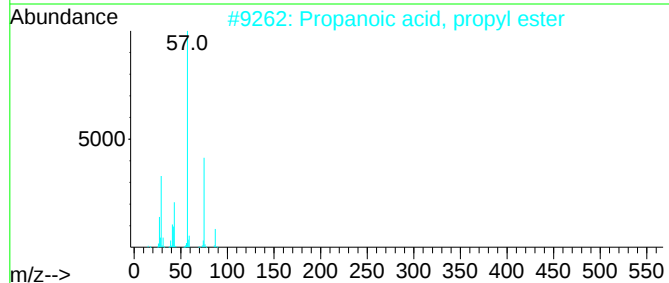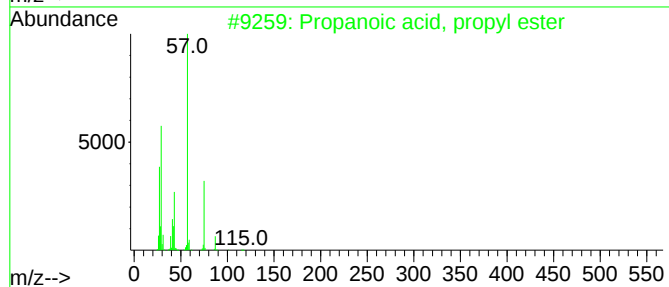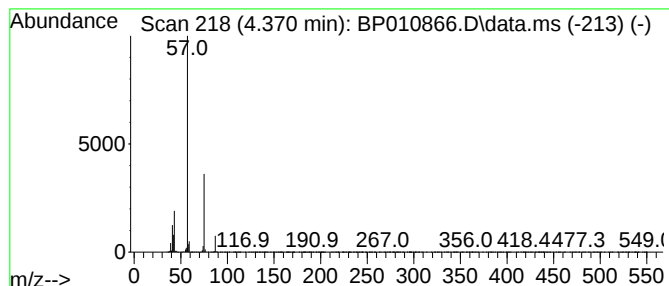

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010866.D
Acq On : 26 Jun 2022 13:34
Operator : CG/JU
Sample : N3392-05 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Acetic acid, butyl ester Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.434	2.25 ng/ul	331698	1,4-Dichlorobenzene-d4	7.711

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Acetic acid, butyl ester	116	C6H12O2	000123-86-4	78		
2	Acetic acid, butyl ester	116	C6H12O2	000123-86-4	72		
3	Acetic acid, butyl ester	116	C6H12O2	000123-86-4	59		
4	Acetic acid, butyl ester	116	C6H12O2	000123-86-4	38		
5	Isopropyl acetate	102	C5H10O2	000108-21-4	9		

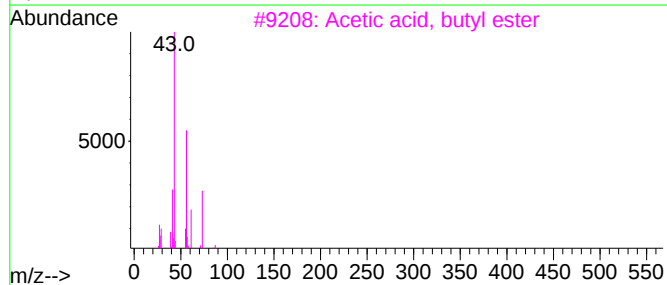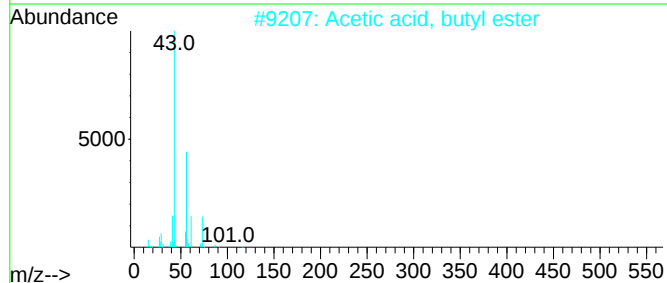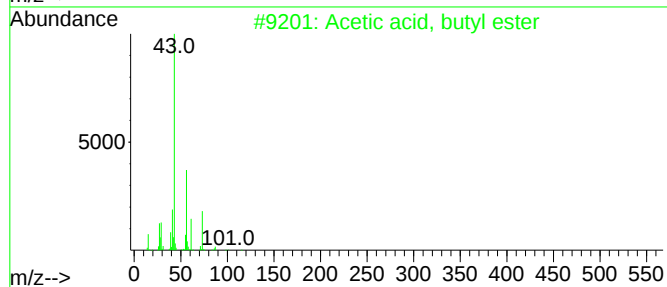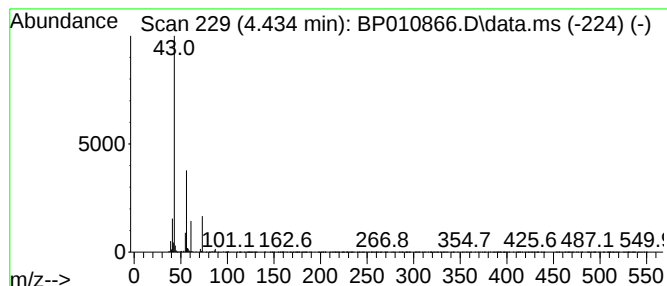

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010866.D
Acq On : 26 Jun 2022 13:34
Operator : CG/JU
Sample : N3392-05 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Isopropyl butyrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.817	5.51 ng/ul	813026	1,4-Dichlorobenzene-d4	7.711

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl butyrate	130	C7H14O2	000638-11-9	95
2			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
3			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
4			Isopropyl butyrate	130	C7H14O2	000638-11-9	86
5			Propanoic acid, 2-methyl-, 1-met...	130	C7H14O2	000617-50-5	64

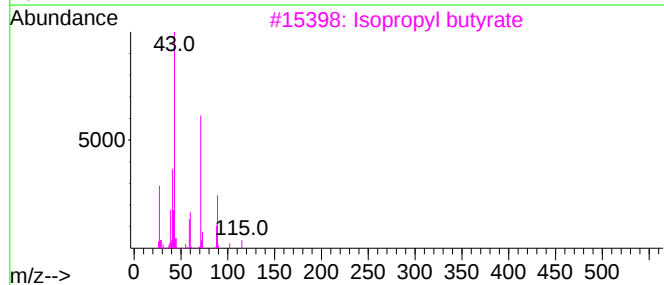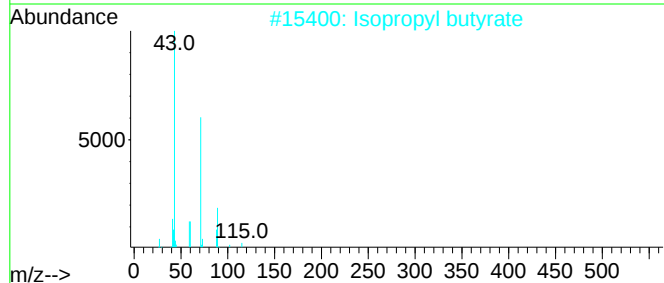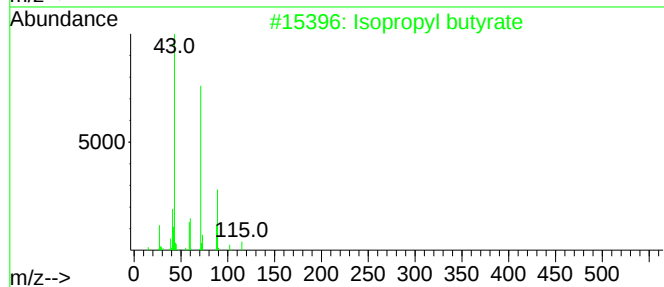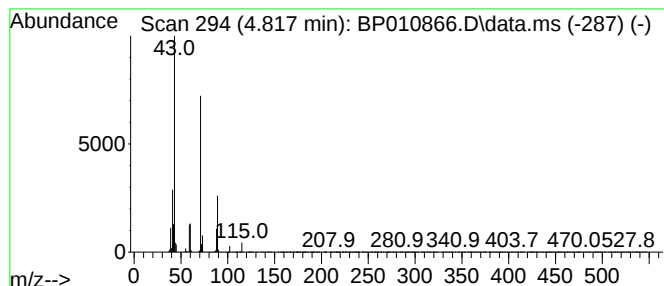

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010866.D
Acq On : 26 Jun 2022 13:34
Operator : CG/JU
Sample : N3392-05 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isobutyl acetate	3.917	2.1	ng/ul	318168	1	7.711	2953130	20.0
Propanoic acid,...	4.370	4.7	ng/ul	698990	1	7.711	2953130	20.0
Acetic acid, bu...	4.434	2.3	ng/ul	331698	1	7.711	2953130	20.0
Isopropyl butyrate	4.817	5.5	ng/ul	813026	1	7.711	2953130	20.0