
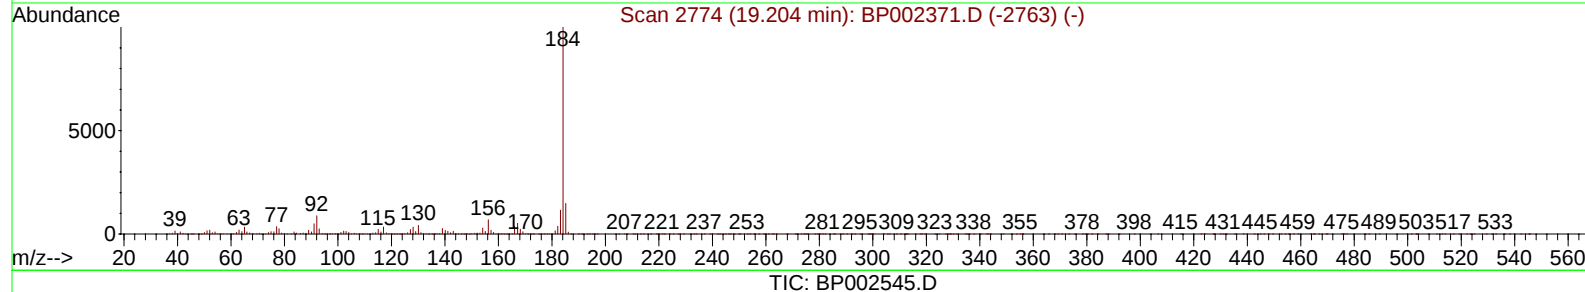
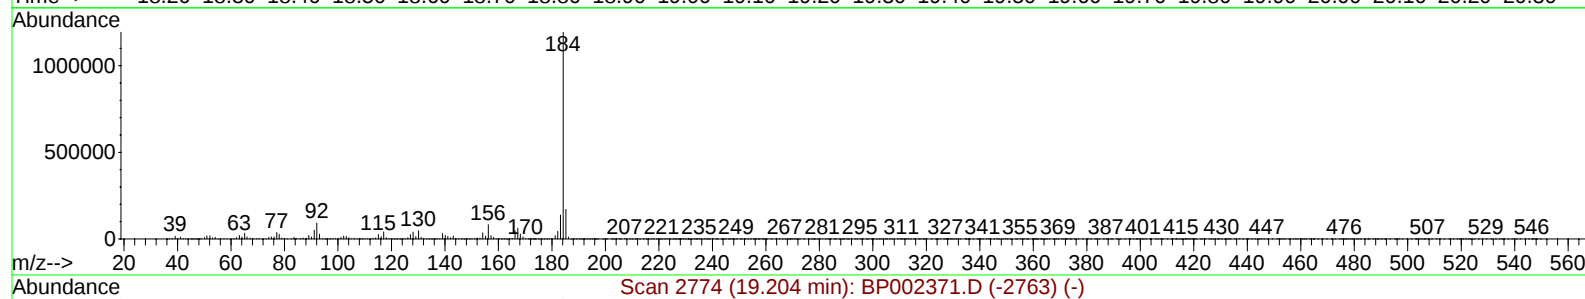


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062620\
 Data File : BP002545.D
 Acq On : 26 Jun 2020 09:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 19:01:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 24 13:54:06 2020
 Response via : Initial Calibration

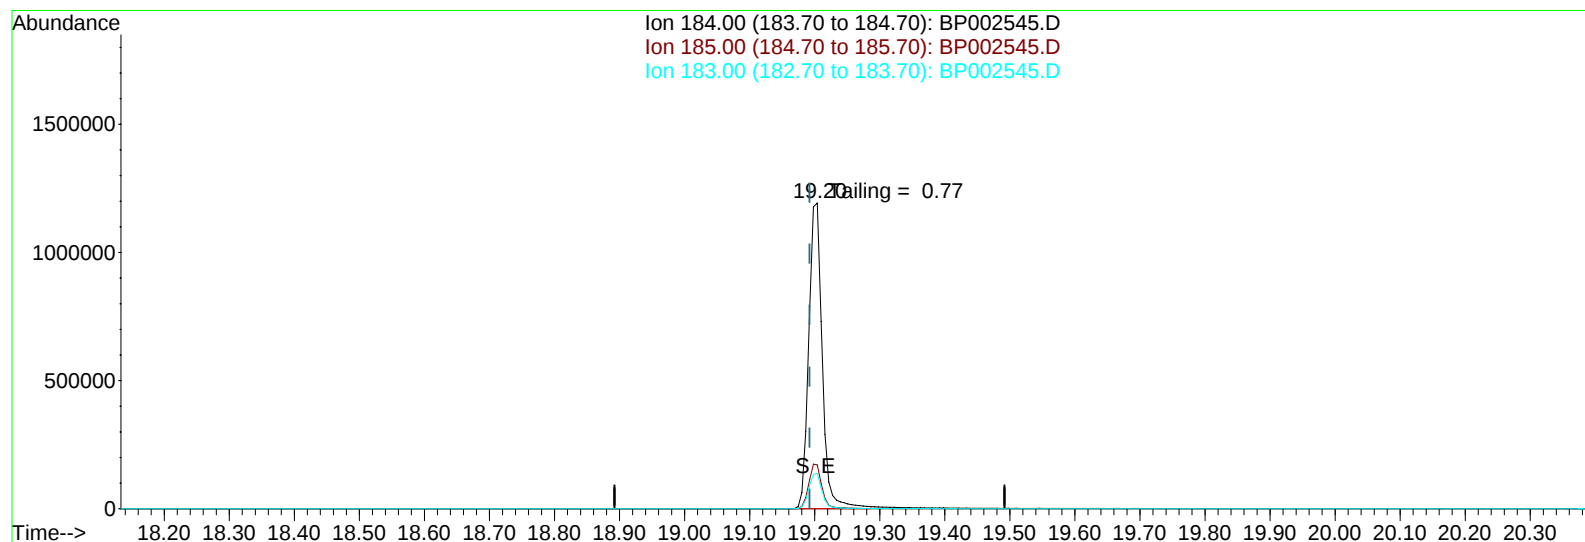

(77) Benzidine




19.204min (+0.012) 858091.98ng

response 1744842

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.32
183.00	11.50	11.58
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062620\
 Data File : BP002545.D
 Acq On : 26 Jun 2020 09:28
 Operator : CG/JU
 Sample : DF TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 19:01:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 24 13:54:06 2020
 Response via : Initial Calibration

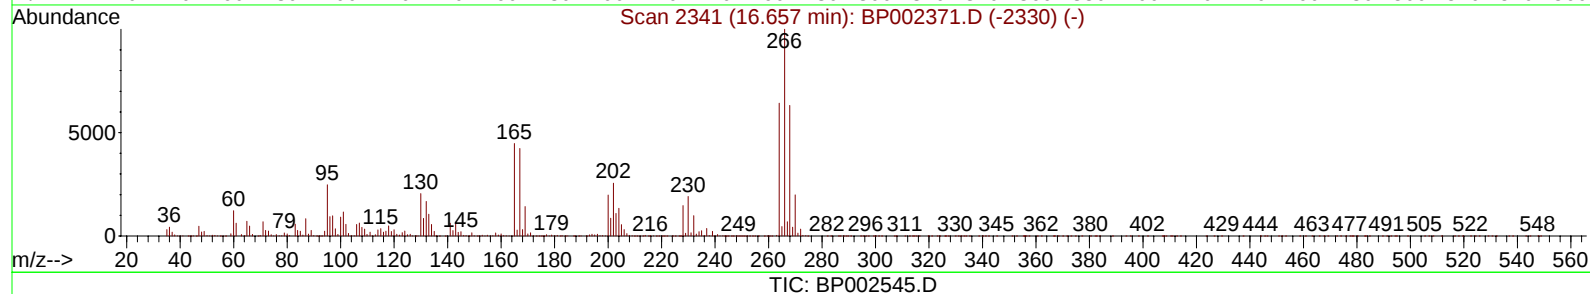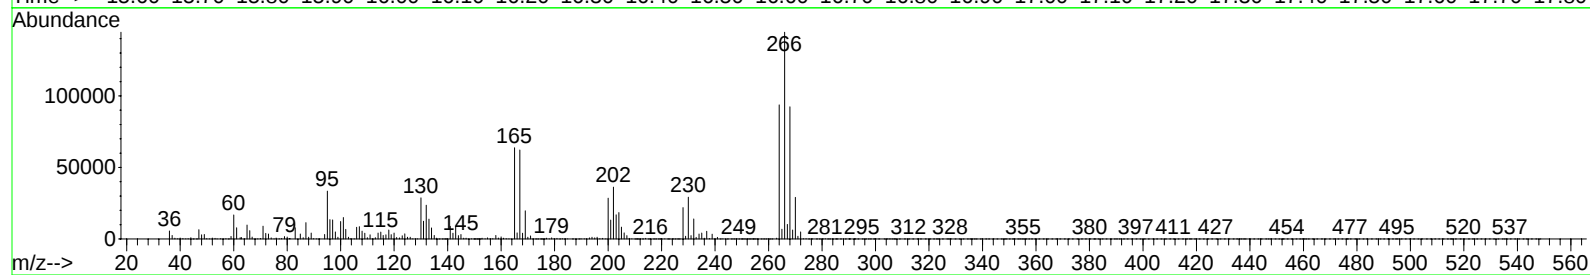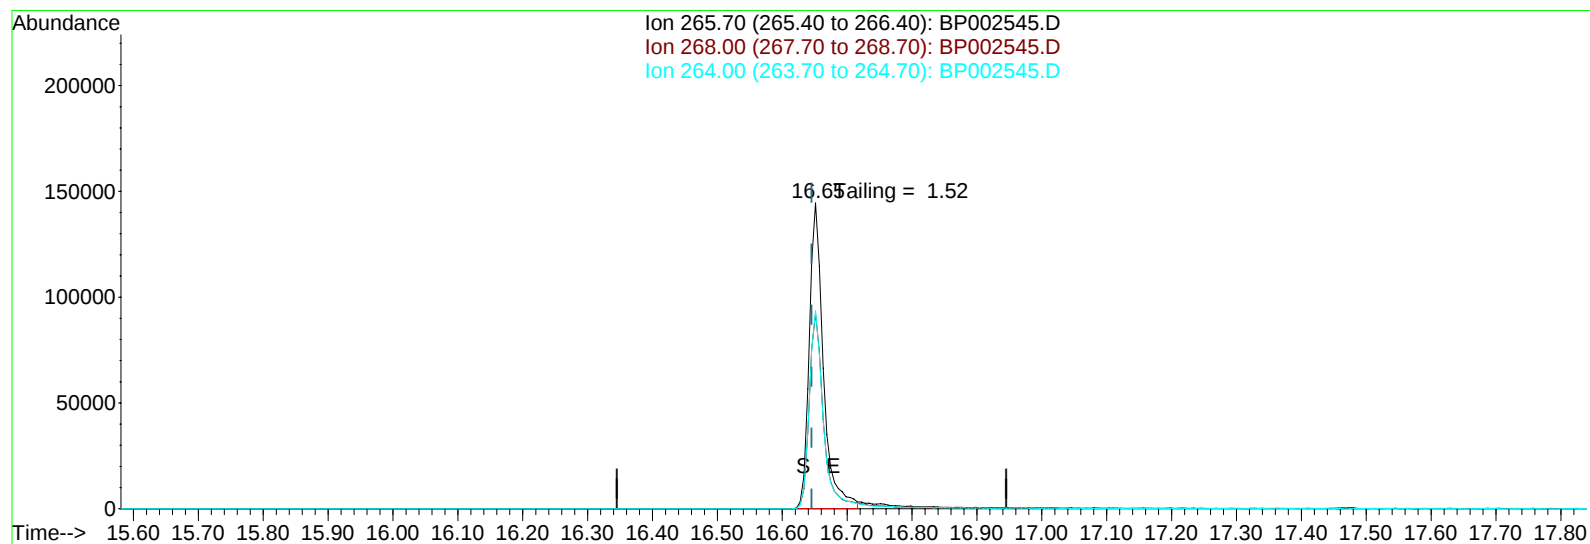

TIC: BP002545.D

(70) Pentachlorophenol (C)

16.651min (+0.006) 3200463.05ng

response 230974

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.96
264.00	64.80	64.83
0.00	0.00	0.00