

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062620\
 Data File : BP002550.D
 Acq On : 26 Jun 2020 14:27
 Operator : CG/JU
 Sample : PB129799BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB129799BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.204	388	394	408	rBV	1977345	2860986	40.43%	7.896%
2	6.775	653	661	680	rBV	1764312	2859004	40.41%	7.891%
3	7.581	791	798	812	rBV	587996	905609	12.80%	2.499%
4	7.898	844	852	873	rBV	2306293	3734924	52.79%	10.308%
5	8.728	982	993	1010	rBV	1679719	2858627	40.40%	7.890%
6	10.351	1261	1269	1287	rBV	638138	1138129	16.09%	3.141%
7	12.845	1685	1693	1718	rBV	3680401	5785503	81.77%	15.967%
8	14.228	1921	1928	1946	rBV	939970	1440107	20.35%	3.975%
9	15.733	2176	2184	2214	rBV	1507397	2729335	38.57%	7.533%
10	16.992	2391	2398	2411	rBV	1082304	1681299	23.76%	4.640%
11	19.580	2832	2838	2853	rBV	5484267	7075562	100.00%	19.528%
12	21.098	3091	3096	3106	rBV	1216402	1620588	22.90%	4.473%
13	23.298	3464	3470	3484	rVB2	768953	1543548	21.82%	4.260%




Sum of corrected areas: 36233221

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062620\
Data File : BP002550.D
Acq On : 26 Jun 2020 14:27
Operator : CG/JU
Sample : PB129799BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129799BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

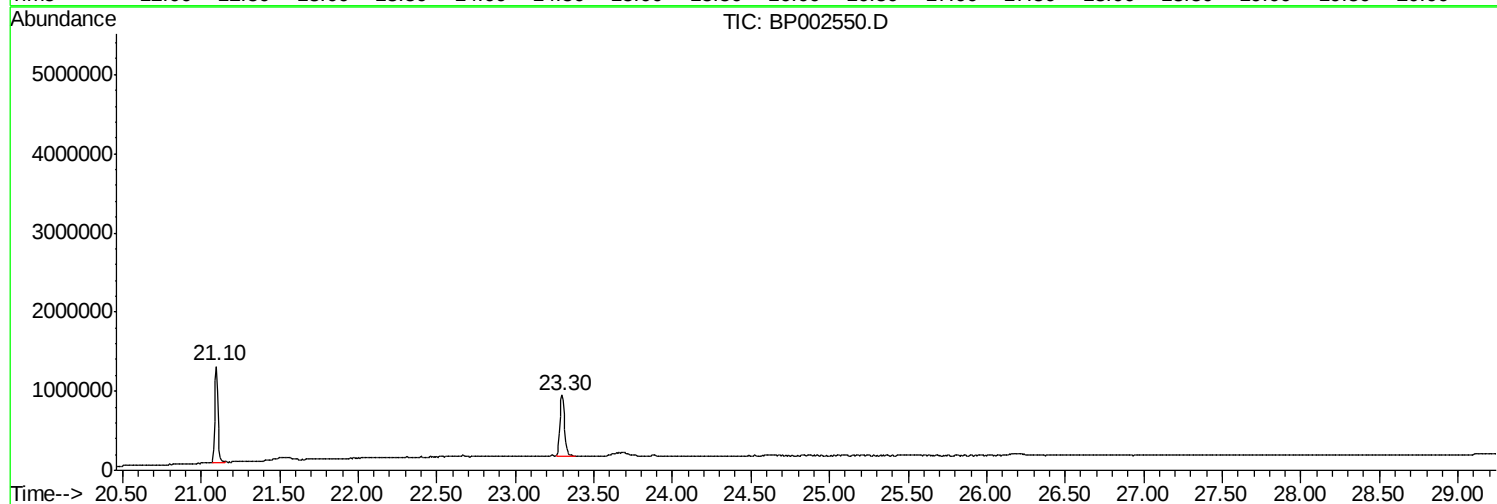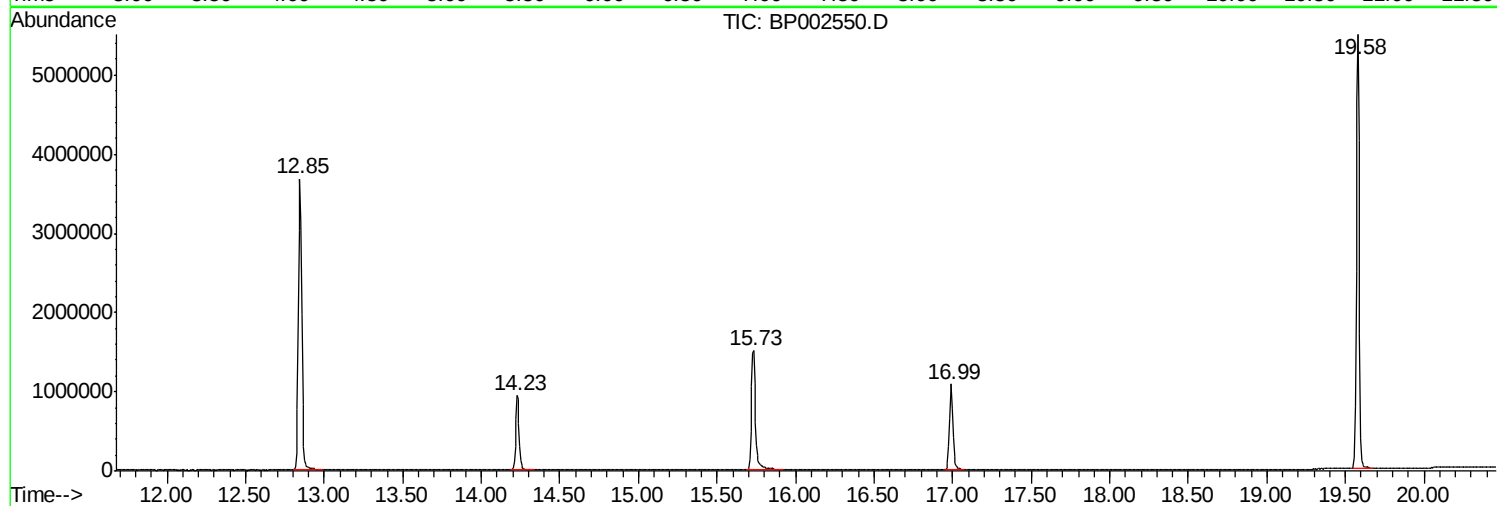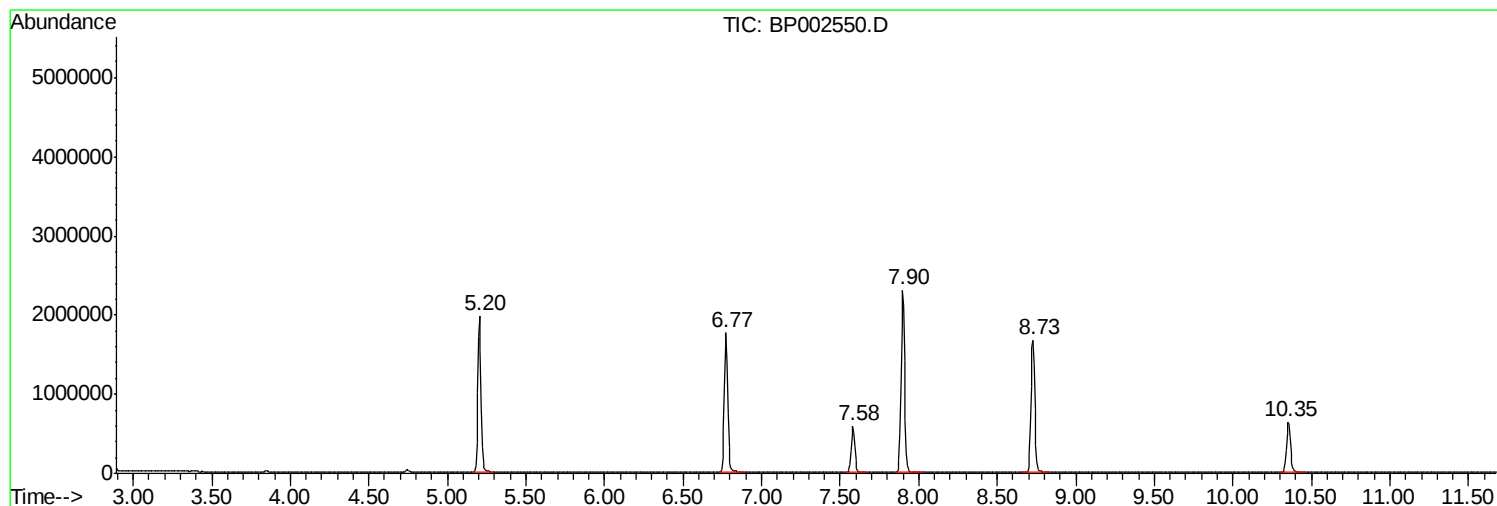

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP062620\
Data File : BP002550.D
Acq On : 26 Jun 2020 14:27
Operator : CG/JU
Sample : PB129799BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129799BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP062620\
Data File : BP002550.D
Acq On : 26 Jun 2020 14:27
Operator : CG/JU
Sample : PB129799BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129799BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc