

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062620\
 Data File : BP002554.D
 Acq On : 26 Jun 2020 16:48
 Operator : CG/JU
 Sample : L3049-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WEST-2-18.0

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.134	376	382	387	rBV	101096	144414	1.41%	0.119%
2	5.199	387	393	399	rVV	1304209	1918908	18.72%	1.577%
3	5.263	399	404	405	rVV	255677	328361	3.20%	0.270%
4	5.281	405	407	420	rVB	275316	384551	3.75%	0.316%
5	5.622	459	465	475	rVB	509571	754431	7.36%	0.620%
6	6.099	539	546	557	rBV	173593	273195	2.67%	0.225%
7	6.581	620	628	636	rBV	384022	573344	5.59%	0.471%
8	6.687	640	646	651	rVV	1364992	2019203	19.70%	1.659%
9	6.752	651	657	658	rVV	652908	1025273	10.00%	0.843%
10	6.769	658	660	665	rVV	777747	1053562	10.28%	0.866%
11	6.822	665	669	683	rVB	809415	1186120	11.57%	0.975%
12	6.987	690	697	707	rBV	951562	1451231	14.16%	1.193%
13	7.240	729	740	747	rBV	2903667	4583332	44.71%	3.767%
14	7.493	779	783	790	rVB	167527	244718	2.39%	0.201%
15	7.581	790	798	803	rVV	780352	1218553	11.89%	1.001%
16	7.634	803	807	812	rVV	286045	434261	4.24%	0.357%
17	7.699	812	818	832	rVB	1096965	1890476	18.44%	1.554%
18	7.899	842	852	857	rBV	2540984	4082342	39.82%	3.355%
19	7.952	857	861	875	rVV	884364	1370284	13.37%	1.126%
20	8.081	875	883	887	rVV	292058	441014	4.30%	0.362%
21	8.134	887	892	900	rVV	637270	964939	9.41%	0.793%
22	8.228	901	908	913	rVV2	1064895	1681145	16.40%	1.382%
23	8.275	913	916	924	rVB	139451	197165	1.92%	0.162%
24	8.387	929	935	952	rVB	469598	756706	7.38%	0.622%
25	8.540	952	961	965	rBV	610406	947298	9.24%	0.778%
26	8.587	965	969	977	rVB	581287	870026	8.49%	0.715%
27	8.687	979	986	989	rBV	1117470	1802672	17.59%	1.481%
28	8.728	989	993	996	rVV	1943283	3222887	31.44%	2.649%
29	8.757	996	998	1007	rVB2	840729	1282041	12.51%	1.054%
30	8.940	1017	1029	1035	rBV4	181800	427953	4.17%	0.352%
31	9.016	1035	1042	1048	rVV2	360176	591145	5.77%	0.486%
32	9.087	1048	1054	1059	rVB2	96052	155724	1.52%	0.128%
33	9.204	1069	1074	1079	rVV	520321	767009	7.48%	0.630%
34	9.263	1079	1084	1092	rVB	846841	1326840	12.94%	1.090%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP062620\
 Data File : BP002554.D
 Acq On : 26 Jun 2020 16:48
 Operator : CG/JU
 Sample : L3049-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WEST-2-18.0

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	9.469	1109	1119	1123	rBV	116762	198351	1.93%	0.163%
36	9.516	1123	1127	1131	rBV	113539	153385	1.50%	0.126%
37	9.616	1131	1144	1149	rBV2	1187138	2318259	22.61%	1.905%
38	9.763	1158	1169	1176	rBV2	2355003	4564668	44.53%	3.751%
39	9.846	1176	1183	1193	rVV3	281844	569441	5.55%	0.468%
40	9.934	1193	1198	1200	rVV	161114	266886	2.60%	0.219%
41	9.999	1203	1209	1216	rVV	2154772	3654869	35.65%	3.004%
42	10.075	1216	1222	1230	rVB2	160720	287992	2.81%	0.237%
43	10.287	1246	1258	1261	rBV2	240060	529508	5.17%	0.435%
44	10.351	1261	1269	1274	rVV2	1540530	3013605	29.40%	2.477%
45	10.404	1274	1278	1286	rVV3	888215	2041353	19.91%	1.678%
46	10.481	1286	1291	1299	rVV	546786	957408	9.34%	0.787%
47	10.587	1300	1309	1317	rVB	146219	247547	2.41%	0.203%
48	10.822	1339	1349	1359	rVB	730319	1304948	12.73%	1.072%
49	10.940	1359	1369	1374	rBV	556583	977416	9.53%	0.803%
50	11.022	1374	1383	1389	rVV2	462451	925734	9.03%	0.761%
51	11.275	1420	1426	1435	rVB	649634	1047948	10.22%	0.861%
52	11.469	1454	1459	1466	rVB	523517	848999	8.28%	0.698%
53	11.551	1466	1473	1483	rBV	1931574	3403707	33.20%	2.797%
54	11.698	1494	1498	1502	rVB	109724	148557	1.45%	0.122%
55	11.751	1502	1507	1511	rVV	391015	642448	6.27%	0.528%
56	11.875	1517	1528	1530	rBV2	115712	307128	3.00%	0.252%
57	11.916	1530	1535	1542	rVB	1418114	2286150	22.30%	1.879%
58	12.028	1542	1554	1560	rBV	1319856	2323766	22.67%	1.910%
59	12.245	1585	1591	1595	rBV	927021	1466569	14.31%	1.205%
60	12.293	1595	1599	1604	rVV2	619831	1113341	10.86%	0.915%
61	12.345	1604	1608	1610	rVV3	178360	337638	3.29%	0.277%
62	12.369	1610	1612	1618	rVB	246287	304125	2.97%	0.250%
63	12.481	1627	1631	1638	rBV3	79561	142209	1.39%	0.117%
64	12.551	1638	1643	1649	rVV2	210901	455311	4.44%	0.374%
65	12.604	1649	1652	1657	rVB	197016	265242	2.59%	0.218%
66	12.710	1666	1670	1675	rBV	126910	164545	1.61%	0.135%
67	12.775	1675	1681	1686	rVV	240540	375189	3.66%	0.308%
68	12.845	1686	1693	1700	rVV	4295141	6768162	66.02%	5.562%
69	12.934	1704	1708	1713	rVB	111649	170327	1.66%	0.140%
70	13.057	1724	1729	1737	rVB	458742	674922	6.58%	0.555%
71	13.175	1739	1749	1754	rBV	563960	1005913	9.81%	0.827%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062620\
 Data File : BP002554.D
 Acq On : 26 Jun 2020 16:48
 Operator : CG/JU
 Sample : L3049-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WEST-2-18.0

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	13.228	1754	1758	1761	rBV2	237750	392143	3.83%	0.322%
73	13.392	1780	1786	1798	rVB3	343893	936452	9.14%	0.770%
74	13.545	1803	1812	1817	rBV2	598411	1353559	13.20%	1.112%
75	13.598	1817	1821	1829	rVB2	546653	880416	8.59%	0.724%
76	13.692	1829	1837	1843	rBV	718482	1022720	9.98%	0.840%
77	13.787	1849	1853	1856	rBV	186706	297816	2.91%	0.245%
78	13.816	1856	1858	1864	rVB2	191327	249378	2.43%	0.205%
79	13.951	1876	1881	1887	rBV3	120835	185370	1.81%	0.152%
80	14.228	1918	1928	1934	rBV3	1485680	2586157	25.23%	2.125%
81	14.287	1934	1938	1941	rVV2	119556	173833	1.70%	0.143%
82	14.328	1941	1945	1949	rVB2	134583	190067	1.85%	0.156%
83	14.445	1961	1965	1974	rVB	98879	228921	2.23%	0.188%
84	14.645	1991	1999	2005	rVB4	174977	336298	3.28%	0.276%
85	14.716	2005	2011	2016	rBV	133026	192119	1.87%	0.158%
86	14.863	2030	2036	2039	rBV	132131	231022	2.25%	0.190%
87	14.910	2041	2044	2050	rVB	109772	171361	1.67%	0.141%
88	15.081	2068	2073	2078	rVB3	104930	202408	1.97%	0.166%
89	15.216	2086	2096	2102	rVB2	59871	154649	1.51%	0.127%
90	15.281	2102	2107	2112	rBV2	139919	216528	2.11%	0.178%
91	15.410	2121	2129	2133	rVV	330719	492380	4.80%	0.405%
92	15.728	2176	2183	2194	rBV	3450423	5437042	53.04%	4.468%
93	16.351	2284	2289	2294	rBV2	180586	277532	2.71%	0.228%
94	16.986	2387	2397	2402	rBV	1686033	2508467	24.47%	2.061%
95	17.028	2402	2404	2410	rVB	109762	138981	1.36%	0.114%
96	19.580	2832	2838	2843	rBV	7541465	10251179	100.00%	8.424%
97	20.839	3047	3052	3057	rBV2	419715	606663	5.92%	0.499%
98	20.886	3057	3060	3070	rVB	182784	255931	2.50%	0.210%
99	21.092	3090	3095	3110	rBV	2038861	2651365	25.86%	2.179%
100	23.292	3462	3469	3481	rVB2	1312544	2428576	23.69%	1.996%


Sum of corrected areas: 121684022

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062620\
Data File : BP002554.D
Acq On : 26 Jun 2020 16:48
Operator : CG/JU
Sample : L3049-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WEST-2-18.0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

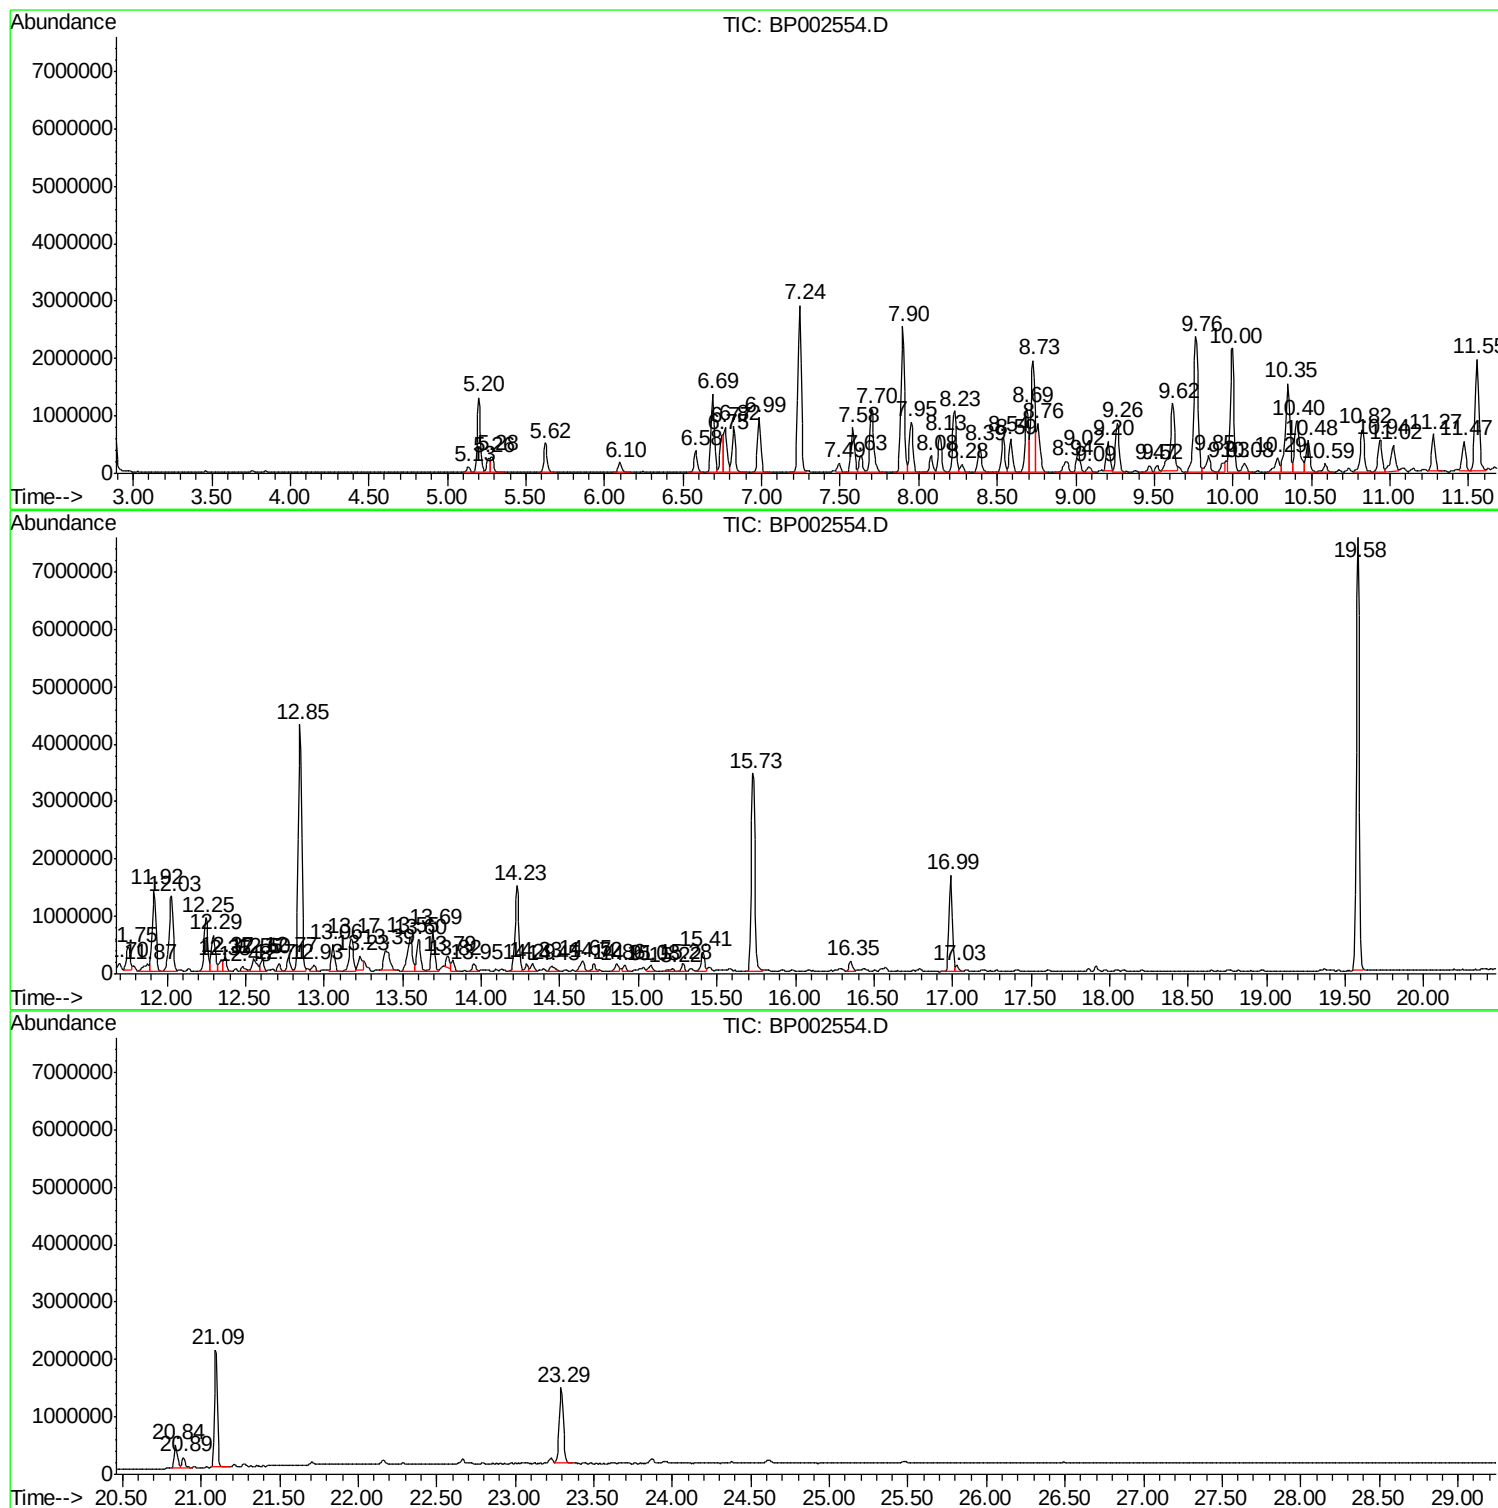

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP062620\
Data_File : BP002554.D
Acq_On : 26 Jun 2020 16:488
Operator : CG/JUU
Sample : L3049-044
Misc :
ALS_Vial : 10 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
WEST-2-18.0

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
