


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062620\
 Data File : BP002545.D
 Acq On : 26 Jun 2020 09:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 24 13:54:06 2020

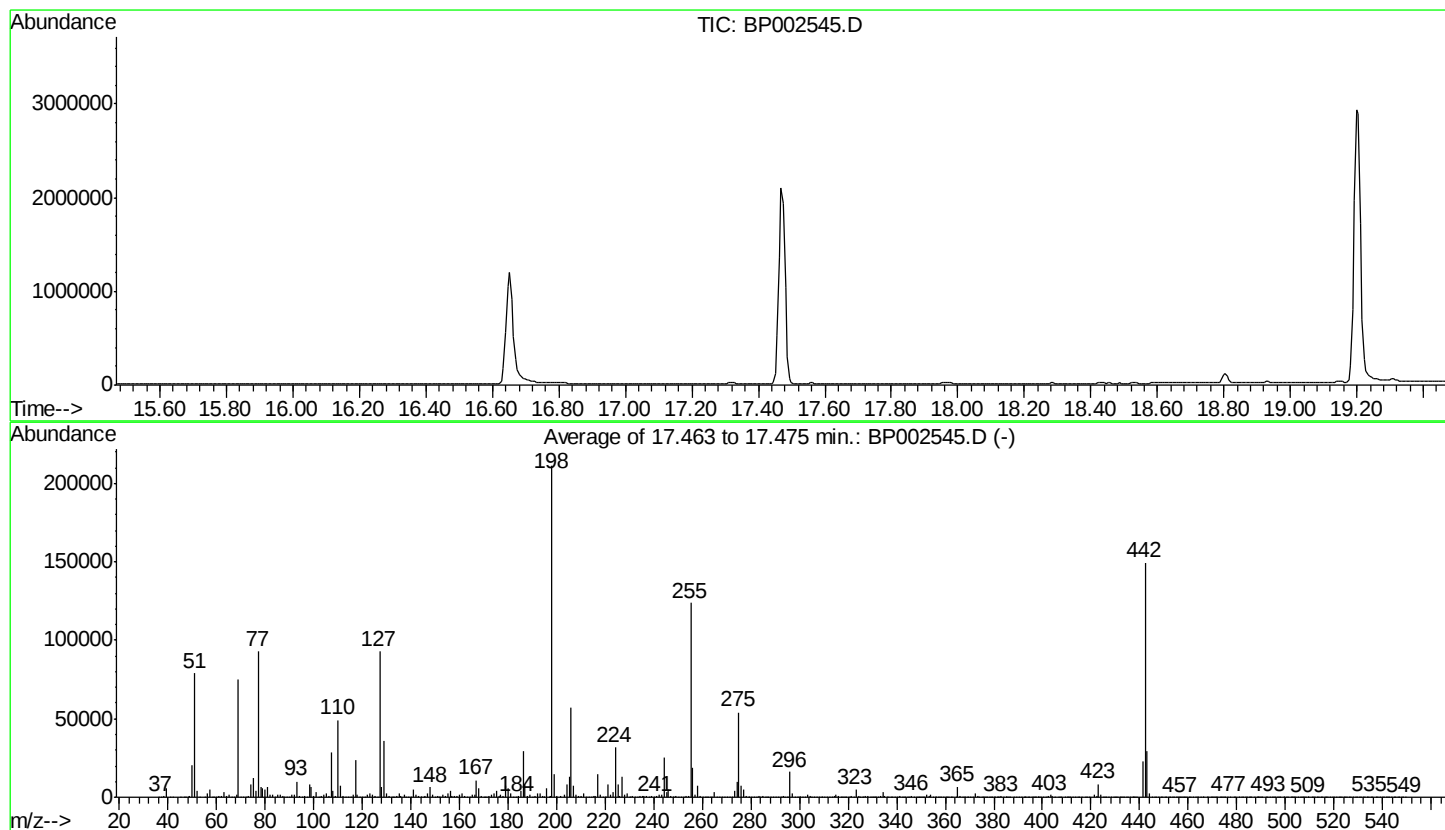

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	79089	PASS
68	69	0.00	2	1.7	1286	PASS
69	198	0.00	100	35.6	75170	PASS
70	69	0.00	2	0.4	320	PASS
127	198	10	80	44.0	92928	PASS
197	198	0.00	2	0.3	612	PASS
198	198	100	100	100.0	211334	PASS
199	198	5	9	7.0	14742	PASS
275	198	10	60	25.5	53928	PASS
365	198	1	100	3.3	6910	PASS
441	198	0.01	100	10.7	22531	PASS
442	198	50	100	70.8	149554	PASS
443	442	15	24	19.9	29802	PASS