

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062624\
 Data File : BP020646.D
 Acq On : 26 Jun 2024 11:55
 Operator : MA/JU
 Sample : PB161716BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK716

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020646.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	12	rVB	89303	105038	2.03%	0.198%
2	3.276	46	49	56	rVB	55503	73368	1.42%	0.139%
3	3.687	116	119	135	rBV	679521	1007503	19.50%	1.903%
4	4.005	169	173	177	rBV2	13075	18026	0.35%	0.034%
5	6.922	661	669	683	rBV	810945	1353507	26.20%	2.556%
6	7.093	691	698	709	rVB	688919	1051415	20.35%	1.986%
7	7.287	724	731	747	rVB	805960	1343606	26.01%	2.537%
8	7.752	802	810	818	rBV	754740	1202529	23.28%	2.271%
9	8.446	921	928	942	rBV	1039616	1711055	33.12%	3.231%
10	8.893	997	1004	1015	rBV	842673	1364100	26.41%	2.576%
11	9.605	1118	1125	1136	rBV	685358	1111057	21.51%	2.098%
12	10.140	1208	1216	1232	rBV	896922	1742046	33.72%	3.290%
13	10.516	1271	1280	1289	rBV	1004845	1780009	34.46%	3.361%
14	10.652	1296	1303	1322	rBV	824313	1489868	28.84%	2.813%
15	12.110	1545	1551	1561	rBV	14358	29022	0.56%	0.055%
16	13.334	1754	1759	1764	rVB7	3482	7140	0.14%	0.013%
17	13.775	1827	1834	1844	rBV	1958590	2756467	53.36%	5.205%
18	14.057	1873	1882	1897	rBV	2167293	3243354	62.78%	6.125%
19	14.369	1927	1935	1945	rBV	1712833	2504047	48.47%	4.729%
20	14.581	1963	1971	1984	rBV	663696	1200864	23.25%	2.268%
21	14.710	1991	1993	1996	rVB4	7124	6072	0.12%	0.011%
22	15.381	2099	2107	2119	rBV	2528202	4023485	77.89%	7.598%
23	15.510	2122	2129	2141	rVV	836032	1215284	23.53%	2.295%
24	15.616	2144	2147	2155	rVB2	14212	26304	0.51%	0.050%
25	15.904	2190	2196	2199	rBV4	6299	9869	0.19%	0.019%
26	16.181	2238	2243	2249	rBV2	10092	16669	0.32%	0.031%
27	16.851	2353	2357	2362	rVB8	4352	6202	0.12%	0.012%
28	16.963	2369	2376	2383	rBV4	6574	13256	0.26%	0.025%
29	17.181	2405	2413	2423	rBV	2021145	3044271	58.93%	5.749%
30	17.287	2424	2431	2445	rVV	3084406	4418979	85.54%	8.345%
31	18.116	2567	2572	2577	rBV9	17216	35296	0.68%	0.067%
32	19.210	2754	2758	2763	rBV2	38532	67890	1.31%	0.128%
33	19.286	2768	2771	2778	rVB	34810	52385	1.01%	0.099%
34	19.469	2799	2802	2805	rBV5	9989	13319	0.26%	0.025%
35	19.669	2829	2836	2846	rBV	3685597	5165877	100.00%	9.755%
36	21.633	3164	3170	3180	rBV	1829732	2994800	57.97%	5.655%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062624\
Data File : BP020646.D
Acq On : 26 Jun 2024 11:55
Operator : MA/JU
Sample : PB161716BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK716

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Title : SVOA CALIBRATION

37	24.763	3692	3702	3718	rVB	1539337	4088222	79.14%	7.720%
38	24.986	3731	3740	3753	rVB	920893	2662215	51.53%	5.027%




Sum of corrected areas: 52954416

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062624\
Data File : BP020646.D
Acq On : 26 Jun 2024 11:55
Operator : MA/JU
Sample : PB161716BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK716

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

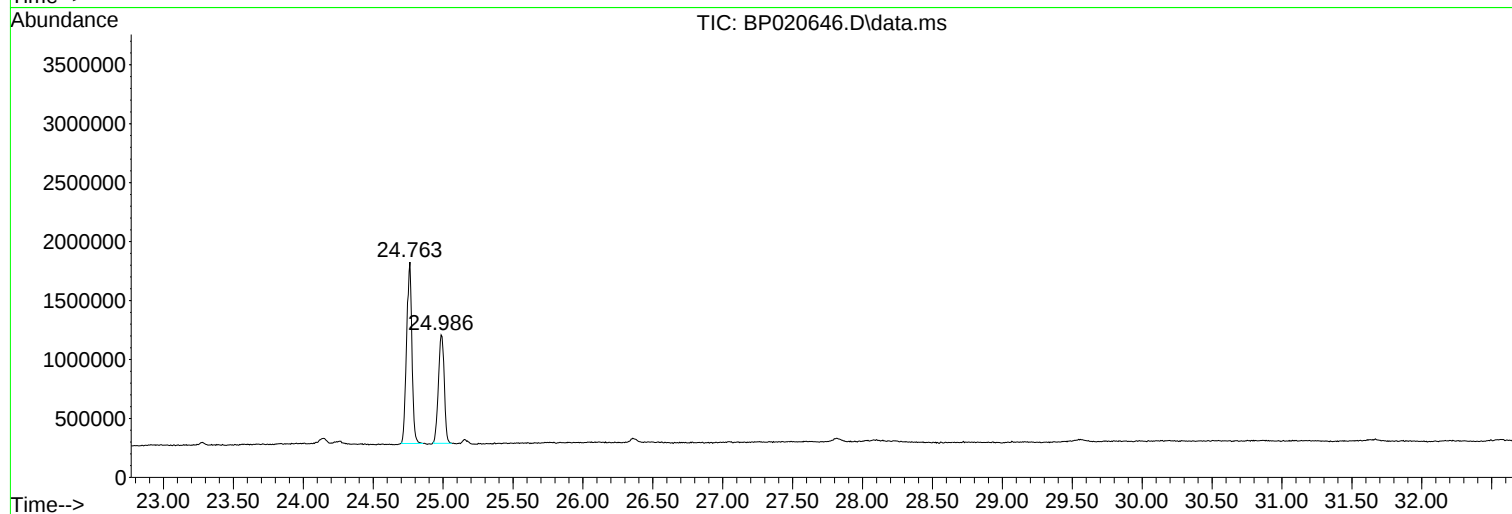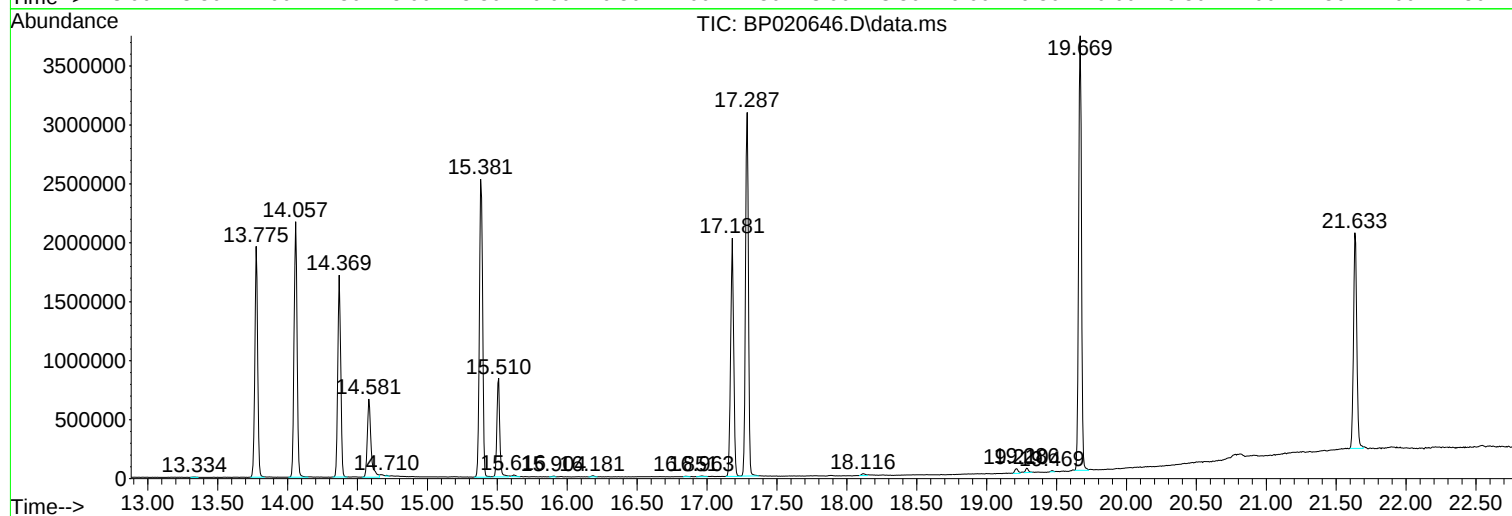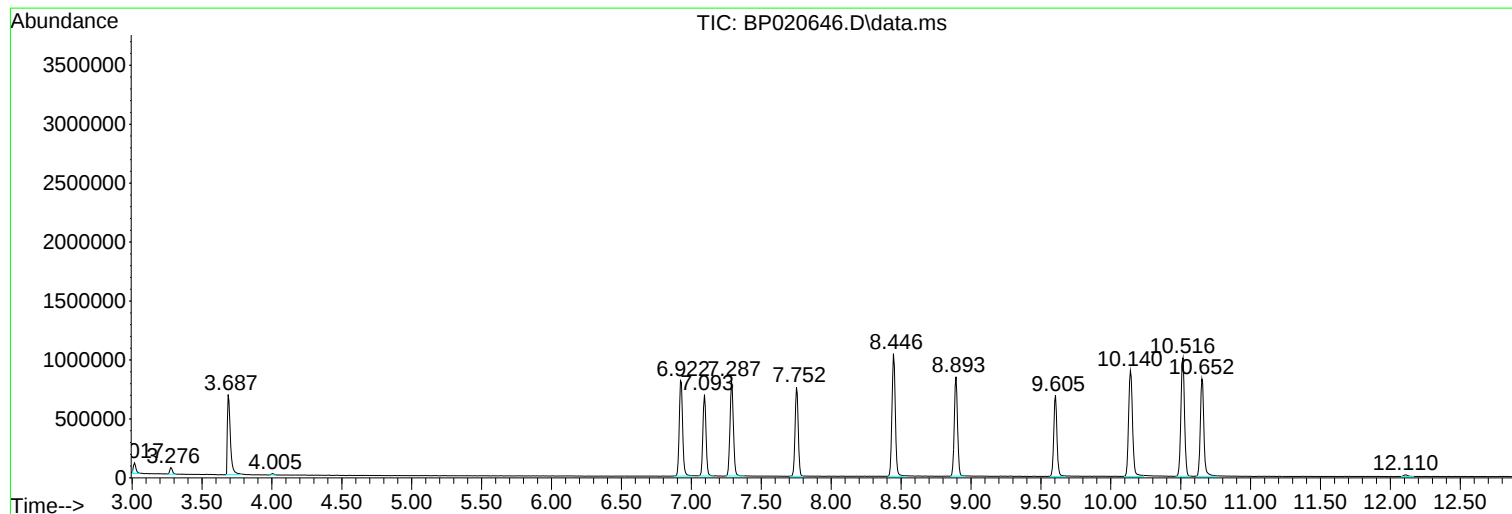

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062624\
Data File : BP020646.D
Acq On : 26 Jun 2024 11:55
Operator : MA/JU
Sample : PB161716BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK716

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062624\
Data File : BP020646.D
Acq On : 26 Jun 2024 11:55
Operator : MA/JU
Sample : PB161716BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK716

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------