

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010873.D
 Acq On : 27 Jun 2022 12:34
 Operator : CG/JU
 Sample : N3392-07 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Jun 27 23:15:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 27 23:12:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.710	152	340648	20.000	ng/ul	0.00
20) Naphthalene-d8	10.504	136	1353070	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.369	164	701096	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.133	188	1345502	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.245	240	1345893	20.000	ng/ul	# 0.00
88) Perylene-d12	23.609	264	1482866	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.204	96	26149	2.904	ng/uL	0.00
4) Pyridine-d5	3.616	84	138935	5.796	ng/ul	0.00
7) Phenol-d5	6.887	99	206068	7.642	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.051	67	666620	37.800	ng/ul	0.00
11) 2-Chlorophenol-d4	7.245	132	652779	29.178	ng/ul	0.00
15) 4-Methylphenol-d8	8.422	113	384185	18.023	ng/ul	0.00
21) Nitrobenzene-d5	8.869	128	387234	44.956	ng/ul	0.00
24) 2-Nitrophenol-d4	9.592	143	331522	46.521	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	595409	33.815	ng/ul	0.00
31) 4-Chloroaniline-d4	10.651	131	855274	29.757	ng/ul	0.00
46) Dimethylphthalate-d6	13.786	166	1840599	38.325	ng/ul	0.00
49) Acenaphthylene-d8	14.057	160	2294543	37.435	ng/ul	0.00
54) 4-Nitrophenol-d4	14.580	143	45678	6.089	ng/ul	0.00
60) Fluorene-d10	15.363	176	1626781	39.472	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.486	200	144112	32.328	ng/ul	0.00
73) Anthracene-d10	17.233	188	2515381	42.019	ng/ul	0.00
81) Pyrene-d10	19.480	212	2852496	38.902	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.456	264	3170899	43.273	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.539	105	35567	1.086	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010873.D
Acq On : 27 Jun 2022 12:34
Operator : CG/JU
Sample : N3392-07 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: Jun 27 23:15:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 27 23:12:49 2022
Response via : Initial Calibration

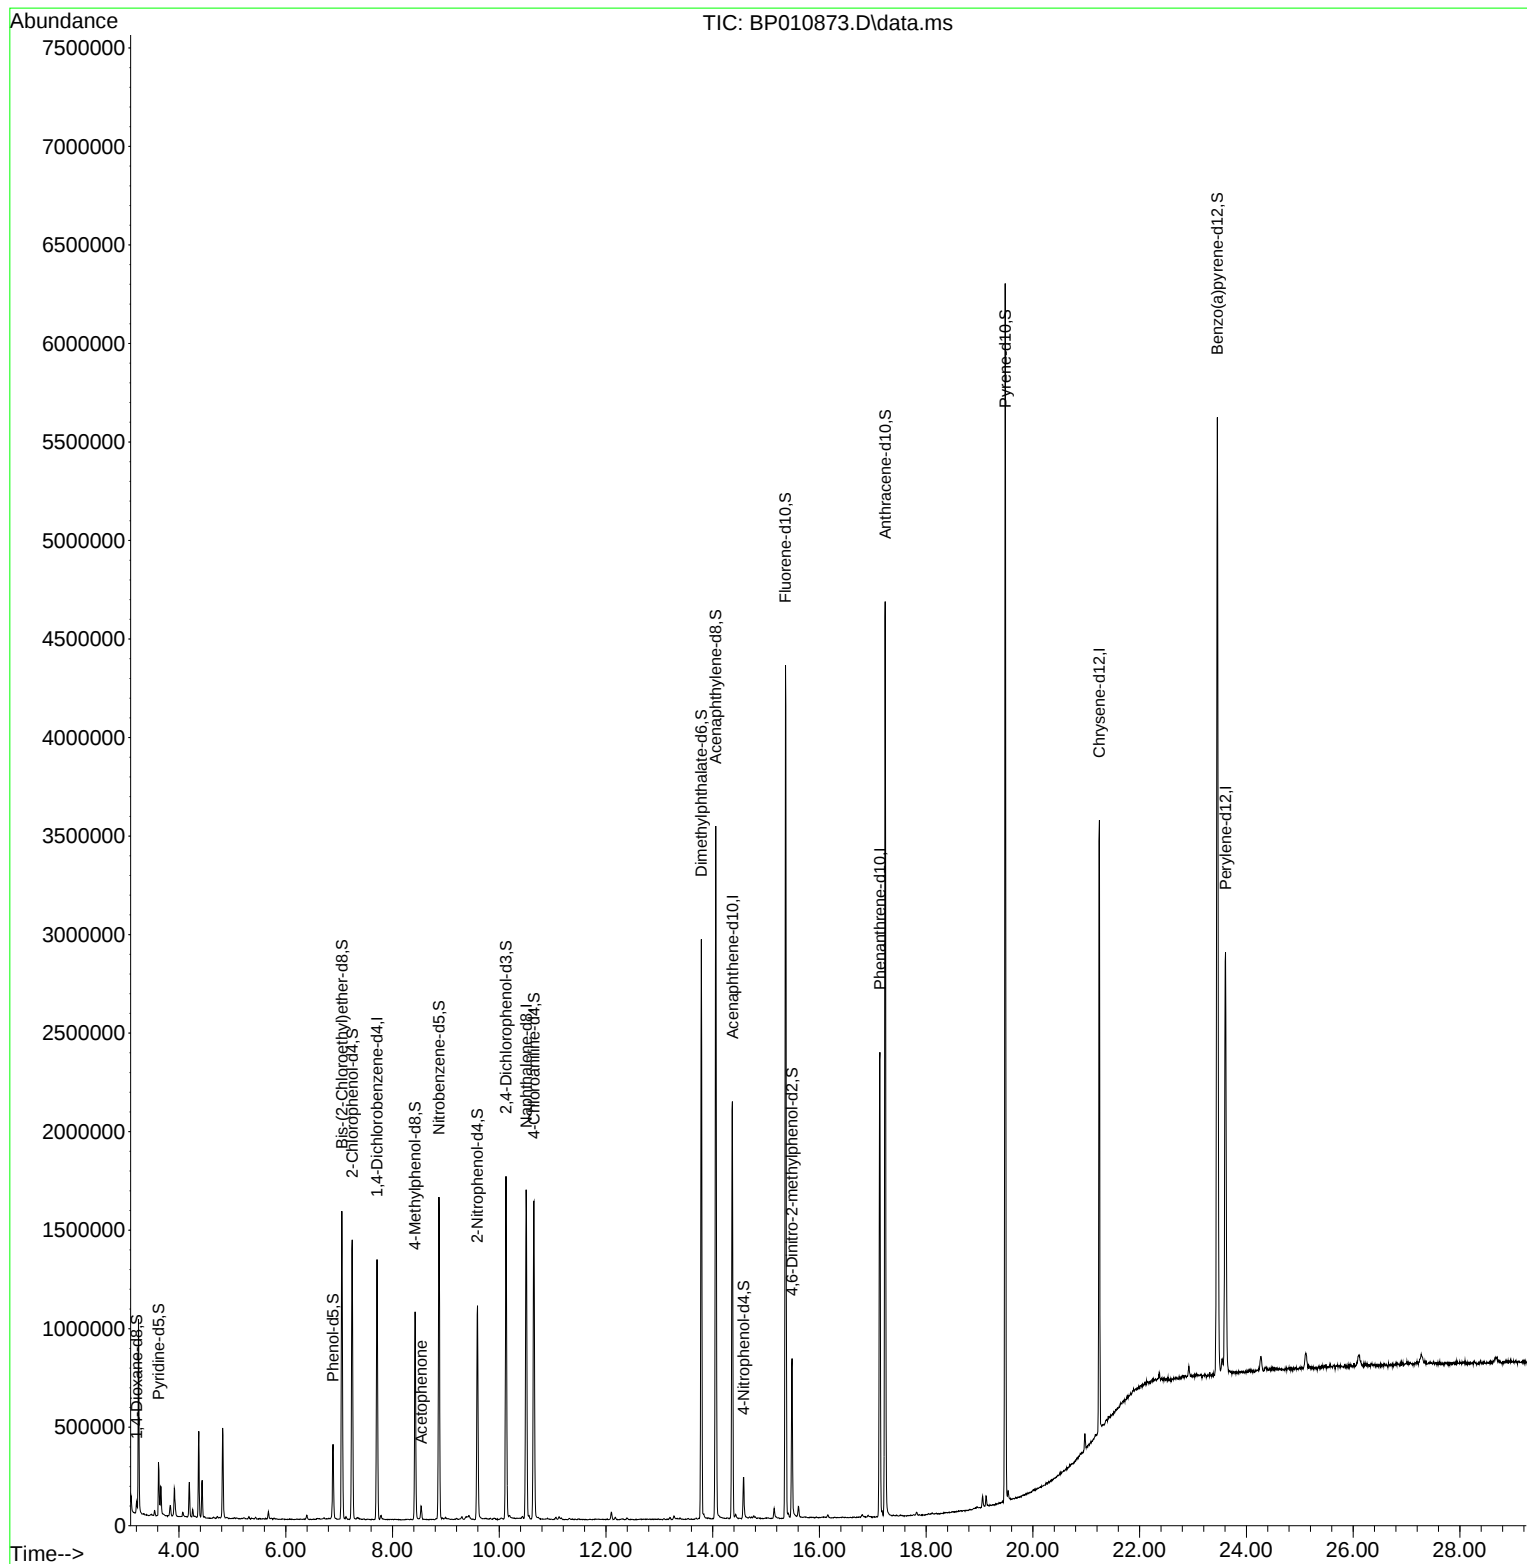

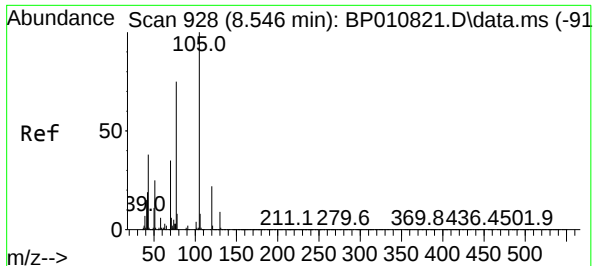

#16
 Acetophenone
 Concen: 1.086 ng/ul
 RT: 8.539 min Scan# 91
 Delta R.T. 0.006 min
 Lab File: BP010873.D
 Acq: 27 Jun 2022 12:34

Instrument :
 BNA_P
 ClientSampleId :

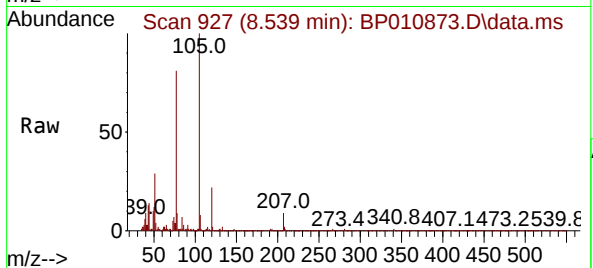

Tgt Ion:105 Resp: 35567
 Ion Ratio Lower Upper
 105 100
 77 81.1 67.5 101.3
 51 29.5 29.6 44.4#

