

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010874.D
 Acq On : 27 Jun 2022 13:08
 Operator : CG/JU
 Sample : N3392-11 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Jun 27 23:15:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 27 23:12:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.710	152	379983	20.000	ng/ul	0.00
20) Naphthalene-d8	10.504	136	1515335	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.369	164	794646	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.128	188	1579127	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.245	240	1601469	20.000	ng/ul	# 0.00
88) Perylene-d12	23.610	264	1720302	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	31281	3.114	ng/uL	0.00
4) Pyridine-d5	3.616	84	270668	10.123	ng/ul	0.00
7) Phenol-d5	6.887	99	272704	9.066	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.052	67	825804	41.979	ng/ul	0.00
11) 2-Chlorophenol-d4	7.246	132	839744	33.649	ng/ul	0.00
15) 4-Methylphenol-d8	8.422	113	506536	21.302	ng/ul	0.00
21) Nitrobenzene-d5	8.869	128	486132	50.394	ng/ul	0.00
24) 2-Nitrophenol-d4	9.593	143	439510	55.071	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	764615	38.774	ng/ul	0.00
31) 4-Chloroaniline-d4	10.651	131	1142366	35.489	ng/ul	0.00
46) Dimethylphthalate-d6	13.787	166	2510653	46.123	ng/ul	0.00
49) Acenaphthylene-d8	14.057	160	3039951	43.758	ng/ul	0.00
54) 4-Nitrophenol-d4	14.575	143	69276	8.148	ng/ul	0.00
60) Fluorene-d10	15.363	176	2220946	47.545	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.486	200	227777	43.537	ng/ul	0.00
73) Anthracene-d10	17.228	188	3446685	49.058	ng/ul	0.00
81) Pyrene-d10	19.480	212	3966620	45.463	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.457	264	4362437	51.317	ng/ul	0.00
Target Compounds						Qvalue
16) Acetophenone	8.534	105	41805	1.145	ng/ul	90
30) Naphthalene	10.557	128	159663	2.022	ng/ul	100
36) 2-Methylnaphthalene	12.175	142	53677	1.050	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010874.D
Acq On : 27 Jun 2022 13:08
Operator : CG/JU
Sample : N3392-11 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Jun 27 23:15:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 27 23:12:49 2022
Response via : Initial Calibration




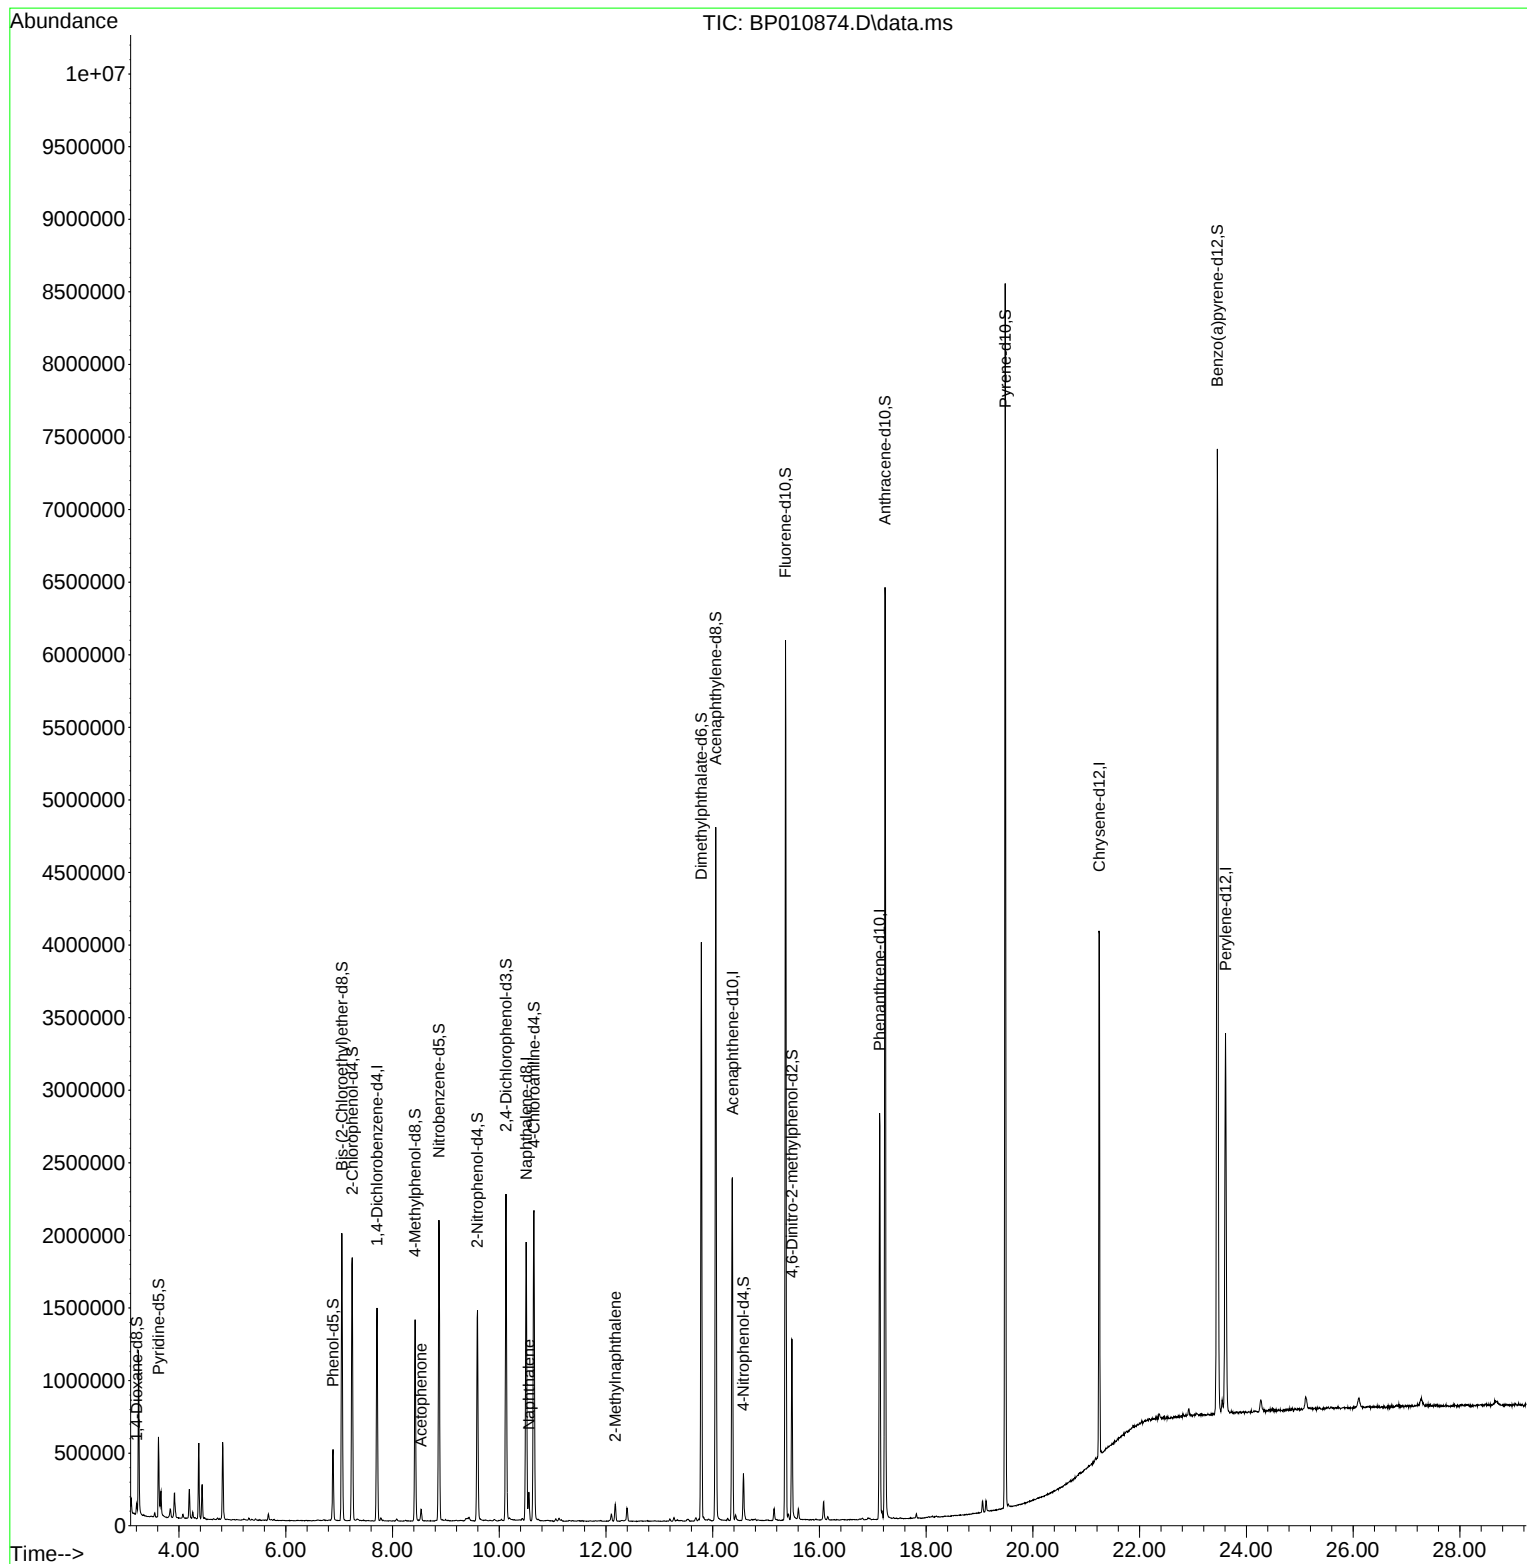


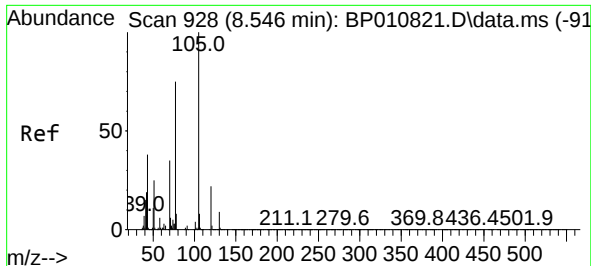

#16
Acetophenone
Concen: 1.145 ng/ul
RT: 8.534 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP010874.D
Acq: 27 Jun 2022 13:08




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:105 Resp: 41805
Ion Ratio Lower Upper
105 100
77 75.3 67.5 101.3
51 31.3 29.6 44.4

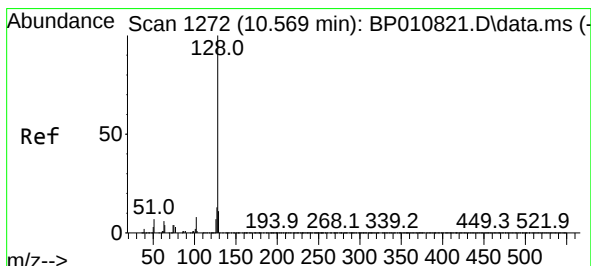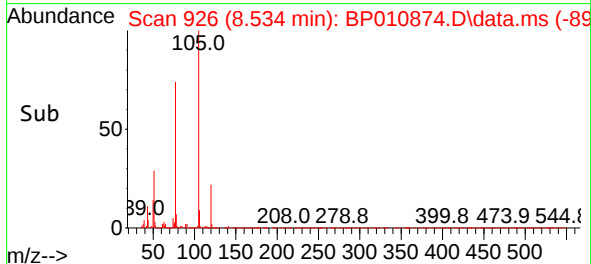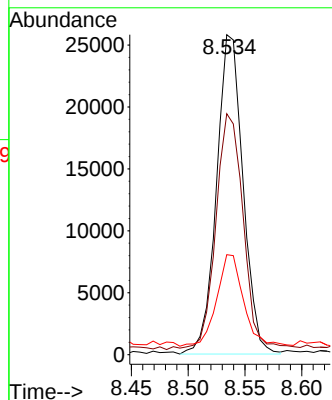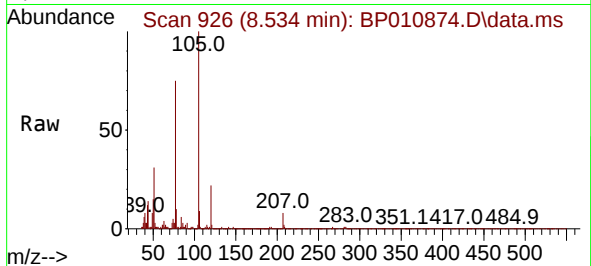

#30
Naphthalene
Concen: 2.022 ng/ul
RT: 10.557 min Scan# 1270
Delta R.T. 0.000 min
Lab File: BP010874.D
Acq: 27 Jun 2022 13:08

Tgt Ion:128 Resp: 159663
Ion Ratio Lower Upper
128 100
129 10.8 8.7 13.1
127 12.9 10.2 15.4

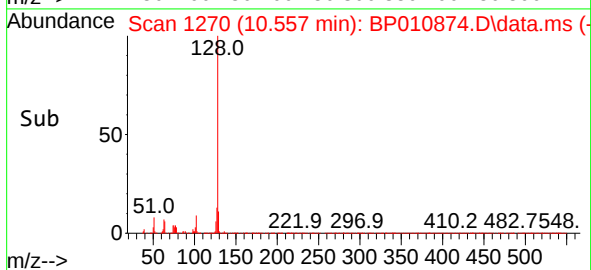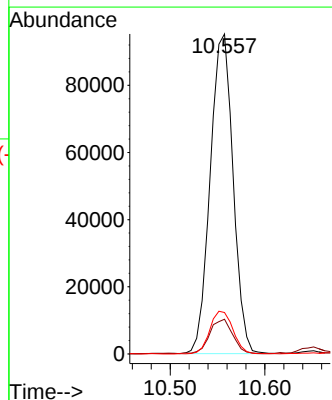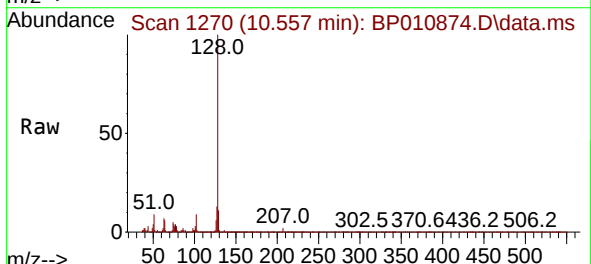

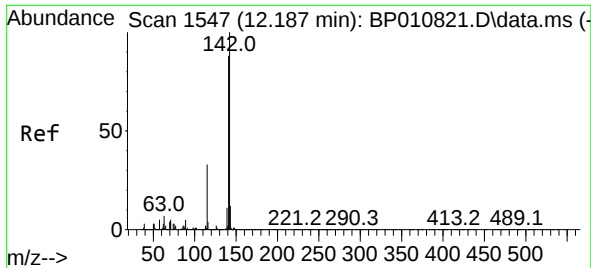

#36

2-Methylnaphthalene

Concen: 1.050 ng/ul

RT: 12.175 min Scan# 1

Delta R.T. 0.000 min


Lab File: BP010874.D

Acq: 27 Jun 2022 13:08

Instrument :

BNA_P

ClientSampleId :

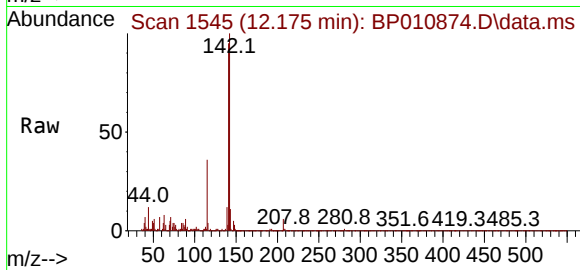

Tgt Ion:142 Resp: 53677

Ion Ratio Lower Upper

142 100

141 95.4 70.1 105.1

