

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010880.D
 Acq On : 27 Jun 2022 16:32
 Operator : CG/JU
 Sample : N3392-08 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Jun 27 23:16:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 27 23:12:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.711	152	513130	20.000	ng/u1	0.00
20) Naphthalene-d8	10.505	136	2173930	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.363	164	1201870	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.128	188	2161958	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.239	240	1544719	20.000	ng/u1	# 0.00
88) Perylene-d12	23.604	264	1493375	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	35628	2.627	ng/uL	0.00
4) Pyridine-d5	3.617	84	305228	8.453	ng/u1	0.00
7) Phenol-d5	6.887	99	314568	7.744	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.052	67	988883	37.225	ng/u1	0.00
11) 2-Chlorophenol-d4	7.240	132	964605	28.623	ng/u1	0.00
15) 4-Methylphenol-d8	8.422	113	600038	18.687	ng/u1	0.00
21) Nitrobenzene-d5	8.869	128	595615	43.038	ng/u1	0.00
24) 2-Nitrophenol-d4	9.593	143	550548	48.085	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	931554	32.928	ng/u1	0.00
31) 4-Chloroaniline-d4	10.646	131	1360648	29.464	ng/u1	0.00
46) Dimethylphthalate-d6	13.787	166	3143062	38.177	ng/u1	0.00
49) Acenaphthylene-d8	14.057	160	3779582	35.971	ng/u1	0.00
54) 4-Nitrophenol-d4	14.575	143	68646	5.338	ng/u1	0.00
60) Fluorene-d10	15.363	176	2618307	37.060	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.487	200	247586	34.566	ng/u1	0.00
73) Anthracene-d10	17.228	188	3761756	39.108	ng/u1	0.00
81) Pyrene-d10	19.481	212	3704827	44.023	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.451	264	3021154	40.939	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.534	105	50279	1.020	ng/u1#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010880.D
Acq On : 27 Jun 2022 16:32
Operator : CG/JU
Sample : N3392-08 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: Jun 27 23:16:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 27 23:12:49 2022
Response via : Initial Calibration

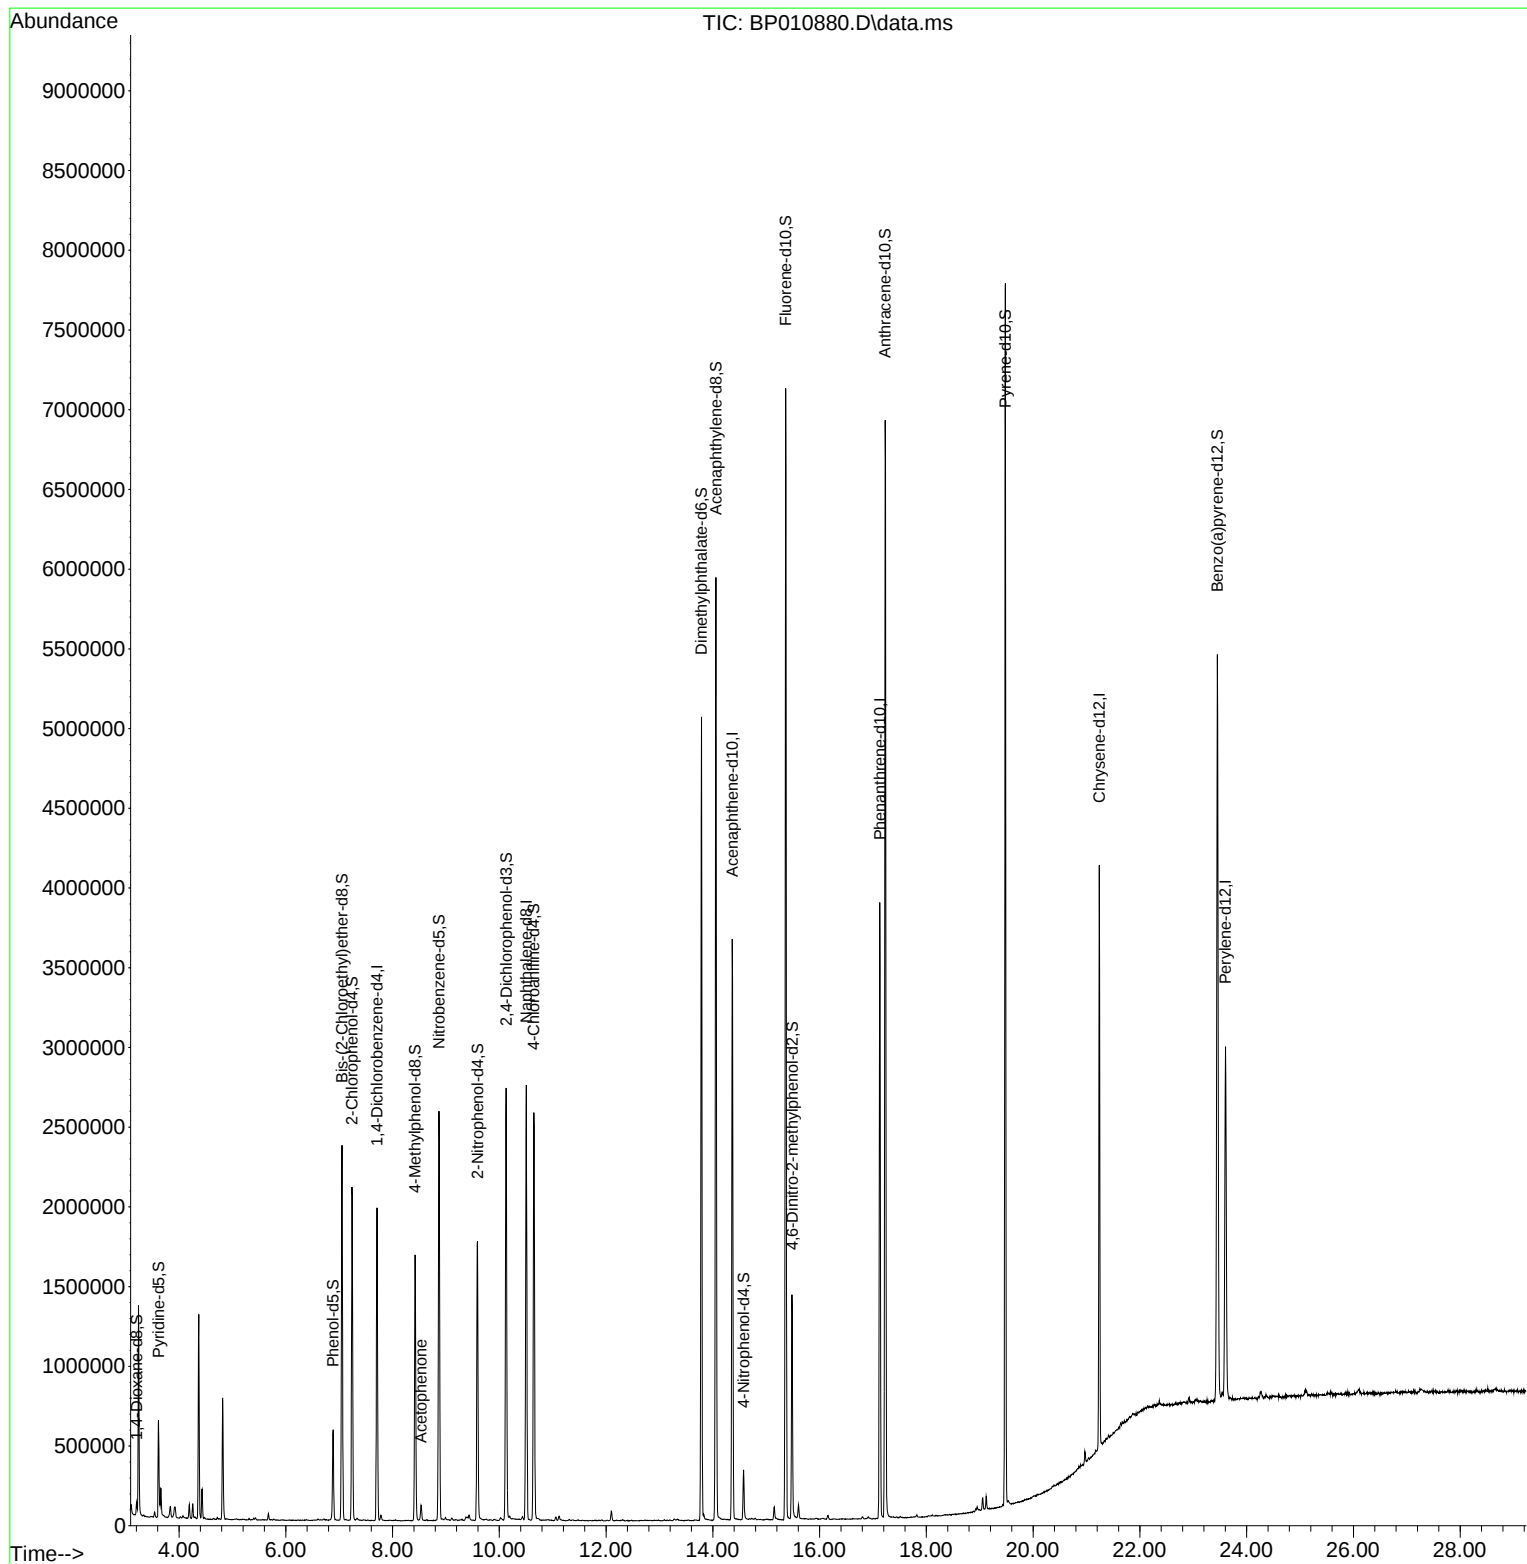

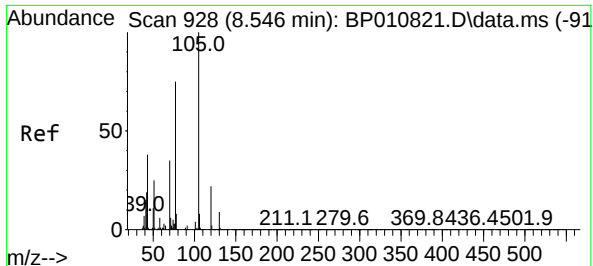

#16
 Acetophenone
 Concen: 1.020 ng/ul
 RT: 8.534 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BP010880.D
 Acq: 27 Jun 2022 16:32

Instrument :
 BNA_P
 ClientSampleId :

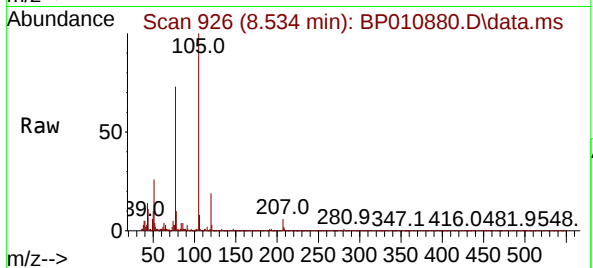

Tgt Ion:105 Resp: 50279
 Ion Ratio Lower Upper
 105 100
 77 73.0 67.5 101.3
 51 26.1 29.6 44.4#

