

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010883.D
 Acq On : 27 Jun 2022 18:14
 Operator : CG/JU
 Sample : N3392-21 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Jun 27 23:16:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 27 23:12:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.710	152	459907	20.000	ng/ul	0.00
20) Naphthalene-d8	10.504	136	1927070	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.363	164	1051460	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.128	188	1895251	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.239	240	1432051	20.000	ng/ul	# 0.00
88) Perylene-d12	23.604	264	1432626	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	39166	3.221	ng/uL	0.00
4) Pyridine-d5	3.616	84	323557	9.998	ng/ul	0.00
7) Phenol-d5	6.887	99	327720	9.002	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.052	67	1069390	44.914	ng/ul	0.00
11) 2-Chlorophenol-d4	7.240	132	1029477	34.083	ng/ul	0.00
15) 4-Methylphenol-d8	8.422	113	627405	21.800	ng/ul	0.00
21) Nitrobenzene-d5	8.869	128	643375	52.445	ng/ul	0.00
24) 2-Nitrophenol-d4	9.593	143	586008	57.739	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	983193	39.206	ng/ul	0.00
31) 4-Chloroaniline-d4	10.646	131	1555549	38.000	ng/ul	0.00
46) Dimethylphthalate-d6	13.787	166	3280561	45.547	ng/ul	0.00
49) Acenaphthylene-d8	14.057	160	3982954	43.328	ng/ul	0.00
54) 4-Nitrophenol-d4	14.575	143	70702	6.285	ng/ul	0.00
60) Fluorene-d10	15.363	176	2762182	44.689	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200	260650	41.510	ng/ul	0.00
73) Anthracene-d10	17.228	188	3957215	46.930	ng/ul	0.00
81) Pyrene-d10	19.480	212	3957315	50.723	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.457	264	3471822	49.041	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.534	105	46480	1.052	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010883.D
Acq On : 27 Jun 2022 18:14
Operator : CG/JU
Sample : N3392-21 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: Jun 27 23:16:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 27 23:12:49 2022
Response via : Initial Calibration

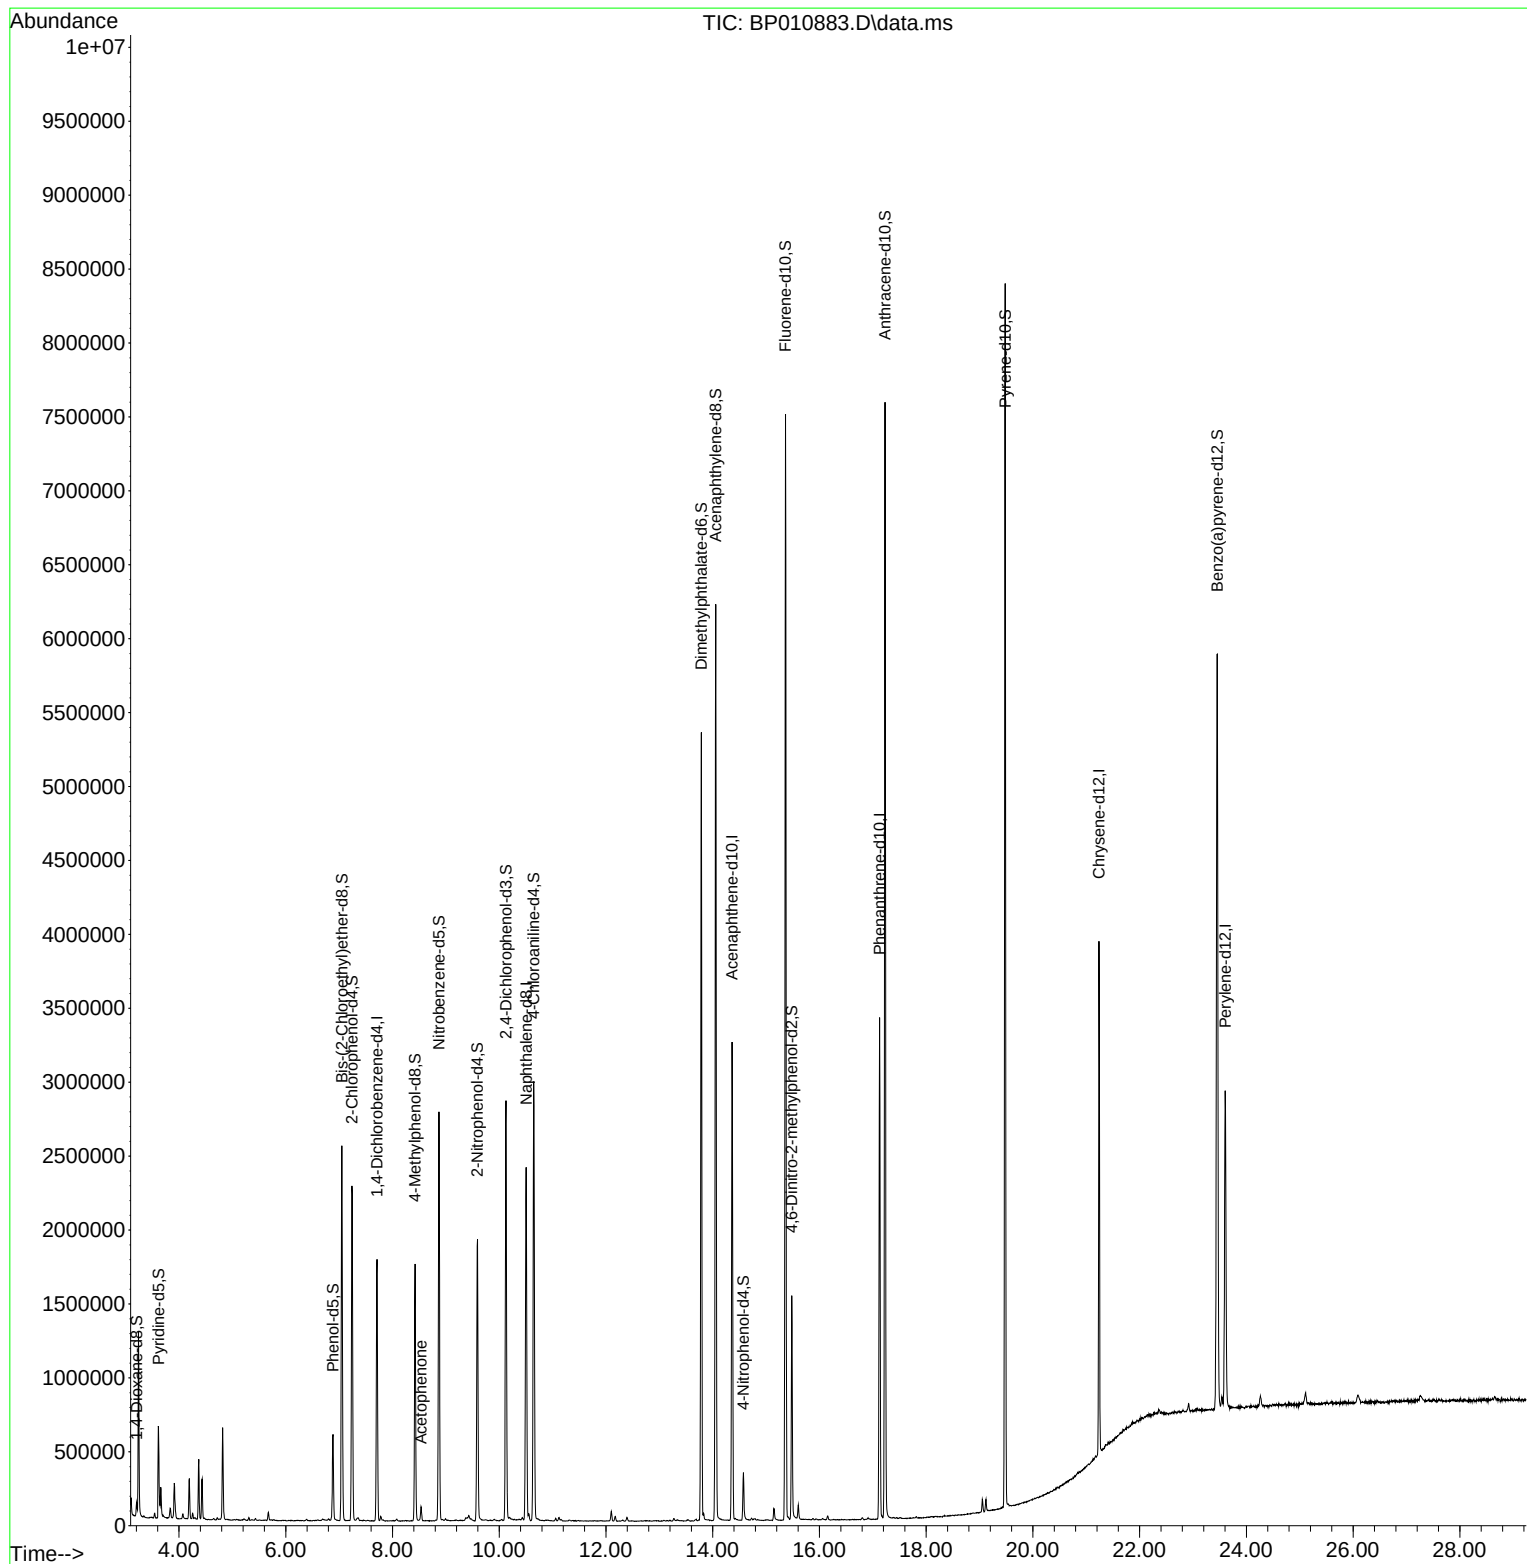

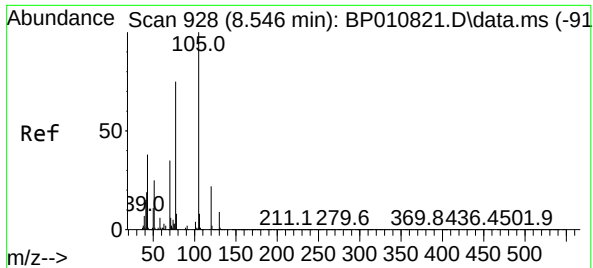

#16
 Acetophenone
 Concen: 1.052 ng/ul
 RT: 8.534 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BP010883.D
 Acq: 27 Jun 2022 18:14

Instrument :
 BNA_P
 ClientSampleId :

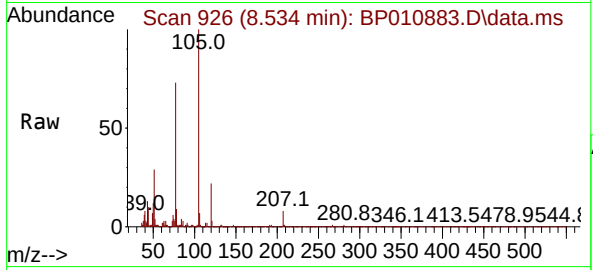

Tgt Ion:	105	Resp:	46480
Ion	Ratio	Lower	Upper
105	100		
77	73.2	67.5	101.3
51	29.5	29.6	44.4#

