

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010886.D
 Acq On : 27 Jun 2022 19:56
 Operator : CG/JU
 Sample : N3425-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Jun 27 23:17:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 27 23:12:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.710	152	437866	20.000	ng/ul	0.00
20) Naphthalene-d8	10.504	136	1751939	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.363	164	878488	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.127	188	1575696	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.239	240	1465528	20.000	ng/ul	# 0.00
88) Perylene-d12	23.603	264	1662397	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.204	96	62529	5.402	ng/uL	0.00
4) Pyridine-d5	3.616	84	95733	3.107	ng/ul	0.00
7) Phenol-d5	6.887	99	295888	8.536	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.051	67	756133	33.356	ng/ul	0.00
11) 2-Chlorophenol-d4	7.240	132	780342	27.135	ng/ul	0.00
15) 4-Methylphenol-d8	8.422	113	491020	17.920	ng/ul	0.00
21) Nitrobenzene-d5	8.869	128	433139	38.837	ng/ul	0.00
24) 2-Nitrophenol-d4	9.586	143	384635	41.686	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	682744	29.947	ng/ul	0.00
31) 4-Chloroaniline-d4	10.645	131	303158	8.146	ng/ul	0.00
46) Dimethylphthalate-d6	13.786	166	2135113	35.481	ng/ul	0.00
49) Acenaphthylene-d8	14.057	160	2588785	33.707	ng/ul	0.00
54) 4-Nitrophenol-d4	14.574	143	70484	7.499	ng/ul	0.00
60) Fluorene-d10	15.363	176	1866731	36.148	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.480	200	188733	36.153	ng/ul	0.00
73) Anthracene-d10	17.227	188	2932547	41.831	ng/ul	0.00
81) Pyrene-d10	19.480	212	3182653	39.862	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.450	264	3530214	42.974	ng/ul	0.00
Target Compounds						Qvalue
16) Acetophenone	8.534	105	55899	1.328	ng/ul#	95
19) Hexachloroethane	8.810	117	14407	1.198	ng/ul#	4
30) Naphthalene	10.551	128	100960	1.106	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010886.D
Acq On : 27 Jun 2022 19:56
Operator : CG/JU
Sample : N3425-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Jun 27 23:17:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 27 23:12:49 2022
Response via : Initial Calibration




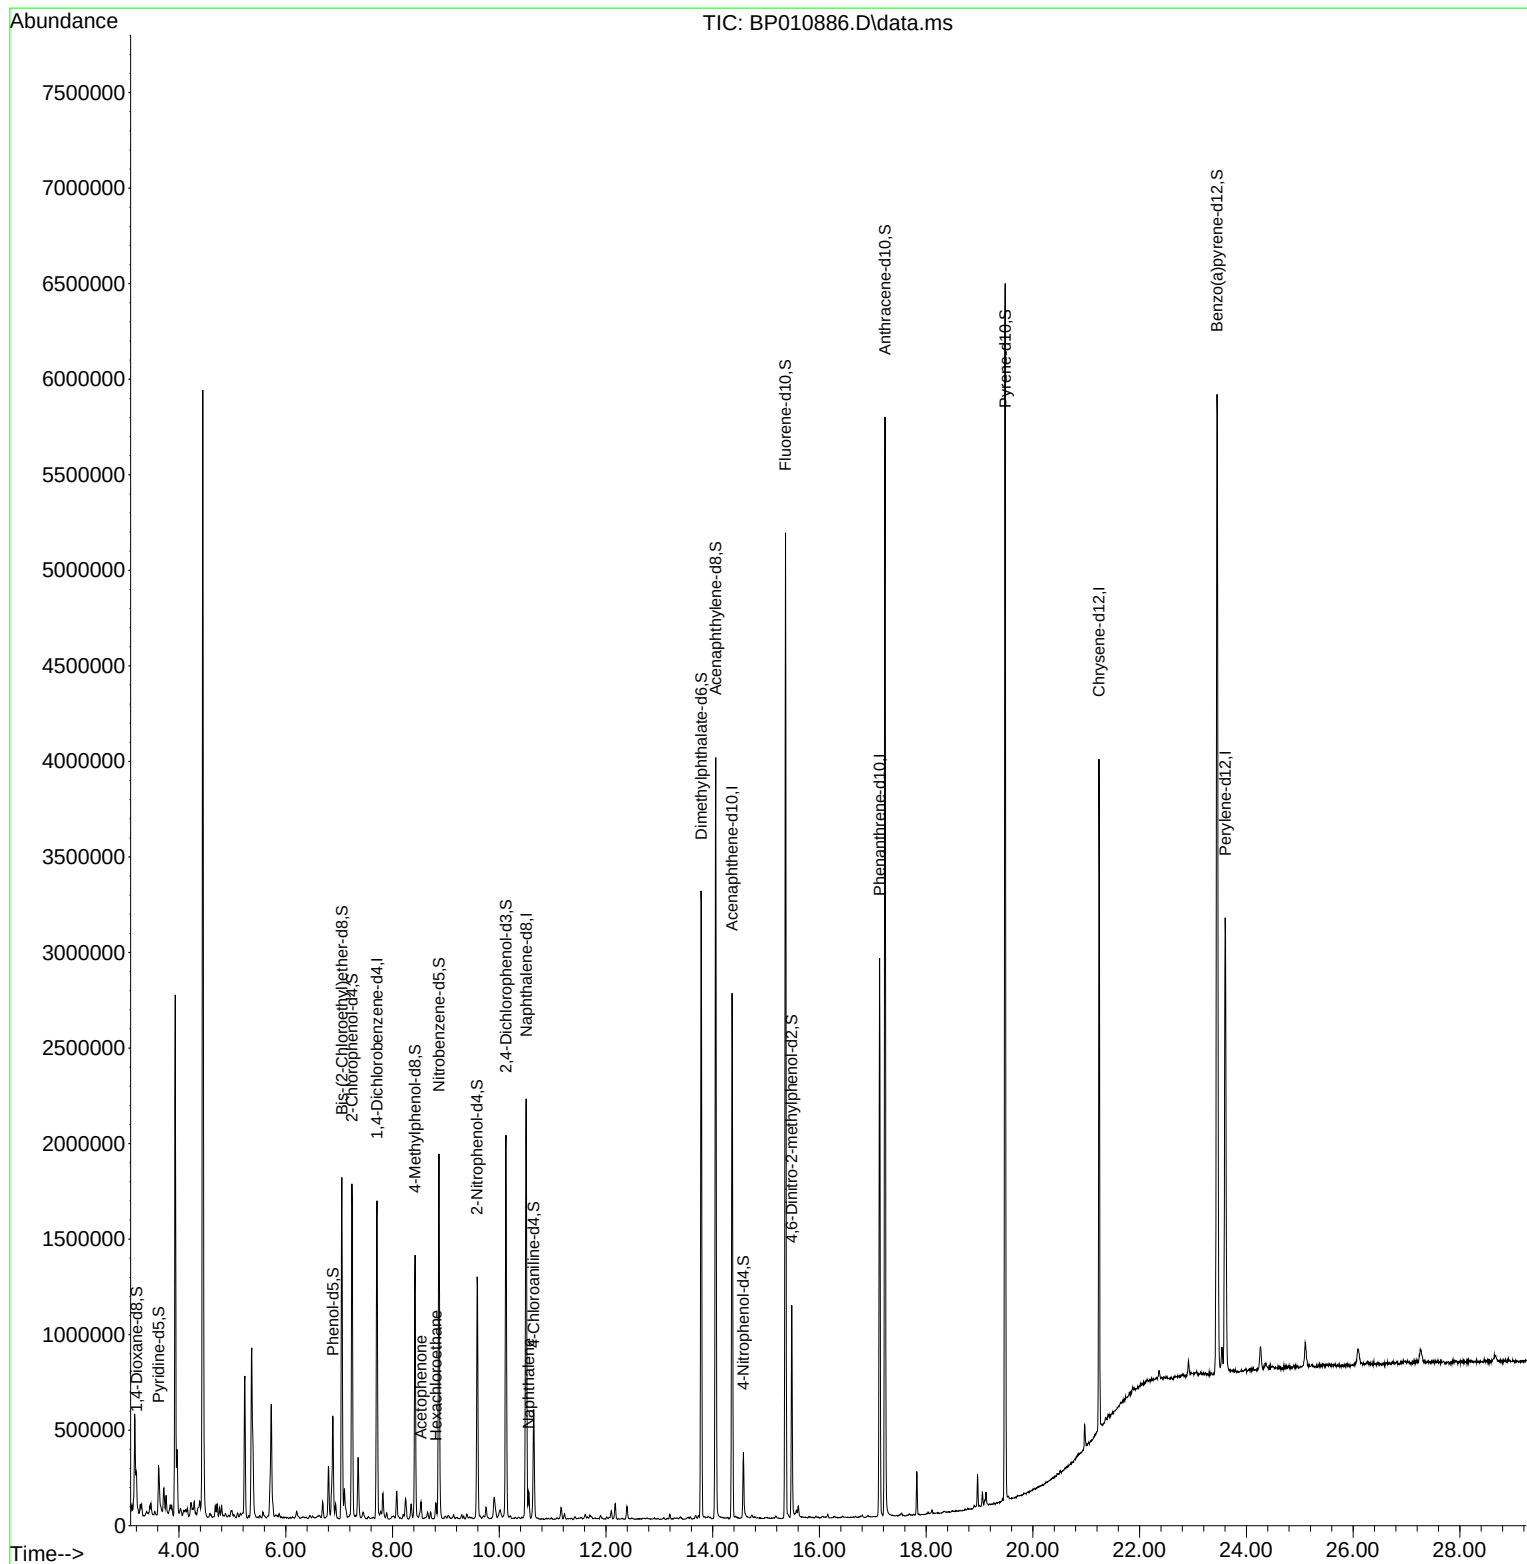


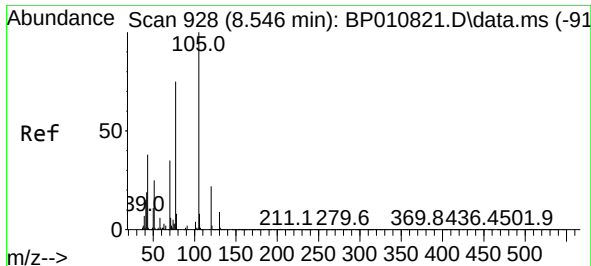

#16
Acetophenone
Concen: 1.328 ng/ul
RT: 8.534 min Scan# 91
Delta R.T. -0.000 min
Lab File: BP010886.D
Acq: 27 Jun 2022 19:56




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:105 Resp: 55899
Ion Ratio Lower Upper
105 100
77 82.6 67.5 101.3
51 29.5 29.6 44.4#

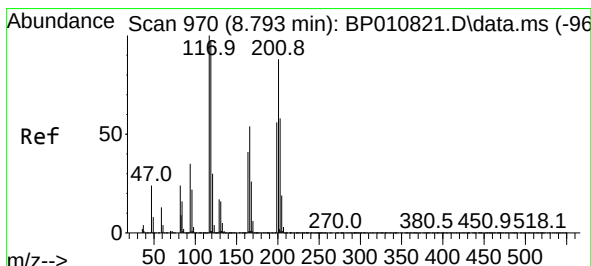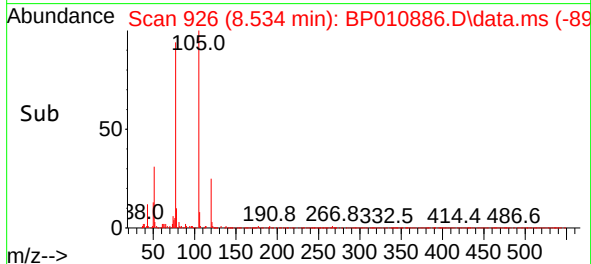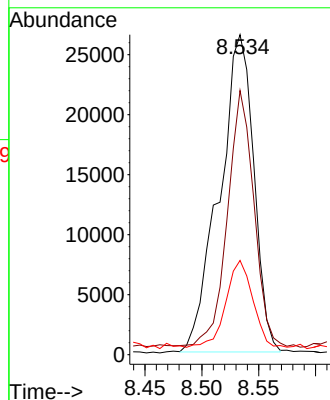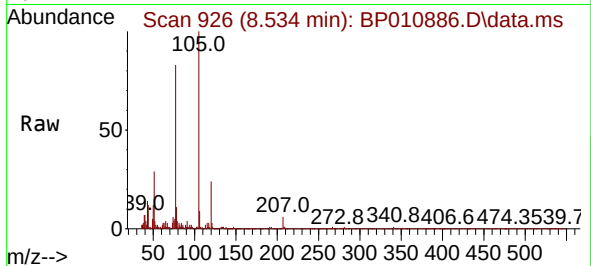

#19
Hexachloroethane
Concen: 1.198 ng/ul
RT: 8.810 min Scan# 973
Delta R.T. 0.023 min
Lab File: BP010886.D
Acq: 27 Jun 2022 19:56

Tgt Ion:117 Resp: 14407
Ion Ratio Lower Upper
117 100
201 0.2 85.7 128.5#
199 0.0 57.4 86.0#

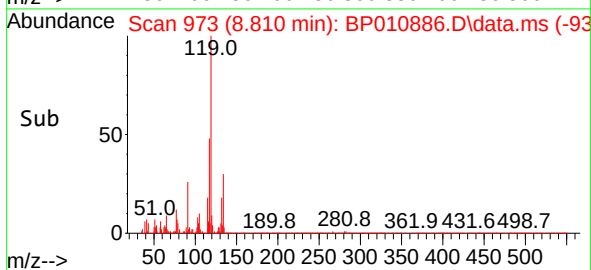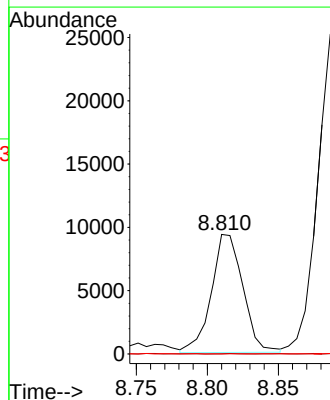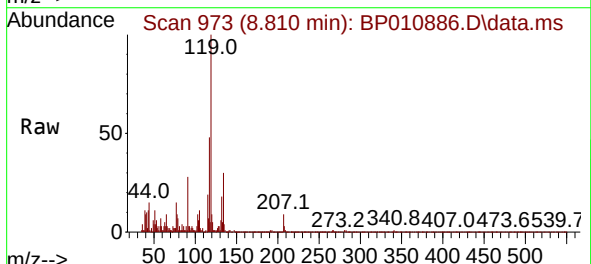

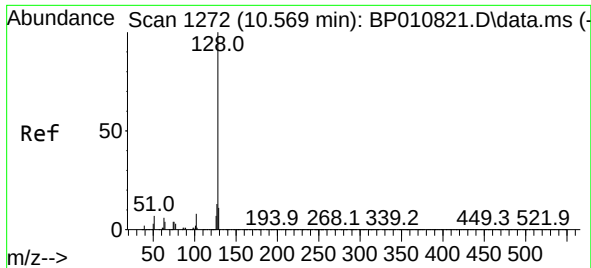

#30

Naphthalene

Concen: 1.106 ng/ul

RT: 10.551 min Scan# 11

Delta R.T. -0.006 min


Lab File: BP010886.D

Acq: 27 Jun 2022 19:56

Instrument :

BNA_P

ClientSampleId :

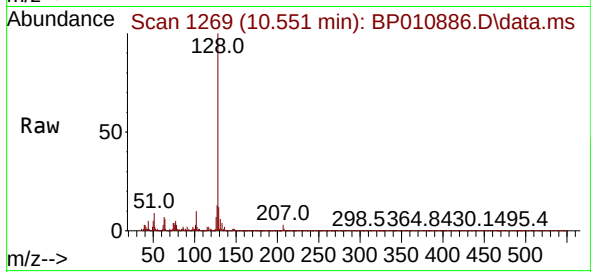

Tgt Ion:128 Resp: 100960

Ion Ratio Lower Upper

128 100

129 12.1 8.7 13.1

127 13.4 10.2 15.4

