

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010894.D
 Acq On : 28 Jun 2022 01:01
 Operator : CG/JU
 Sample : N3374-01DL 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4S6DL

Manual Integrations APPROVED

Reviewed By :Jagrut
 Upadhyay
 06/30/2022

Supervised By :mohammad
 ahmed
 07/01/2022

Quant Time: Jun 28 01:37:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 27 23:12:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.704	152	425102	20.000	ng/ul	0.00
20) Naphthalene-d8	10.504	136	1583631	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.363	164	857124	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.127	188	1602115	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.239	240	1513717	20.000	ng/ul	# 0.00
88) Perylene-d12	23.603	264	1687170	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	3333	0.297	ng/uL	0.00
4) Pyridine-d5	3.628	84	60689m	2.029	ng/ul	0.02
7) Phenol-d5	6.887	99	31410	0.933	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.051	67	64282	2.921	ng/ul	0.00
11) 2-Chlorophenol-d4	7.240	132	88989	3.187	ng/ul	0.00
15) 4-Methylphenol-d8	8.422	113	55552	2.088	ng/ul	0.00
21) Nitrobenzene-d5	8.869	128	33711m	3.344	ng/ul	0.00
24) 2-Nitrophenol-d4	9.586	143	42866	5.139	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.122	165	83718	4.062	ng/ul	0.00
31) 4-Chloroaniline-d4	10.657	131	91192	2.711	ng/ul	0.00
46) Dimethylphthalate-d6	13.786	166	159483	2.716	ng/ul	0.00
49) Acenaphthylene-d8	14.051	160	187729	2.505	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.363	176	148086	2.939	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.480	200	13783	2.597	ng/ul	0.00
73) Anthracene-d10	17.227	188	208834	2.930	ng/ul	0.00
81) Pyrene-d10	19.474	212	234283	2.841	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.445	264	238171	2.857	ng/ul	-0.01
Target Compounds						
8) Phenol	6.910	94	1315135	36.540	ng/ul#	85
18) 4-Methylphenol	8.487	108	67473	2.418	ng/ul	96
26) 2,4-Dimethylphenol	9.687	107	432017m	15.656	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010894.D
Acq On : 28 Jun 2022 01:01
Operator : CG/JU
Sample : N3374-01DL 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
EW4S6DL


Quant Time: Jun 28 01:37:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 27 23:12:49 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Jagrut
Upadhyay
06/30/2022


Supervised By :mohammad
ahmed
07/01/2022

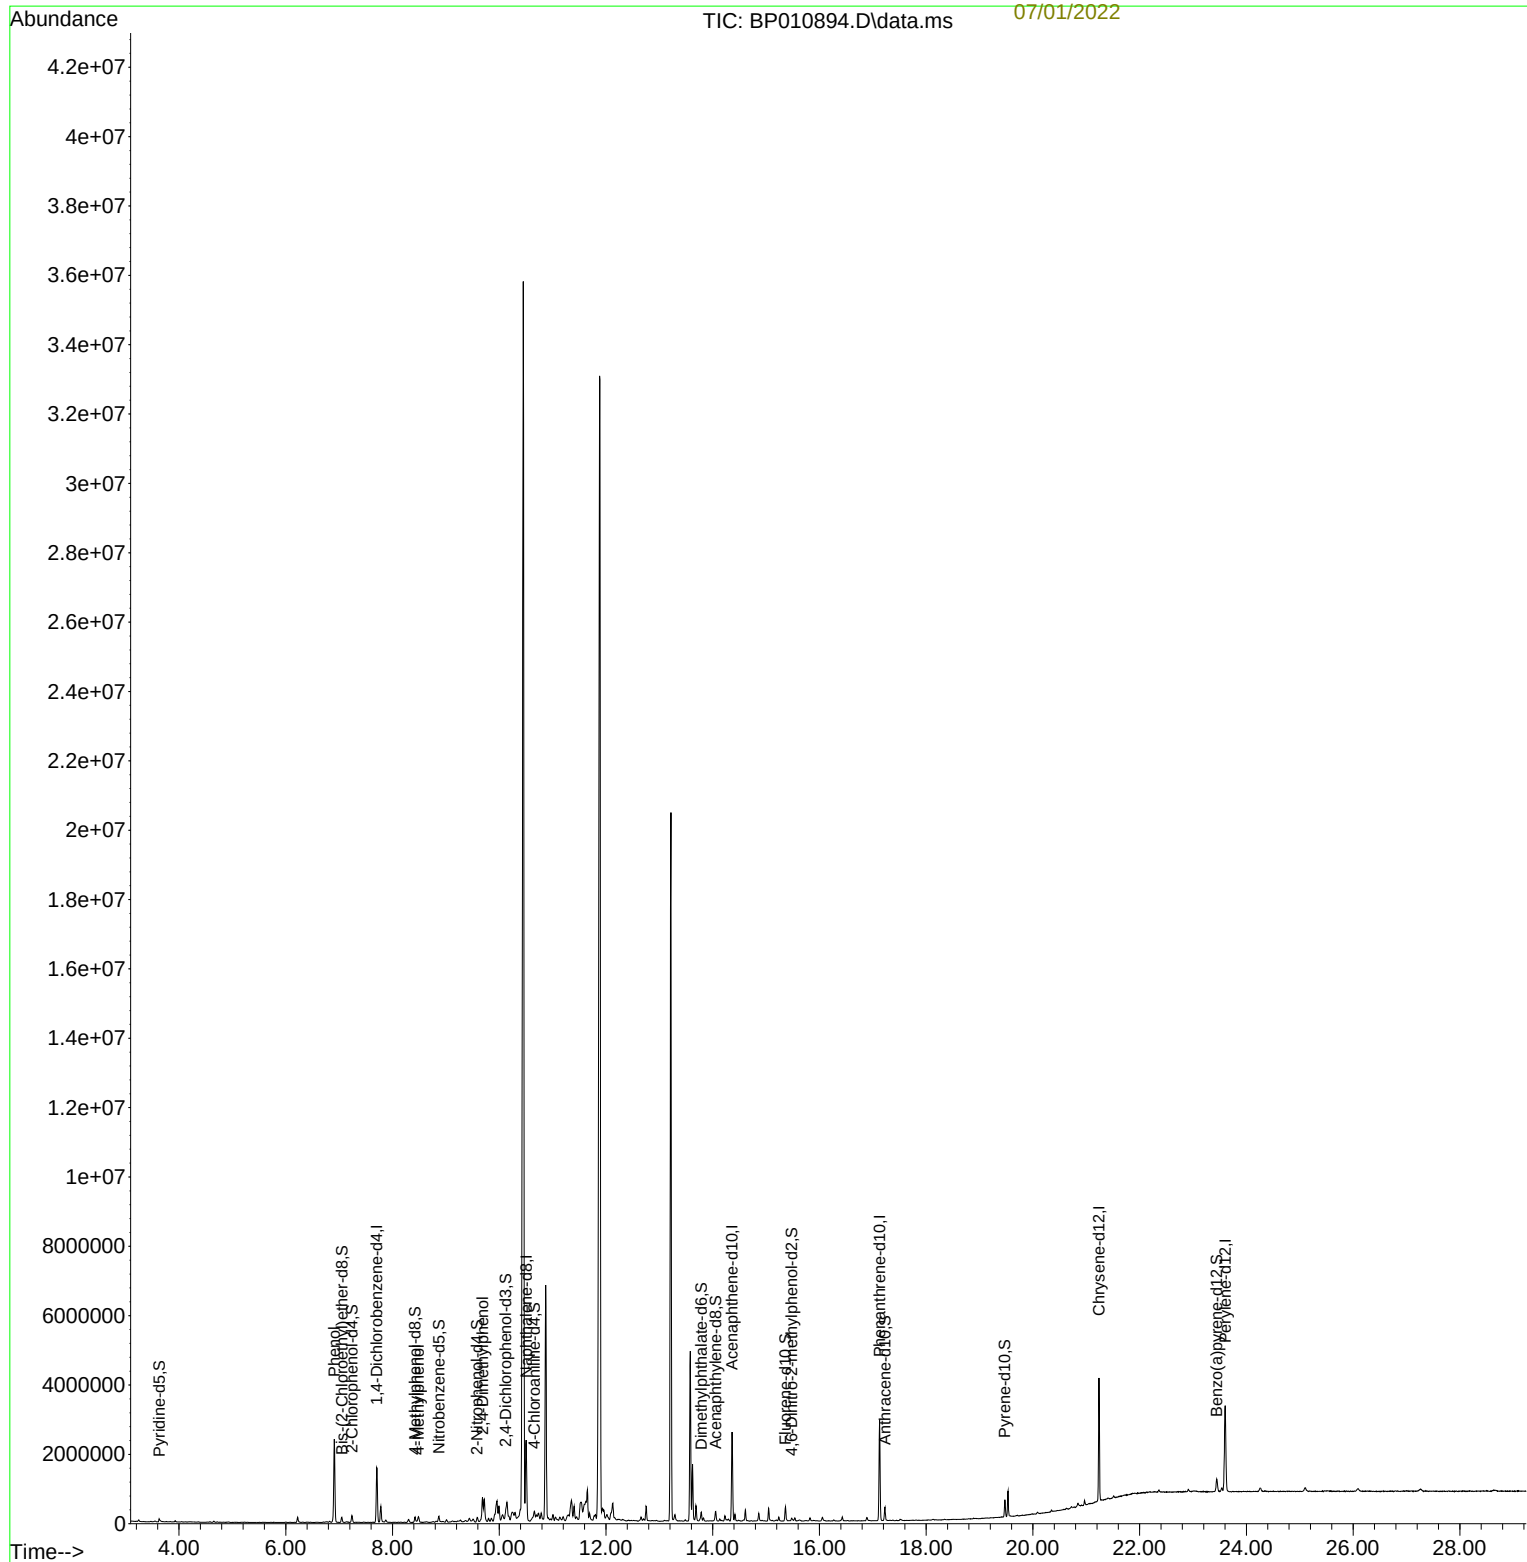

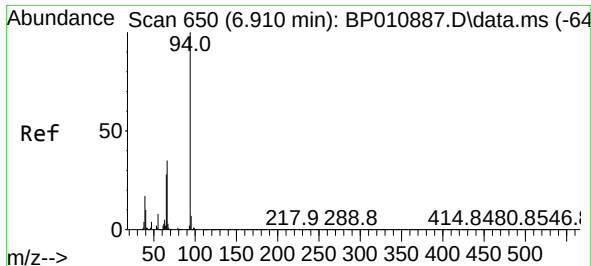

#8
Phenol
Concen: 36.540 ng/ul
RT: 6.910 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP010894.D
Acq: 28 Jun 2022 01:01

Instrument :
BNA_P
ClientSampleId :
EW4S6DL



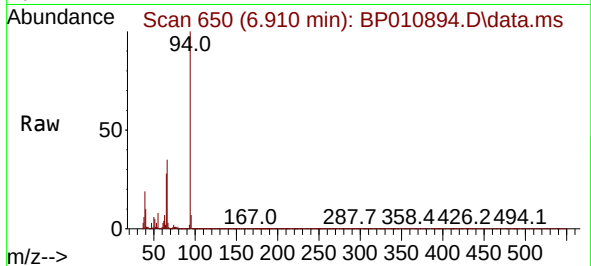


Tgt Ion: 94 Resp: 131513
Ion Ratio Lower Upper
94 100
65 27.5 27.4 41.2
66 35.4 37.4 56.2

Manual Integrations
APPROVED




Reviewed By :Jagrut
Upadhyay
06/30/2022


Supervised By :mohammad
ahmed
07/01/2022

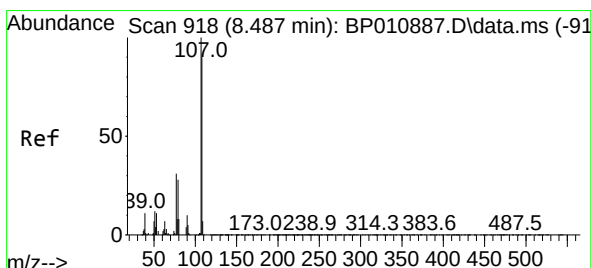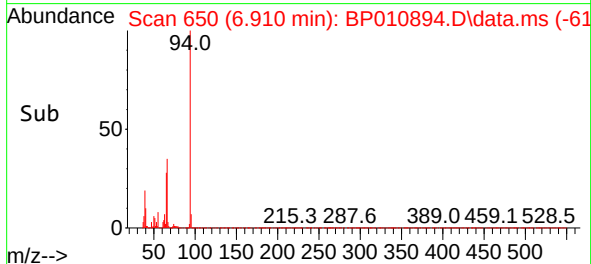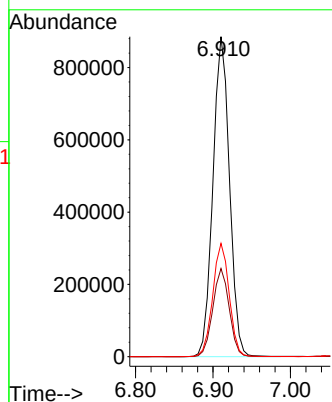

#18
4-Methylphenol
Concen: 2.418 ng/ul
RT: 8.487 min Scan# 918
Delta R.T. -0.000 min
Lab File: BP010894.D
Acq: 28 Jun 2022 01:01


Tgt Ion:108 Resp: 67473
Ion Ratio Lower Upper
108 100
107 105.9 88.3 132.5

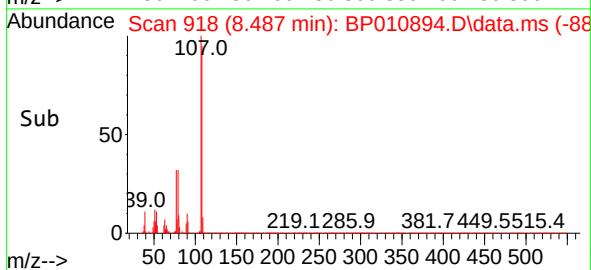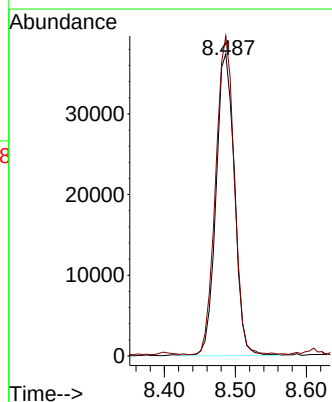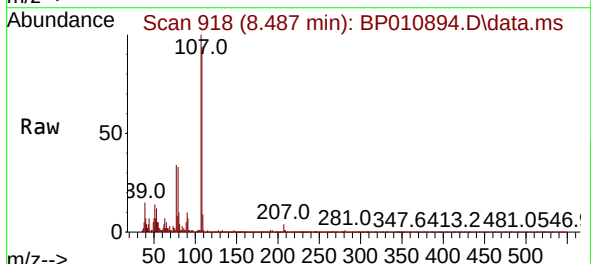

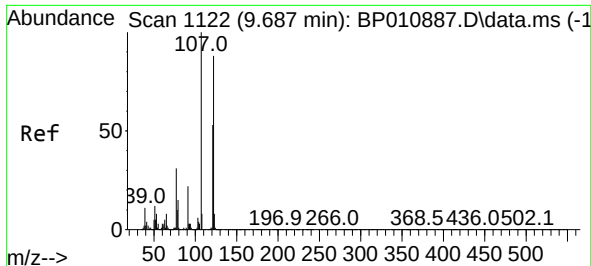

#26
2,4-Dimethylphenol
Concen: 15.656 ng/ul m
RT: 9.687 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP010894.D
Acq: 28 Jun 2022 01:01

Instrument :
BNA_P
ClientSampleId :
EW4S6DL

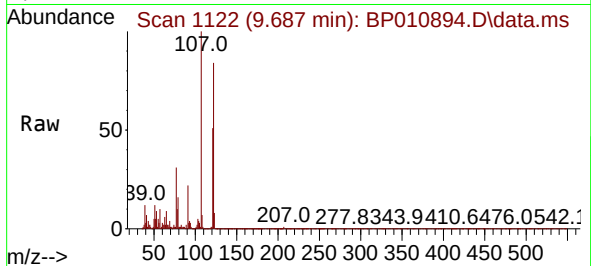

Tgt Ion:107 Resp: 43201
Ion Ratio Lower Upper
107 100
121 50.8 39.1 58.7
122 84.2 66.1 99.1

Manual Integrations
APPROVED

Reviewed By :Jagrut
Upadhyay
06/30/2022

Supervised By :mohammad
ahmed
07/01/2022

