

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010871.D
 Acq On : 27 Jun 2022 11:26
 Operator : CG/JU
 Sample : PB145767BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK767

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	27	rVB	162101	190076	2.68%	0.226%
2	3.611	85	89	115	rBV	1873137	2659556	37.46%	3.162%
3	3.928	139	143	150	rVB	33588	46618	0.66%	0.055%
4	6.887	638	646	658	rBV	1971320	2949606	41.54%	3.507%
5	7.052	667	674	683	rVB	1677651	2491123	35.09%	2.962%
6	7.246	700	707	718	rBV	2005683	3087110	43.48%	3.670%
7	7.711	778	786	794	rVB	1433464	2168443	30.54%	2.578%
8	8.422	897	907	918	rBV	2305259	3607857	50.82%	4.290%
9	8.869	976	983	994	rBV	1699288	2741423	38.61%	3.259%
10	9.593	1098	1106	1113	rBV	1247878	1940434	27.33%	2.307%
11	10.128	1189	1197	1208	rBV	2033420	3249885	45.77%	3.864%
12	10.505	1252	1261	1270	rBV	1838811	3013221	42.44%	3.583%
13	10.652	1276	1286	1298	rBV	2162844	3609613	50.84%	4.292%
14	12.104	1526	1533	1542	rVB	39522	70777	1.00%	0.084%
15	12.316	1564	1569	1572	rBV7	4968	8911	0.13%	0.011%
16	13.093	1697	1701	1705	rVB7	4398	7145	0.10%	0.008%
17	13.787	1812	1819	1826	rBV	3151199	4129036	58.16%	4.909%
18	14.057	1857	1865	1880	rBV	3755252	5238511	73.78%	6.228%
19	14.369	1911	1918	1927	rBV	2261774	3337338	47.01%	3.968%
20	14.575	1947	1953	1969	rBV	1240734	1840515	25.92%	2.188%
21	14.734	1976	1980	1987	rVV10	4191	10798	0.15%	0.013%
22	14.793	1987	1990	1998	rVB10	7389	14928	0.21%	0.018%
23	15.363	2080	2087	2101	rBV	4427699	6285345	88.53%	7.473%
24	15.487	2101	2108	2124	rVV	790609	1167477	16.44%	1.388%
25	15.604	2124	2128	2138	rVB	55887	84350	1.19%	0.100%
26	16.157	2217	2222	2232	rVB4	17468	26797	0.38%	0.032%
27	16.804	2328	2332	2338	rVB9	8333	11409	0.16%	0.014%
28	17.128	2378	2387	2394	rBV	2340951	3326974	46.86%	3.956%
29	17.228	2398	2404	2419	rVV2	4346301	6171106	86.92%	7.337%
30	17.510	2449	2452	2455	rBV5	8164	11172	0.16%	0.013%
31	19.057	2711	2715	2719	rBV2	53127	66493	0.94%	0.079%
32	19.128	2723	2727	2732	rVB2	42709	61194	0.86%	0.073%
33	19.481	2781	2787	2793	rBV	5175062	6461048	91.00%	7.682%
34	21.239	3082	3086	3094	rBV	2512231	3277088	46.16%	3.896%
35	23.457	3456	3463	3473	rVB	3719890	7099833	100.00%	8.441%
36	23.610	3483	3489	3501	rVB2	1880617	3644700	51.34%	4.333%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010871.D
Acq On : 27 Jun 2022 11:26
Operator : CG/JU
Sample : PB145767BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK767

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION




Sum of corrected areas: 84107910

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010871.D
Acq On : 27 Jun 2022 11:26
Operator : CG/JU
Sample : PB145767BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK767

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

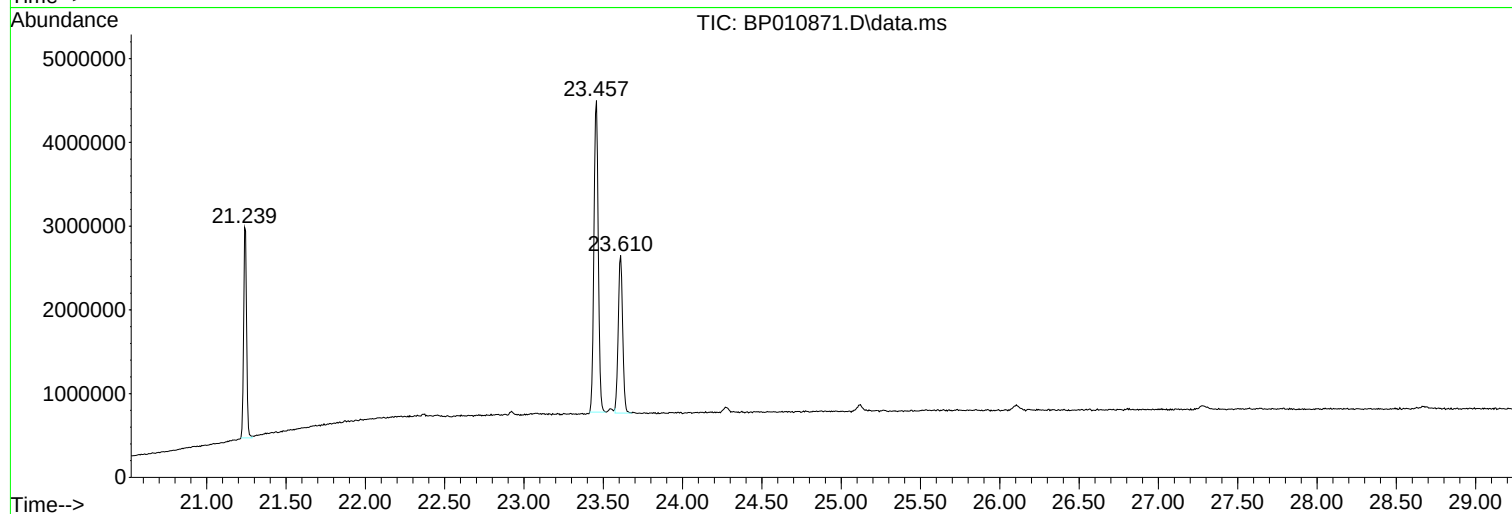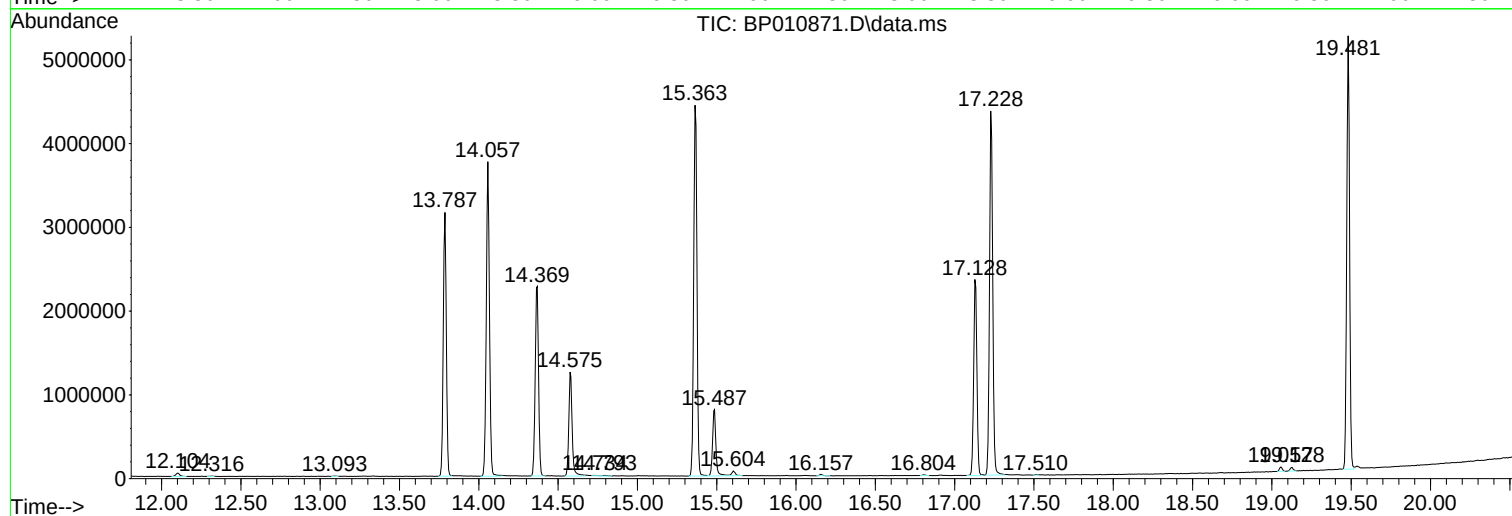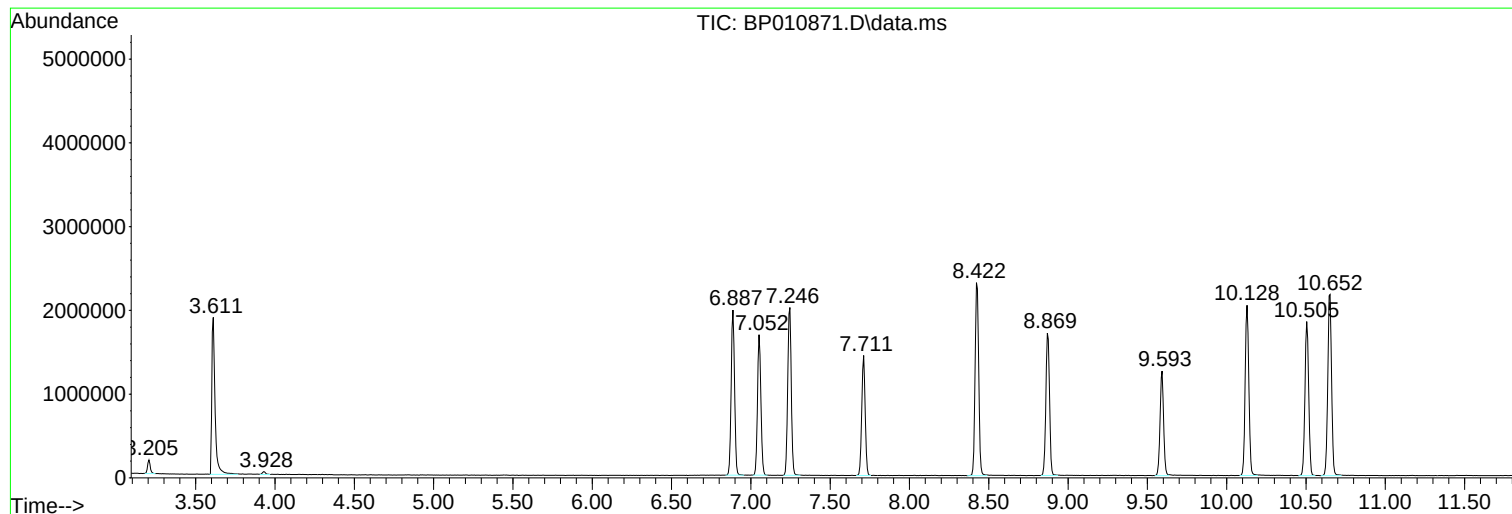

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010871.D
Acq On : 27 Jun 2022 11:26
Operator : CG/JU
Sample : PB145767BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK767

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010871.D
Acq On : 27 Jun 2022 11:26
Operator : CG/JU
Sample : PB145767BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK767

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------