

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010881.D
 Acq On : 27 Jun 2022 17:06
 Operator : CG/JU
 Sample : N3392-04 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	22	rBV	60817	75120	0.85%	0.084%
2	3.240	22	26	38	rVV	1090461	1227836	13.84%	1.375%
3	3.340	41	43	47	rVB5	11283	11684	0.13%	0.013%
4	3.540	74	77	82	rVB	29396	36498	0.41%	0.041%
5	3.611	86	89	95	rVV	619533	849125	9.57%	0.951%
6	3.658	95	97	111	rVB	177739	241782	2.73%	0.271%
7	3.834	122	127	134	rVB	59495	92010	1.04%	0.103%
8	3.911	134	140	155	rVB2	150900	270703	3.05%	0.303%
9	4.069	162	167	173	rVV	27333	36068	0.41%	0.040%
10	4.152	177	181	183	rVV3	7031	10643	0.12%	0.012%
11	4.193	183	188	193	rVV	198511	250567	2.82%	0.281%
12	4.258	195	199	203	rVV	42838	53265	0.60%	0.060%
13	4.299	204	206	213	rVB8	8399	10493	0.12%	0.012%
14	4.369	213	218	224	rBV	471257	585109	6.60%	0.655%
15	4.434	224	229	234	rVB	188570	244659	2.76%	0.274%
16	4.652	263	266	270	rVB4	7005	9000	0.10%	0.010%
17	4.716	272	277	280	rBV4	11299	17246	0.19%	0.019%
18	4.816	286	294	304	rVV	525856	698873	7.88%	0.783%
19	5.040	327	332	336	rBV	39884	53707	0.61%	0.060%
20	5.311	374	378	384	rBV5	11509	17158	0.19%	0.019%
21	5.434	393	399	404	rVB	11555	19422	0.22%	0.022%
22	5.675	434	440	446	rBV	43000	61234	0.69%	0.069%
23	6.710	608	616	622	rBV10	7539	19518	0.22%	0.022%
24	6.887	636	646	653	rBV	356287	564032	6.36%	0.632%
25	7.052	665	674	684	rBV	1717779	2572079	29.00%	2.881%
26	7.128	684	687	691	rVB	6329	9482	0.11%	0.011%
27	7.240	699	706	717	rBV	1522565	2355216	26.55%	2.638%
28	7.334	719	722	725	rBV4	7348	11980	0.14%	0.013%
29	7.710	777	786	793	rBV	1644594	2521655	28.43%	2.824%
30	7.781	794	798	803	rVV	22770	33624	0.38%	0.038%
31	8.422	900	907	917	rBV	1105602	1691075	19.06%	1.894%
32	8.534	920	926	933	rVB	68755	116592	1.31%	0.131%
33	8.869	976	983	991	rVV	1821011	2861787	32.26%	3.205%
34	8.993	1000	1004	1009	rVV5	10378	15077	0.17%	0.017%
35	9.293	1048	1055	1060	rVB2	16608	32545	0.37%	0.036%
36	9.375	1062	1069	1071	rBV5	15759	26689	0.30%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010881.D
 Acq On : 27 Jun 2022 17:06
 Operator : CG/JU
 Sample : N3392-04 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	9.434	1075	1079	1085	rVB6	20708	39629	0.45%	0.044%
38	9.587	1096	1105	1121	rBV	1220291	1971222	22.22%	2.208%
39	9.904	1155	1159	1162	rBV6	8738	12432	0.14%	0.014%
40	10.128	1189	1197	1205	rBV	1868903	3019039	34.03%	3.381%
41	10.193	1205	1208	1212	rVB6	13572	21585	0.24%	0.024%
42	10.434	1244	1249	1253	rVB5	13331	21158	0.24%	0.024%
43	10.504	1253	1261	1276	rVB	2127867	3508280	39.55%	3.929%
44	10.646	1276	1285	1297	rBV	1866456	3048933	34.37%	3.415%
45	11.057	1351	1355	1361	rVV	16993	27054	0.30%	0.030%
46	11.122	1361	1366	1369	rVV2	20664	34002	0.38%	0.038%
47	11.157	1369	1372	1378	rVB	18020	29885	0.34%	0.033%
48	11.310	1392	1398	1403	rBV10	6132	12155	0.14%	0.014%
49	11.475	1420	1426	1428	rBV7	5408	8941	0.10%	0.010%
50	12.016	1514	1518	1523	rBV6	6621	13191	0.15%	0.015%
51	12.098	1526	1532	1538	rVB	43404	70875	0.80%	0.079%
52	12.304	1563	1567	1573	rVB9	5672	12445	0.14%	0.014%
53	13.198	1715	1719	1724	rVB2	17535	25342	0.29%	0.028%
54	13.281	1727	1733	1736	rBV5	9156	18958	0.21%	0.021%
55	13.328	1737	1741	1749	rVB7	7723	15777	0.18%	0.018%
56	13.787	1812	1819	1825	rBV	3179958	4445968	50.12%	4.979%
57	14.057	1857	1865	1884	rBV	3862764	5551704	62.59%	6.218%
58	14.275	1898	1902	1910	rVB3	24666	34546	0.39%	0.039%
59	14.363	1910	1917	1924	rBV	2674685	3857188	43.48%	4.320%
60	14.428	1924	1928	1935	rVB2	25916	40552	0.46%	0.045%
61	14.575	1948	1953	1963	rBV	193829	293193	3.31%	0.328%
62	14.734	1975	1980	1982	rBV6	8381	13258	0.15%	0.015%
63	14.898	2005	2008	2013	rVB7	5898	10145	0.11%	0.011%
64	15.145	2046	2050	2061	rBV	56232	91802	1.03%	0.103%
65	15.234	2061	2065	2070	rVB	37537	47845	0.54%	0.054%
66	15.363	2080	2087	2094	rBV	5027633	6926684	78.09%	7.758%
67	15.481	2101	2107	2118	rBV	923026	1260523	14.21%	1.412%
68	15.604	2123	2128	2132	rBV	53410	83022	0.94%	0.093%
69	15.792	2156	2160	2166	rBV9	8013	17363	0.20%	0.019%
70	16.104	2209	2213	2216	rBV	53165	66859	0.75%	0.075%
71	16.904	2345	2349	2355	rBV2	47826	64933	0.73%	0.073%
72	16.957	2355	2358	2363	rVB5	17595	24575	0.28%	0.028%
73	17.128	2381	2387	2393	rBV	2755582	3909192	44.07%	4.378%
74	17.228	2398	2404	2420	rVV	5112354	7111416	80.17%	7.965%
75	17.651	2472	2476	2481	rBV2	38826	49631	0.56%	0.056%
76	17.822	2501	2505	2510	rVB	98644	123710	1.39%	0.139%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010881.D
Acq On : 27 Jun 2022 17:06
Operator : CG/JU
Sample : N3392-04 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION

77	18.327	2588	2591	2596	rBV	29803	40480	0.46%	0.045%
78	18.963	2696	2699	2705	rVB2	111403	131282	1.48%	0.147%
79	19.057	2711	2715	2719	rVB	61616	79162	0.89%	0.089%
80	19.122	2723	2726	2730	rVB	55644	64027	0.72%	0.072%
81	19.480	2781	2787	2794	rBV	5941762	7755414	87.43%	8.686%
82	21.239	3081	3086	3095	rBV2	3359252	4148184	46.76%	4.646%
83	23.457	3456	3463	3473	rVB2	4641079	8870531	100.00%	9.935%
84	23.604	3482	3488	3500	rVB2	2291402	4557928	51.38%	5.105%




Sum of corrected areas: 89285573

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010881.D
Acq On : 27 Jun 2022 17:06
Operator : CG/JU
Sample : N3392-04 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

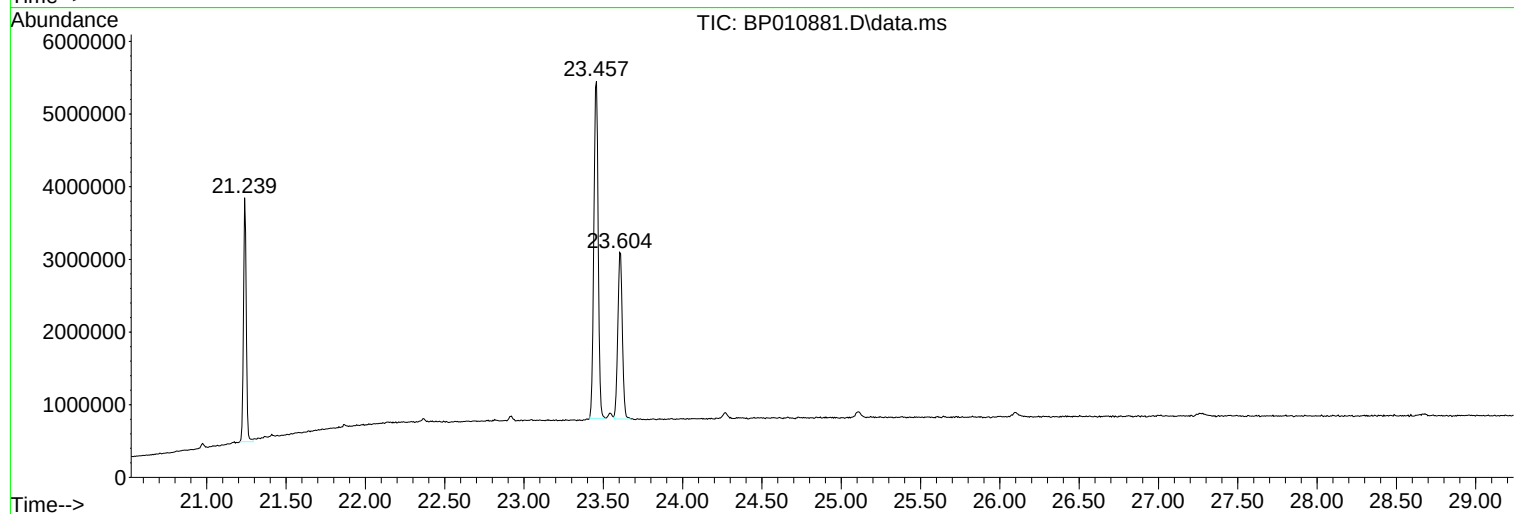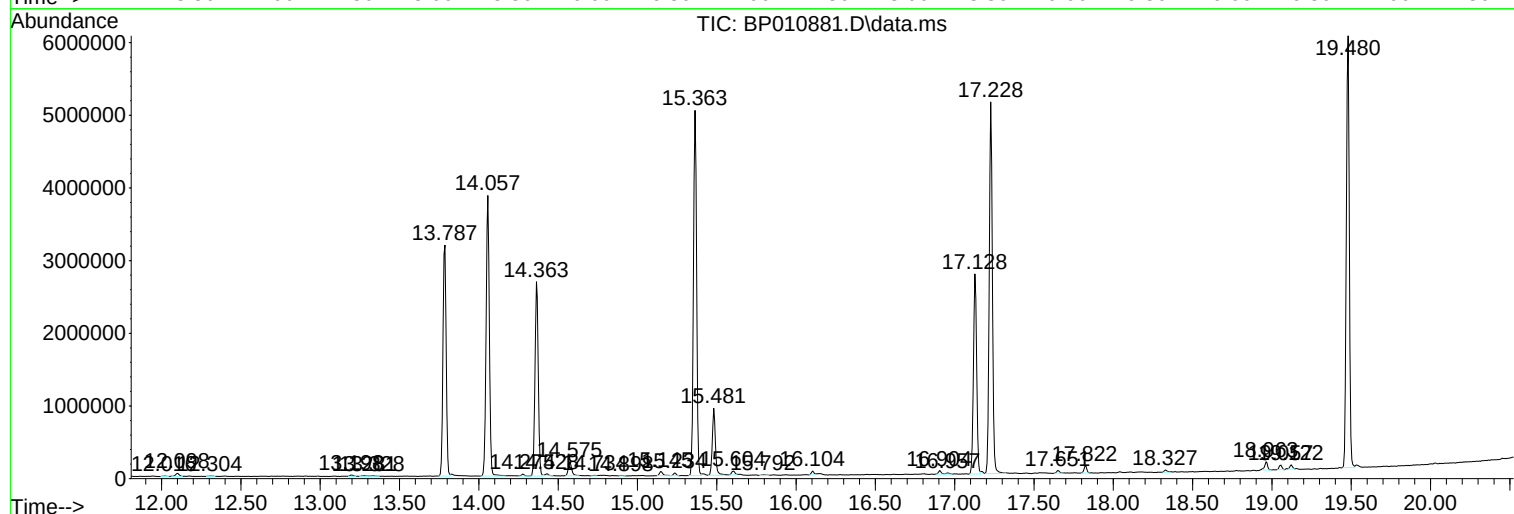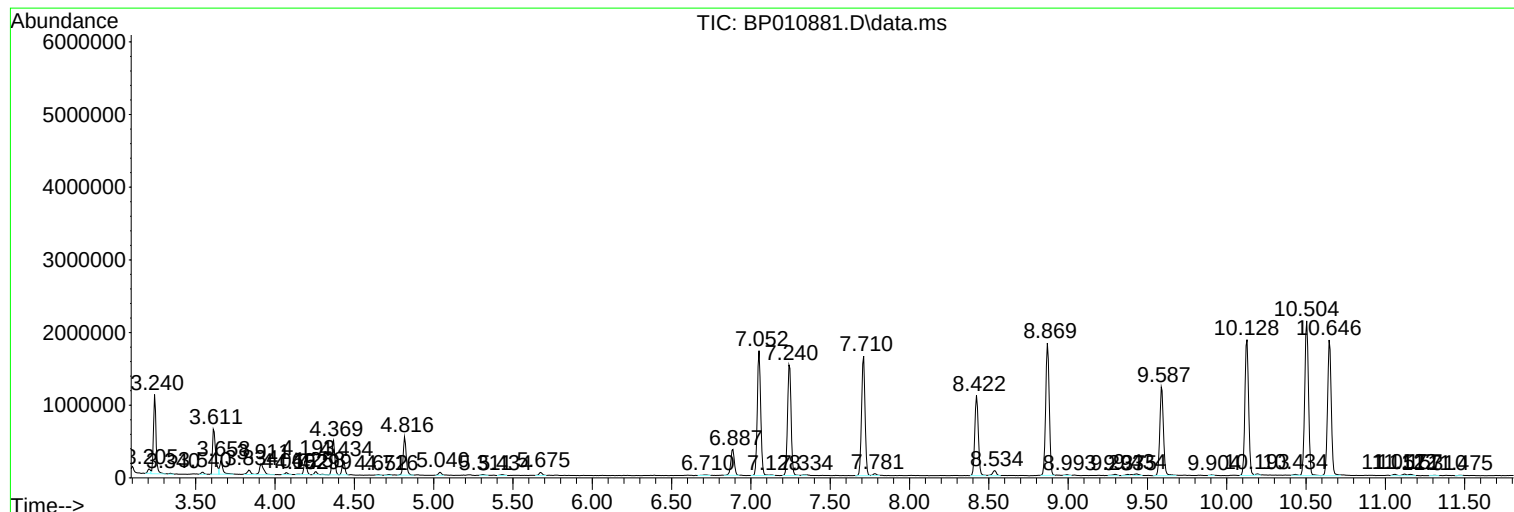

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010881.D
Acq On : 27 Jun 2022 17:06
Operator : CG/JU
Sample : N3392-04 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isobutyl acetate Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.911	2.15 ng/ul	270703	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isobutyl acetate	116	C6H12O2	000110-19-0	78
2			Isobutyl acetate	116	C6H12O2	000110-19-0	72
3			Isobutyl acetate	116	C6H12O2	000110-19-0	59
4			Isobutyl acetate	116	C6H12O2	000110-19-0	50
5			Isobutyl acetate	116	C6H12O2	000110-19-0	50

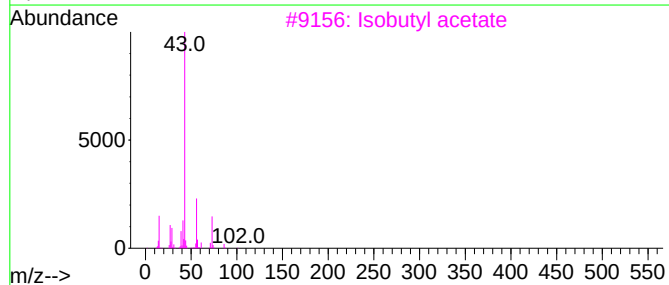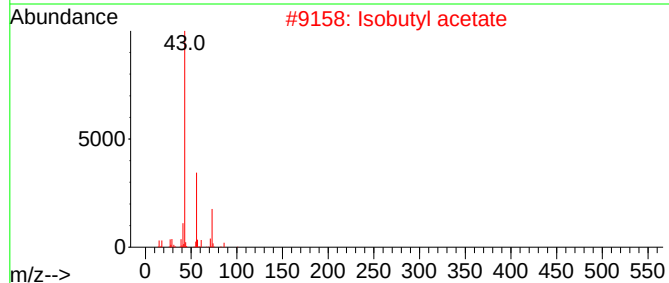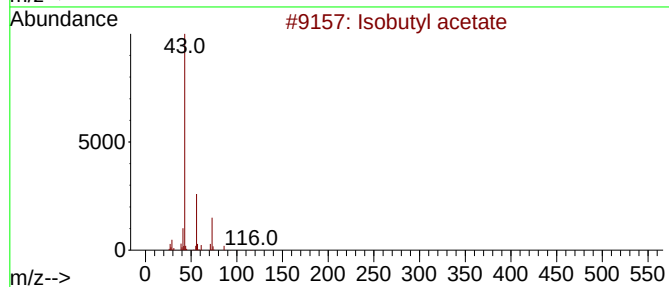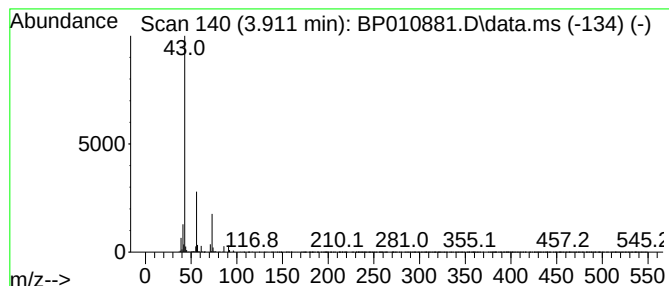

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010881.D
Acq On : 27 Jun 2022 17:06
Operator : CG/JU
Sample : N3392-04 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Propanoic acid, propyl ester Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.369	4.64 ng/ul	585109	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	83
2			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
3			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
4			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
5			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	64

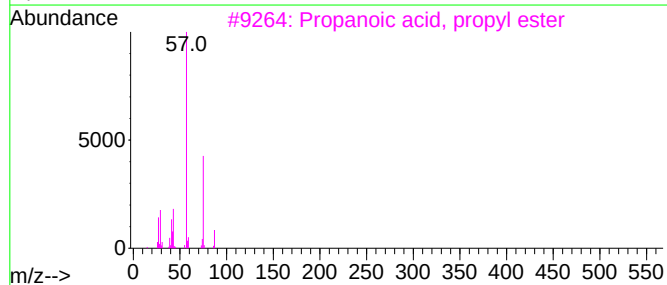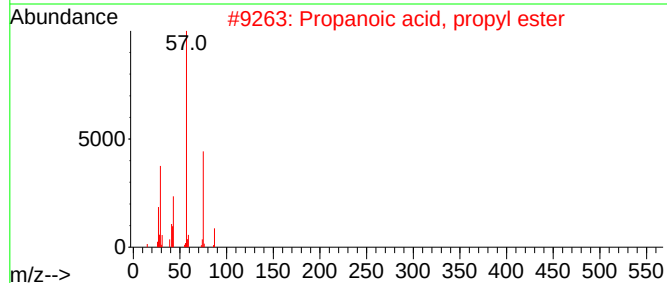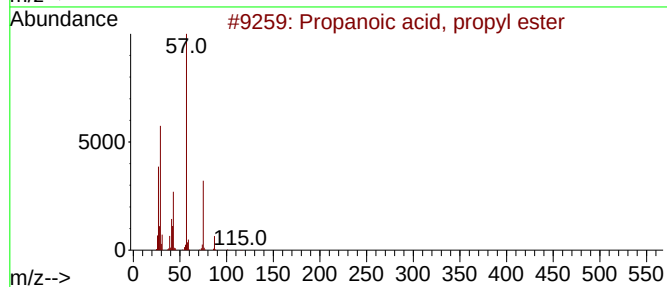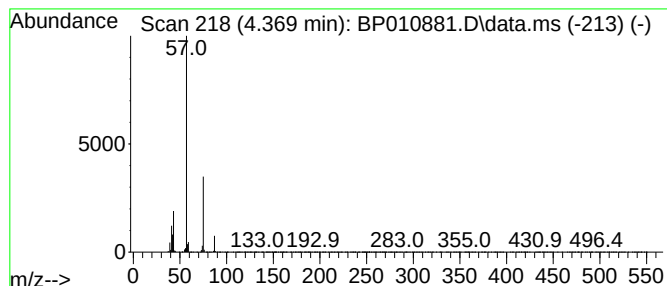

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010881.D
Acq On : 27 Jun 2022 17:06
Operator : CG/JU
Sample : N3392-04 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Isopropyl butyrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.816	5.54 ng/ul	698873	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl butyrate	130	C7H14O2	000638-11-9	91
2			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
3			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
4			Isopropyl butyrate	130	C7H14O2	000638-11-9	86
5			Propanoic acid, 2-methyl-, 1-met...	130	C7H14O2	000617-50-5	72

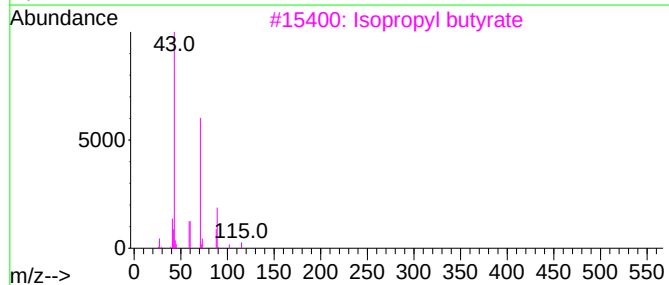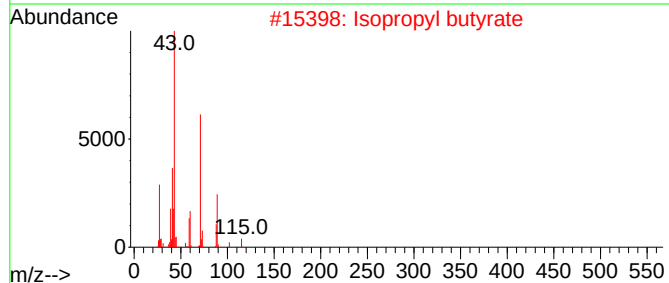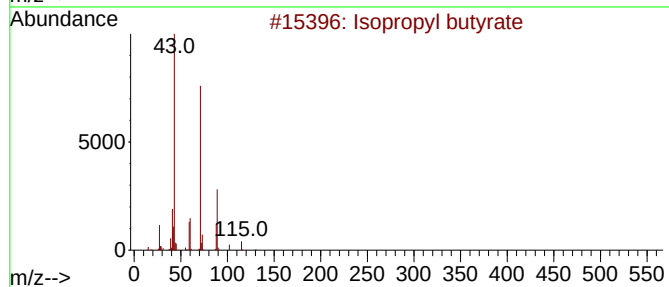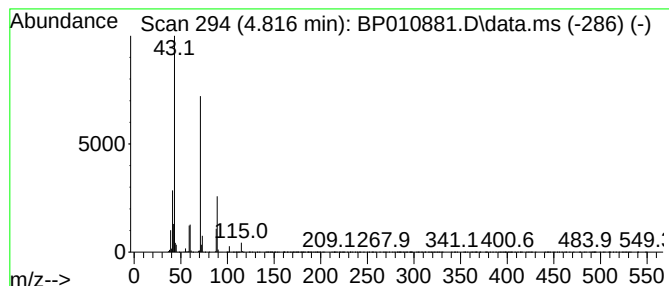

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010881.D
Acq On : 27 Jun 2022 17:06
Operator : CG/JU
Sample : N3392-04 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isobutyl acetate	3.911	2.1	ng/ul	270703	1	7.710	2521660	20.0
Propanoic acid,...	4.369	4.6	ng/ul	585109	1	7.710	2521660	20.0
Isopropyl butyrate	4.816	5.5	ng/ul	698873	1	7.710	2521660	20.0