

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010884.D
 Acq On : 27 Jun 2022 18:48
 Operator : CG/JU
 Sample : N3392-05 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	22	rBV	73240	86908	0.95%	0.080%
2	3.240	22	26	36	rVB	1257923	1400067	15.30%	1.295%
3	3.546	74	78	81	rVB	31508	37288	0.41%	0.035%
4	3.611	86	89	95	rVV	726793	986572	10.78%	0.913%
5	3.658	95	97	112	rVB	194412	271346	2.96%	0.251%
6	3.840	121	128	133	rVV	59514	95277	1.04%	0.088%
7	3.911	134	140	150	rVB2	195753	322977	3.53%	0.299%
8	4.075	163	168	175	rVV2	29831	46527	0.51%	0.043%
9	4.152	177	181	183	rVV3	14788	20175	0.22%	0.019%
10	4.193	183	188	195	rVV	220255	286584	3.13%	0.265%
11	4.258	195	199	203	rVV	48391	63034	0.69%	0.058%
12	4.305	203	207	210	rVV5	9836	15310	0.17%	0.014%
13	4.369	213	218	224	rVV	544634	687963	7.52%	0.637%
14	4.434	224	229	234	rVV	250384	325160	3.55%	0.301%
15	4.481	234	237	241	rVB3	9746	13265	0.14%	0.012%
16	4.646	262	265	272	rVB2	9479	15178	0.17%	0.014%
17	4.716	272	277	281	rBV3	12978	18726	0.20%	0.017%
18	4.816	286	294	304	rVV	608407	803153	8.77%	0.743%
19	5.040	328	332	337	rBV2	17143	25862	0.28%	0.024%
20	5.222	359	363	368	rVB4	8334	14384	0.16%	0.013%
21	5.311	374	378	382	rBV3	15745	21407	0.23%	0.020%
22	5.434	395	399	404	rBV	12583	19801	0.22%	0.018%
23	5.675	435	440	444	rBV	45723	61765	0.67%	0.057%
24	5.775	453	457	461	rVB7	6246	9159	0.10%	0.008%
25	6.393	556	562	569	rVB	35402	60131	0.66%	0.056%
26	6.716	610	617	622	rBV8	9468	20291	0.22%	0.019%
27	6.881	638	645	661	rVB	503561	798927	8.73%	0.739%
28	7.052	667	674	683	rBV	2098337	3155056	34.47%	2.919%
29	7.122	683	686	692	rVB2	8115	16050	0.18%	0.015%
30	7.240	699	706	716	rBV	1924274	2974732	32.50%	2.752%
31	7.340	720	723	727	rVB4	9593	13026	0.14%	0.012%
32	7.710	779	786	793	rBV	1959066	3004935	32.83%	2.780%
33	7.781	793	798	803	rVB	24421	38537	0.42%	0.036%
34	8.422	900	907	916	rBV	1516001	2284237	24.96%	2.114%
35	8.534	921	926	933	rVB	84343	134547	1.47%	0.124%
36	8.869	976	983	991	rBV	2307737	3605101	39.39%	3.336%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010884.D
 Acq On : 27 Jun 2022 18:48
 Operator : CG/JU
 Sample : N3392-05 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	8.993	999	1004	1009	rBV6	13767	20962	0.23%	0.019%
38	9.040	1009	1012	1018	rVB8	5798	9316	0.10%	0.009%
39	9.293	1046	1055	1060	rVB3	13724	32205	0.35%	0.030%
40	9.381	1062	1070	1073	rBV8	16996	41142	0.45%	0.038%
41	9.428	1076	1078	1087	rVB4	27403	45772	0.50%	0.042%
42	9.587	1097	1105	1123	rBV	1597832	2564596	28.02%	2.373%
43	9.904	1153	1159	1162	rBV8	6015	11768	0.13%	0.011%
44	10.040	1174	1182	1188	rBV8	7740	19198	0.21%	0.018%
45	10.128	1188	1197	1205	rBV	2375268	3872648	42.31%	3.583%
46	10.187	1205	1207	1215	rVB7	17172	31026	0.34%	0.029%
47	10.428	1244	1248	1253	rBV5	12304	20867	0.23%	0.019%
48	10.504	1253	1261	1270	rBV	2596852	4293622	46.91%	3.973%
49	10.646	1276	1285	1295	rBV	2338542	3821595	41.75%	3.536%
50	10.922	1323	1332	1335	rVB10	4299	10625	0.12%	0.010%
51	11.057	1351	1355	1360	rBV2	19427	28659	0.31%	0.027%
52	11.116	1360	1365	1369	rBV	25879	41104	0.45%	0.038%
53	12.098	1526	1532	1539	rVB	51817	85366	0.93%	0.079%
54	12.316	1564	1569	1575	rVB10	5383	11130	0.12%	0.010%
55	13.198	1714	1719	1723	rBV5	10679	16244	0.18%	0.015%
56	13.275	1726	1732	1736	rBV2	29095	49221	0.54%	0.046%
57	13.328	1738	1741	1746	rVV4	5227	9278	0.10%	0.009%
58	13.787	1810	1819	1825	rBV	4371638	5890448	64.35%	5.450%
59	13.828	1825	1826	1830	rVB	20100	19113	0.21%	0.018%
60	14.057	1856	1865	1882	rBV	5124679	7260375	79.32%	6.718%
61	14.281	1899	1903	1909	rVB7	7888	12408	0.14%	0.011%
62	14.363	1909	1917	1926	rBV	3519151	5000785	54.63%	4.627%
63	14.575	1947	1953	1967	rBV	273073	425547	4.65%	0.394%
64	14.728	1975	1979	1984	rVB8	7346	11194	0.12%	0.010%
65	14.798	1985	1991	1996	rVB10	8669	15119	0.17%	0.014%
66	14.857	1996	2001	2005	rBV7	6657	9607	0.10%	0.009%
67	15.016	2022	2028	2035	rVB7	4841	12097	0.13%	0.011%
68	15.151	2045	2051	2058	rBV	78204	125723	1.37%	0.116%
69	15.234	2062	2065	2069	rVB4	12541	14812	0.16%	0.014%
70	15.363	2080	2087	2101	rBV	6273202	8905328	97.29%	8.240%
71	15.481	2101	2107	2119	rVV	1263041	1731317	18.91%	1.602%
72	15.604	2123	2128	2137	rVB2	70704	116933	1.28%	0.108%
73	15.933	2178	2184	2185	rBV6	6487	11463	0.13%	0.011%
74	16.051	2202	2204	2210	rBV7	5249	11780	0.13%	0.011%
75	16.104	2210	2213	2216	rVV	21005	26210	0.29%	0.024%
76	16.157	2218	2222	2228	rVB4	24732	36895	0.40%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010884.D
 Acq On : 27 Jun 2022 18:48
 Operator : CG/JU
 Sample : N3392-05 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

77	16.804	2328	2332	2337	rVB6	11097	14346	0.16%	0.013%
78	16.904	2345	2349	2354	rBV4	23559	35052	0.38%	0.032%
79	17.128	2380	2387	2397	rBV	3693345	5039822	55.06%	4.663%
80	17.228	2397	2404	2417	rBV2	6465005	8984687	98.16%	8.313%
81	17.539	2454	2457	2463	rVB8	18783	29725	0.32%	0.028%
82	17.651	2473	2476	2481	rBV5	15081	23638	0.26%	0.022%
83	17.822	2500	2505	2510	rVV	117108	147818	1.61%	0.137%
84	18.039	2539	2542	2545	rBV5	7544	9220	0.10%	0.009%
85	18.333	2588	2592	2595	rBV6	10039	19229	0.21%	0.018%
86	18.963	2696	2699	2703	rVB	177625	186768	2.04%	0.173%
87	19.051	2711	2714	2718	rBV	69830	86635	0.95%	0.080%
88	19.098	2718	2722	2723	rVV2	47904	47571	0.52%	0.044%
89	19.122	2723	2726	2731	rVB	70656	84540	0.92%	0.078%
90	19.480	2781	2787	2794	rBV	6990693	9153397	100.00%	8.469%
91	20.968	3038	3040	3046	rBV3	89867	110398	1.21%	0.102%
92	21.239	3081	3086	3093	rBV	3559607	4377928	47.83%	4.051%
93	23.451	3455	3462	3474	rBV2	4513236	8728756	95.36%	8.076%
94	23.604	3482	3488	3502	rVB2	2351986	4570025	49.93%	4.229%

Sum of corrected areas: 108076511

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010884.D
Acq On : 27 Jun 2022 18:48
Operator : CG/JU
Sample : N3392-05 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isobutyl acetate Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.911	2.15 ng/ul	322977	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isobutyl acetate	116	C6H12O2	000110-19-0	78
2			Isobutyl acetate	116	C6H12O2	000110-19-0	78
3			Isobutyl acetate	116	C6H12O2	000110-19-0	78
4			Isobutyl acetate	116	C6H12O2	000110-19-0	64
5			Isobutyl acetate	116	C6H12O2	000110-19-0	59

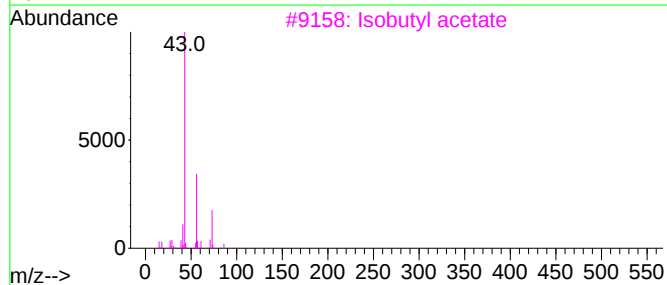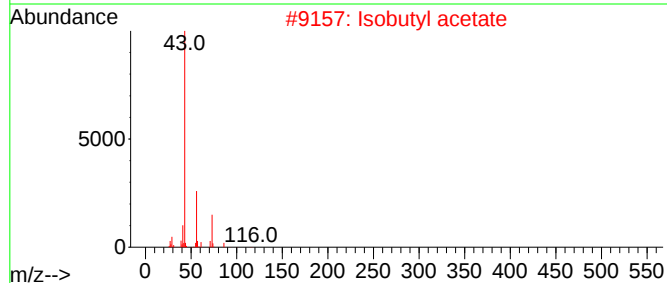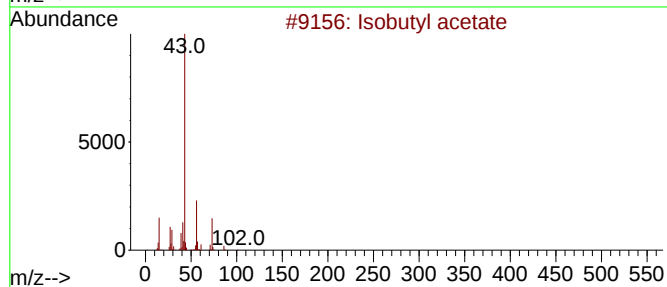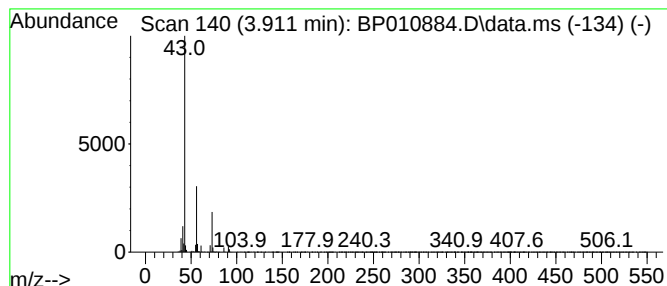

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010884.D
Acq On : 27 Jun 2022 18:48
Operator : CG/JU
Sample : N3392-05 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Propanoic acid, propyl ester Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.369	4.58 ng/ul	687963	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	83
2			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	83
3			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	78
4			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	64
5			Propanoic acid, propyl ester	116	C6H12O2	000106-36-5	64

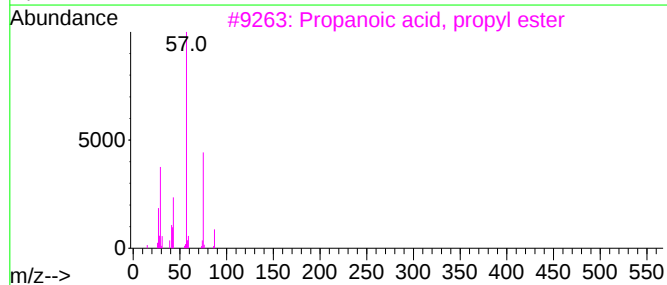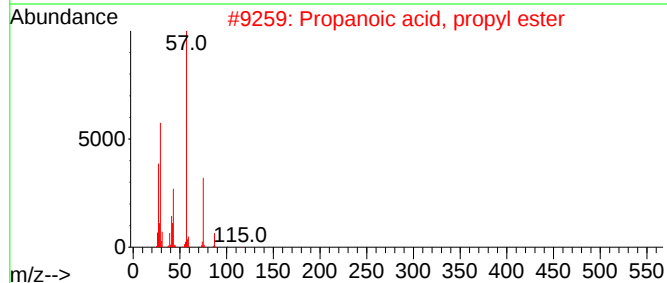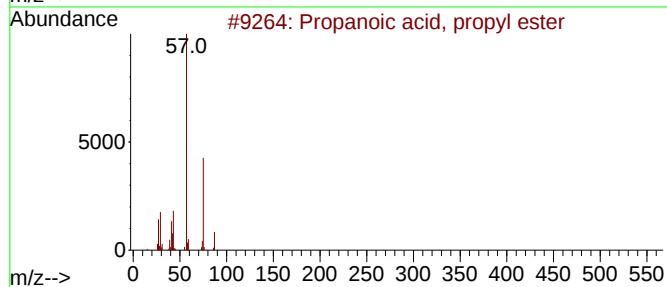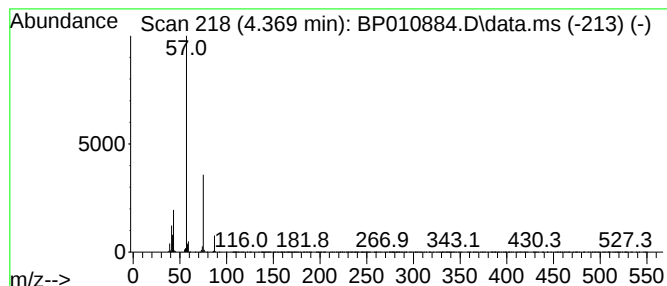

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010884.D
Acq On : 27 Jun 2022 18:48
Operator : CG/JU
Sample : N3392-05 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Acetic acid, butyl ester Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.434	2.16 ng/ul	325160	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Acetic acid, butyl ester		116	C6H12O2	000123-86-4	64	
2	Acetic acid, butyl ester		116	C6H12O2	000123-86-4	59	
3	Acetic acid, butyl ester		116	C6H12O2	000123-86-4	50	
4	Acetic acid, butyl ester		116	C6H12O2	000123-86-4	43	
5	Isobutyl acetate		116	C6H12O2	000110-19-0	36	

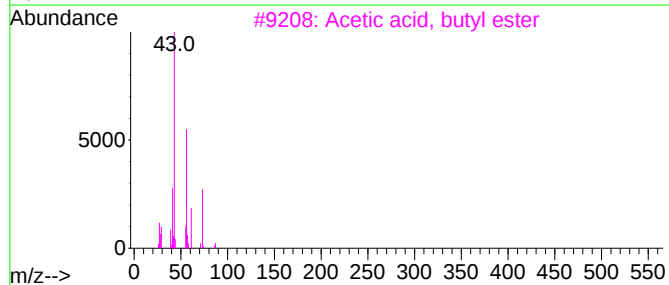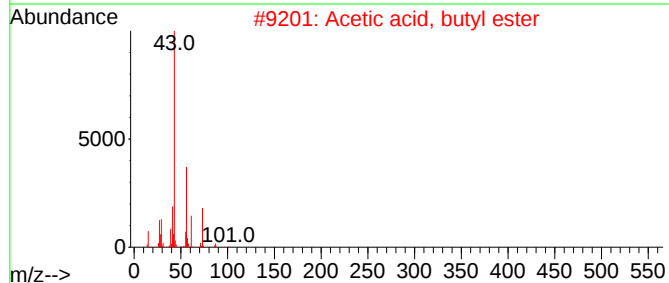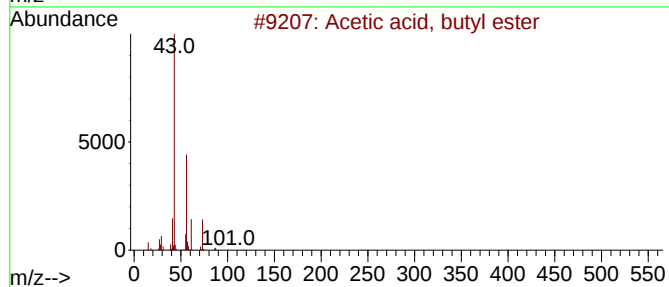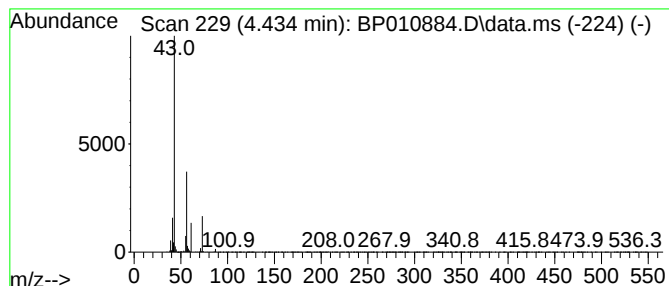

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010884.D
Acq On : 27 Jun 2022 18:48
Operator : CG/JU
Sample : N3392-05 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Isopropyl butyrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.816	5.35 ng/ul	803153	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
2			Isopropyl butyrate	130	C7H14O2	000638-11-9	86
3			Isopropyl butyrate	130	C7H14O2	000638-11-9	86
4			Propanoic acid, 2-methyl-, 1-met...	130	C7H14O2	000617-50-5	64
5			Isopropyl butyrate	130	C7H14O2	000638-11-9	64

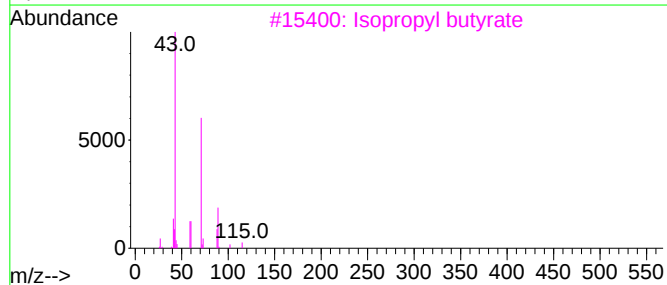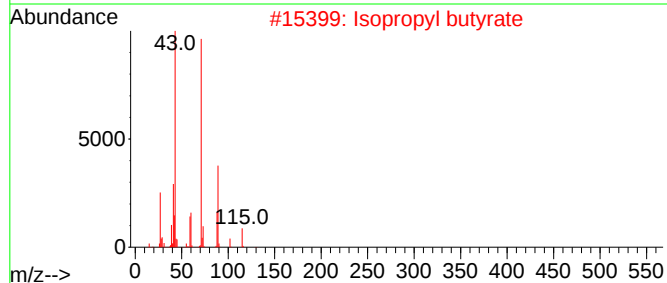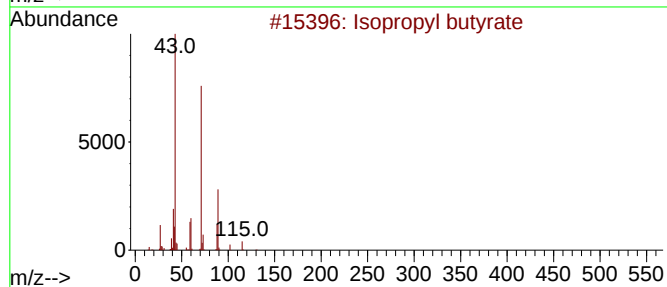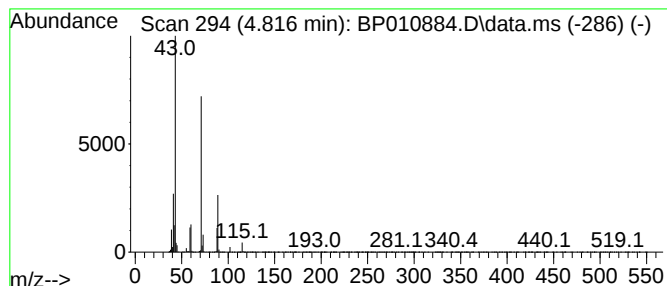

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010884.D
Acq On : 27 Jun 2022 18:48
Operator : CG/JU
Sample : N3392-05 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isobutyl acetate	3.911	2.1	ng/ul	322977	1	7.710	3004940	20.0
Propanoic acid,...	4.369	4.6	ng/ul	687963	1	7.710	3004940	20.0
Acetic acid, bu...	4.434	2.2	ng/ul	325160	1	7.710	3004940	20.0
Isopropyl butyrate	4.816	5.3	ng/ul	803153	1	7.710	3004940	20.0