

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010888.D
 Acq On : 27 Jun 2022 21:37
 Operator : CG/JU
 Sample : PB145835BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK835

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010888.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	15	20	30	rVB	198624	252550	2.93%	0.222%
2	3.605	85	88	108	rBV	2293297	3325459	38.64%	2.917%
3	3.929	139	143	149	rVB	56512	74607	0.87%	0.065%
4	6.217	528	532	537	rBV7	3705	8619	0.10%	0.008%
5	6.881	638	645	660	rBV	2477787	3786518	43.99%	3.321%
6	7.052	667	674	683	rVB	2147400	3207688	37.27%	2.814%
7	7.240	699	706	720	rBV	2591399	3952645	45.92%	3.467%
8	7.705	778	785	796	rVB	2055095	3257807	37.85%	2.858%
9	8.422	900	907	922	rBV	3091136	4721886	54.86%	4.142%
10	8.869	972	983	992	rBV	2337955	3633042	42.21%	3.187%
11	9.587	1097	1105	1122	rBV	1646395	2632889	30.59%	2.309%
12	10.122	1189	1196	1207	rBV	2601927	4303037	50.00%	3.775%
13	10.505	1253	1261	1268	rBV	2850993	4665399	54.21%	4.092%
14	10.646	1277	1285	1300	rBV	2950313	4753738	55.23%	4.170%
15	12.099	1526	1532	1539	rBV	50935	83328	0.97%	0.073%
16	12.310	1563	1568	1572	rBV7	6834	13091	0.15%	0.011%
17									

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010888.D
Acq On : 27 Jun 2022 21:37
Operator : CG/JU
Sample : PB145835BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK835

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION

37 23.604 3481 3488 3497 rVB2 2409120 4751525 55.21% 4.168%




Sum of corrected areas: 114002723

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010888.D
Acq On : 27 Jun 2022 21:37
Operator : CG/JU
Sample : PB145835BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK835

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

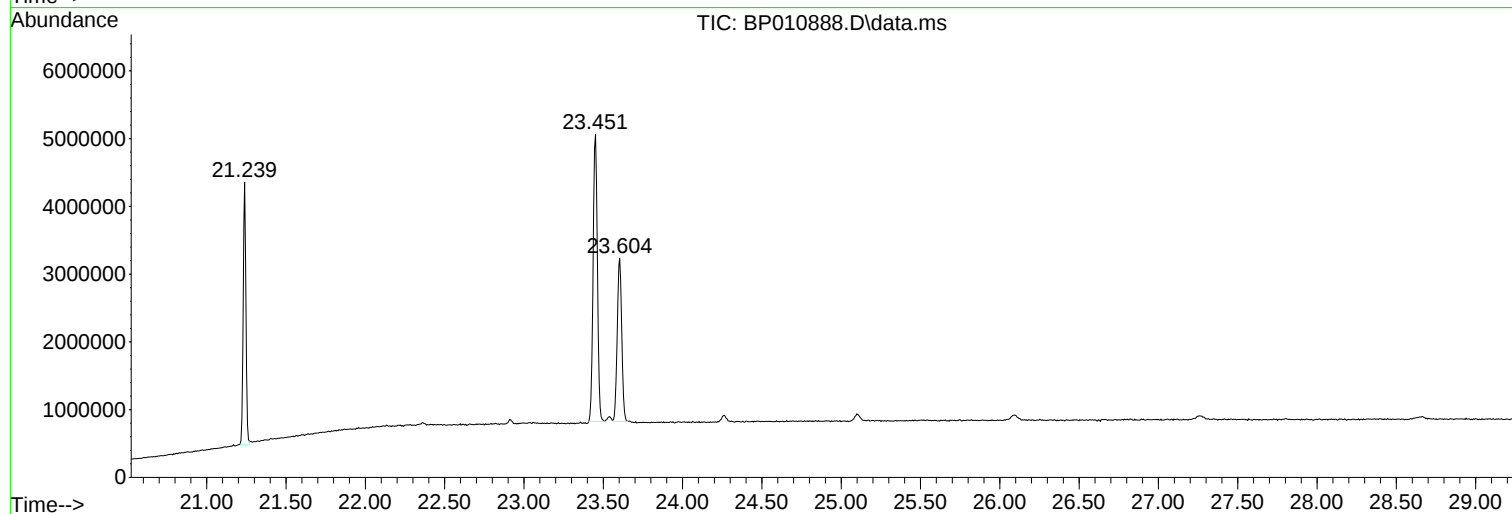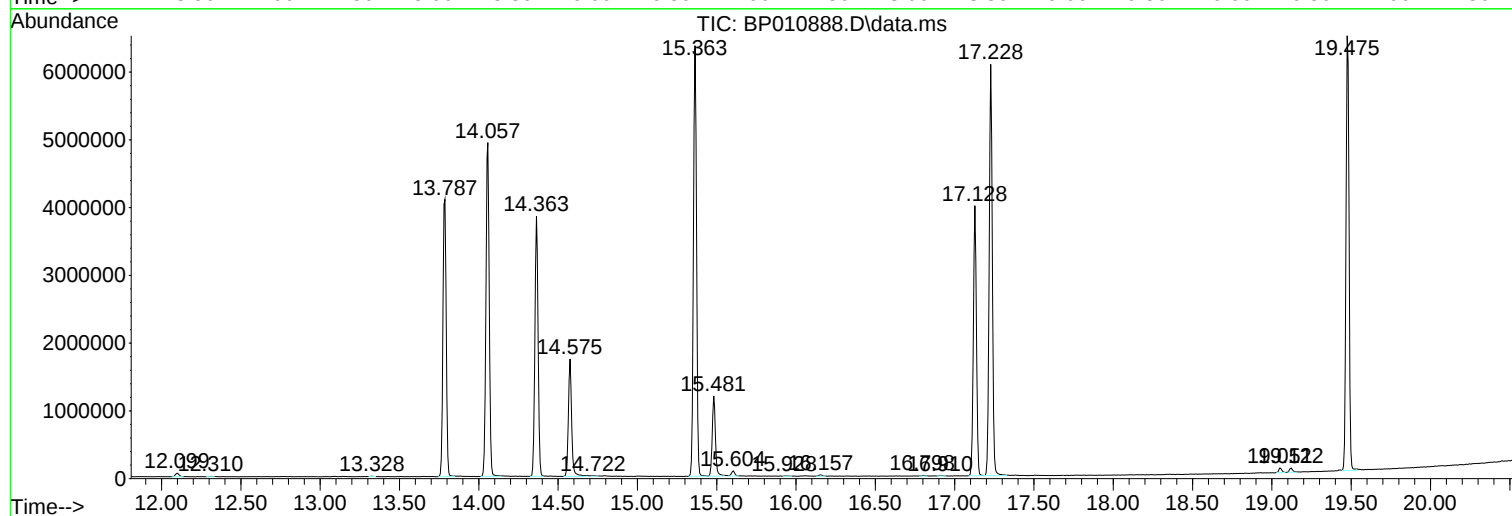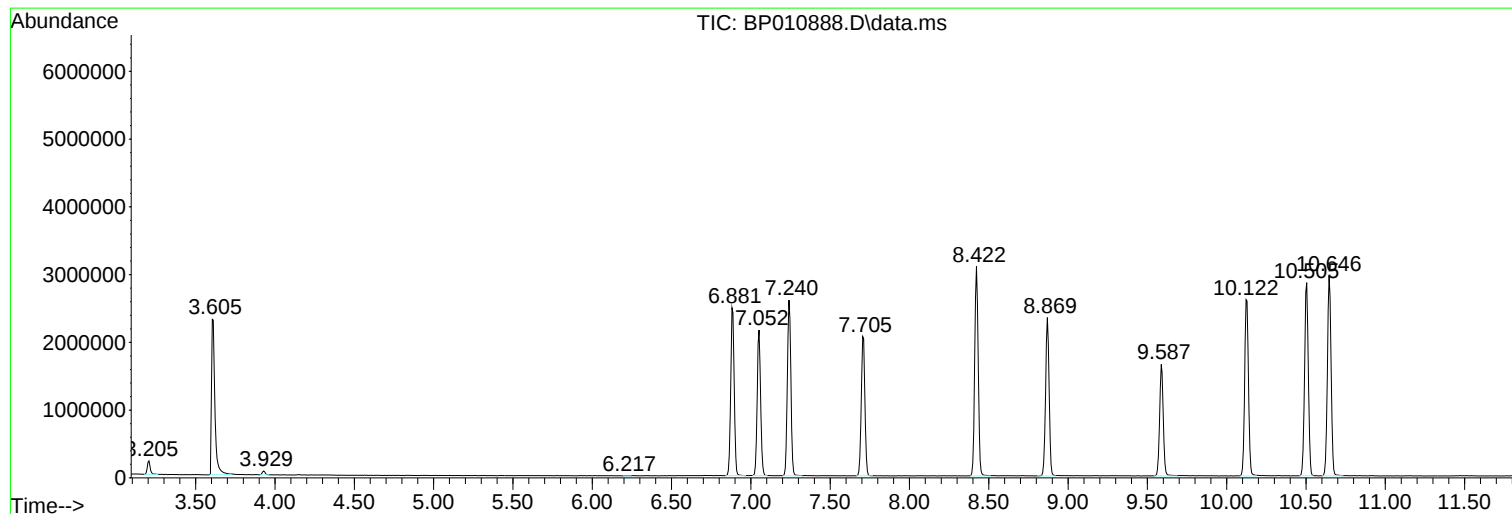

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010888.D
Acq On : 27 Jun 2022 21:37
Operator : CG/JU
Sample : PB145835BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK835

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010888.D
Acq On : 27 Jun 2022 21:37
Operator : CG/JU
Sample : PB145835BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK835

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------