

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010889.D
 Acq On : 27 Jun 2022 22:11
 Operator : CG/JU
 Sample : PB145713BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK713

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010889.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	27	rVB	158883	200794	2.79%	0.216%
2	3.611	85	89	105	rBV	1874413	2749664	38.19%	2.955%
3	3.928	138	143	148	rBV	44001	57092	0.79%	0.061%
4	4.840	293	298	301	rVB7	4227	7227	0.10%	0.008%
5	6.881	639	645	656	rBV	1997033	3024625	42.01%	3.251%
6	7.052	667	674	683	rVB	1746854	2592898	36.01%	2.787%
7	7.240	699	706	719	rBV	2096840	3166794	43.98%	3.403%
8	7.710	776	786	793	rBV	1772330	2797392	38.85%	3.006%
9	8.422	899	907	922	rBV	2436527	3731577	51.83%	4.010%
10	8.869	972	983	992	rBV	1836652	2871876	39.89%	3.086%
11	9.587	1098	1105	1116	rBV	1259583	2003553	27.83%	2.153%
12	10.122	1189	1196	1211	rBV	2090131	3360264	46.67%	3.611%
13	10.504	1253	1261	1269	rBV	2357701	3949967	54.86%	4.245%
14	10.645	1277	1285	1301	rBV	2317428	3750920	52.10%	4.031%
15	12.098	1525	1532	1538	rBV	45113	71389	0.99%	0.077%
16	12.310	1565	1568	1574	rVB7	5135	9706	0.13%	0.010%
17	13.092	1696	1701	1706	rBV6	5602	7869	0.11%	0.008%
18	13.275	1725	1732	1735	rBV3	19140	31012	0.43%	0.033%
19	13.334	1737	1742	1745	rVB6	5998	8454	0.12%	0.009%
20	13.781	1812	1818	1828	rBV	3141770	4385409	60.91%	4.713%
21	14.057	1856	1865	1880	rBV	3661312	5421210	75.29%	5.826%
22	14.363	1909	1917	1928	rBV	3158576	4484809	62.29%	4.820%
23	14.575	1946	1953	1974	rBV	1346155	1970757	27.37%	2.118%
24	14.798	1987	1991	1995	rVB7	5459	9462	0.13%	0.010%
25	15.363	2080	2087	2100	rBV	4833829	6634296	92.14%	7.130%
26	15.481	2101	2107	2123	rVV	897688	1269705	17.63%	1.365%
27	15.604	2123	2128	2138	rVB	58521	96808	1.34%	0.104%
28	16.151	2217	2221	2227	rBV4	17936	25772	0.36%	0.028%
29	16.804	2328	2332	2337	rVB8	9447	15381	0.21%	0.017%
30	16.910	2346	2350	2354	rBV4	9068	14516	0.20%	0.016%
31	17.127	2380	2387	2397	rBV	3455846	4567798	63.44%	4.909%
32	17.227	2397	2404	2417	rVV	4887931	6549968	90.97%	7.039%
33	19.051	2710	2714	2718	rBV2	55330	79342	1.10%	0.085%
34	19.122	2722	2726	2730	rVV	51294	64990	0.90%	0.070%
35	19.474	2781	2786	2794	rBV	5301425	6964700	96.73%	7.485%
36	21.239	3081	3086	3092	rBV	3629757	4360071	60.56%	4.686%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010889.D
Acq On : 27 Jun 2022 22:11
Operator : CG/JU
Sample : PB145713BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK713

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION

37	23.451	3456	3462	3473	rVB2	3826402	7200035	100.00%	7.738%
38	23.604	3482	3488	3497	rVB2	2298805	4539658	63.05%	4.879%




Sum of corrected areas: 93047760

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010889.D
Acq On : 27 Jun 2022 22:11
Operator : CG/JU
Sample : PB145713BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK713

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

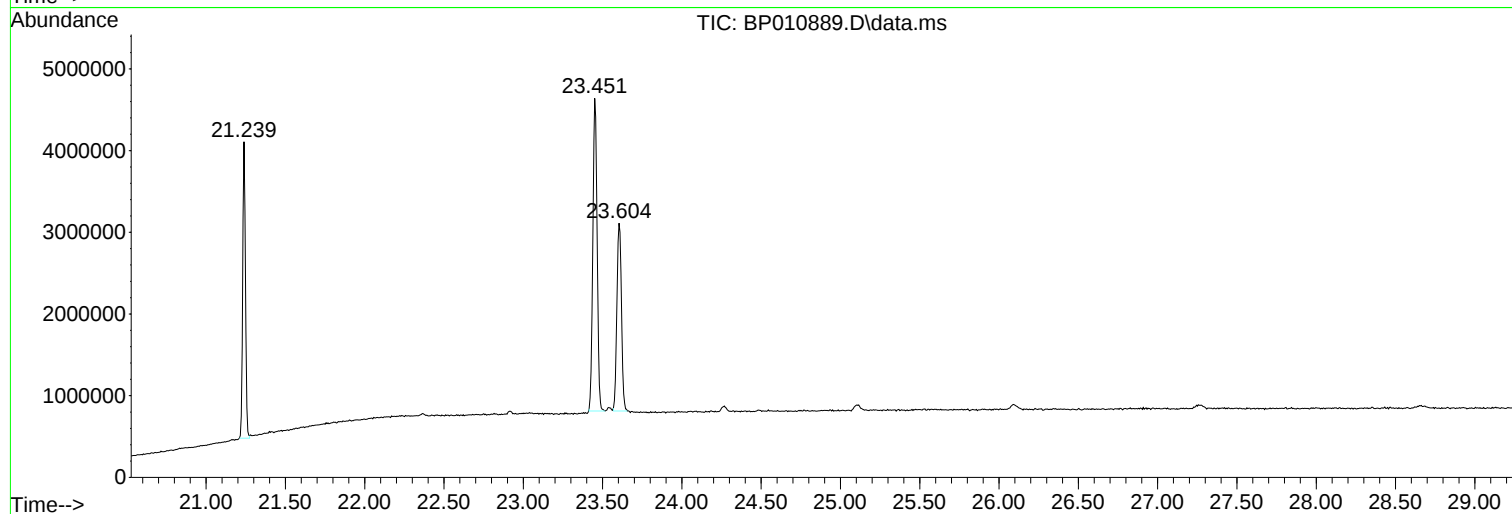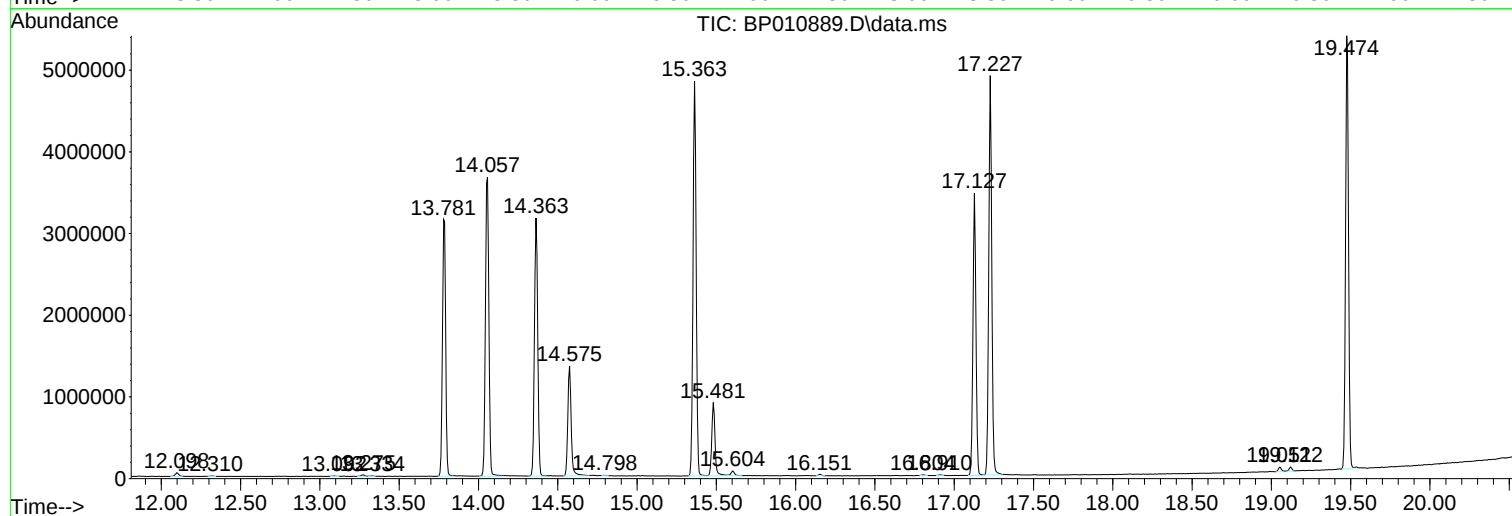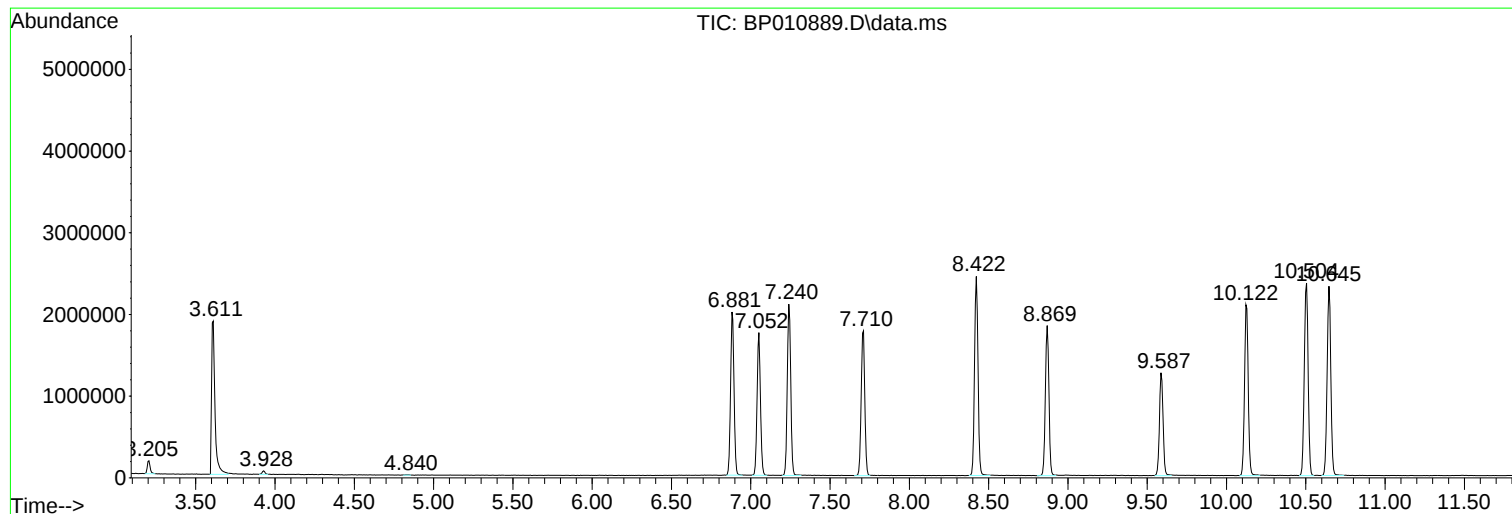

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010889.D
Acq On : 27 Jun 2022 22:11
Operator : CG/JU
Sample : PB145713BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK713

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010889.D
Acq On : 27 Jun 2022 22:11
Operator : CG/JU
Sample : PB145713BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK713

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------