

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
 Data File : BP010899.D
 Acq On : 28 Jun 2022 03:50
 Operator : CG/JU
 Sample : PB145729BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK729

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	3	6	11	rVB	4186394	4414172	79.53%	13.026%
2	3.423	54	57	59	rBV4	10023	11824	0.21%	0.035%
3	3.458	59	63	69	rVB	115576	138787	2.50%	0.410%
4	3.546	74	78	82	rBV6	8102	12568	0.23%	0.037%
5	3.923	138	142	146	rVB	53862	63879	1.15%	0.189%
6	4.846	295	299	302	rBV	12283	15079	0.27%	0.044%
7	6.652	599	606	609	rVB9	4426	8626	0.16%	0.025%
8	6.852	637	640	644	rBV6	4054	7838	0.14%	0.023%
9	7.705	778	785	797	rVB	2298229	3428383	61.77%	10.117%
10	10.505	1252	1261	1270	rVV	2792492	4695935	84.60%	13.858%
11	11.163	1369	1373	1374	rBV4	4587	5572	0.10%	0.016%
12	11.863	1488	1492	1495	rBV6	4453	7037	0.13%	0.021%
13	13.087	1695	1700	1705	rVB9	7379	9794	0.18%	0.029%
14	13.804	1816	1822	1825	rBV8	3900	6888	0.12%	0.020%
15	14.363	1910	1917	1926	rBV	3686772	5344079	96.28%	15.770%
16	15.363	2084	2087	2090	rBV5	5582	6120	0.11%	0.018%
17	16.904	2346	2349	2355	rBV5	11017	20643	0.37%	0.061%
18	17.128	2380	2387	2401	rBV	3896659	5550592	100.00%	16.380%
19	21.239	3081	3086	3092	rBV	4024410	5091241	91.72%	15.024%
20	23.604	3481	3488	3500	rVB2	2498452	5047653	90.94%	14.896%




Sum of corrected areas: 33886710

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010899.D
Acq On : 28 Jun 2022 03:50
Operator : CG/JU
Sample : PB145729BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK729

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

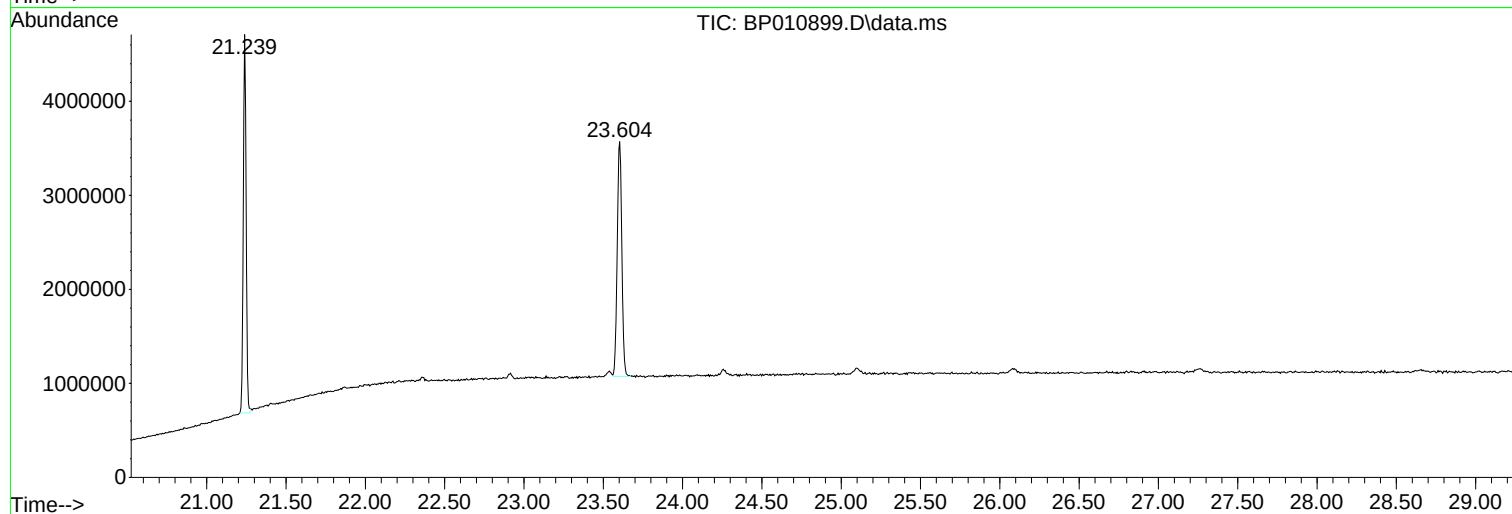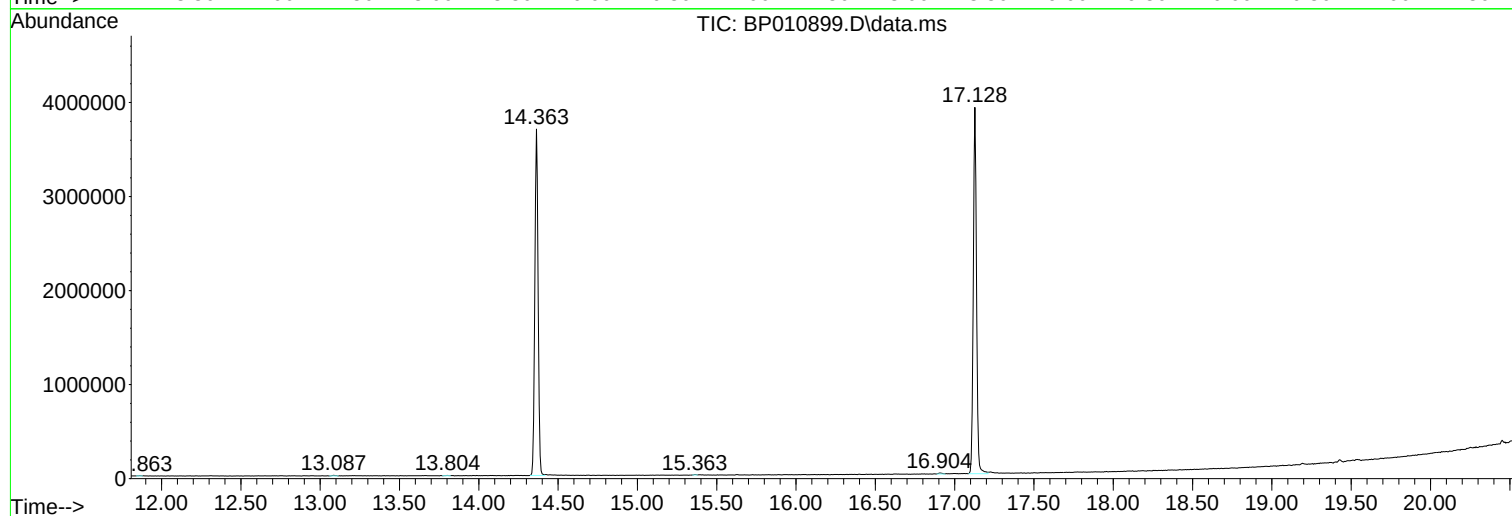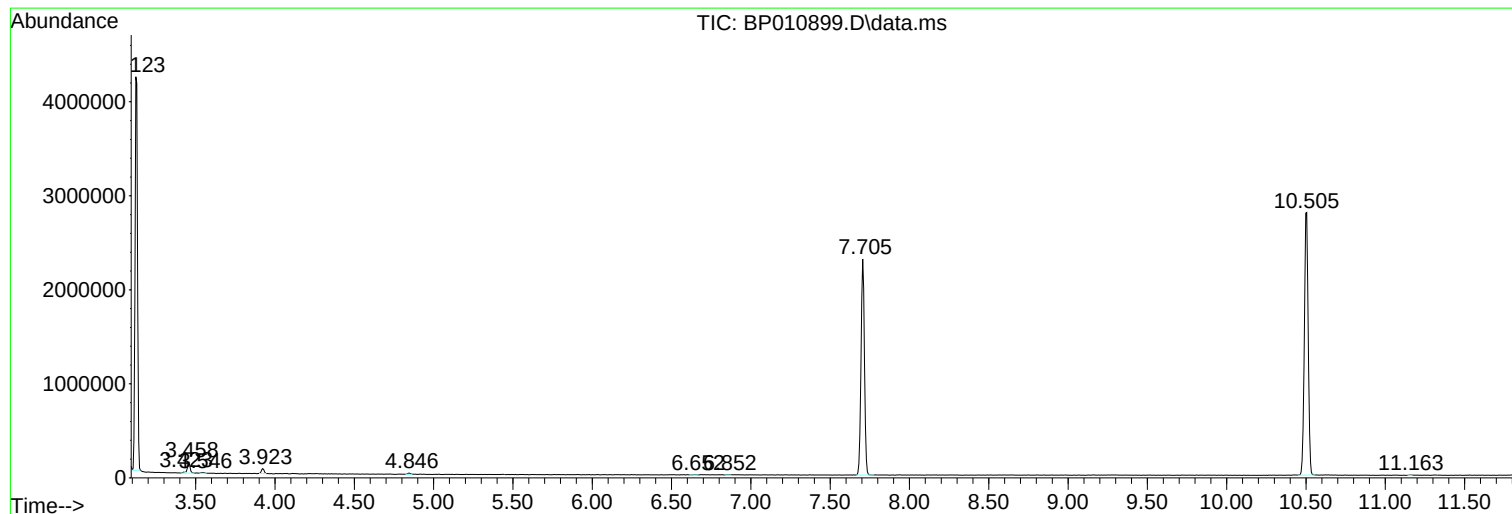

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010899.D
Acq On : 28 Jun 2022 03:50
Operator : CG/JU
Sample : PB145729BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK729










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.123	25.75 ng/ul	4414170	1,4-Dichlorobenzene-d4	7.705

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	95
2			Heptane	100	C7H16	000142-82-5	94
3			Heptane	100	C7H16	000142-82-5	87
4			Heptane	100	C7H16	000142-82-5	87
5			Oxalic acid, isobutyl pentyl ester	216	C11H20O4	1000309-37-0	59

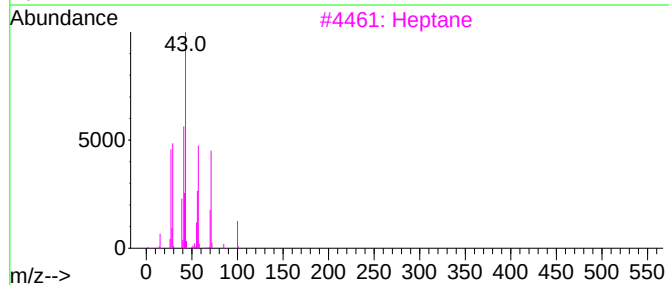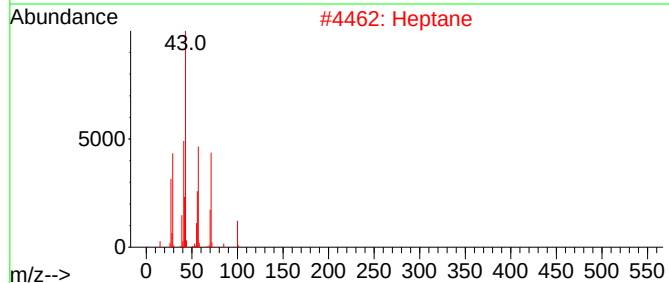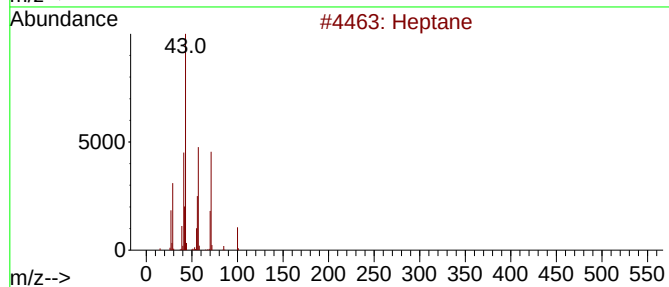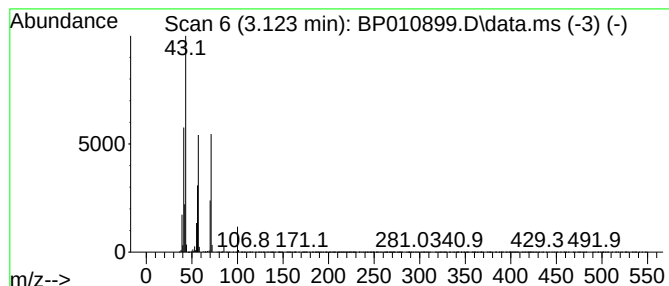

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062722\
Data File : BP010899.D
Acq On : 28 Jun 2022 03:50
Operator : CG/JU
Sample : PB145729BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK729

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.123	25.8	ng/u1	4414170	1	7.705	3428380	20.0