

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020706.D
Acq On : 29 Jun 2024 00:51
Operator : MA/JU
Sample : P2897-14
Misc :
ALS Vial : 64 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 06/29/2024

Quant Time: Jun 29 01:20:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

06/29/2024
Supervised By :mohammad
ahmed

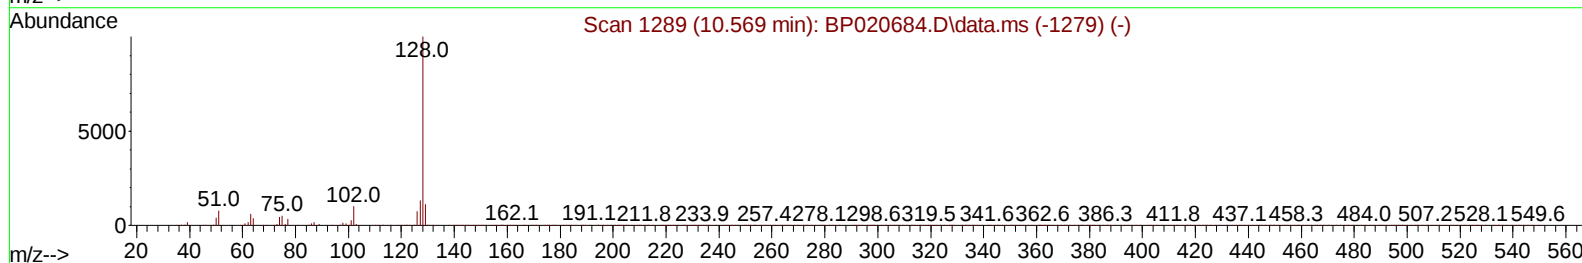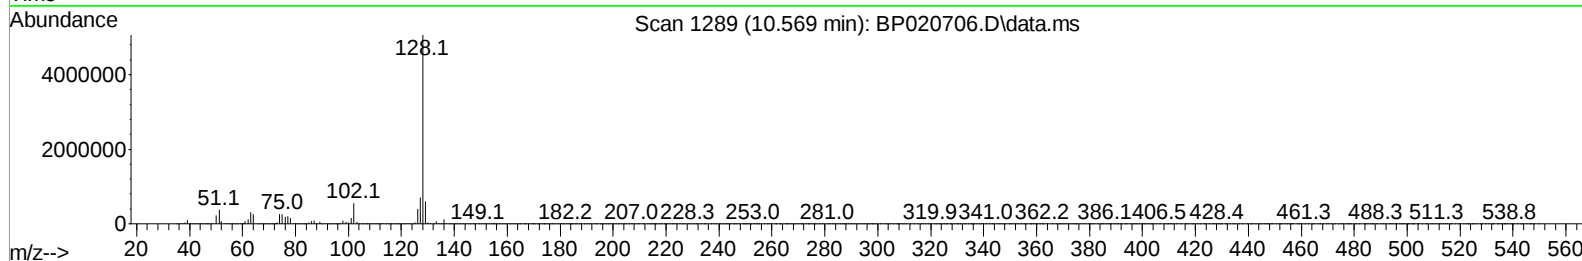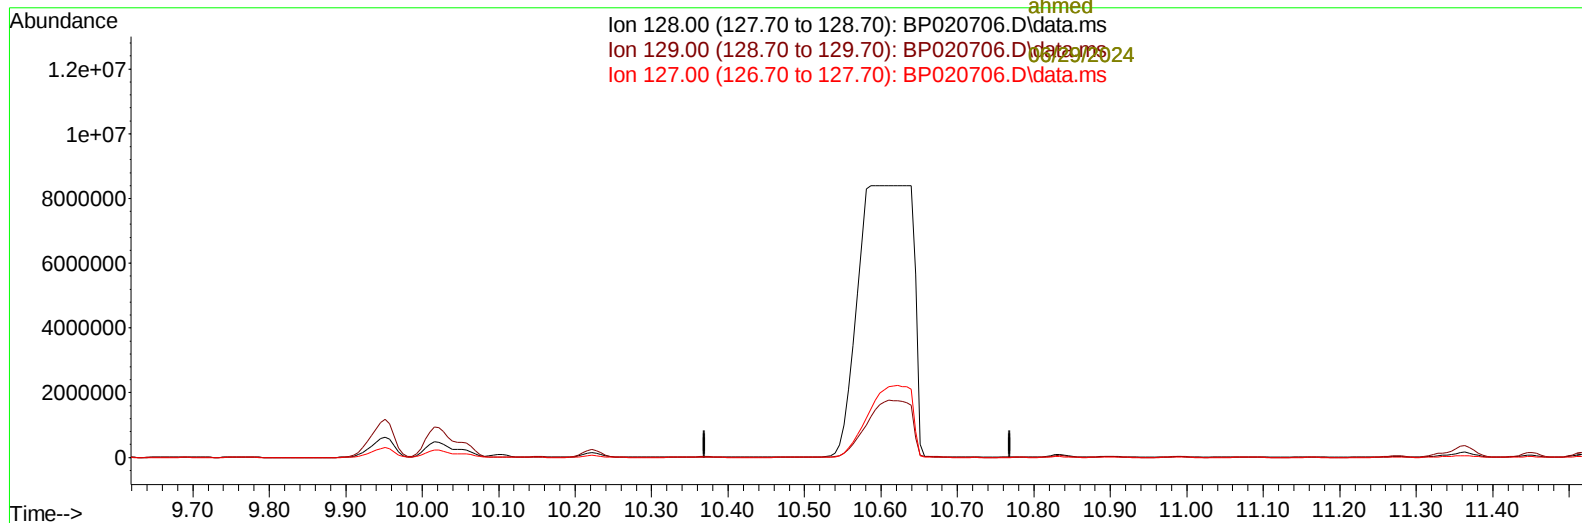

TIC: BP020706.D\data.ms

(30) Naphthalene

10.569min (-10.569) 0.00 ng/u1

response 0

Ion	Exp%	Act%
128.00	100.00	0.00
129.00	10.90	0.00#
127.00	13.20	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020706.D
 Acq On : 29 Jun 2024 00:51
 Operator : MA/JU
 Sample : P2897-14
 Misc :
 ALS Vial : 64 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
 Supervised By :mohammad ahmed 06/29/2024

06/29/2024
 Supervised By :mohammad
 ahmed

Quant Time: Jun 29 01:20:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

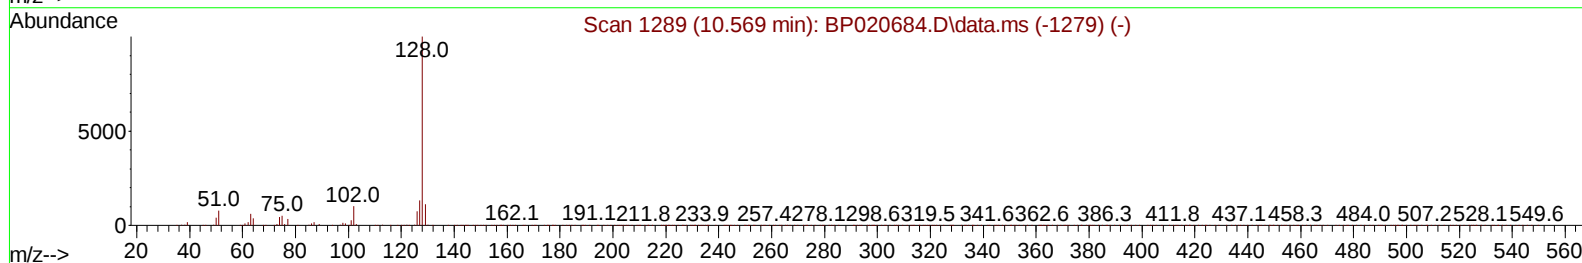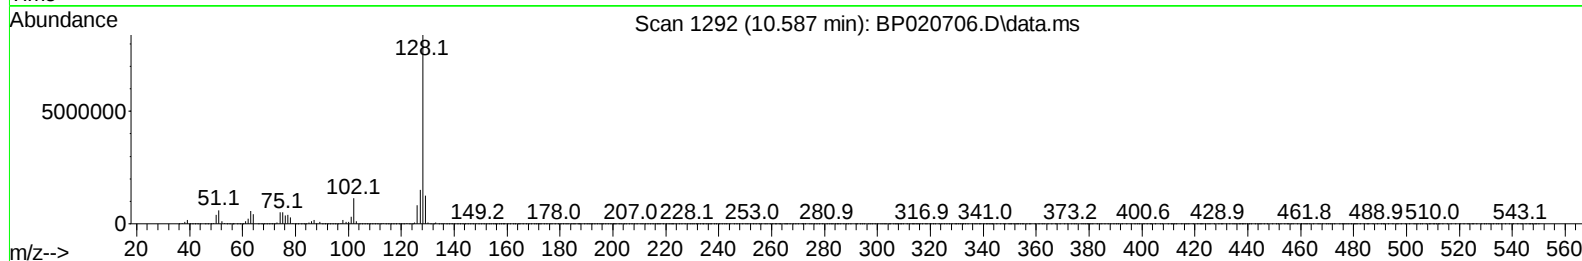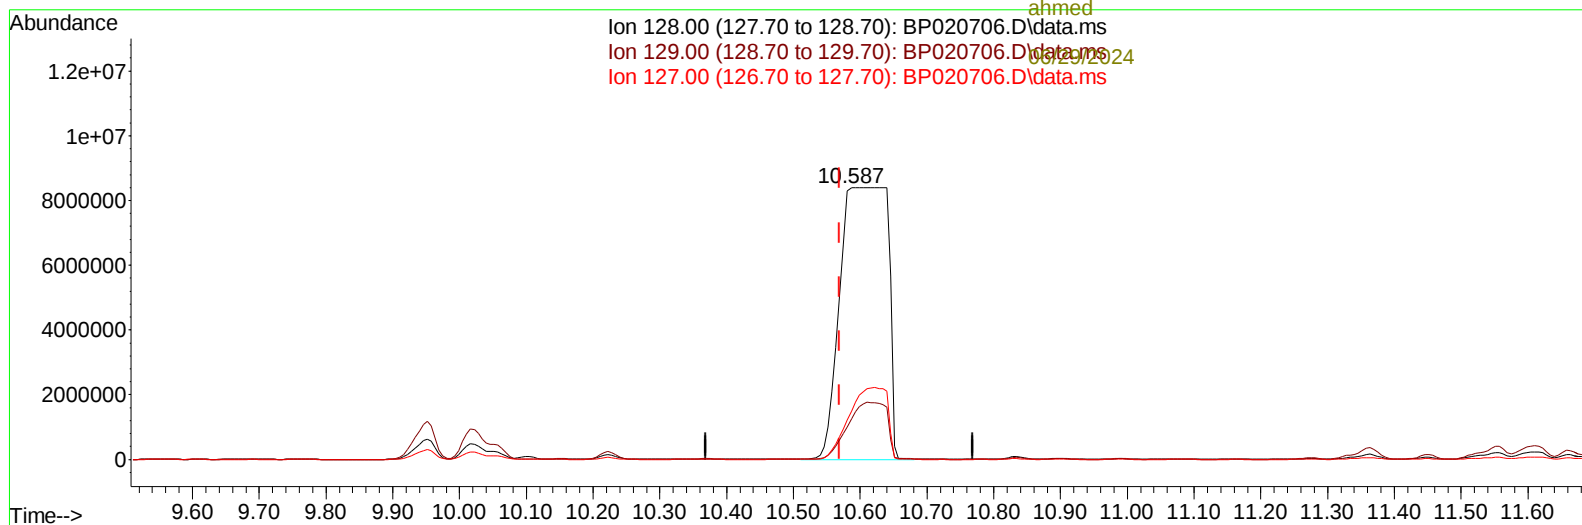

TIC: BP020706.D\data.ms

(30) Naphthalene

10.587min (+ 0.018) 980.69 ng/ul m

response 41376394

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	10.90	14.91#
127.00	13.20	17.85#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020706.D
Acq On : 29 Jun 2024 00:51
Operator : MA/JU
Sample : P2897-14
Misc :
ALS Vial : 64 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 06/29/2024

Quant Time: Jun 29 01:25:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

06/29/2024
Supervised By :mohammad
ahmed

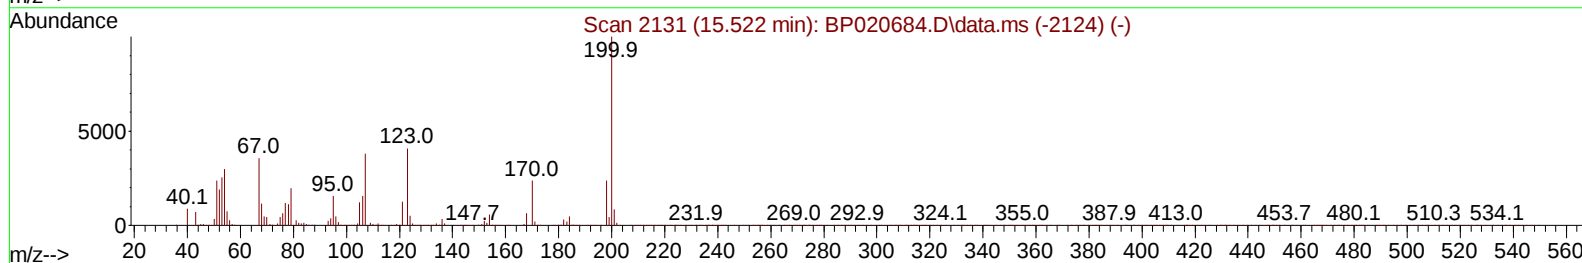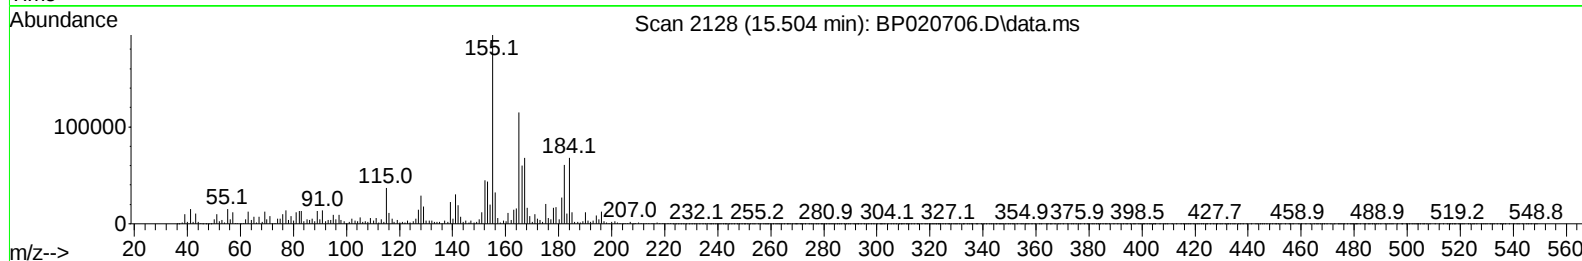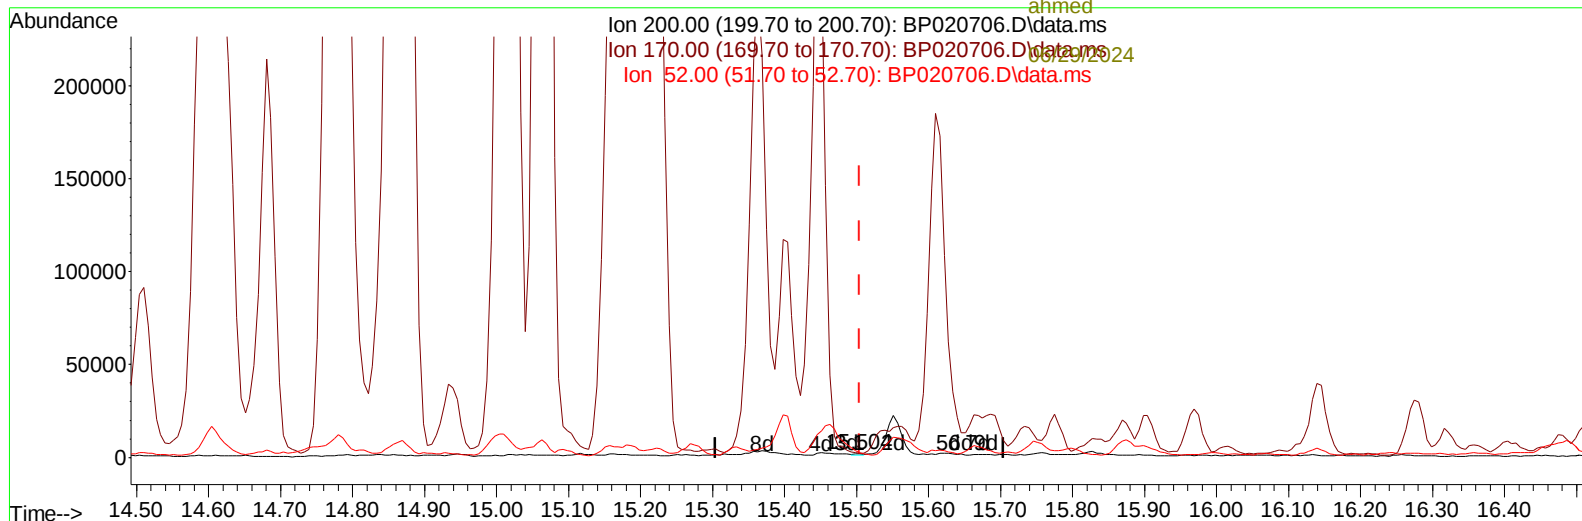

TIC: BP020706.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.504min (-0.000) 0.16 ng/u1

response 743

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	20.80	109.18#
52.00	45.40	124.01#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020706.D
 Acq On : 29 Jun 2024 00:51
 Operator : MA/JU
 Sample : P2897-14
 Misc :
 ALS Vial : 64 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 C0T61

Manual IntegrationsAPPROVED

Quant Time: Jun 29 01:25:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/29/2024
 Supervised By :mohammad ahmed 06/29/2024

06/29/2024
 Supervised By :mohammad
 ahmed

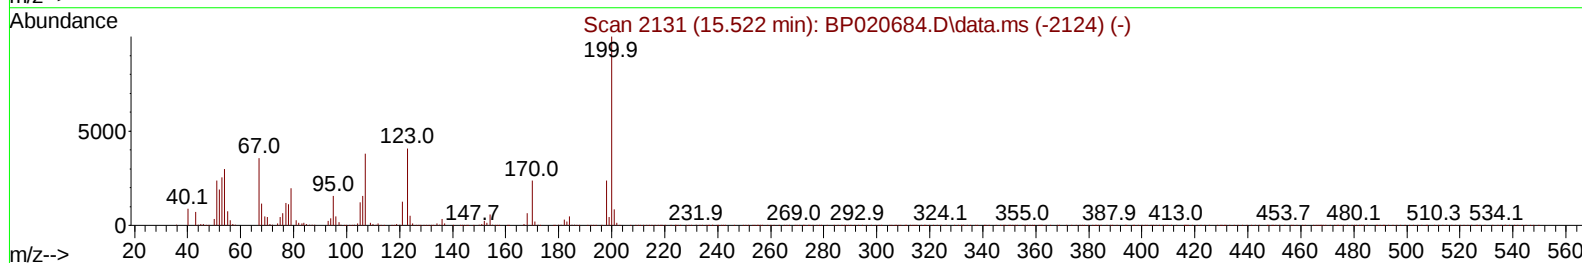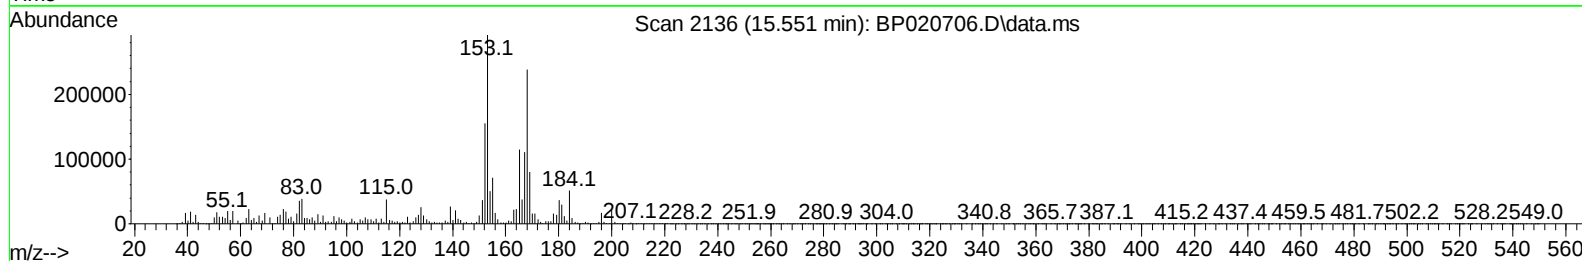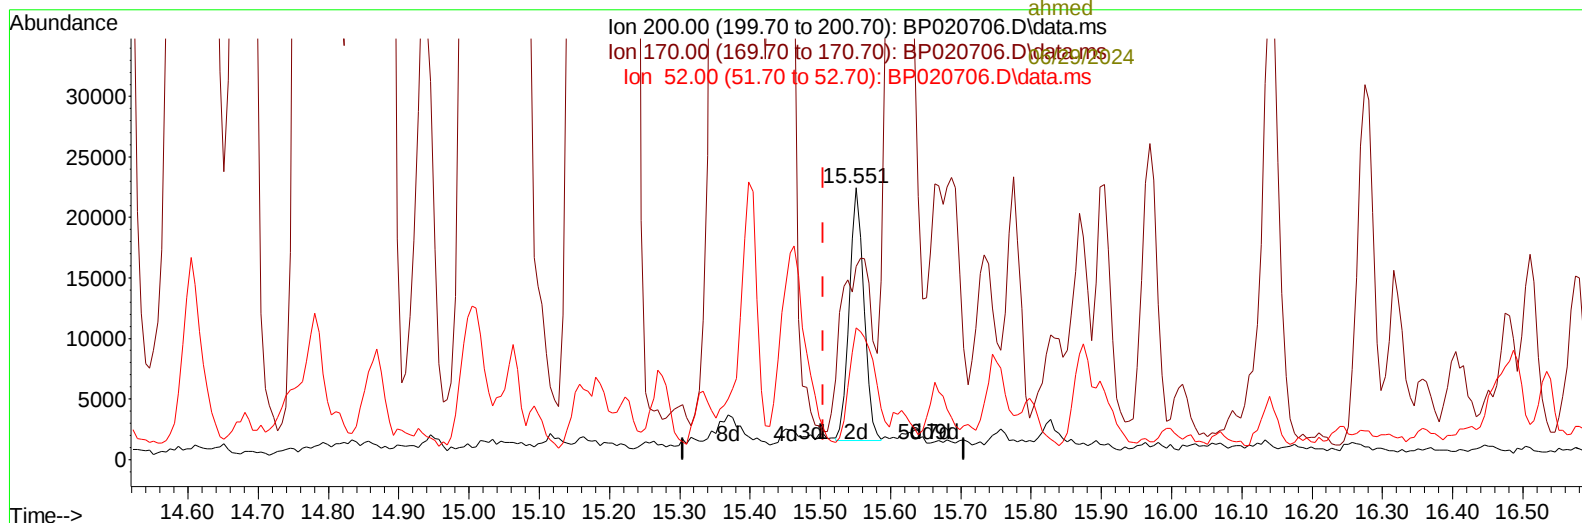

TIC: BP020706.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.551min (+ 0.047) 6.67 ng/ul m

response 30099

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	20.80	71.16#
52.00	45.40	48.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020706.D
Acq On : 29 Jun 2024 00:51
Operator : MA/JU
Sample : P2897-14
Misc :
ALS Vial : 64 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 06/29/2024

Quant Time: Jun 29 01:21:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

06/29/2024
Supervised By :mohammad
ahmed

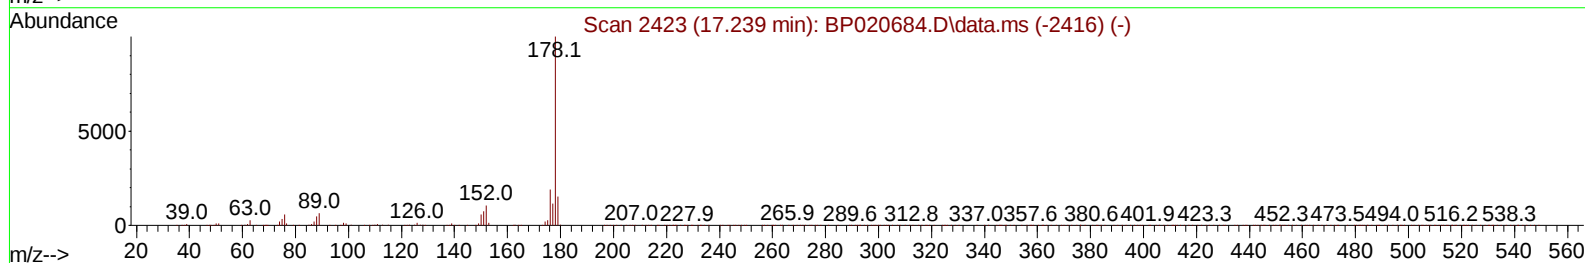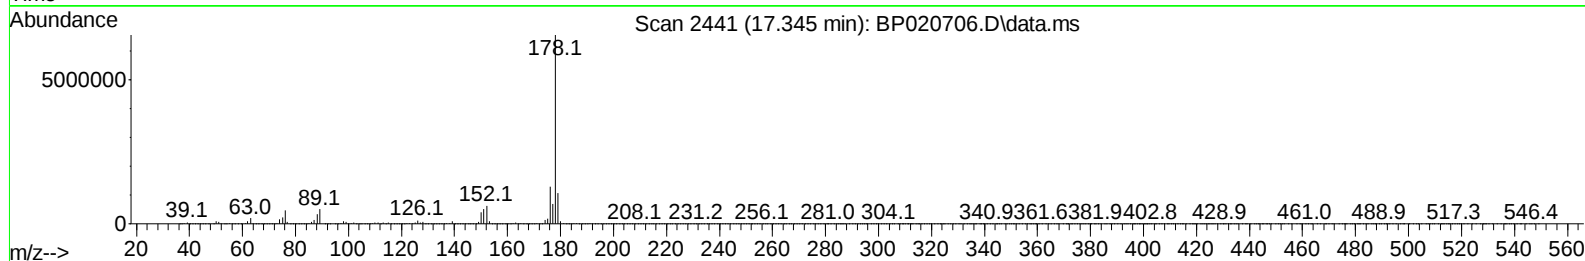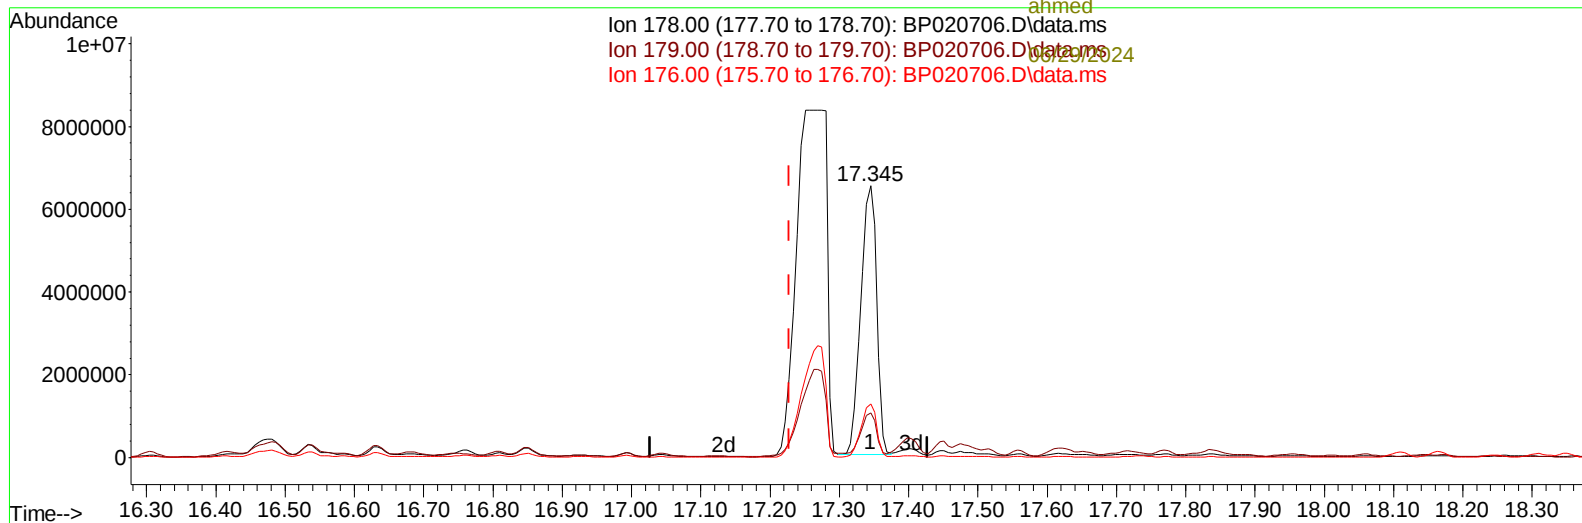

TIC: BP020706.D\data.ms

(72) Phenanthrene

17.345min (+ 0.118) 222.21 ng/u1

response 10420010

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.50	16.33
176.00	19.30	19.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020706.D
Acq On : 29 Jun 2024 00:51
Operator : MA/JU
Sample : P2897-14
Misc :
ALS Vial : 64 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 06/29/2024

Quant Time: Jun 29 01:21:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

06/29/2024
Supervised By :mohammad
ahmed

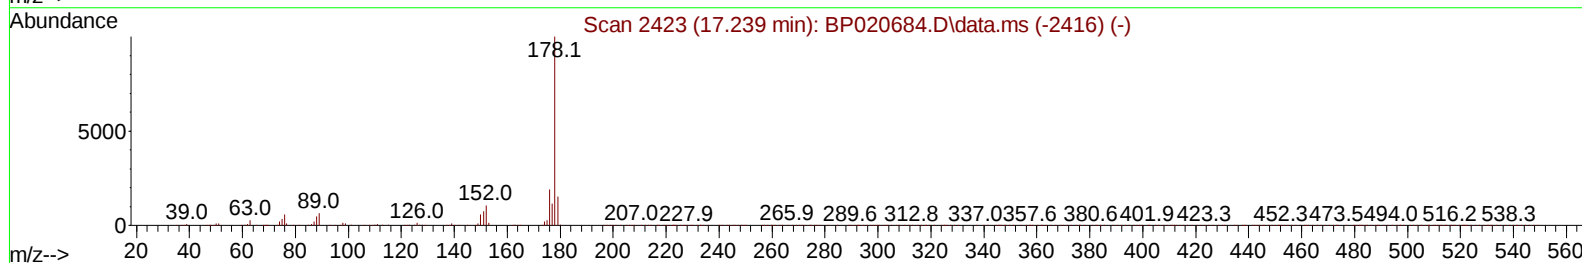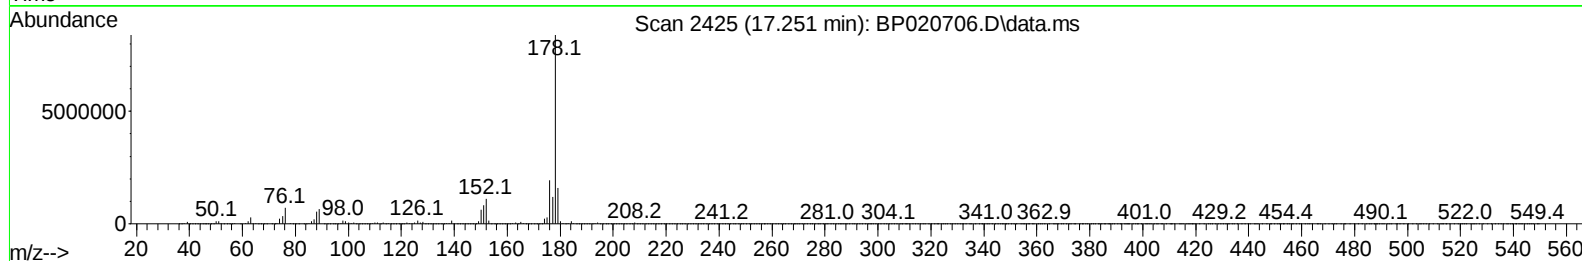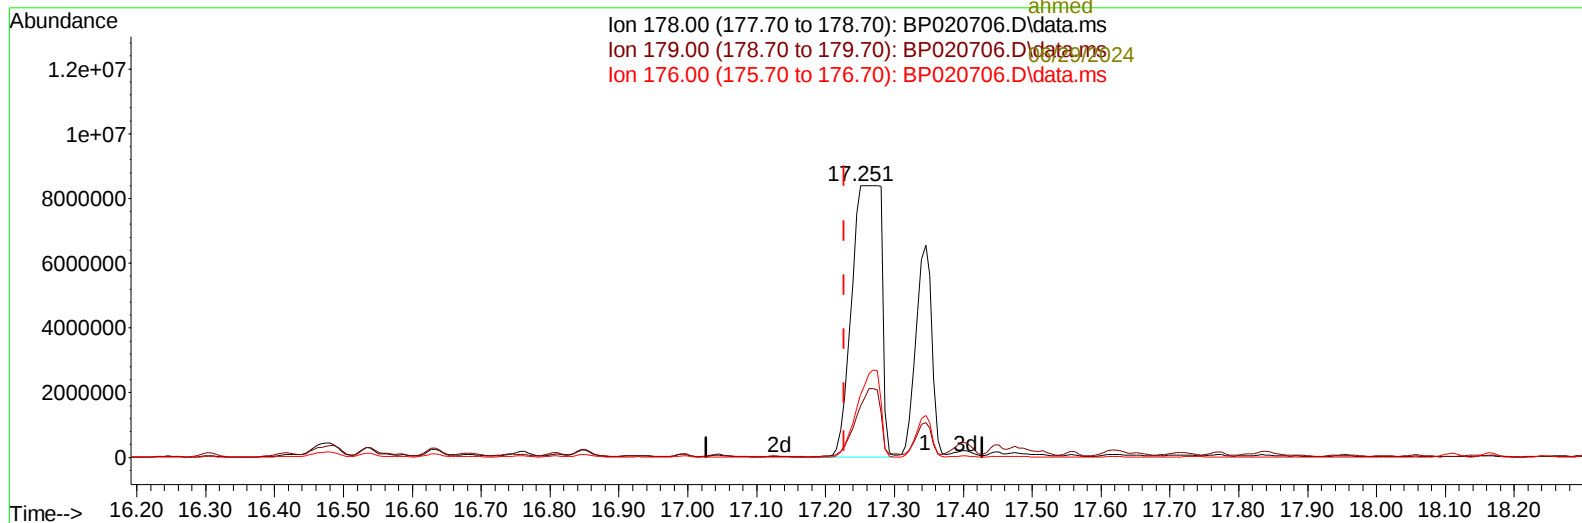

TIC: BP020706.D\data.ms

(72) Phenanthrene

17.251min (+ 0.024) 537.22 ng/u1 m

response 25191311

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.50	19.04#
176.00	19.30	23.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020706.D
 Acq On : 29 Jun 2024 00:51
 Operator : MA/JU
 Sample : P2897-14
 Misc :
 ALS Vial : 64 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
 Supervised By :mohammad ahmed 06/29/2024

Quant Time: Jun 29 01:22:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

06/29/2024
 Supervised By :mohammad
 ahmed

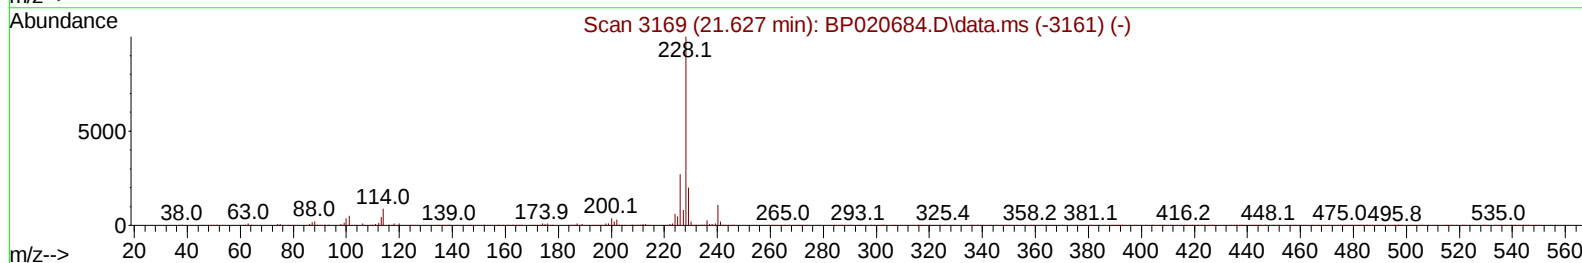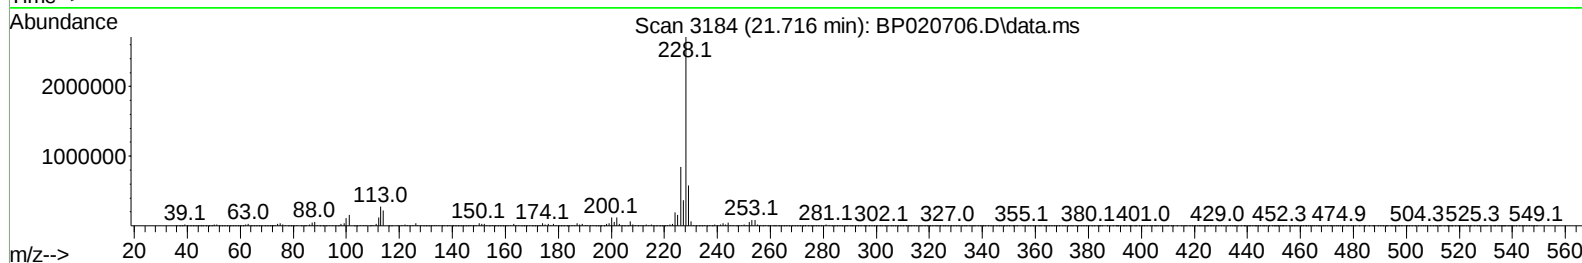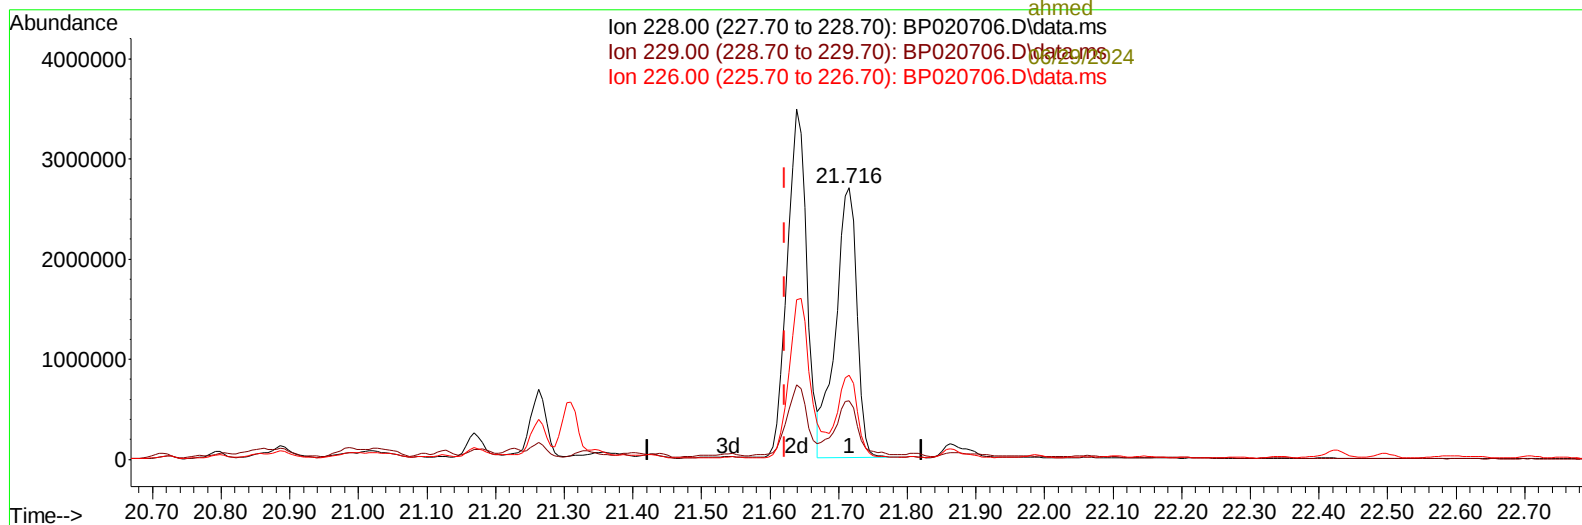

TIC: BP020706.D\data.ms

(85) Benzo(a)anthracene

21.716min (+ 0.094) 126.04 ng/u1

response 5841553

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.00	21.49
226.00	26.40	31.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020706.D
 Acq On : 29 Jun 2024 00:51
 Operator : MA/JU
 Sample : P2897-14
 Misc :
 ALS Vial : 64 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
 Supervised By :mohammad ahmed 06/29/2024

Quant Time: Jun 29 01:22:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

06/29/2024
 Supervised By :mohammad
 ahmed

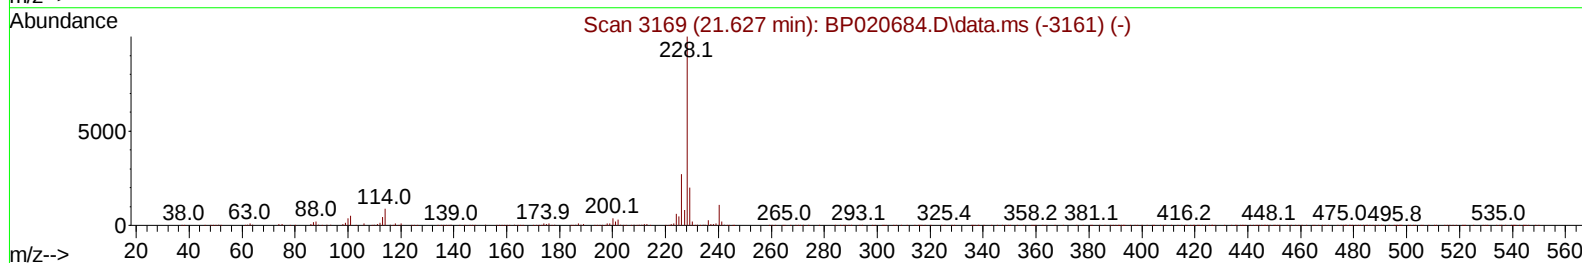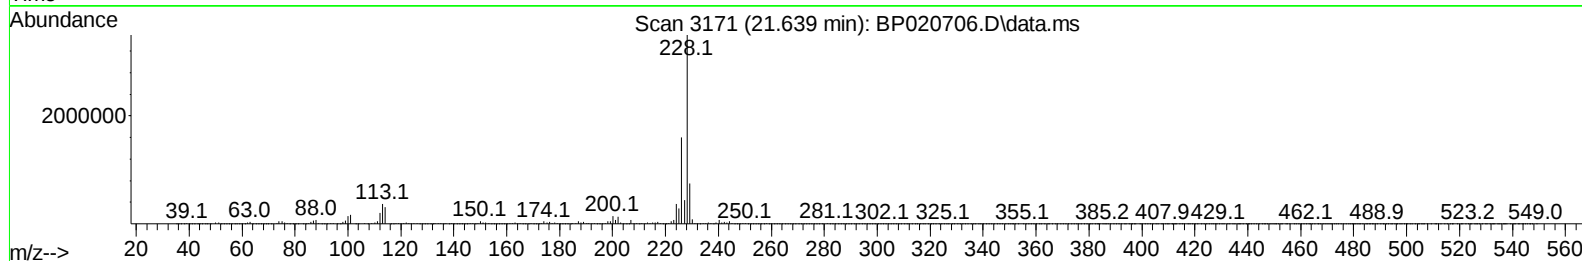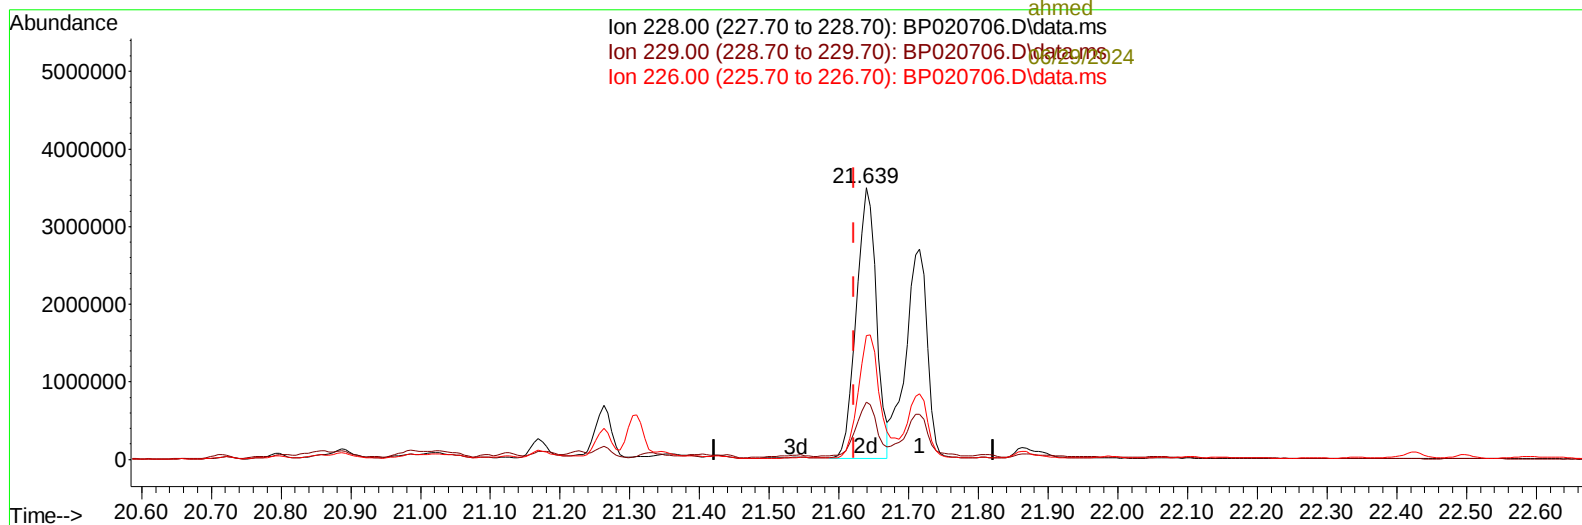

TIC: BP020706.D\data.ms

(85) Benzo(a)anthracene

21.639min (+ 0.018) 149.72 ng/ul m

response 6938844

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.00	21.23
226.00	26.40	45.62#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020706.D
 Acq On : 29 Jun 2024 00:51
 Operator : MA/JU
 Sample : P2897-14
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0T61




Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
 Supervised By :mohammad ahmed 06/29/2024

06/29/2024
 Supervised By :mohammad
 ahmed

Quant Time: Jun 29 01:23:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

Ion 252.00 (251.70 to 252.70): BP020706.D\data.ms
 Ion 253.00 (252.70 to 253.70): BP020706.D\data.ms
 Ion 125.00 (124.70 to 125.70): BP020706.D\data.ms

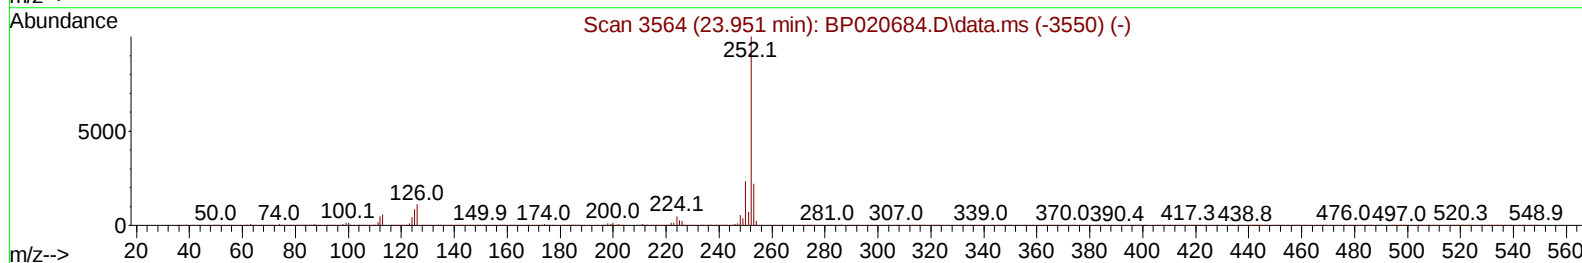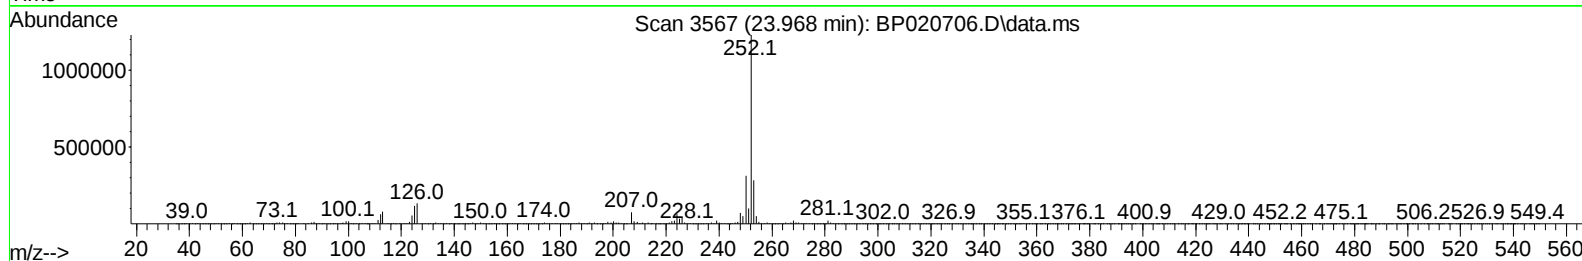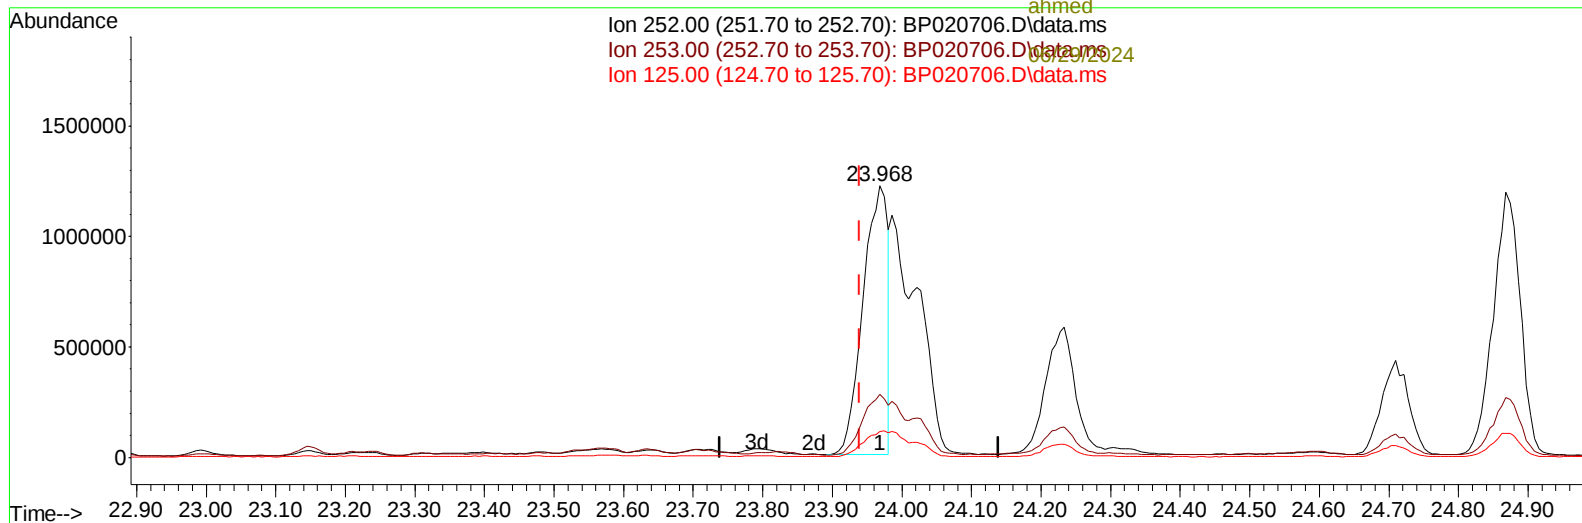

TIC: BP020706.D\data.ms

(90) Benzo(b)fluoranthene

23.968min (+ 0.029) 59.44 ng/u1

response 3004848

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.90	23.22
125.00	9.90	9.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020706.D
Acq On : 29 Jun 2024 00:51
Operator : MA/JU
Sample : P2897-14
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0T61




Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 06/29/2024

06/29/2024
Supervised By :mohammad
ahmed

Quant Time: Jun 29 01:23:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

Ion 252.00 (251.70 to 252.70): BP020706.D\data.ms
Ion 253.00 (252.70 to 253.70): BP020706.D\data.ms
Ion 125.00 (124.70 to 125.70): BP020706.D\data.ms

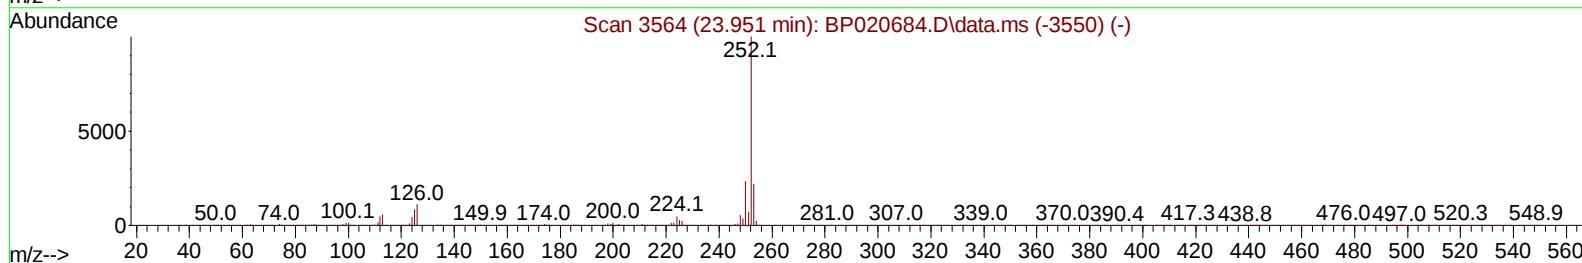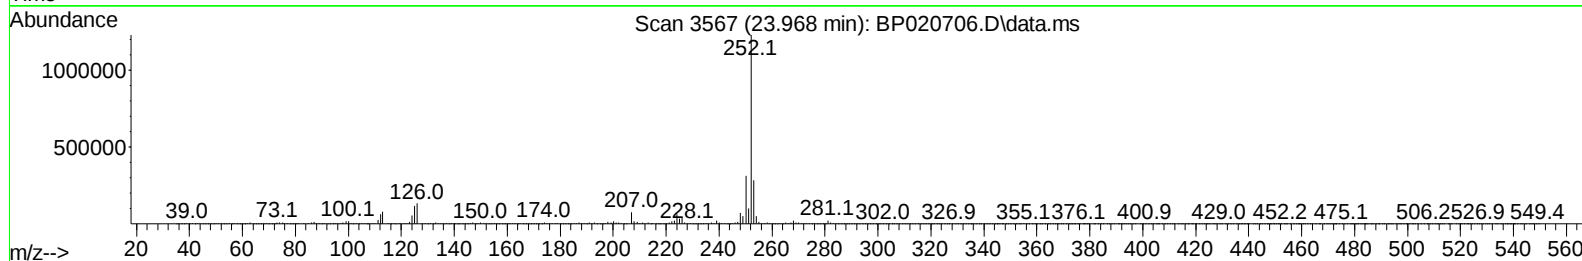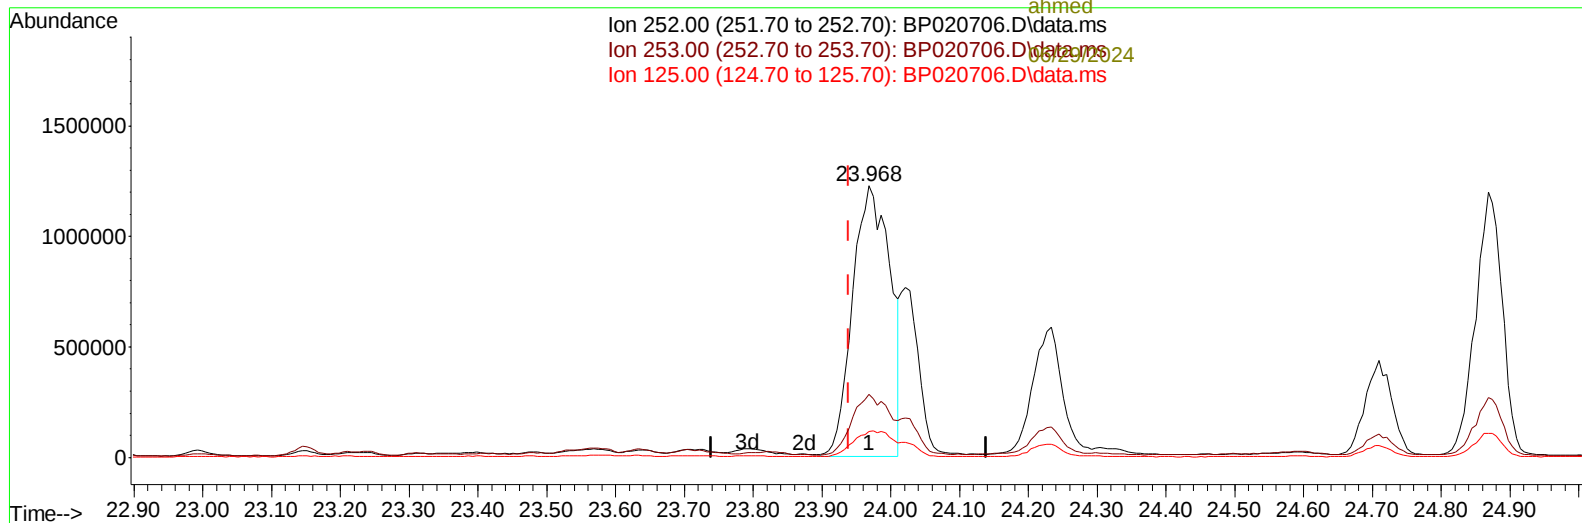

TIC: BP020706.D\data.ms

(90) Benzo(b)fluoranthene

23.968min (+ 0.029) 90.98 ng/ul m

response 4598983

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.90	23.22
125.00	9.90	9.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020706.D
Acq On : 29 Jun 2024 00:51
Operator : MA/JU
Sample : P2897-14
Misc :
ALS Vial : 64 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 06/29/2024

Quant Time: Jun 29 01:23:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

06/29/2024
Supervised By :mohammad
ahmed

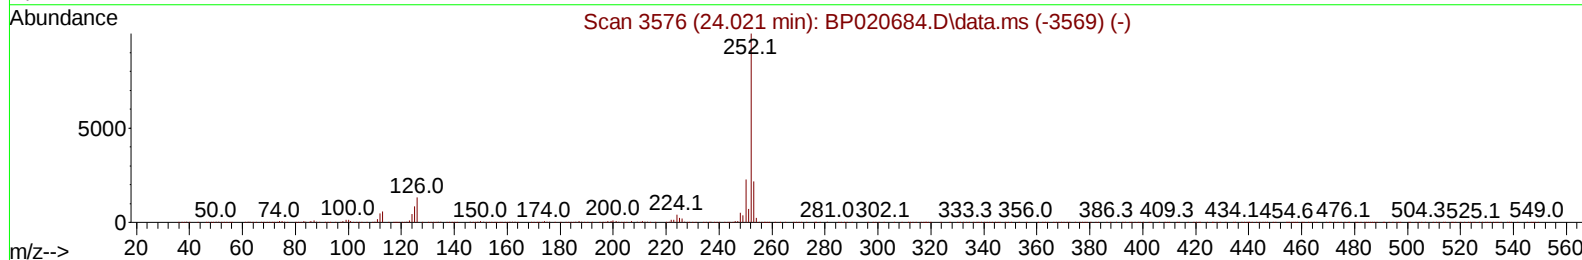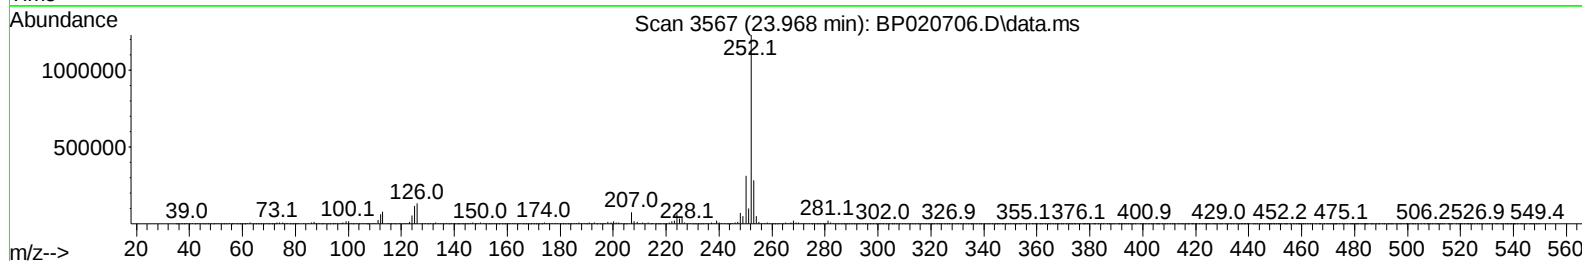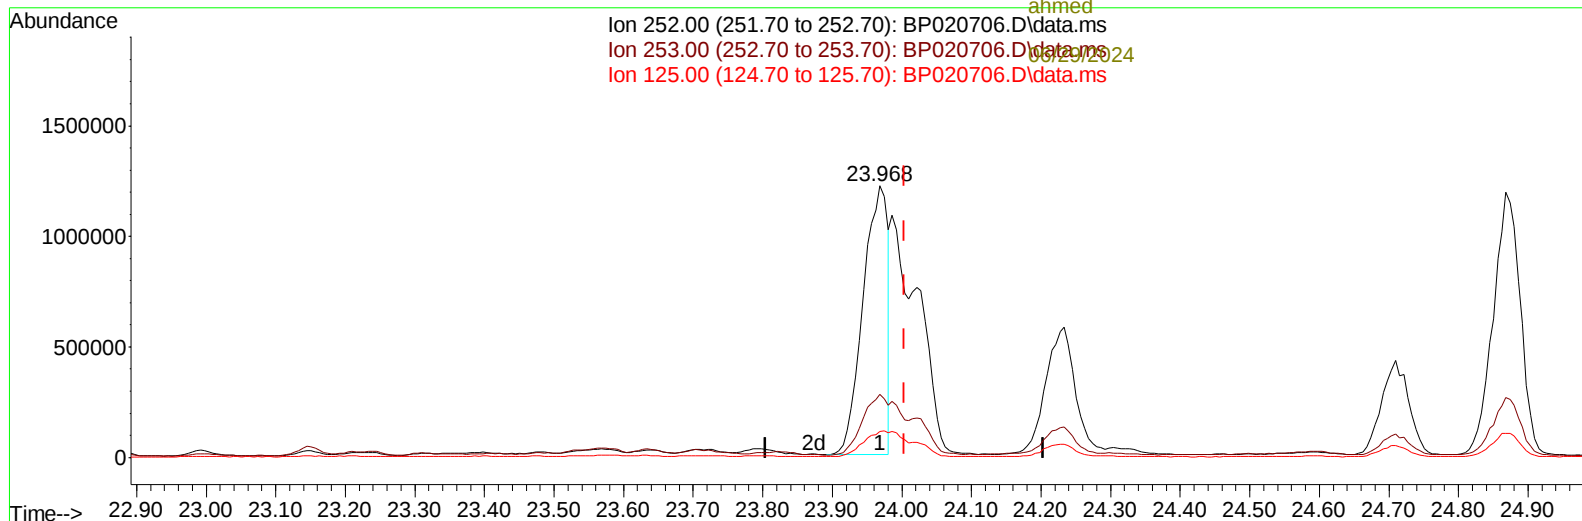

TIC: BP020706.D\data.ms

(91) Benzo(k)fluoranthene

23.968min (-0.035) 58.76 ng/u1

response 3004848

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.00	23.22
125.00	9.90	9.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020706.D
 Acq On : 29 Jun 2024 00:51
 Operator : MA/JU
 Sample : P2897-14
 Misc :
 ALS Vial : 64 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
 Supervised By :mohammad ahmed 06/29/2024

06/29/2024
 Supervised By :mohammad
 ahmed

Quant Time: Jun 29 01:23:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

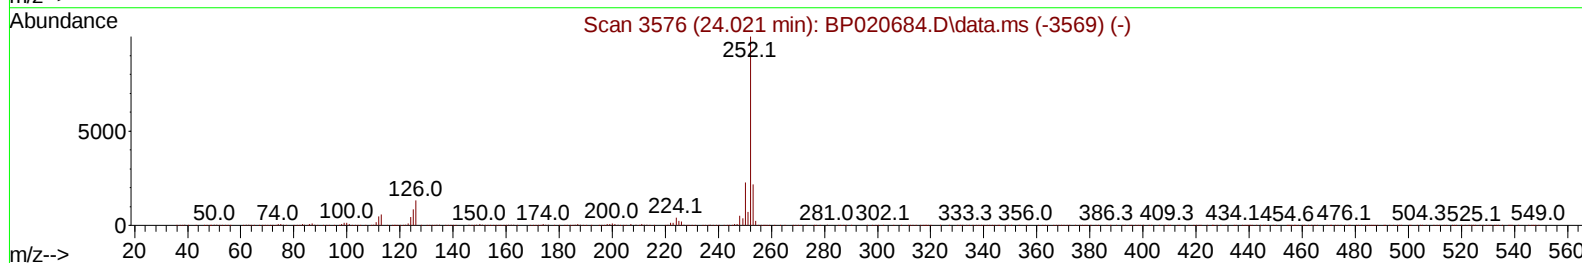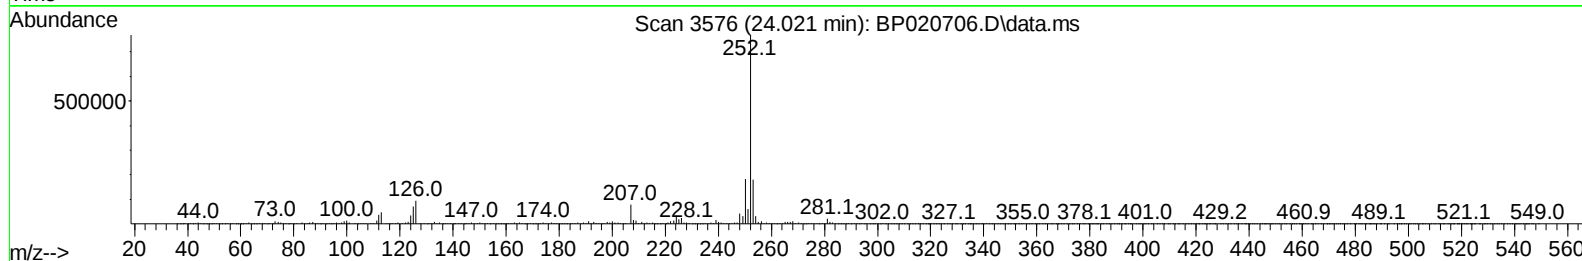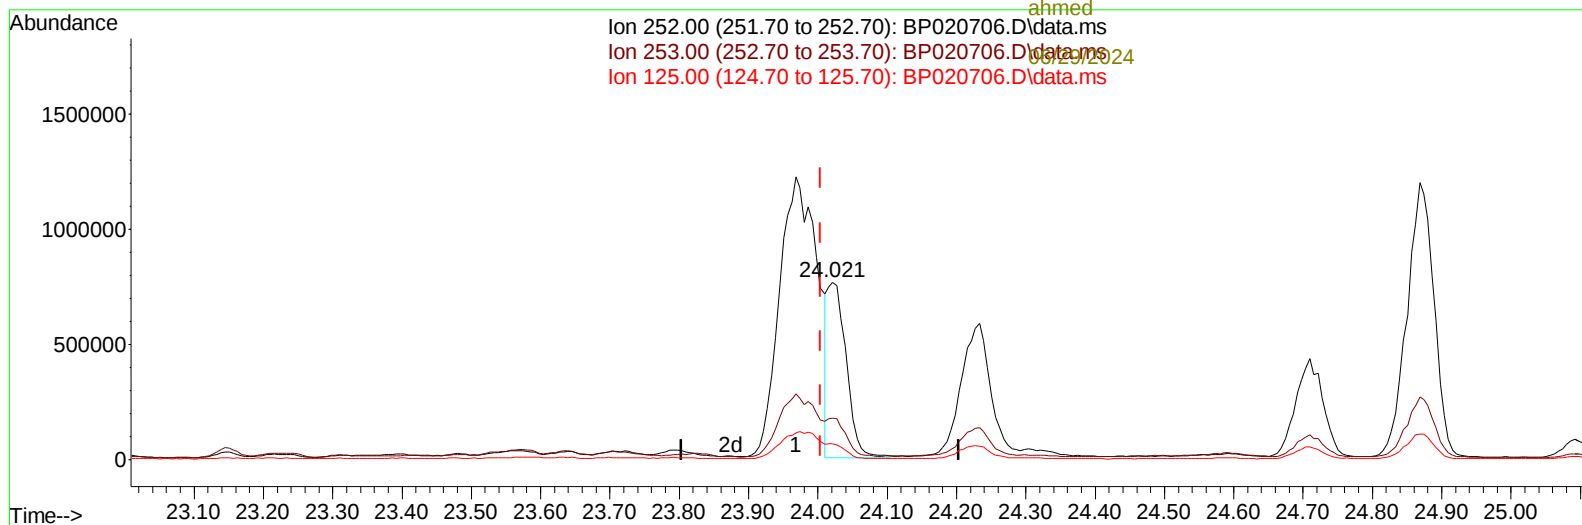

TIC: BP020706.D\data.ms

(91) Benzo(k)fluoranthene

24.021min (+ 0.018) 28.08 ng/ul m

response 1435919

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.00	23.26
125.00	9.90	9.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020706.D
Acq On : 29 Jun 2024 00:51
Operator : MA/JU
Sample : P2897-14
Misc :
ALS Vial : 64 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 06/29/2024

Quant Time: Jun 29 01:24:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

06/29/2024
Supervised By :mohammad
ahmed

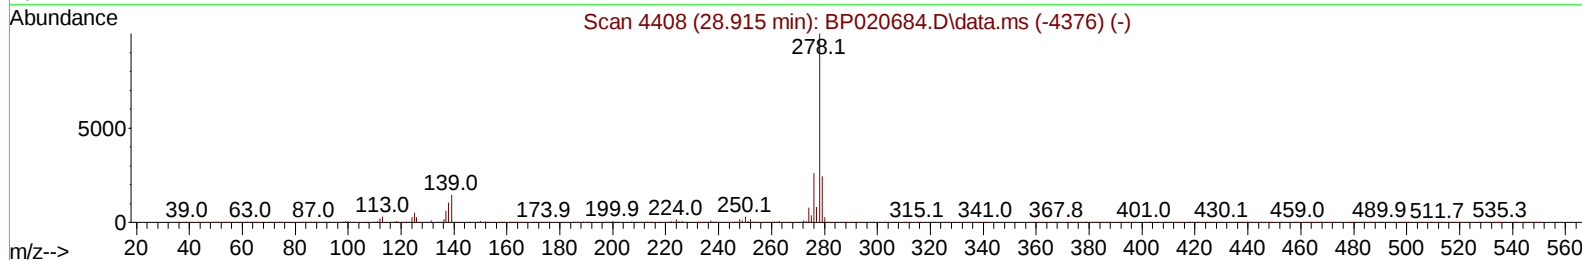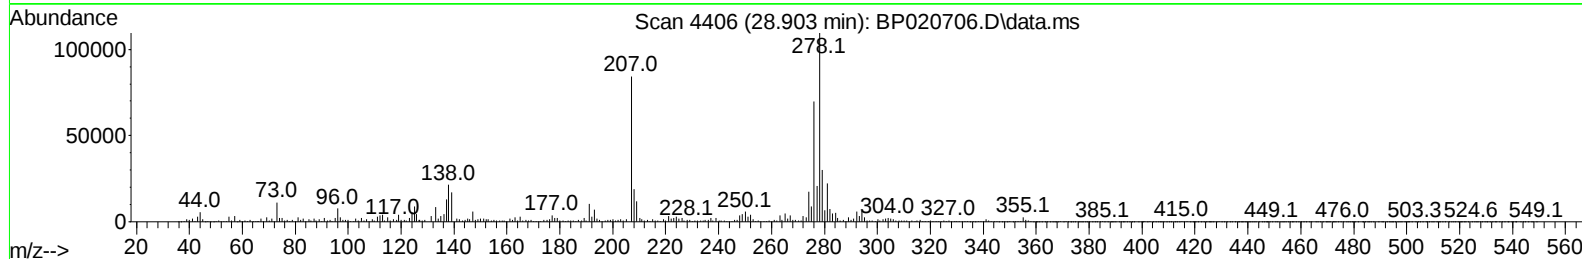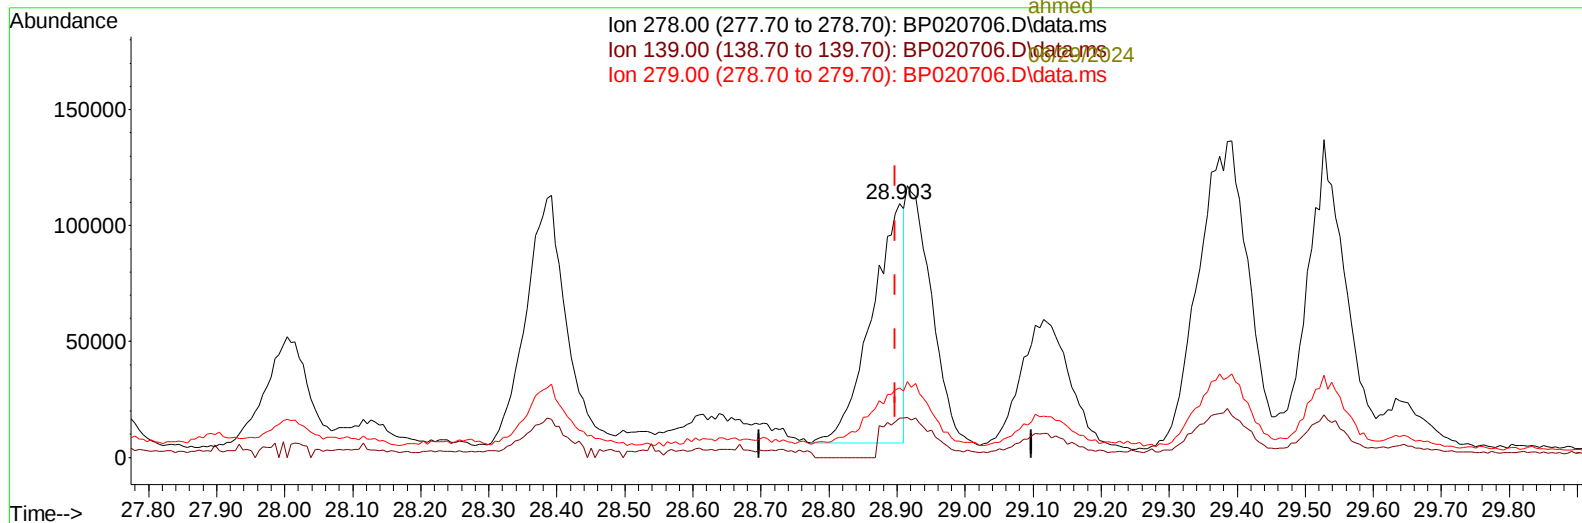

TIC: BP020706.D\data.ms

(95) Dibenzo(a,h)anthracene

28.903min (+ 0.006) 6.82 ng/u1

response 342938

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.90	15.56
279.00	23.40	27.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020706.D
Acq On : 29 Jun 2024 00:51
Operator : MA/JU
Sample : P2897-14
Misc :
ALS Vial : 64 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
C0T61

Quant Time: Jun 29 01:24:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 06/29/2024

06/29/2024
Supervised By :mohammad
ahmed

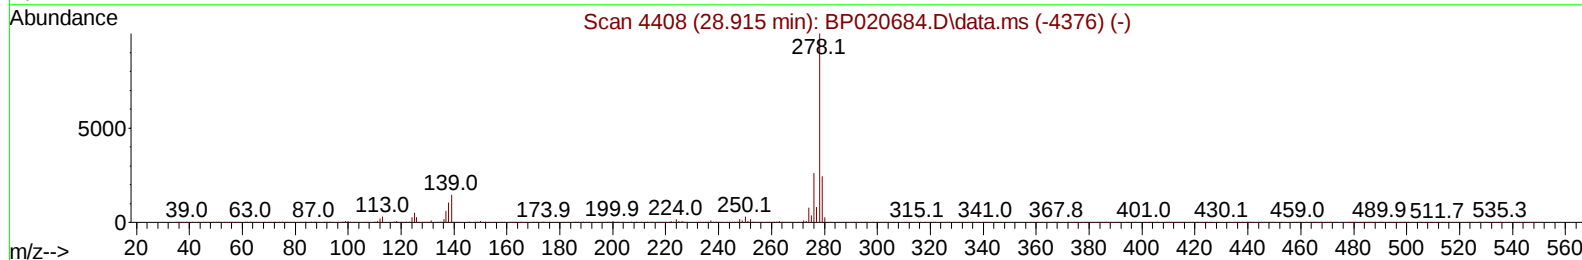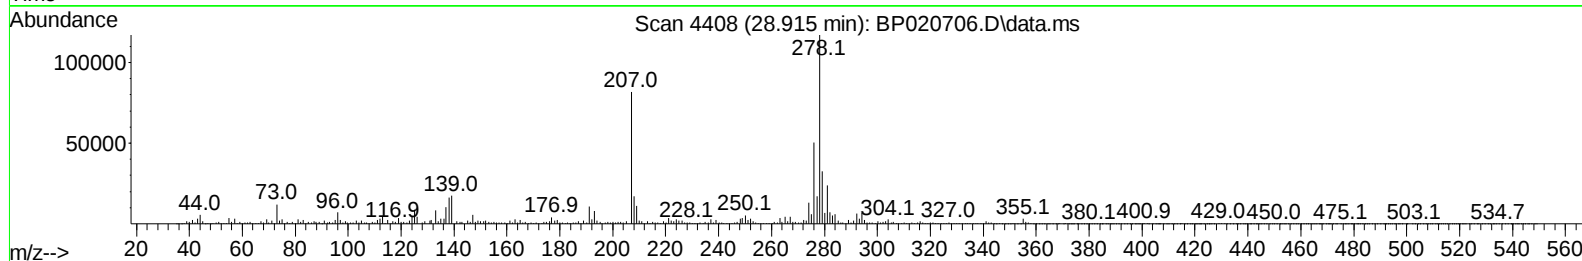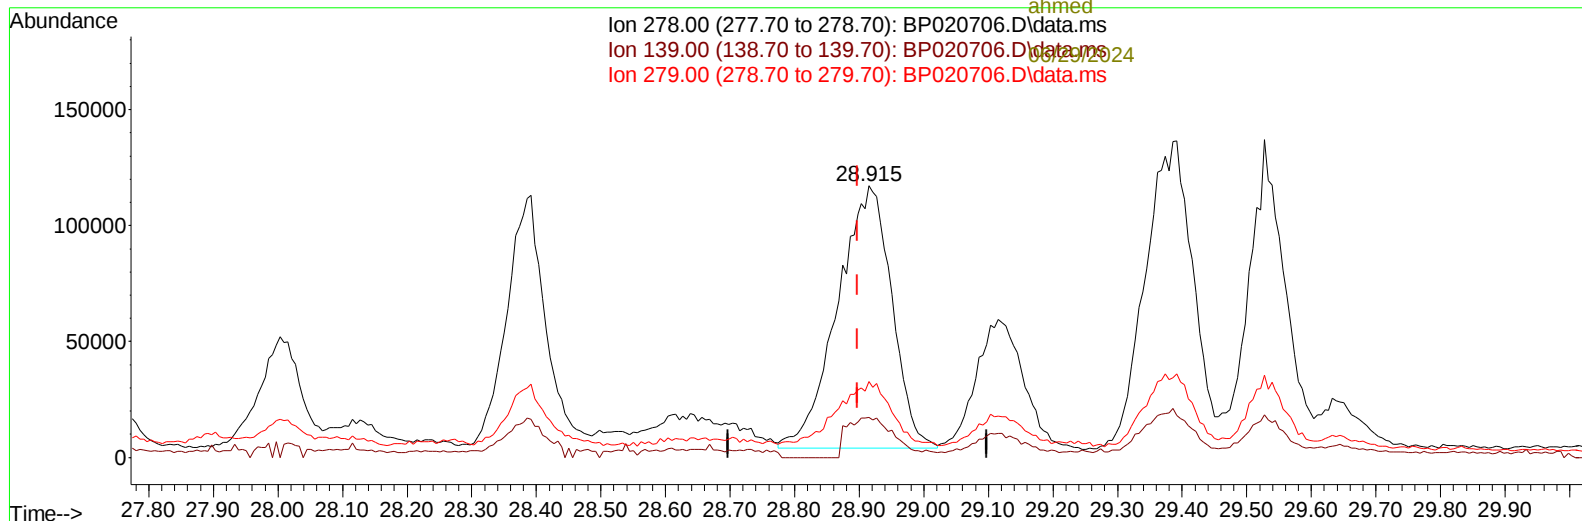

TIC: BP020706.D\data.ms

(95) Dibenzo(a,h)anthracene

28.915min (+ 0.018) 13.12 ng/ul m

response 660188

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.90	14.78
279.00	23.40	27.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020706.D
Acq On : 29 Jun 2024 00:51
Operator : MA/JU
Sample : P2897-14
Misc :
ALS Vial : 64 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
C0T61

Quant Time: Jun 29 01:24:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 06/29/2024

06/29/2024
Supervised By :mohammad
ahmed

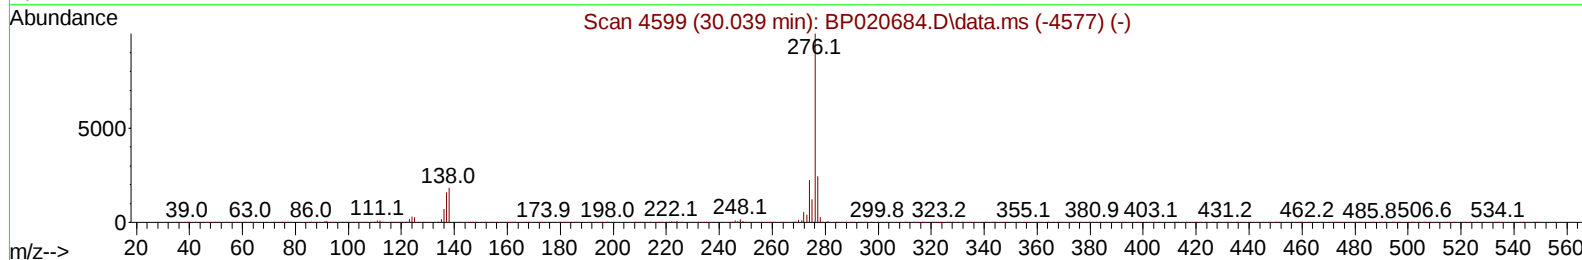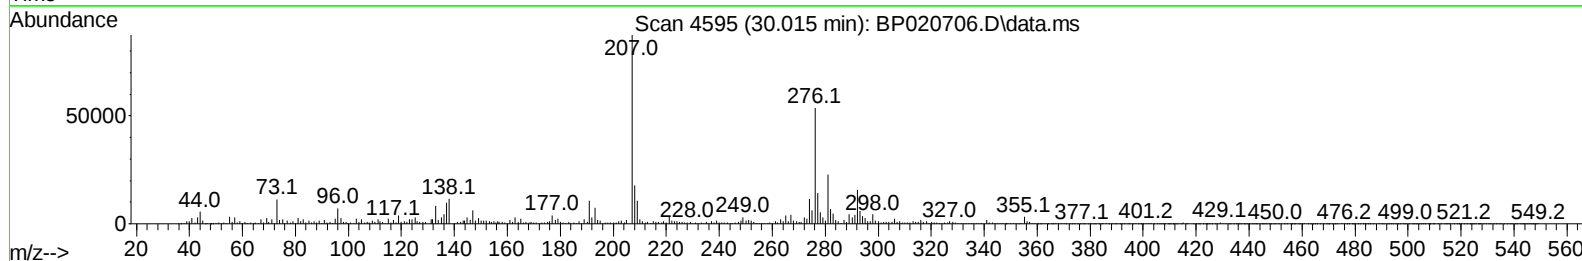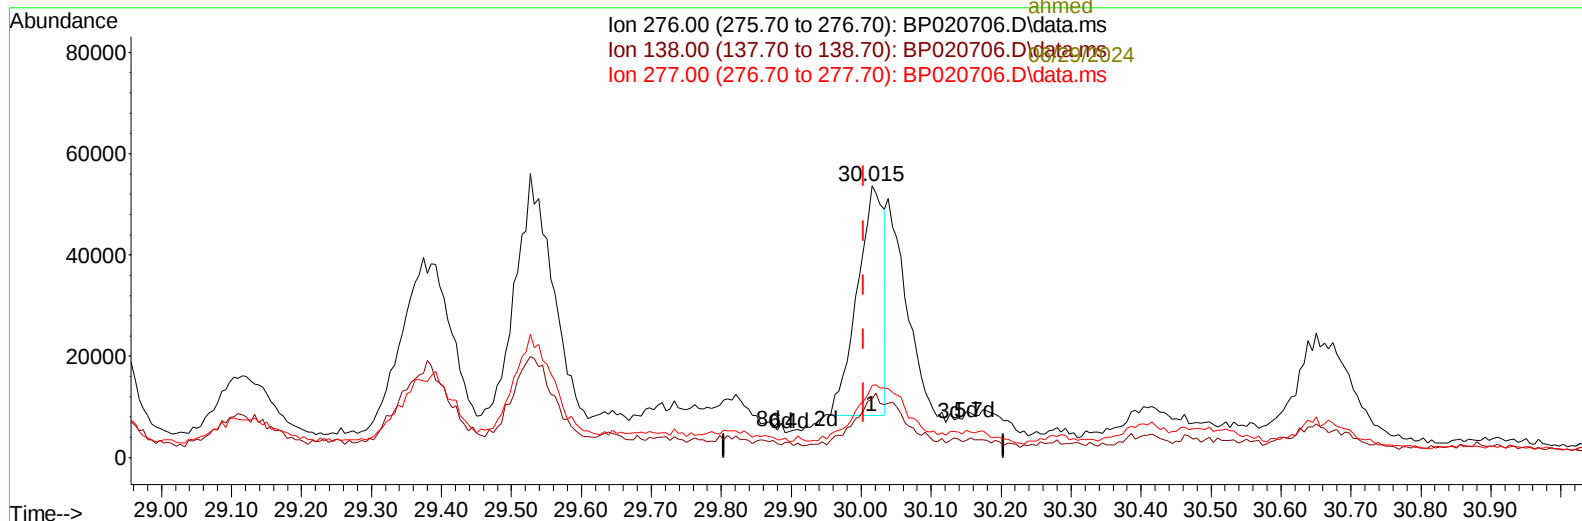

TIC: BP020706.D\data.ms

(96) Benzo(g,h,i)perylene**30.015min (+ 0.012) 2.38 ng/u1****response 118756**

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	20.50	21.52
277.00	23.40	26.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020706.D
Acq On : 29 Jun 2024 00:51
Operator : MA/JU
Sample : P2897-14
Misc :
ALS Vial : 64 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
C0T61

Quant Time: Jun 29 01:24:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 06/29/2024

06/29/2024
Supervised By :mohammad
ahmed

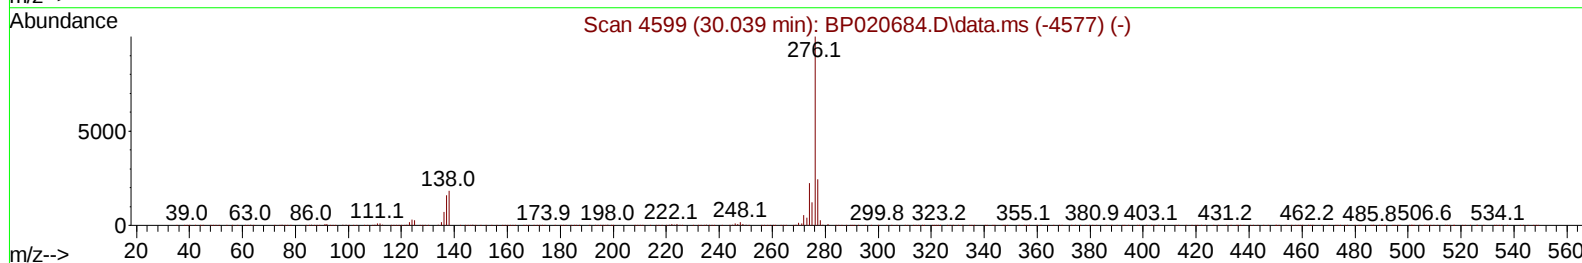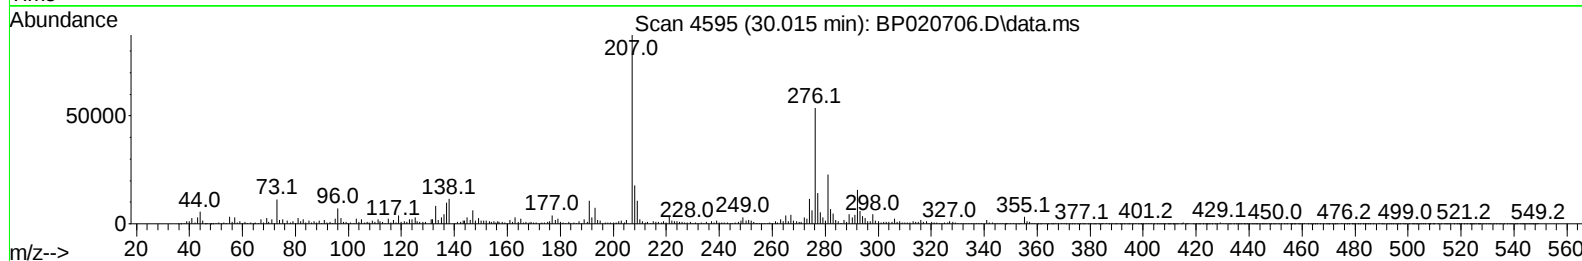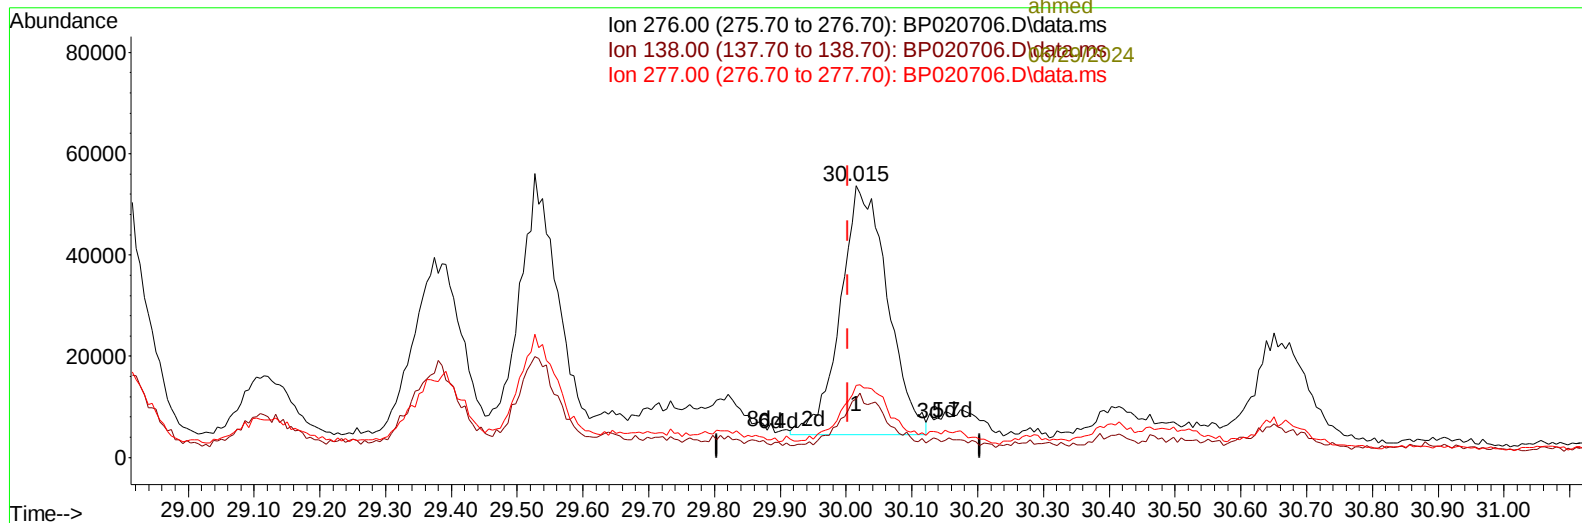

TIC: BP020706.D\data.ms

(96) Benzo(g,h,i)perylene

30.015min (+ 0.012) 4.89 ng/ul m

response 244150

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	20.50	21.52
277.00	23.40	26.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020706.D
 Acq On : 29 Jun 2024 00:51
 Operator : MA/JU
 Sample : P2897-14
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
 Supervised By :mohammad ahmed 06/29/2024

Quant Time: Jun 29 01:27:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

06/29/2024
 Supervised By :mohammad
 ahmed

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----06/29/2024						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.746	152	205739	20.000	ng/ul	0.00
20) Naphthalene-d8	10.546	136	788260	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.387	164	583927	20.000	ng/ul	0.02
64) Phenanthrene-d10	17.204	188	895482	20.000	ng/ul	0.02
79) Chrysene-d12	21.663	240	661226	20.000	ng/ul	0.02
88) Perylene-d12	25.015	264	834414	20.000	ng/ul	# 0.02

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	21582	4.505	ng/uL	0.00
4) Pyridine-d5	3.693	84	74486	5.334	ng/ul	0.00
7) Phenol-d5	6.922	99	460981	27.318	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.087	67	295035	27.579	ng/ul	0.00
11) 2-Chlorophenol-d4	7.281	132	396871	28.777	ng/ul	0.00
15) 4-Methylphenol-d8	8.446	113	382608	27.917	ng/ul	0.00
21) Nitrobenzene-d5	8.893	128	212734	36.554	ng/ul	0.00
24) 2-Nitrophenol-d4	9.610	143	226883	38.957	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.151	165	392410	32.710	ng/ul	0.01
31) 4-Chloroaniline-d4	10.663	131	359253	21.369	ng/ul	0.01
46) Dimethylphthalate-d6	13.792	166	1238979	30.517	ng/ul	0.01
49) Acenaphthylene-d8	14.081	160	1357428	28.020	ng/ul	0.02
54) 4-Nitrophenol-d4	14.604	143	137800	22.214	ng/ul	0.01
60) Fluorene-d10	15.398	176	941625	27.562	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.551	200	30099m	6.670	ng/ul	0.05
73) Anthracene-d10	17.304	188	1311209	32.626	ng/ul	0.02
81) Pyrene-d10	19.686	212	1079234	27.168	ng/ul	0.02
92) Benzo(a)pyrene-d12	24.798	264	892002	21.976	ng/ul	0.04

Target Compounds				Qvalue		
30) Naphthalene	10.587	128	41376394m	980.695	ng/ul	
36) 2-Methylnaphthalene	12.216	142	27012116	955.766	ng/ul	99
37) 1-Methylnaphthalene	12.440	142	17149409	593.574	ng/ul	99
43) 1,1'-Biphenyl	13.204	154	5251312	120.250	ng/ul	98
50) Acenaphthylene	14.110	152	4375234	79.952	ng/ul#	90
52) Acenaphthene	14.469	153	12459503	343.228	ng/ul	98
56) Dibenzofuran	14.787	168	1513493	30.941	ng/ul	94
61) Fluorene	15.463	166	9923178	252.484	ng/ul	98
72) Phenanthrene	17.251	178	25191311m	537.216	ng/ul	
74) Anthracene	17.345	178	10415647	215.936	ng/ul	97
77) Carbazole	17.616	167	251204	6.310	ng/ul#	79
80) Fluoranthene	19.345	202	12213565	251.708	ng/ul	98
82) Pyrene	19.727	202	14298273	287.323	ng/ul	99
85) Benzo(a)anthracene	21.639	228	6938844m	149.716	ng/ul	
87) Chrysene	21.716	228	5823517	132.934	ng/ul	97
90) Benzo(b)fluoranthene	23.968	252	4598983m	90.979	ng/ul	
91) Benzo(k)fluoranthene	24.021	252	1435919m	28.082	ng/ul	
93) Benzo(a)pyrene	24.868	252	3230904	67.708	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	28.851	276	1571315	25.672	ng/ul	98
95) Dibenzo(a,h)anthracene	28.915	278	660188m	13.124	ng/ul	
96) Benzo(g,h,i)perylene	30.015	276	244150m	4.886	ng/ul	

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020706.D
Acq On : 29 Jun 2024 00:51
Operator : MA/JU
Sample : P2897-14
Misc :
ALS Vial : 64 Sample Multiplier: 1

Quant Time: Jun 29 01:27:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

Instrument :
BNA_P
ClientSampleId :
C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 06/29/2024

06/29/2024
Supervised By :mohammad
ahmed

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
----------	------	---	-----	----------	------	-------	----------

-----06/29/2024

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020706.D
Acq On : 29 Jun 2024 00:51
Operator : MA/JU
Sample : P2897-14
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0T61

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 06/29/2024

06/29/2024
Supervised By :mohammad
ahmed

06/29/2024

Quant Time: Jun 29 01:27:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

