

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020667.D
 Acq On : 27 Jun 2024 18:47
 Operator : MA/JU
 Sample : P2909-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4CP2

Quant Time: Jun 27 22:39:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.740	152	201468	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.522	136	814682	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.387	164	507598	20.000	ng/ul	0.02
64) Phenanthrene-d10	17.192	188	945870	20.000	ng/ul	0.00
79) Chrysene-d12	21.651	240	703022	20.000	ng/ul	0.01
88) Perylene-d12	25.004	264	878640	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	17517	3.734	ng/uL	0.00
4) Pyridine-d5	3.693	84	45691	3.342	ng/ul	0.00
7) Phenol-d5	6.928	99	405496	24.540	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.087	67	255100	24.352	ng/ul	0.00
11) 2-Chlorophenol-d4	7.287	132	344927	25.541	ng/ul	0.00
15) 4-Methylphenol-d8	8.440	113	311974	23.246	ng/ul	0.00
21) Nitrobenzene-d5	8.893	128	166339	27.655	ng/ul	0.00
24) 2-Nitrophenol-d4	9.604	143	185307	30.786	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.146	165	327961	26.451	ng/ul	0.00
31) 4-Chloroaniline-d4	10.657	131	189400	10.900	ng/ul	0.00
46) Dimethylphthalate-d6	13.787	166	985976	27.937	ng/ul	0.00
49) Acenaphthylene-d8	14.075	160	1083375	25.725	ng/ul	0.01
54) 4-Nitrophenol-d4	14.598	143	123560	22.914	ng/ul	0.00
60) Fluorene-d10	15.392	176	794468	26.751	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	119893	25.152	ng/ul	0.02
73) Anthracene-d10	17.292	188	1117321	26.320	ng/ul	0.01
81) Pyrene-d10	19.674	212	1119591	26.509	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.774	264	860140	20.125	ng/ul	0.01
Target Compounds						
80) Fluoranthene	19.327	202	63976	1.240	ng/ul#	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020667.D
Acq On : 27 Jun 2024 18:47
Operator : MA/JU
Sample : P2909-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4CP2

Quant Time: Jun 27 22:39:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

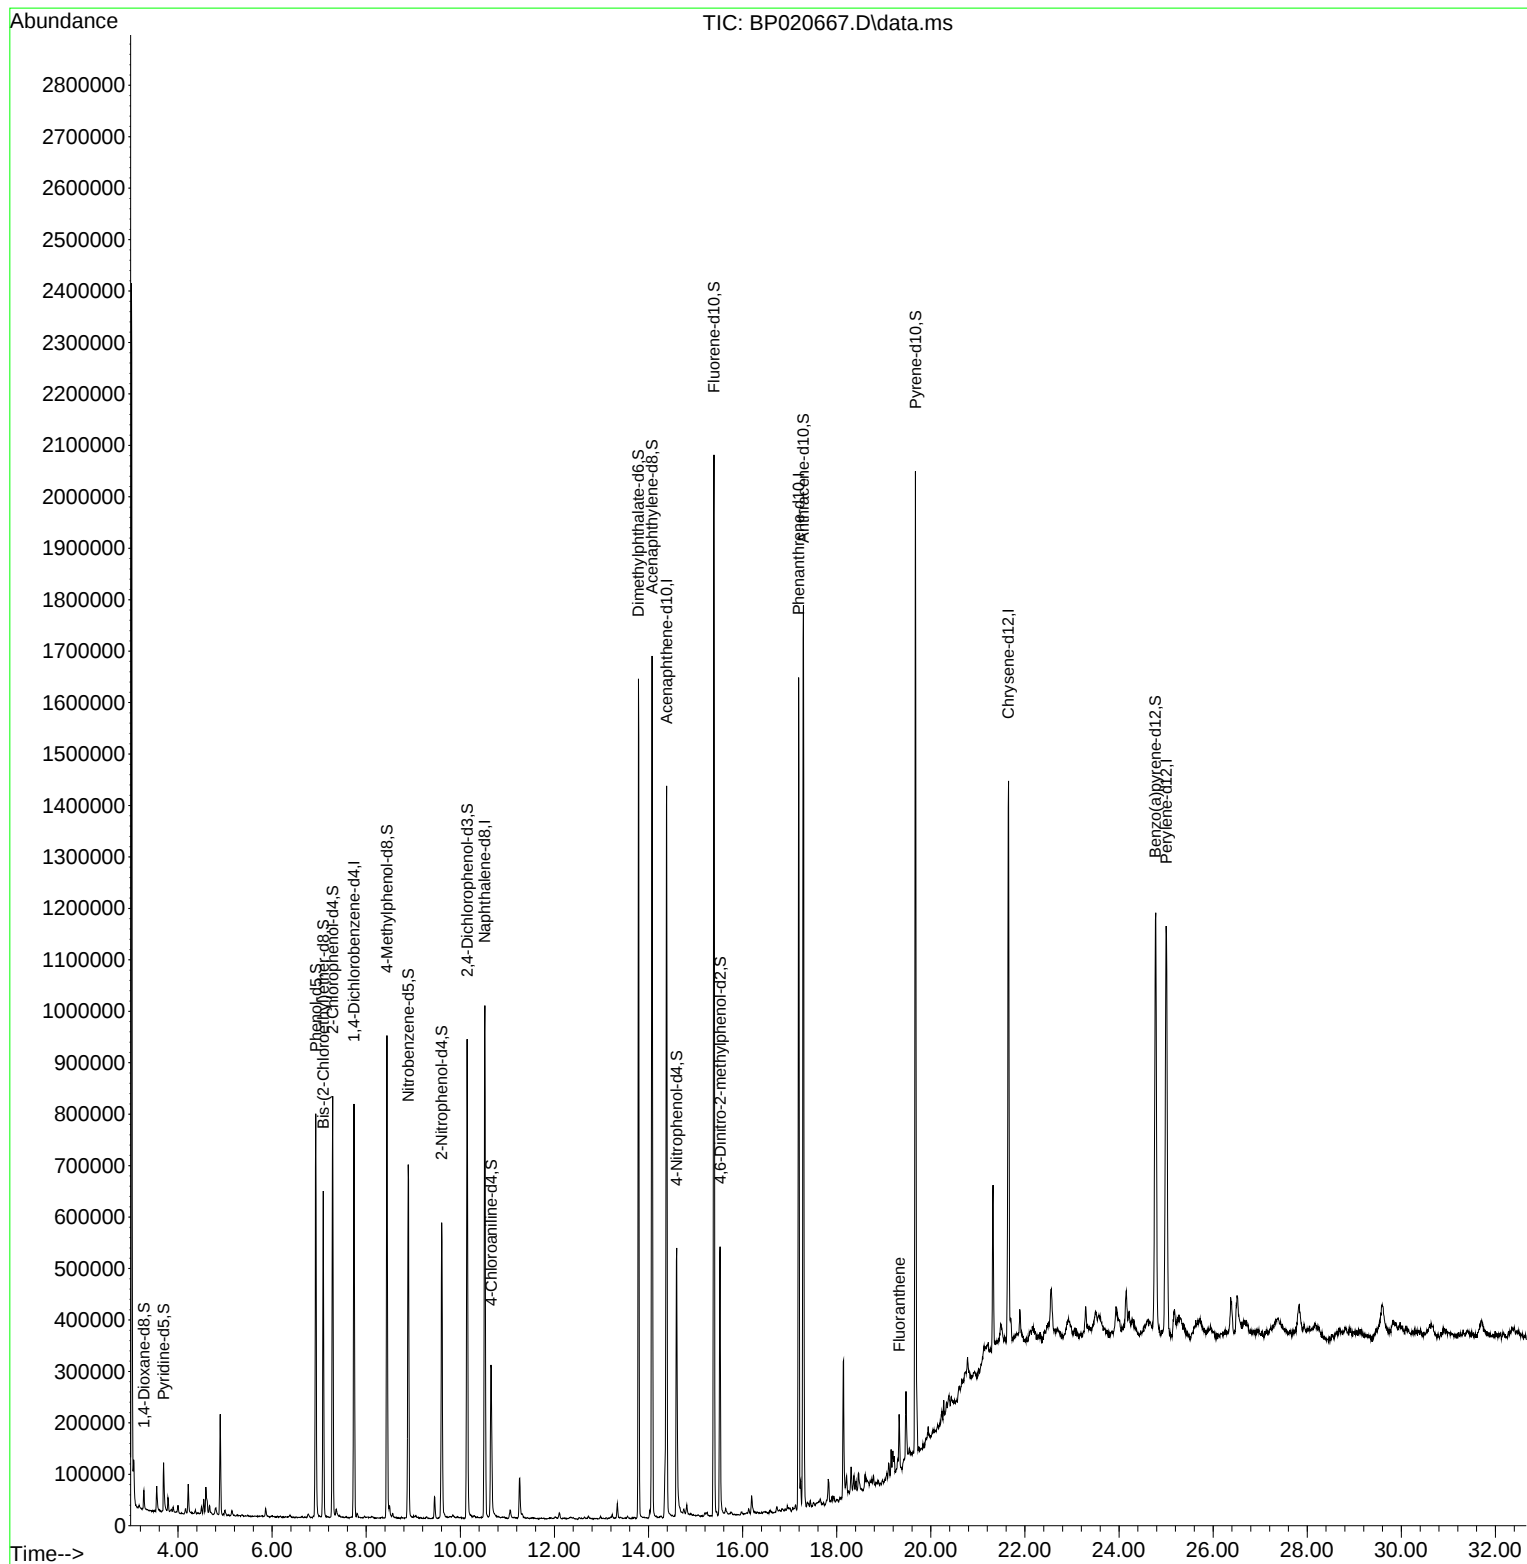

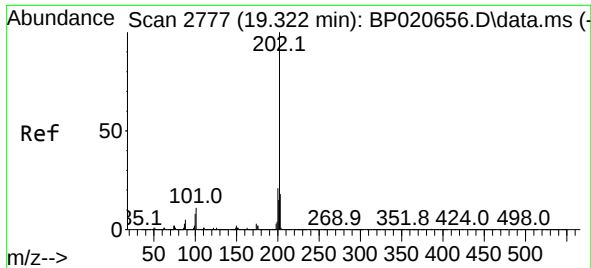

#80
 Fluoranthene
 Concen: 1.240 ng/ul
 RT: 19.327 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP020667.D
 Acq: 27 Jun 2024 18:47

Instrument :
 BNA_P
 ClientSampleId :
 A4CP2

Tgt Ion:202 Resp: 63976
 Ion Ratio Lower Upper
 202 100
 101 12.5 8.2 12.4#
 100 7.9 6.6 10.0

