

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020681.D
 Acq On : 28 Jun 2024 05:32
 Operator : MA/JU
 Sample : P2898-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1GC2

Quant Time: Jun 28 05:58:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.751	152	221168	20.000	ng/u1	0.00
20) Naphthalene-d8	10.516	136	875851	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.380	164	526021	20.000	ng/u1	0.01
64) Phenanthrene-d10	17.198	188	967128	20.000	ng/u1	0.01
79) Chrysene-d12	21.656	240	840619	20.000	ng/u1	0.02
88) Perylene-d12	25.039	264	1002484	20.000	ng/u1	0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	20636	4.007	ng/uL	0.00
4) Pyridine-d5	3.693	84	55346	3.687	ng/u1	0.00
7) Phenol-d5	6.928	99	114338	6.303	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.093	67	388661	33.797	ng/u1	0.00
11) 2-Chlorophenol-d4	7.287	132	376048	25.365	ng/u1	0.00
15) 4-Methylphenol-d8	8.451	113	236234	16.035	ng/u1	0.00
21) Nitrobenzene-d5	8.898	128	261786	40.484	ng/u1	0.00
24) 2-Nitrophenol-d4	9.616	143	267433	41.327	ng/u1	0.01
28) 2,4-Dichlorophenol-d3	10.139	165	437658	32.834	ng/u1	0.00
31) 4-Chloroaniline-d4	10.663	131	461470	24.703	ng/u1	0.01
46) Dimethylphthalate-d6	13.786	166	1670100	45.664	ng/u1	0.00
49) Acenaphthylene-d8	14.069	160	1764182	40.424	ng/u1	0.00
54) 4-Nitrophenol-d4	14.616	143	29658	5.307	ng/u1	0.02
60) Fluorene-d10	15.398	176	1304221	42.377	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.527	200	177837	36.489	ng/u1	0.02
73) Anthracene-d10	17.304	188	1919327	44.219	ng/u1	0.02
81) Pyrene-d10	19.686	212	2099619	41.576	ng/u1	0.02
92) Benzo(a)pyrene-d12	24.797	264	2270374	46.558	ng/u1	0.03
Target Compounds						
					Qvalue	
16) Acetophenone	8.563	105	25520	1.085	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020681.D
Acq On : 28 Jun 2024 05:32
Operator : MA/JU
Sample : P2898-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1GC2


Quant Time: Jun 28 05:58:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

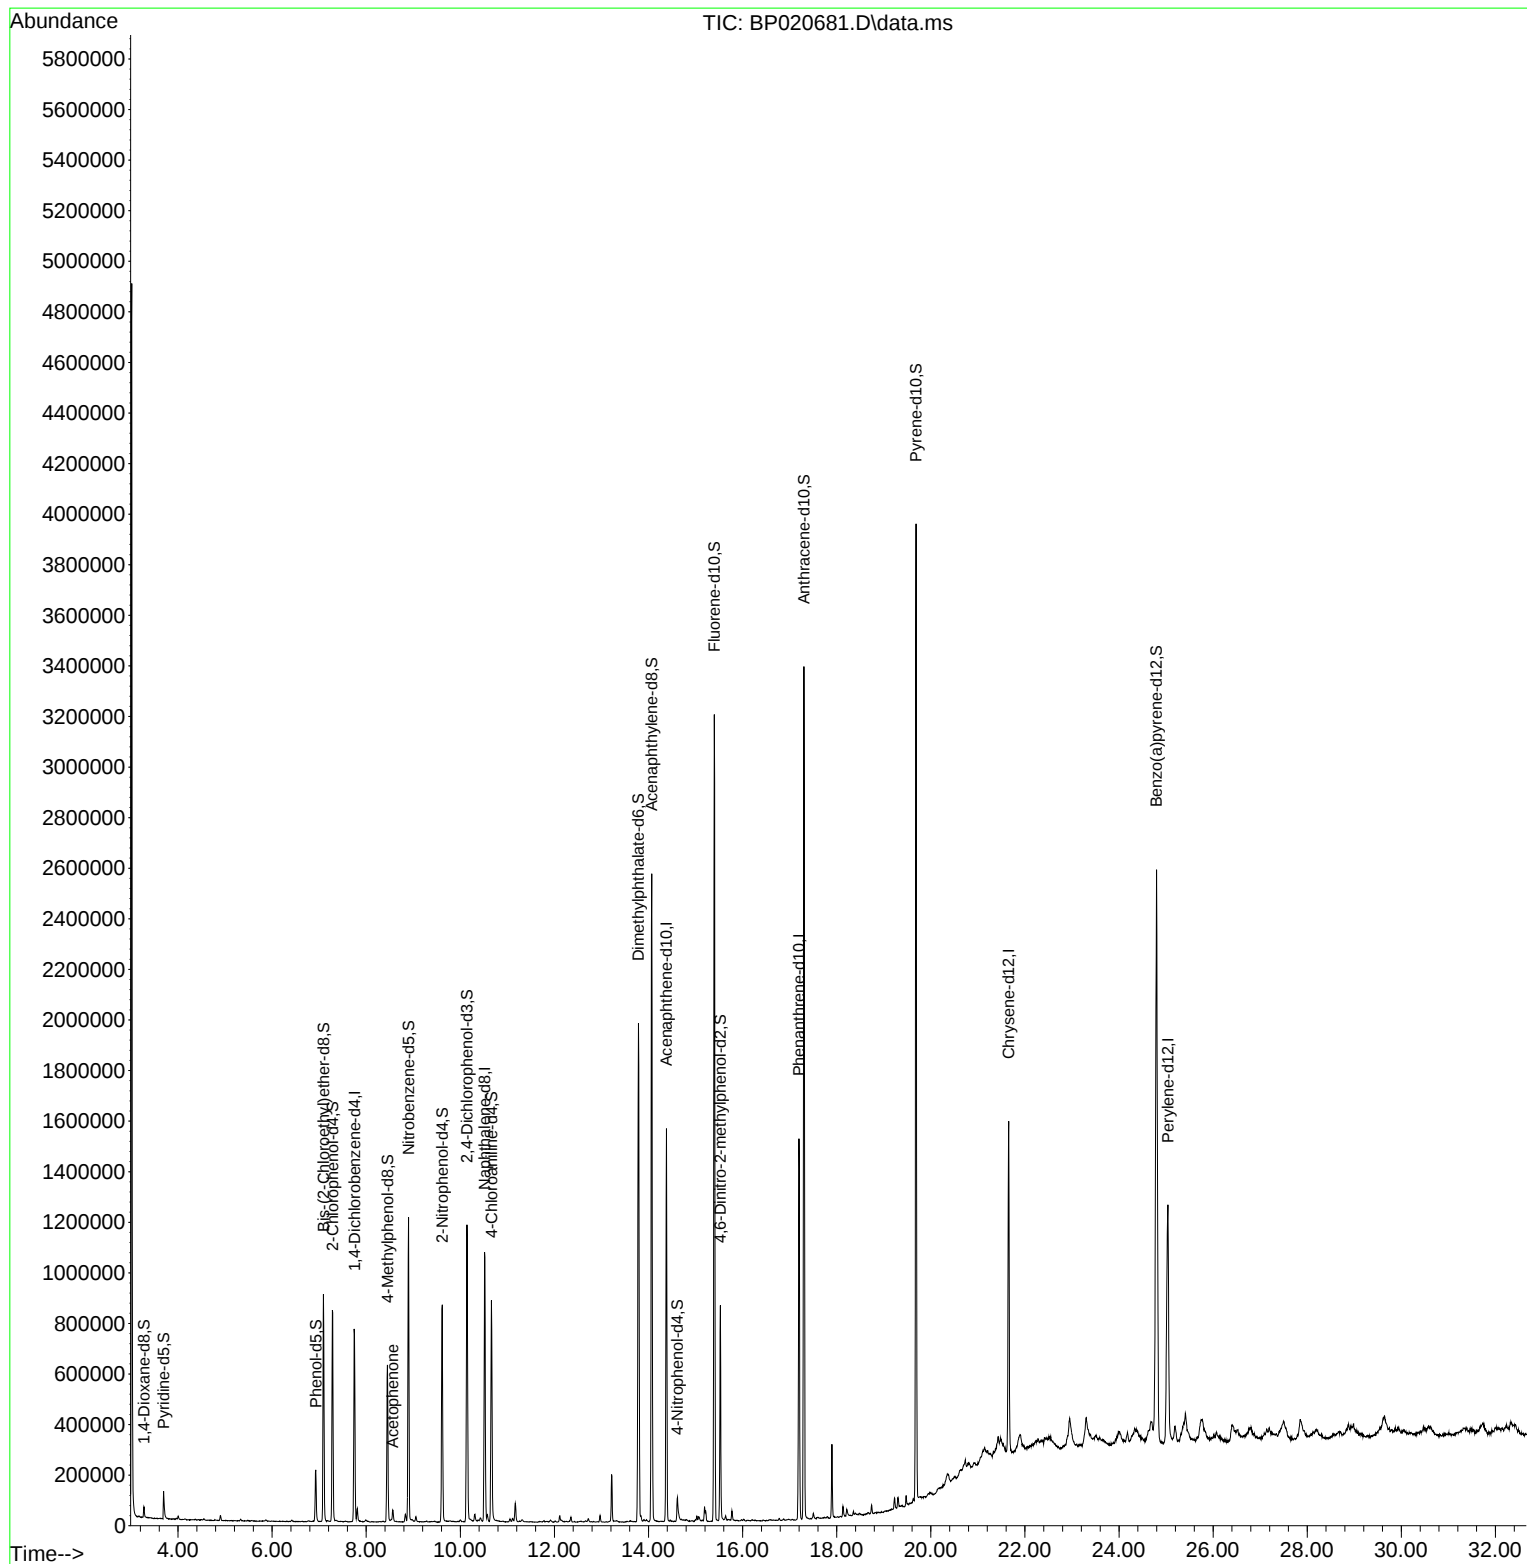

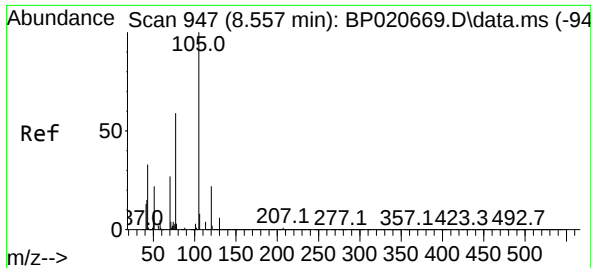

#16
 Acetophenone
 Concen: 1.085 ng/ul
 RT: 8.563 min Scan# 94
 Delta R.T. -0.000 min
 Lab File: BP020681.D
 Acq: 28 Jun 2024 05:32

Instrument :
 BNA_P
 ClientSampleId :
 E1GC2

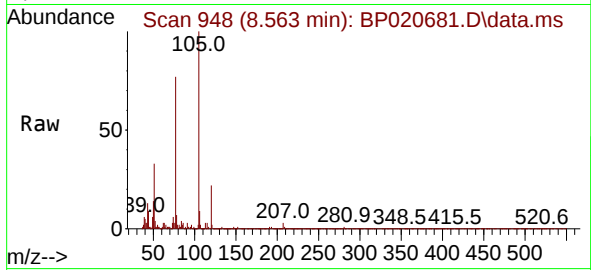

Tgt Ion:	105	Resp:	25520
Ion Ratio	Lower	Upper	
105	100		
77	76.7	62.2	93.4
51	33.3	23.6	35.4

