

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020682.D
 Acq On : 28 Jun 2024 06:15
 Operator : MA/JU
 Sample : P2898-05
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1G83

Quant Time: Jun 28 06:41:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 25 18:30:06 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.746	152	220877	20.000	ng/u1	0.00
20) Naphthalene-d8	10.522	136	890647	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.375	164	548983	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	966793	20.000	ng/u1	0.01
79) Chrysene-d12	21.657	240	842725	20.000	ng/u1	0.02
88) Perylene-d12	25.033	264	1013641	20.000	ng/u1	0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	25865	5.028	ng/uL	0.00
4) Pyridine-d5	3.687	84	165448	11.037	ng/u1	0.00
7) Phenol-d5	6.928	99	175812	9.705	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.093	67	448713	39.070	ng/u1	0.00
11) 2-Chlorophenol-d4	7.287	132	486847	32.882	ng/u1	0.00
15) 4-Methylphenol-d8	8.446	113	324655	22.065	ng/u1	0.00
21) Nitrobenzene-d5	8.899	128	304515	46.310	ng/u1	0.00
24) 2-Nitrophenol-d4	9.616	143	332699	50.559	ng/u1	0.01
28) 2,4-Dichlorophenol-d3	10.140	165	538510	39.729	ng/u1	0.00
31) 4-Chloroaniline-d4	10.663	131	673838	35.473	ng/u1	0.01
46) Dimethylphthalate-d6	13.793	166	1812682	47.489	ng/u1	0.01
49) Acenaphthylene-d8	14.063	160	1917178	42.093	ng/u1	0.00
54) 4-Nitrophenol-d4	14.610	143	51855	8.891	ng/u1	0.02
60) Fluorene-d10	15.398	176	1429133	44.494	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.528	200	214560	44.039	ng/u1	0.02
73) Anthracene-d10	17.304	188	1984574	45.738	ng/u1	0.02
81) Pyrene-d10	19.686	212	2104937	41.577	ng/u1	0.02
92) Benzo(a)pyrene-d12	24.804	264	2371537	48.097	ng/u1	0.04
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.580	149	49778	1.361	ng/u1#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020682.D
Acq On : 28 Jun 2024 06:15
Operator : MA/JU
Sample : P2898-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1G83

Quant Time: Jun 28 06:41:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 25 18:30:06 2024
Response via : Initial Calibration

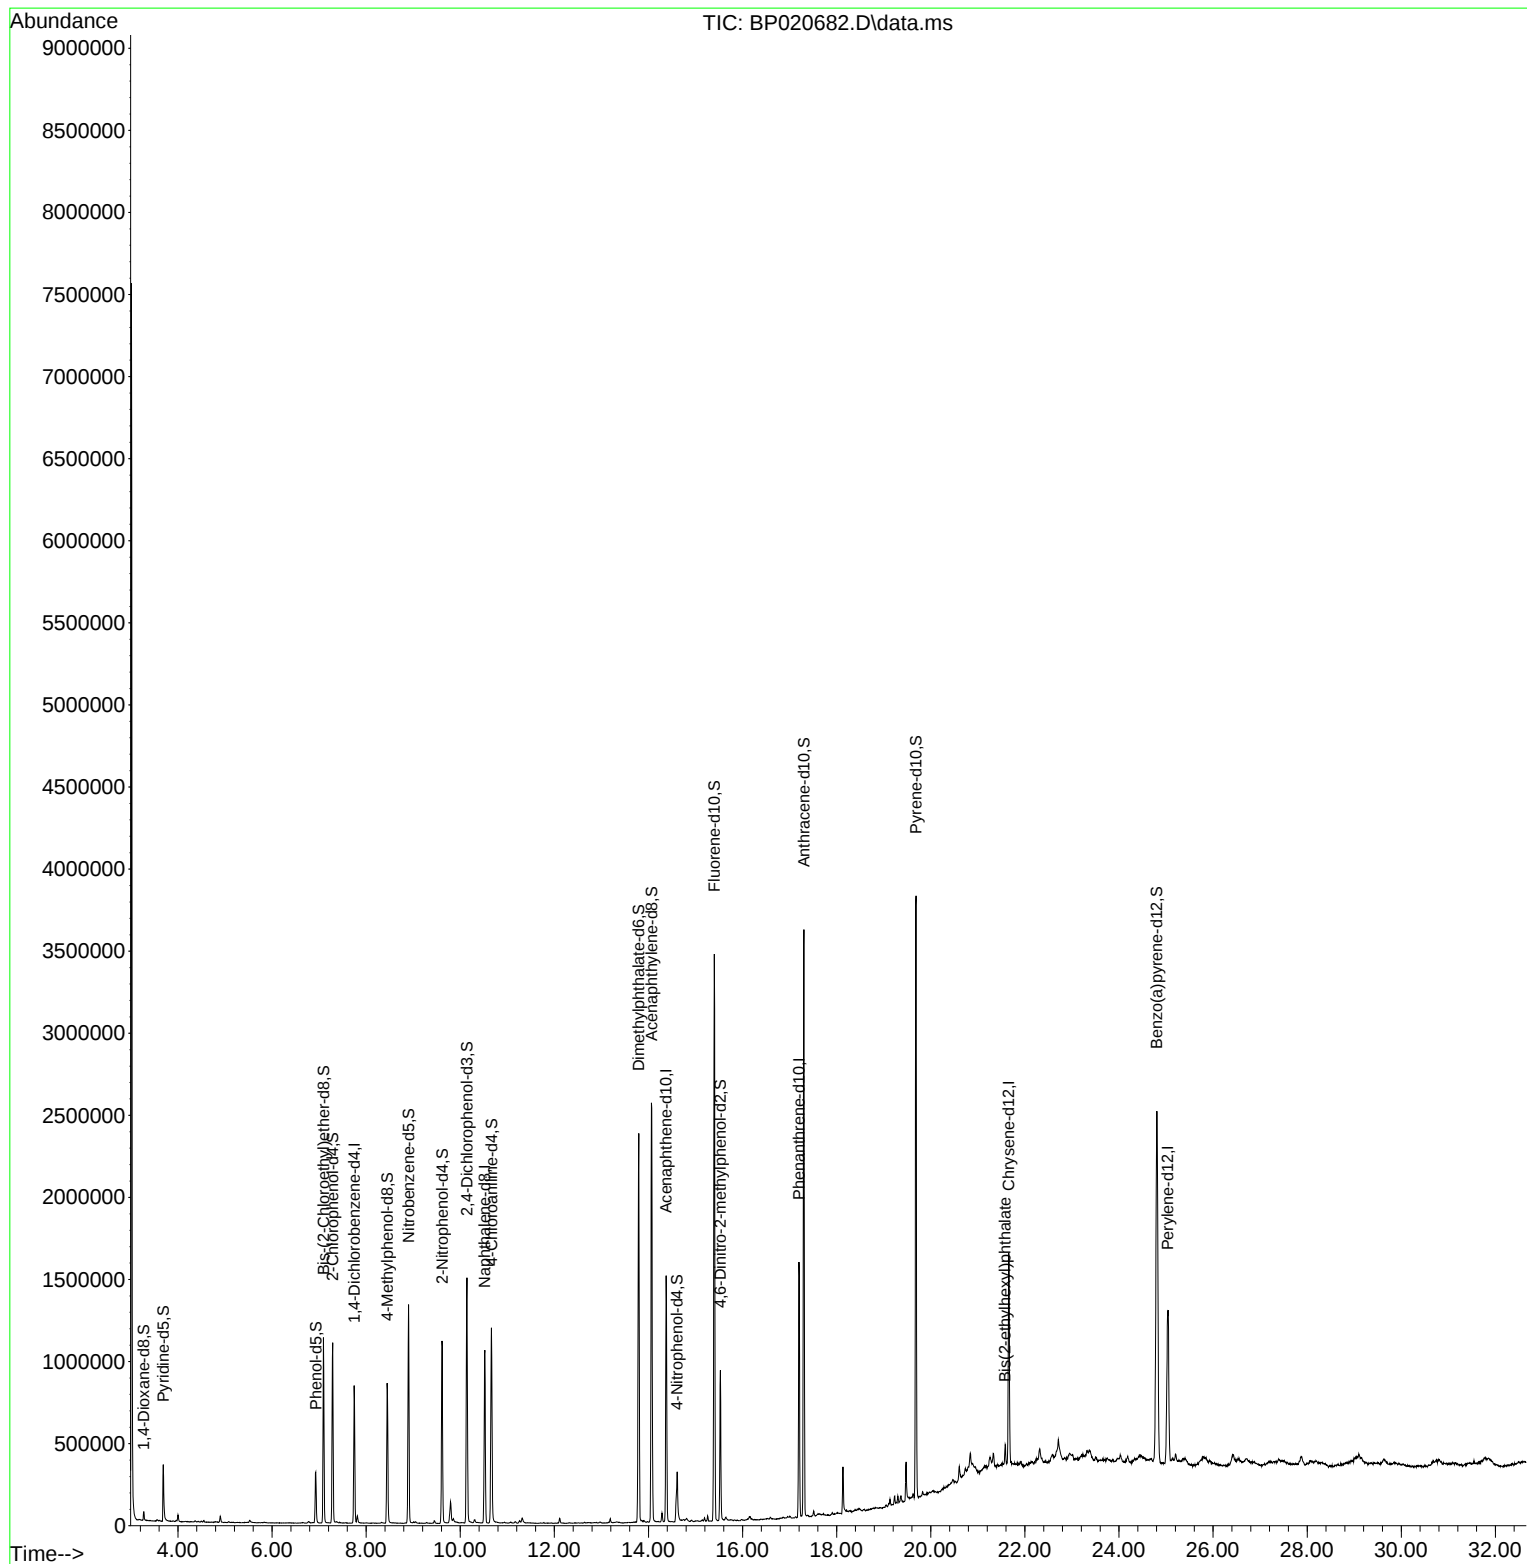

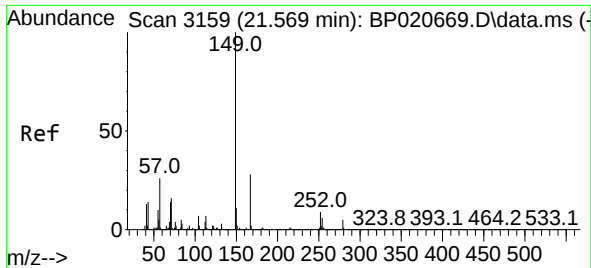

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.361 ng/ul
RT: 21.580 min Scan# 31
Delta R.T. 0.012 min
Lab File: BP020682.D
Acq: 28 Jun 2024 06:15

Instrument :
BNA_P
ClientSampleId :
E1G83

Tgt Ion	Ratio	Lower	Upper
149	100		
167	27.8	22.0	33.0
279	5.0	3.3	4.9

