

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020657.D
 Acq On : 27 Jun 2024 11:31
 Operator : MA/JU
 Sample : PB161614BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK614

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	10	rVB	112215	121747	2.08%	0.202%
2	3.058	10	12	21	rVB2	14418	21537	0.37%	0.036%
3	3.275	45	49	57	rVB	61430	81766	1.40%	0.135%
4	3.687	116	119	141	rBV	790959	1238864	21.20%	2.052%
5	4.005	167	173	179	rBV	16176	27350	0.47%	0.045%
6	4.222	207	210	215	rVB4	5924	8038	0.14%	0.013%
7	4.622	274	278	283	rBV6	5374	8698	0.15%	0.014%
8	6.922	662	669	683	rBV	966900	1549470	26.52%	2.566%
9	7.087	690	697	708	rBV	777822	1170715	20.04%	1.939%
10	7.281	723	730	742	rBV	943720	1563498	26.76%	2.589%
11	7.746	802	809	817	rBV	838792	1385569	23.71%	2.295%
12	8.446	919	928	943	rBV	1195515	1962444	33.59%	3.250%
13	8.893	995	1004	1024	rBV	983255	1581793	27.07%	2.620%
14	9.604	1118	1125	1137	rBV	815858	1305579	22.34%	2.162%
15	10.140	1207	1216	1236	rBV	1046142	1998891	34.21%	3.310%
16	10.522	1272	1281	1294	rVB	1121300	2024472	34.65%	3.353%
17	10.651	1294	1303	1320	rBV	1255334	2049862	35.08%	3.395%
18	11.334	1410	1419	1420	rBV10	3477	7331	0.13%	0.012%
19	12.104	1544	1550	1559	rBV2	19032	34724	0.59%	0.058%
20	13.340	1755	1760	1764	rVB7	3597	6165	0.11%	0.010%
21	13.787	1827	1836	1848	rBV	2062486	3064503	52.45%	5.075%
22	14.063	1873	1883	1893	rBV	2459113	3561152	60.95%	5.897%
23	14.375	1929	1936	1944	rBV	1912349	2762049	47.27%	4.574%
24	14.592	1965	1973	1985	rBV	861457	1460087	24.99%	2.418%
25	15.192	2067	2075	2076	rBV8	4091	6185	0.11%	0.010%
26	15.387	2100	2108	2116	rBV	3014186	4419394	75.64%	7.319%
27	15.510	2122	2129	2144	rBV	1104217	1467302	25.11%	2.430%
28	15.628	2144	2149	2157	rVB2	14607	30976	0.53%	0.051%
29	16.186	2239	2244	2252	rBV8	7591	13141	0.22%	0.022%
30	16.857	2354	2358	2363	rVB7	5163	7019	0.12%	0.012%
31	16.963	2371	2376	2382	rBV4	6544	11146	0.19%	0.018%
32	17.186	2406	2414	2425	rBV	2041176	3402532	58.23%	5.635%
33	17.292	2425	2432	2445	rVV	3470103	4809805	82.32%	7.965%
34	18.122	2569	2573	2578	rBV6	24722	45905	0.79%	0.076%
35	19.216	2754	2759	2764	rBV	43294	69066	1.18%	0.114%
36	19.292	2767	2772	2777	rBV	46059	71861	1.23%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020657.D
Acq On : 27 Jun 2024 11:31
Operator : MA/JU
Sample : PB161614BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK614

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Title : SVOA CALIBRATION

37	19.457	2797	2800	2804	rBV5	18923	28766	0.49%	0.048%
38	19.675	2830	2837	2845	rBV	3775269	5842970	100.00%	9.676%
39	21.639	3165	3171	3185	rVB	2341606	3477987	59.52%	5.760%
40	24.751	3691	3700	3714	rVB3	1542666	4609999	78.90%	7.634%
41	24.992	3733	3741	3754	rVB	1162036	3073986	52.61%	5.091%




Sum of corrected areas: 60384344

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020657.D
Acq On : 27 Jun 2024 11:31
Operator : MA/JU
Sample : PB161614BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK614

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

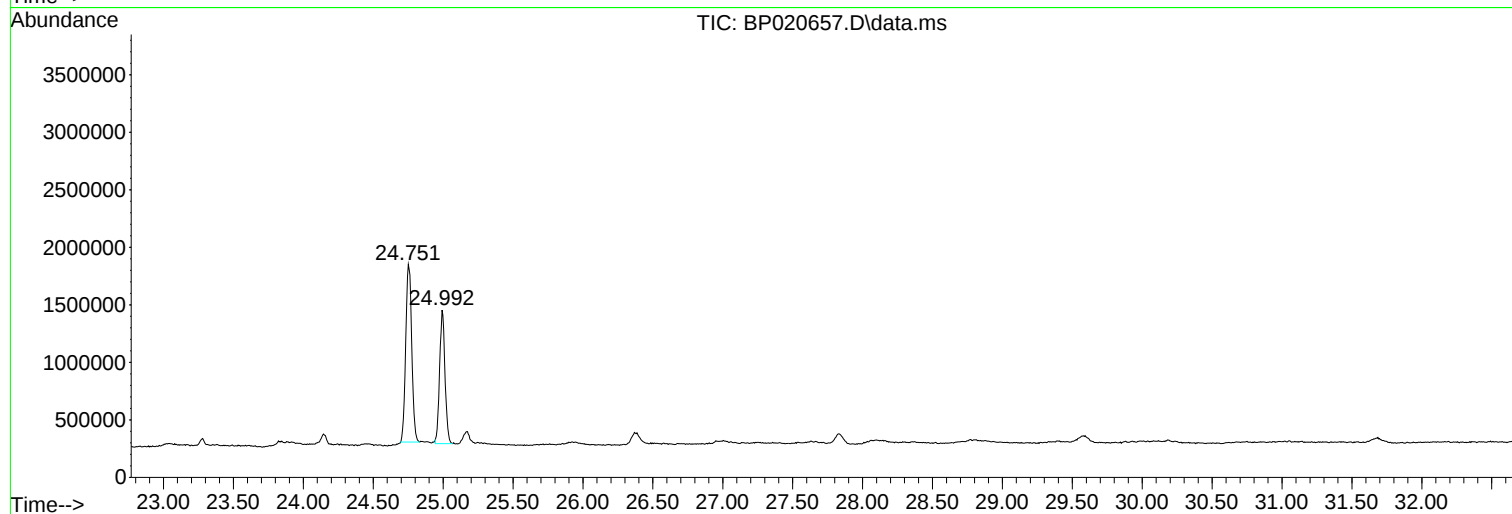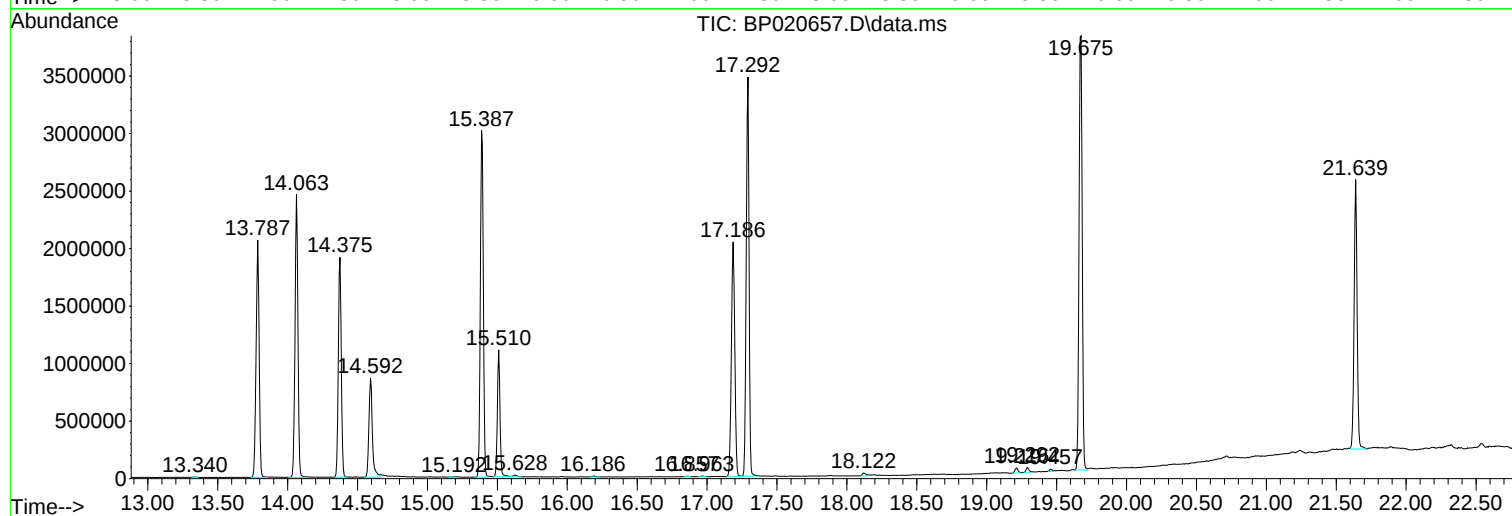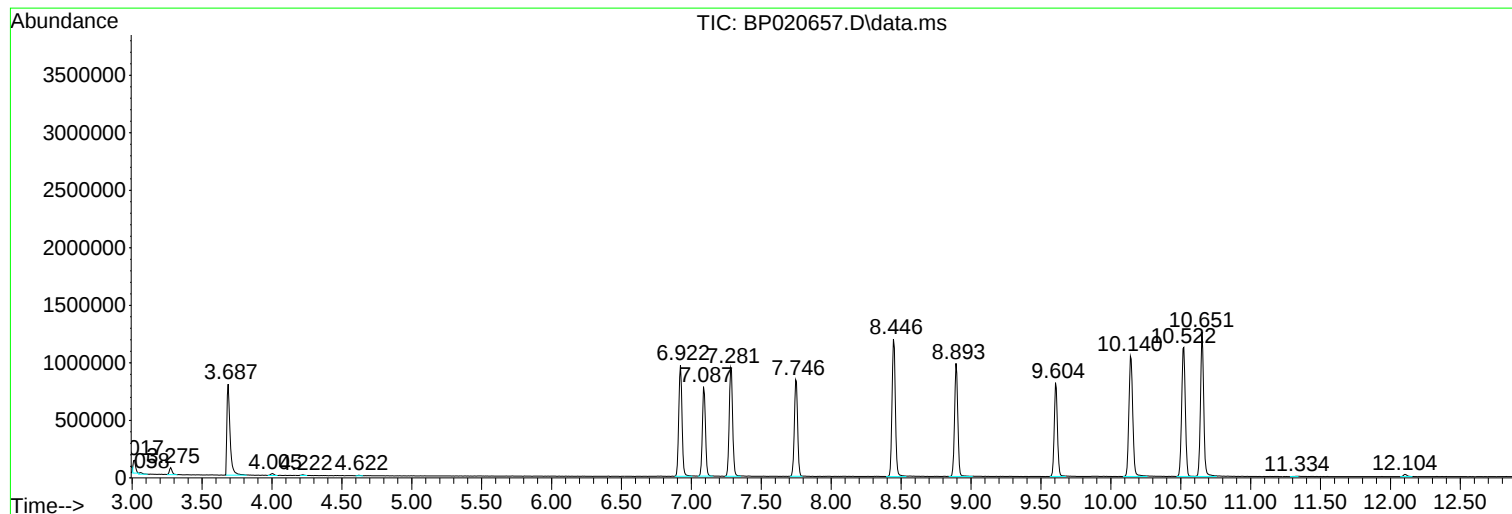

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020657.D
Acq On : 27 Jun 2024 11:31
Operator : MA/JU
Sample : PB161614BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK614

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020657.D
Acq On : 27 Jun 2024 11:31
Operator : MA/JU
Sample : PB161614BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK614

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------