

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020685.D
 Acq On : 28 Jun 2024 09:05
 Operator : MA/JU
 Sample : PB161614BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK614

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020685.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	10	rVB	164433	176165	2.99%	0.228%
2	3.064	10	13	18	rVB	20673	26983	0.46%	0.035%
3	3.275	45	49	56	rVB	85442	109192	1.85%	0.142%
4	3.687	116	119	136	rBV	1175814	1712407	29.05%	2.220%
5	4.005	168	173	179	rVB2	21046	34266	0.58%	0.044%
6	6.787	638	646	653	rBV2	4410	10817	0.18%	0.014%
7	6.928	663	670	683	rBV	1366889	2189445	37.14%	2.838%
8	7.099	691	699	708	rBV	1074976	1671589	28.36%	2.167%
9	7.287	723	731	745	rBV	1340944	2240342	38.01%	2.904%
10	7.752	802	810	824	rBV	1223533	1995915	33.86%	2.588%
11	8.452	920	929	943	rBV	1653663	2785252	47.25%	3.611%
12	8.899	996	1005	1017	rBV	1389234	2225874	37.76%	2.886%
13	9.610	1118	1126	1143	rBV	1176328	1910053	32.40%	2.476%
14	10.146	1208	1217	1233	rBV	1608169	2902171	49.23%	3.762%
15	10.516	1272	1280	1293	rBV	1506936	2884014	48.92%	3.739%
16	10.663	1297	1305	1322	rBV	1696864	2877840	48.82%	3.731%
17	11.322	1411	1417	1418	rBV5	4724	6515	0.11%	0.008%
18	12.110	1544	1551	1559	rBV3	30898	56631	0.96%	0.073%
19	13.334	1756	1759	1763	rBV5	4216	6680	0.11%	0.009%
20	13.792	1827	1837	1847	rBV	2734856	4181519	70.94%	5.421%
21	14.069	1874	1884	1900	rBV2	2805519	4983021	84.53%	6.460%
22	14.381	1929	1937	1945	rBV	2382036	3808578	64.61%	4.938%
23	14.604	1967	1975	1987	rBV	1104994	1810023	30.71%	2.347%
24	15.392	2097	2109	2116	rBV	3907777	5894773	100.00%	7.642%
25	15.522	2124	2131	2143	rBV	1123605	1661357	28.18%	2.154%
26	15.634	2146	2150	2157	rVB	19929	32340	0.55%	0.042%
27	15.969	2202	2207	2212	rBV6	5022	7383	0.13%	0.010%
28	16.186	2240	2244	2250	rVB4	10721	16447	0.28%	0.021%
29	16.857	2354	2358	2365	rVB9	8027	15337	0.26%	0.020%
30	16.963	2372	2376	2381	rBV5	6149	11618	0.20%	0.015%
31	17.192	2408	2415	2426	rBV	2467160	4116323	69.83%	5.337%
32	17.298	2426	2433	2450	rVB2	3965889	5852419	99.28%	7.587%
33	17.498	2463	2467	2473	rBV4	6963	12050	0.20%	0.016%
34	17.892	2532	2534	2539	rVB6	7825	10083	0.17%	0.013%
35	18.133	2570	2575	2578	rBV5	16982	25694	0.44%	0.033%
36	18.480	2630	2634	2641	rVB5	10704	15273	0.26%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020685.D
Acq On : 28 Jun 2024 09:05
Operator : MA/JU
Sample : PB161614BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK614

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Title : SVOA CALIBRATION

37	19.222	2757	2760	2766	rBV3	45785	65077	1.10%	0.084%
38	19.298	2769	2773	2779	rVB	39302	58820	1.00%	0.076%
39	19.680	2832	2838	2845	rBV	4236613	5734201	97.28%	7.434%
40	20.916	3046	3048	3058	rVB	81945	131001	2.22%	0.170%
41	21.651	3166	3173	3186	rVB2	1896577	3347912	56.79%	4.340%
42	24.792	3697	3707	3720	rVB	2252905	5777038	98.00%	7.490%
43	25.015	3736	3745	3759	rVB	1366412	3744075	63.52%	4.854%




Sum of corrected areas: 77134513

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020685.D
Acq On : 28 Jun 2024 09:05
Operator : MA/JU
Sample : PB161614BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK614

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

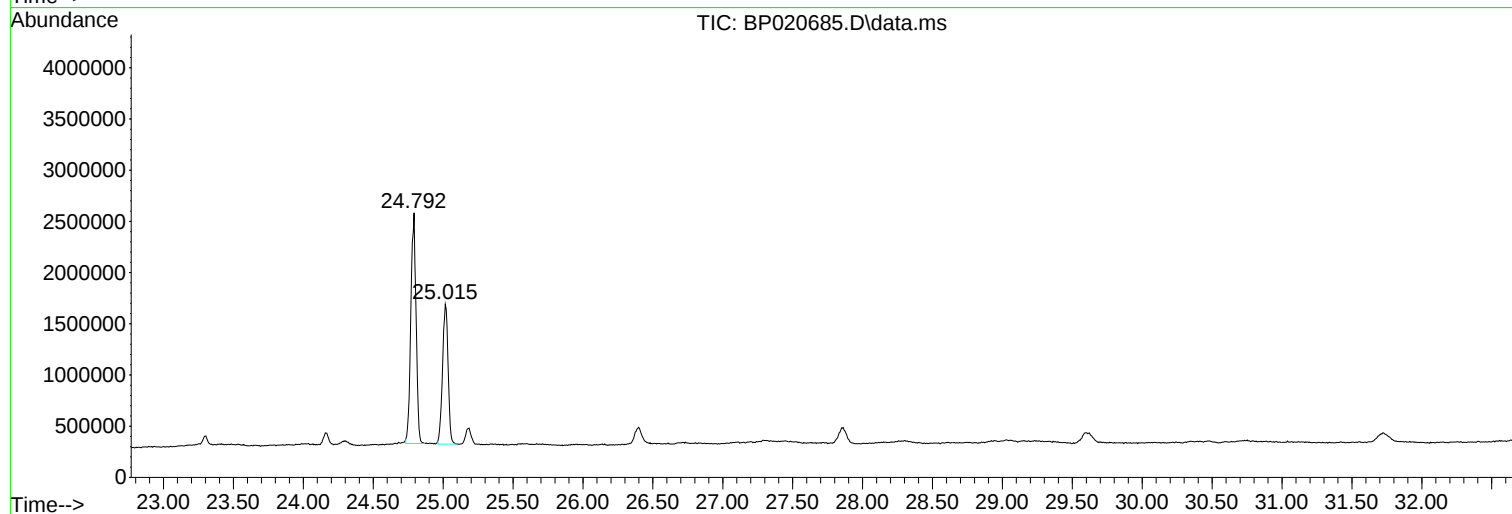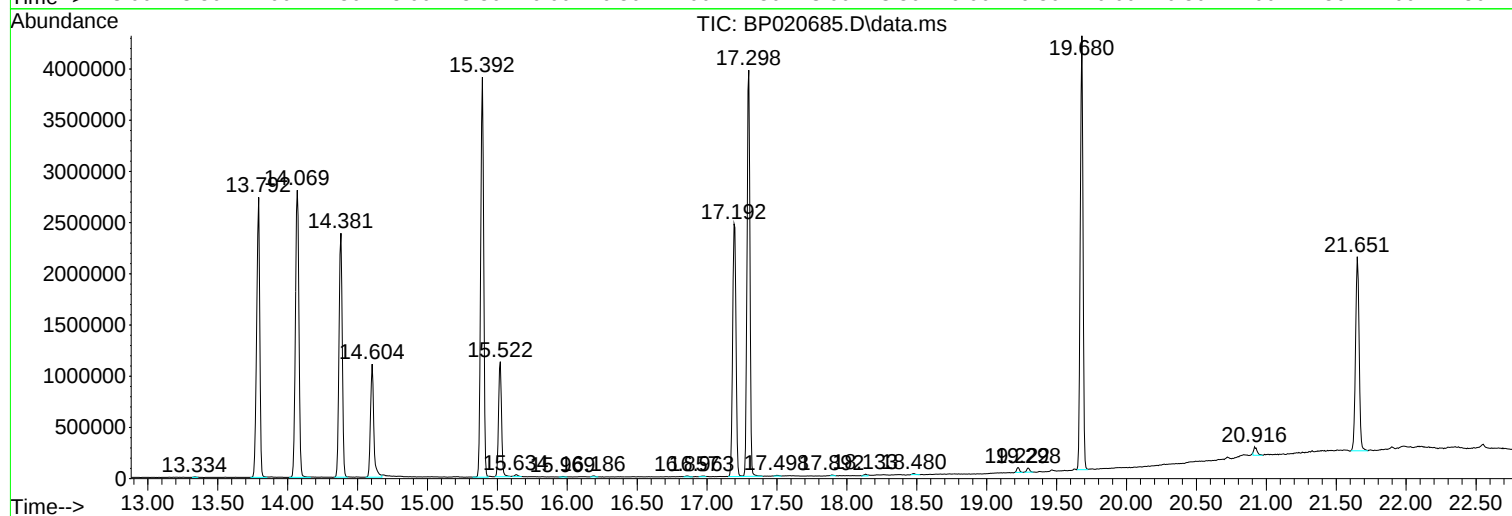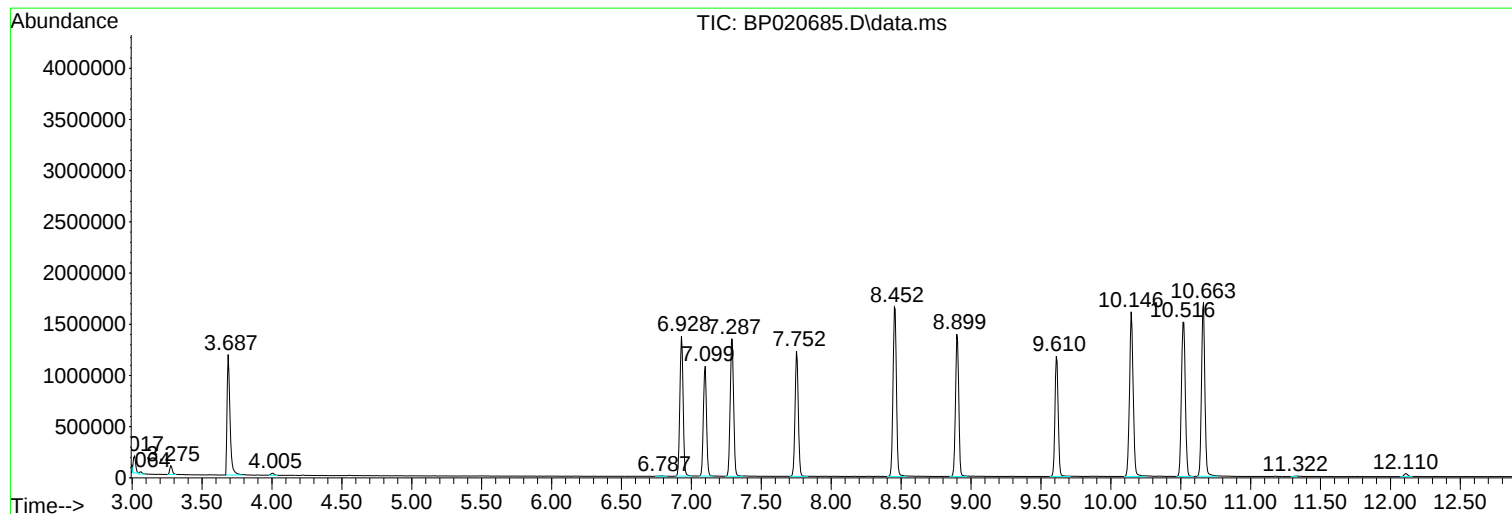

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020685.D
Acq On : 28 Jun 2024 09:05
Operator : MA/JU
Sample : PB161614BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK614

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020685.D
Acq On : 28 Jun 2024 09:05
Operator : MA/JU
Sample : PB161614BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK614

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------