

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020696.D
 Acq On : 28 Jun 2024 17:38
 Operator : MA/JU
 Sample : PB161583BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK583

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	56	rVB	56454	73454	2.00%	0.158%
2	3.681	116	118	134	rBV	719455	1063936	29.00%	2.285%
3	3.999	168	172	176	rBV2	16647	21977	0.60%	0.047%
4	6.922	662	669	683	rBV	843023	1362256	37.14%	2.926%
5	7.087	689	697	709	rVB	662114	1054323	28.74%	2.265%
6	7.281	723	730	745	rVB	882165	1378678	37.59%	2.961%
7	7.734	800	807	818	rBV	776257	1330441	36.27%	2.858%
8	8.440	919	927	940	rBV	1017543	1708211	46.57%	3.669%
9	8.893	996	1004	1016	rBV	791937	1367856	37.29%	2.938%
10	9.604	1117	1125	1136	rBV	656592	1165420	31.77%	2.503%
11	10.140	1208	1216	1229	rBV	1026655	1732528	47.23%	3.721%
12	10.510	1271	1279	1289	rBV	1190103	1913481	52.16%	4.110%
13	10.651	1295	1303	1317	rBV	898319	1741358	47.47%	3.740%
14	10.804	1325	1329	1331	rVB5	3145	3899	0.11%	0.008%
15	12.110	1542	1551	1556	rBV	15571	30240	0.82%	0.065%
16	12.810	1667	1670	1674	rVB6	2295	3838	0.10%	0.008%
17	13.334	1754	1759	1765	rBV9	3406	5908	0.16%	0.013%
18	13.781	1827	1835	1850	rBV	1650332	2397539	65.36%	5.150%
19	13.904	1850	1856	1861	rVB9	2719	5460	0.15%	0.012%
20	14.069	1875	1884	1896	rBV	1906449	2899178	79.04%	6.227%
21	14.381	1929	1937	1953	rBV	1631281	2436026	66.41%	5.232%
22	14.598	1967	1974	1991	rBV	425730	929775	25.35%	1.997%
23	14.804	2004	2009	2015	rVB10	6166	13859	0.38%	0.030%
24	15.392	2100	2109	2124	rBV	2224120	3405115	92.83%	7.314%
25	15.516	2124	2130	2146	rVV	478026	797206	21.73%	1.712%
26	15.628	2146	2149	2156	rVB4	12198	22002	0.60%	0.047%
27	15.969	2205	2207	2213	rVB6	3211	3965	0.11%	0.009%
28	16.192	2240	2245	2250	rBV7	5330	9385	0.26%	0.020%
29	16.857	2353	2358	2361	rBV7	4456	6574	0.18%	0.014%
30	16.969	2372	2377	2381	rBV5	6113	9558	0.26%	0.021%
31	17.186	2407	2414	2424	rBV	1716881	2456895	66.98%	5.277%
32	17.292	2424	2432	2445	rBV	2045821	3245602	88.48%	6.971%
33	17.880	2529	2532	2536	rBV6	5473	7772	0.21%	0.017%
34	18.128	2570	2574	2578	rBV6	13148	19326	0.53%	0.042%
35	19.222	2756	2760	2765	rBV2	27788	40854	1.11%	0.088%
36	19.298	2770	2773	2776	rVB	21816	27549	0.75%	0.059%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020696.D
Acq On : 28 Jun 2024 17:38
Operator : MA/JU
Sample : PB161583BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK583

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Title : SVOA CALIBRATION

37	19.674	2831	2837	2846	rBV2	2301981	3427279	93.43%	7.361%
38	21.645	3167	3172	3182	rVB	1376071	2222666	60.59%	4.774%
39	24.780	3696	3705	3720	rVB2	1335555	3668159	100.00%	7.879%
40	25.027	3738	3747	3760	rVB	918370	2547324	69.44%	5.471%




Sum of corrected areas: 46556872

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020696.D
Acq On : 28 Jun 2024 17:38
Operator : MA/JU
Sample : PB161583BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK583

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

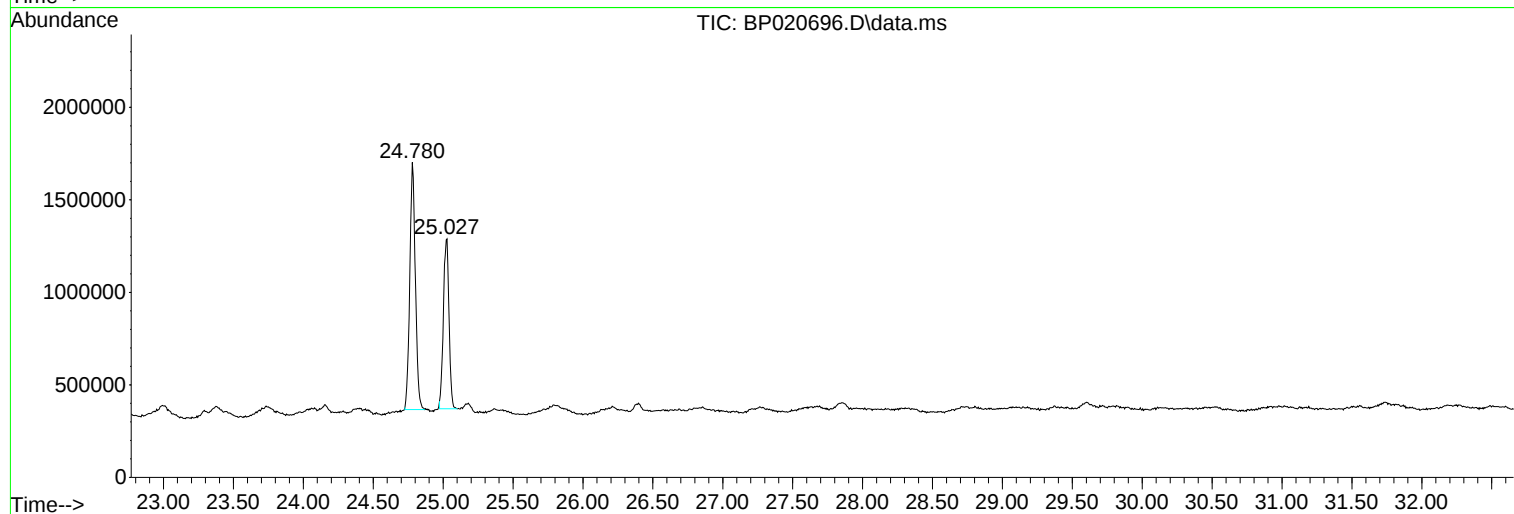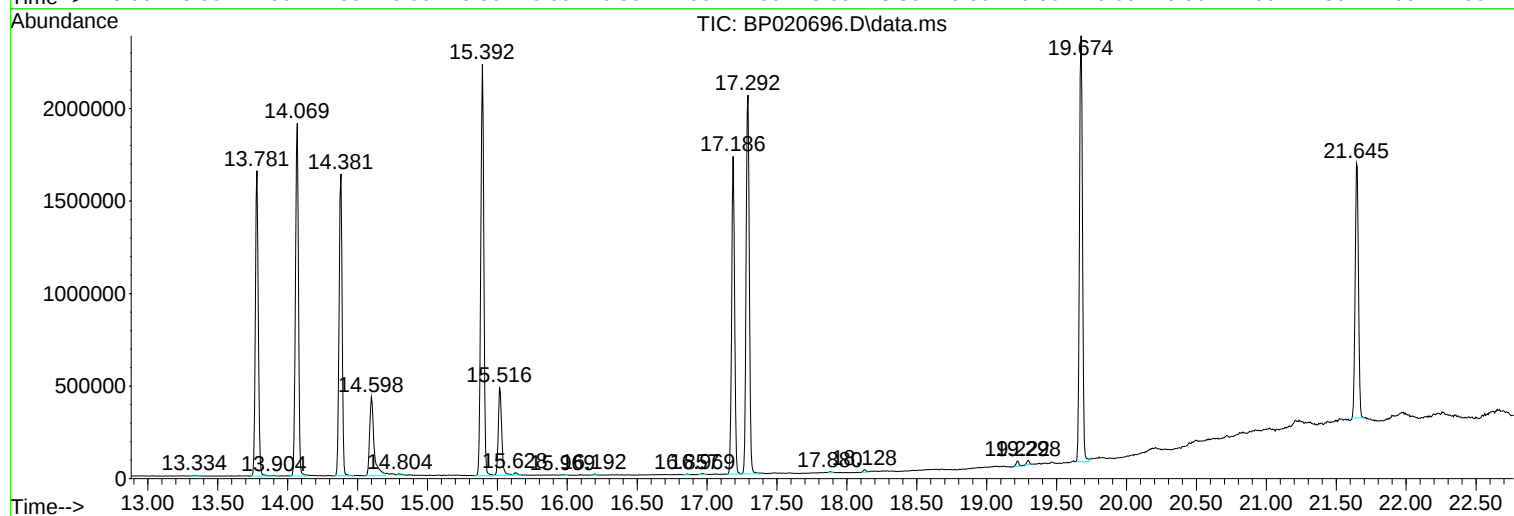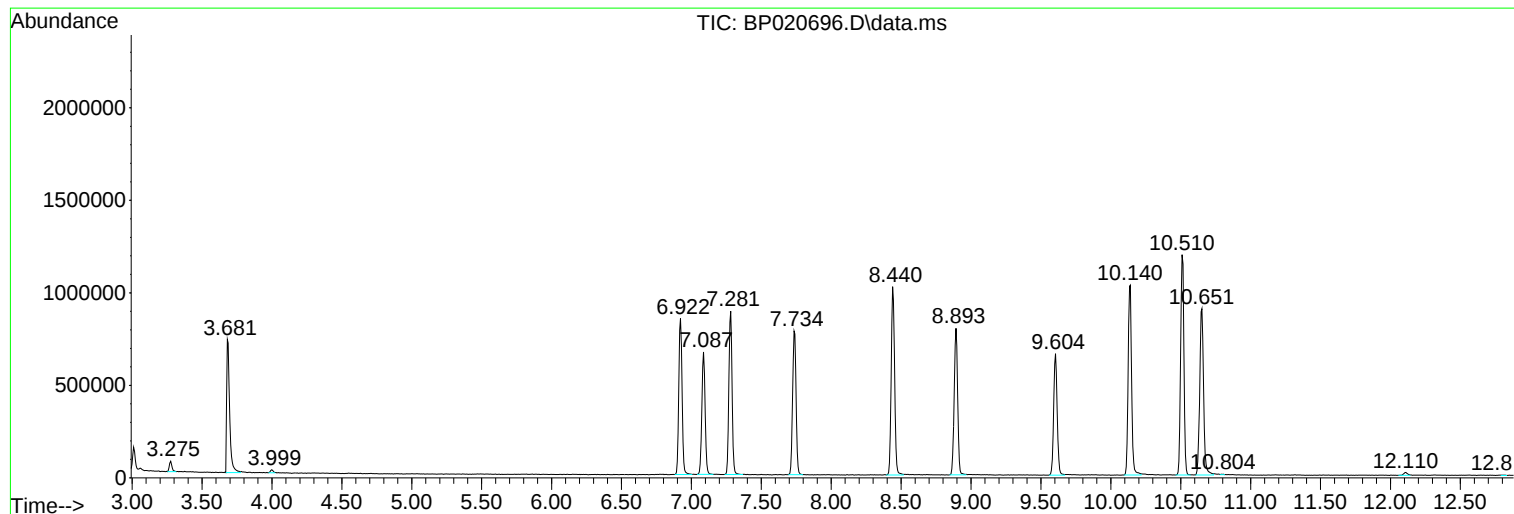

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020696.D
Acq On : 28 Jun 2024 17:38
Operator : MA/JU
Sample : PB161583BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK583

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020696.D
Acq On : 28 Jun 2024 17:38
Operator : MA/JU
Sample : PB161583BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK583

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------