

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020697.D
 Acq On : 28 Jun 2024 18:21
 Operator : MA/JU
 Sample : PB161630BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK630

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	44	48	54	rVB	53523	69681	1.64%	0.136%
2	3.681	116	118	133	rBV	665180	1021807	24.06%	1.988%
3	3.999	169	172	178	rVB	13647	19577	0.46%	0.038%
4	6.922	661	669	684	rBV	872492	1441731	33.95%	2.805%
5	7.087	691	697	707	rBV	733224	1092465	25.73%	2.125%
6	7.281	722	730	741	rBV	905174	1451521	34.19%	2.824%
7	7.746	801	809	816	rBV	736499	1224290	28.83%	2.382%
8	8.446	919	928	940	rBV	1091768	1844530	43.44%	3.589%
9	8.893	997	1004	1015	rBV	948225	1455361	34.28%	2.831%
10	9.605	1116	1125	1135	rBV	812291	1256373	29.59%	2.444%
11	10.140	1207	1216	1236	rBV	1046694	1948507	45.89%	3.791%
12	10.516	1270	1280	1289	rBV	1059453	1827807	43.05%	3.556%
13	10.657	1296	1304	1318	rBV	859310	1552492	36.56%	3.020%
14	11.334	1413	1419	1428	rBV	2891	7222	0.17%	0.014%
15	12.104	1544	1550	1564	rVB	18363	33456	0.79%	0.065%
16	13.787	1826	1836	1845	rBV	1669619	2820977	66.44%	5.488%
17	14.063	1874	1883	1895	rBV	2157383	3379385	79.59%	6.575%
18	14.375	1928	1936	1949	rBV	1736281	2501939	58.92%	4.868%
19	14.604	1967	1975	1987	rBV	661392	1184427	27.89%	2.304%
20	15.393	2100	2109	2116	rBV	2749135	4169968	98.21%	8.113%
21	15.522	2124	2131	2144	rBV	702236	1054476	24.83%	2.052%
22	15.634	2146	2150	2156	rVB4	11720	21202	0.50%	0.041%
23	15.910	2190	2197	2201	rBV4	7774	11610	0.27%	0.023%
24	16.192	2241	2245	2250	rVB4	9895	15639	0.37%	0.030%
25	16.863	2356	2359	2365	rVB8	3779	5896	0.14%	0.011%
26	16.969	2374	2377	2384	rVB3	5169	9369	0.22%	0.018%
27	17.192	2408	2415	2425	rBV	1758821	2862728	67.42%	5.570%
28	17.292	2426	2432	2444	rVV2	2945175	4246047	100.00%	8.261%
29	17.898	2532	2535	2538	rVB5	5783	6643	0.16%	0.013%
30	18.122	2570	2573	2574	rBV3	6873	6648	0.16%	0.013%
31	19.222	2756	2760	2764	rBV4	34761	53014	1.25%	0.103%
32	19.298	2770	2773	2778	rVB	27519	38388	0.90%	0.075%
33	19.681	2831	2838	2848	rBV	2950762	4202904	98.98%	8.177%
34	21.651	3167	3173	3185	rVB2	1268375	2236551	52.67%	4.351%
35	24.786	3697	3706	3719	rVB2	1353676	3828842	90.17%	7.449%
36	25.016	3737	3745	3762	rVB	934223	2496142	58.79%	4.856%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020697.D
Acq On : 28 Jun 2024 18:21
Operator : MA/JU
Sample : PB161630BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK630

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 51399615

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020697.D
Acq On : 28 Jun 2024 18:21
Operator : MA/JU
Sample : PB161630BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK630

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

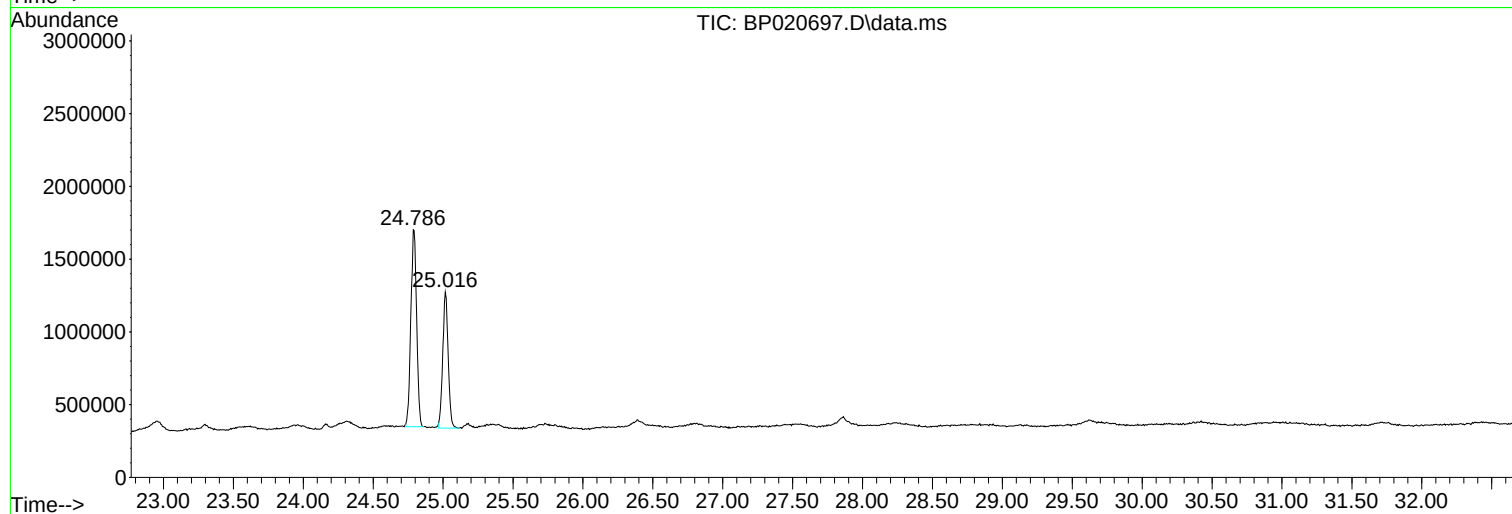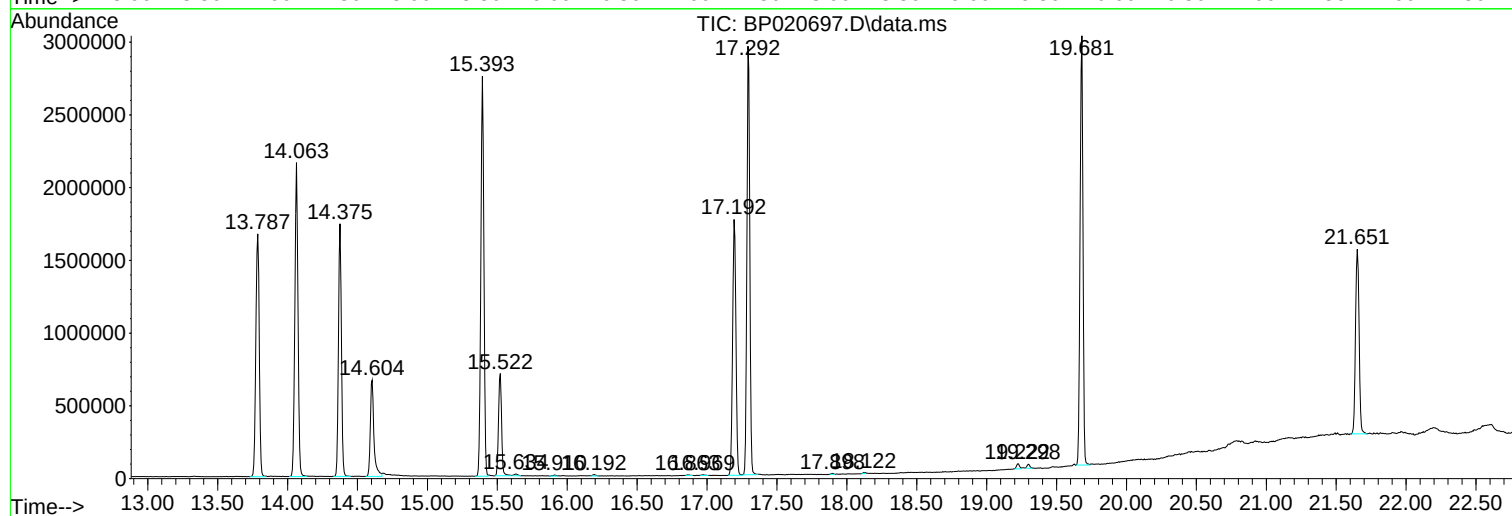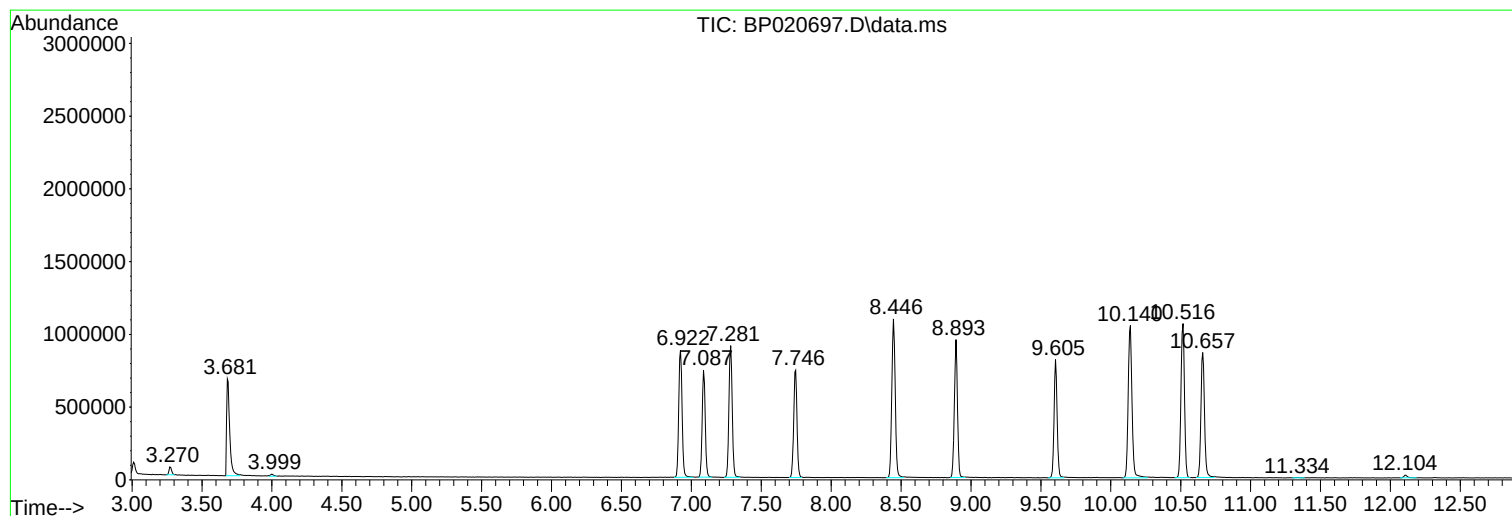

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020697.D
Acq On : 28 Jun 2024 18:21
Operator : MA/JU
Sample : PB161630BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK630

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020697.D
Acq On : 28 Jun 2024 18:21
Operator : MA/JU
Sample : PB161630BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK630

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------