

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
 Data File : BP020699.D
 Acq On : 28 Jun 2024 19:48
 Operator : MA/JU
 Sample : PB161608BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK608

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	10	rVB	122382	127831	3.13%	0.307%
2	3.276	45	49	54	rVB	57116	71084	1.74%	0.171%
3	3.687	115	119	135	rBV	711788	1034691	25.37%	2.483%
4	3.999	169	172	177	rVB	14930	19625	0.48%	0.047%
5	6.928	663	670	682	rBV	748824	1229606	30.15%	2.950%
6	7.087	689	697	707	rBV	659348	966864	23.70%	2.320%
7	7.287	723	731	741	rBV	774852	1297189	31.80%	3.112%
8	7.746	802	809	817	rBV	676741	1092753	26.79%	2.622%
9	8.446	919	928	947	rBV	884061	1492922	36.60%	3.582%
10	8.893	996	1004	1019	rBV	718862	1176192	28.84%	2.822%
11	9.605	1116	1125	1135	rBV	561581	980229	24.03%	2.352%
12	10.140	1207	1216	1235	rBV	802087	1484915	36.41%	3.563%
13	10.522	1271	1281	1289	rBV	844302	1442876	35.37%	3.462%
14	10.658	1293	1304	1319	rBV	843460	1437589	35.25%	3.449%
15	12.104	1545	1550	1555	rBV2	14131	24297	0.60%	0.058%
16	13.346	1758	1761	1767	rVB6	3055	5541	0.14%	0.013%
17	13.793	1830	1837	1846	rBV	1395627	1913792	46.92%	4.592%
18	14.075	1876	1885	1898	rBV	1426583	2371185	58.13%	5.689%
19	14.381	1928	1937	1946	rBV	1039022	1700017	41.68%	4.079%
20	14.604	1968	1975	1987	rBV	447028	832826	20.42%	1.998%
21	14.851	2014	2017	2023	rVB8	3380	6065	0.15%	0.015%
22	15.393	2101	2109	2116	rBV	1919811	2760294	67.67%	6.623%
23	15.522	2124	2131	2146	rBV	471669	714796	17.52%	1.715%
24	15.634	2147	2150	2158	rVV8	10292	20986	0.51%	0.050%
25	16.104	2224	2230	2233	rBV8	2650	5724	0.14%	0.014%
26	16.192	2240	2245	2251	rVB9	4351	8386	0.21%	0.020%
27	16.857	2356	2358	2364	rVB7	4967	8944	0.22%	0.021%
28	16.963	2374	2376	2383	rVB5	3924	5896	0.14%	0.014%
29	17.192	2408	2415	2423	rBV	1379770	1925974	47.22%	4.621%
30	17.292	2425	2432	2444	rVV	2079493	2981179	73.09%	7.153%
31	18.122	2570	2573	2575	rBV4	7828	10005	0.25%	0.024%
32	19.216	2756	2759	2764	rVB3	24701	36262	0.89%	0.087%
33	19.292	2769	2772	2779	rVB	25446	34165	0.84%	0.082%
34	19.675	2831	2837	2845	rBV	2579185	3603092	88.34%	8.645%
35	21.651	3167	3173	3185	rVB2	1209523	2243279	55.00%	5.382%
36	24.792	3698	3707	3719	rVB	1474661	4078841	100.00%	9.787%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020699.D
Acq On : 28 Jun 2024 19:48
Operator : MA/JU
Sample : PB161608BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK608

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Title : SVOA CALIBRATION

37	25.021	3738	3746	3760	rVB	927260	2531935	62.07%	6.075%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 41677847

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020699.D
Acq On : 28 Jun 2024 19:48
Operator : MA/JU
Sample : PB161608BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK608

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

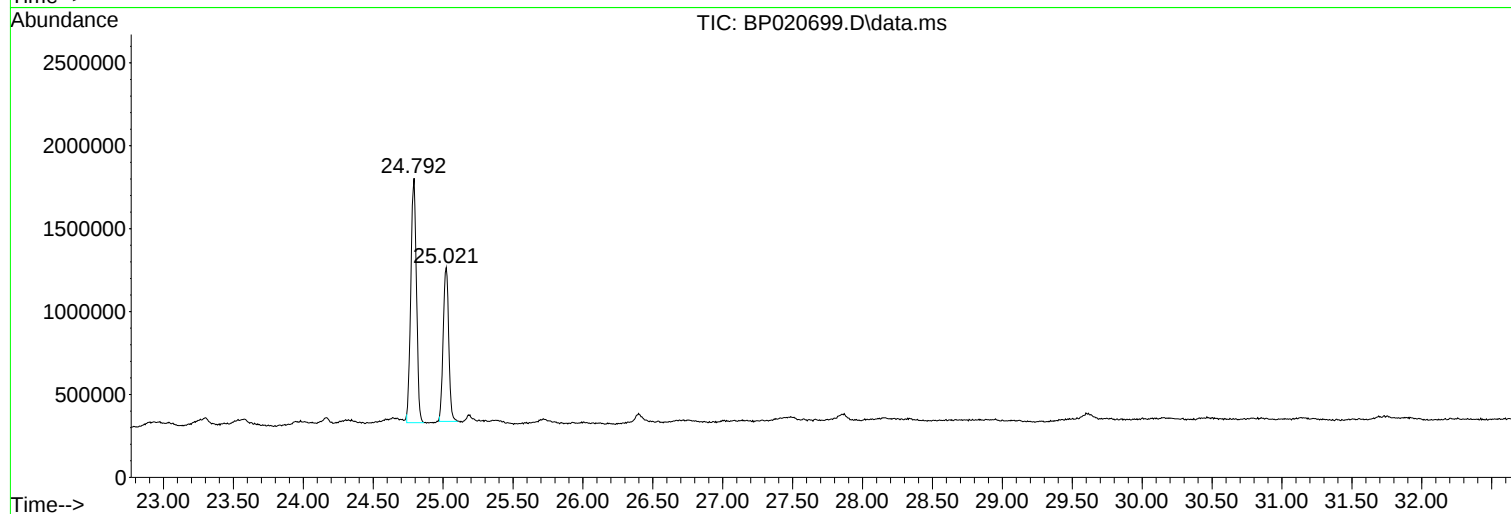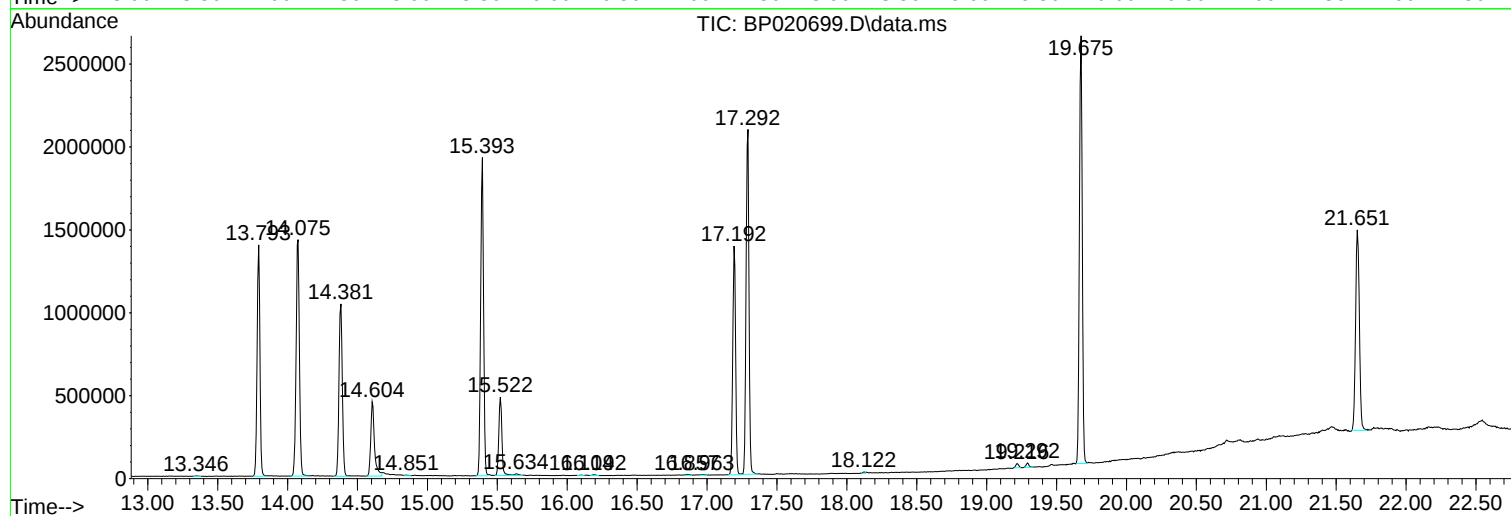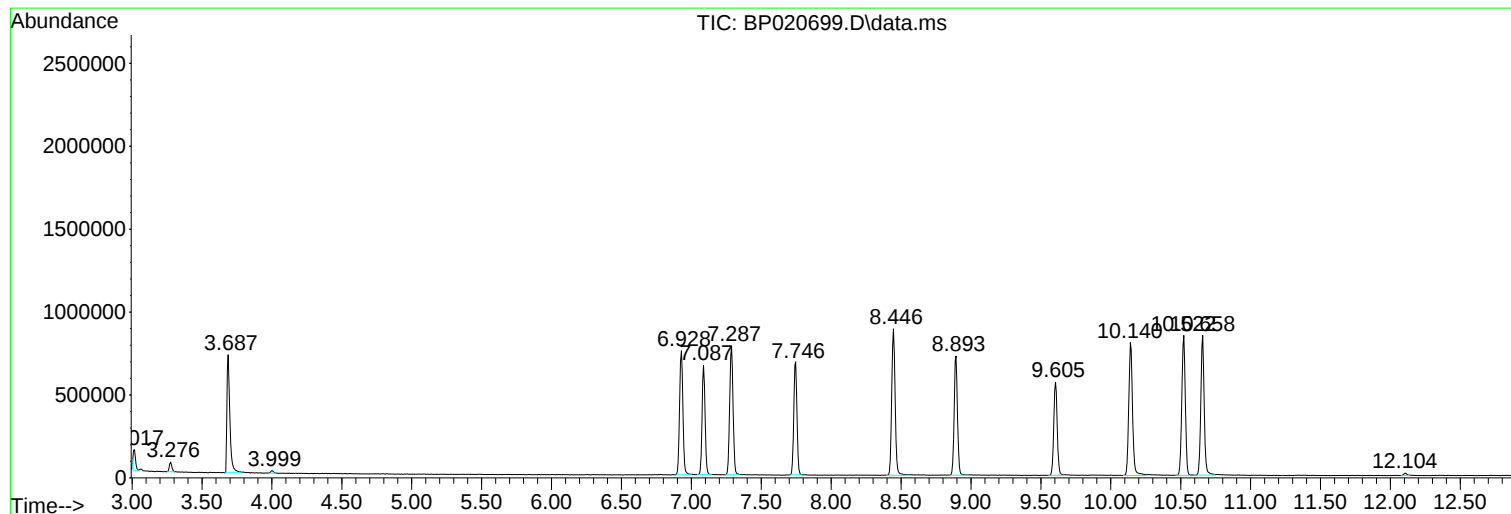

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020699.D
Acq On : 28 Jun 2024 19:48
Operator : MA/JU
Sample : PB161608BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK608

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062724\
Data File : BP020699.D
Acq On : 28 Jun 2024 19:48
Operator : MA/JU
Sample : PB161608BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK608

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc