
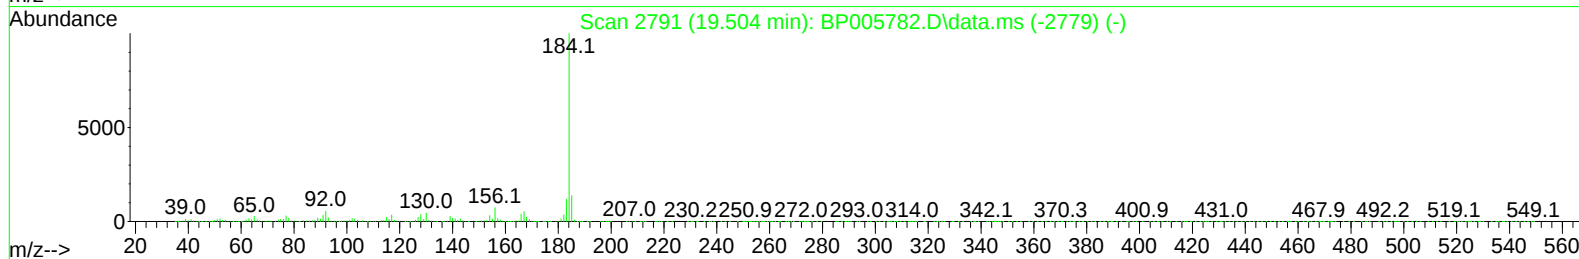
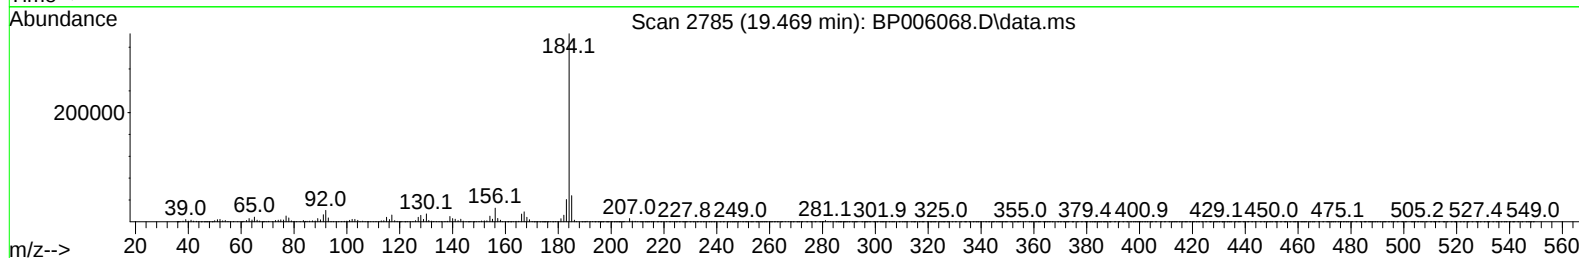


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062821\
 Data File : BP006068.D
 Acq On : 28 Jun 2021 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 11:28:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 22 17:52:38 2021
 Response via : Initial Calibration

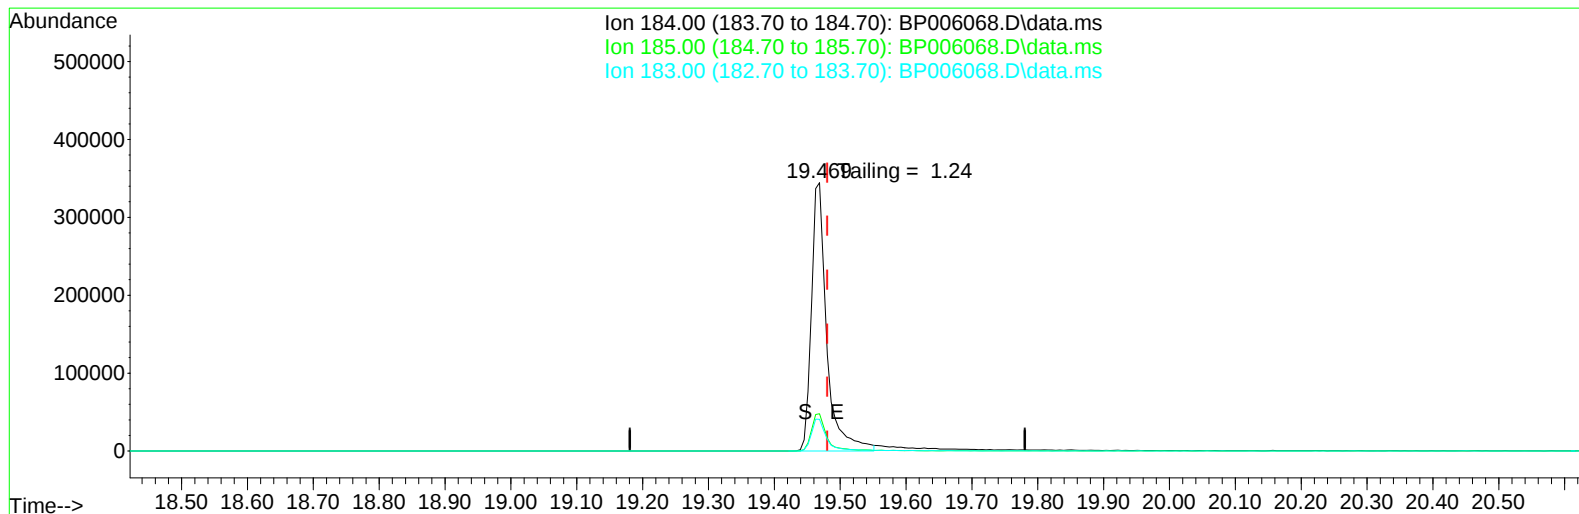




TIC: BP006068.D\data.ms

(77) Benzidine**19.469min (-0.012) 895322.45 ng****response 577526**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.89
183.00	11.90	11.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062821\
 Data File : BP006068.D
 Acq On : 28 Jun 2021 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 11:28:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 22 17:52:38 2021
 Response via : Initial Calibration

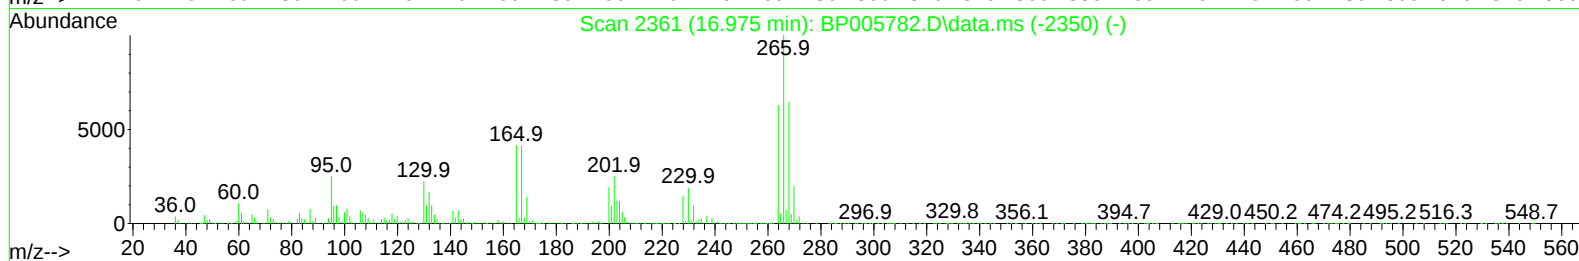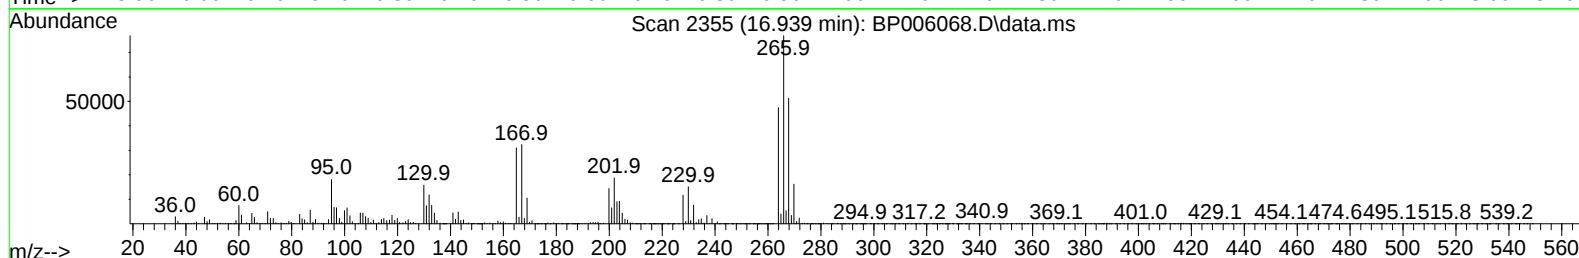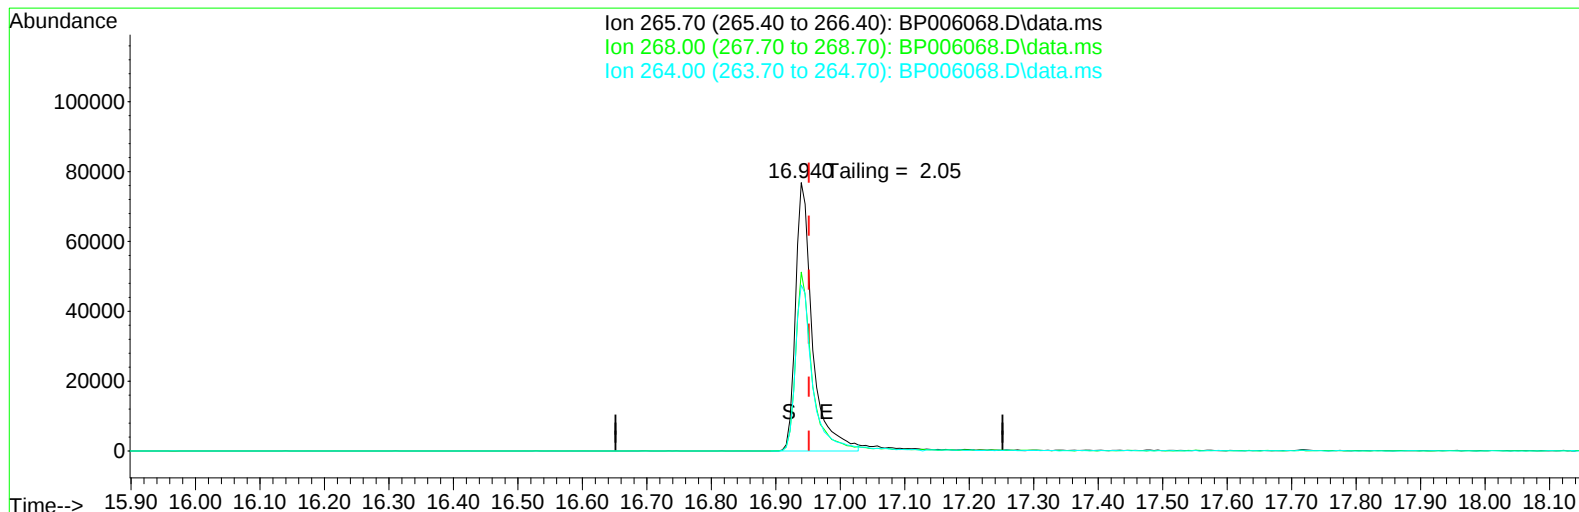

TIC: BP006068.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.012) 712898.25 ng

response 146362

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	66.66
264.00	62.90	61.83
0.00	0.00	0.00