

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062821\
 Data File : BP006083.D
 Acq On : 28 Jun 2021 18:24
 Operator : CG/JU
 Sample : M2857-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SB-14-COMP

Quant Time: Jun 29 02:05:44 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 11:34:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	68929	20.000	ng	0.00
21) Naphthalene-d8	10.704	136	260956	20.000	ng	0.00
39) Acenaphthene-d10	14.534	164	159554	20.000	ng	0.00
64) Phenanthrene-d10	17.281	188	331126	20.000	ng	0.00
76) Chrysene-d12	21.357	240	401630	20.000	ng	0.00
86) Perylene-d12	23.757	264	470030	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	398122	92.681	ng	0.00
7) Phenol-d6	7.081	99	476505	85.583	ng	0.00
23) Nitrobenzene-d5	9.069	82	284719	53.492	ng	0.00
42) 2,4,6-Tribromophenol	16.028	330	236797	86.483	ng	0.00
45) 2-Fluorobiphenyl	13.163	172	661986	54.482	ng	0.00
79) Terphenyl-d14	19.827	244	1154185	53.811	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062821\
Data File : BP006083.D
Acq On : 28 Jun 2021 18:24
Operator : CG/JU
Sample : M2857-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-14-COMP

Quant Time: Jun 29 02:05:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 28 11:34:30 2021
Response via : Initial Calibration




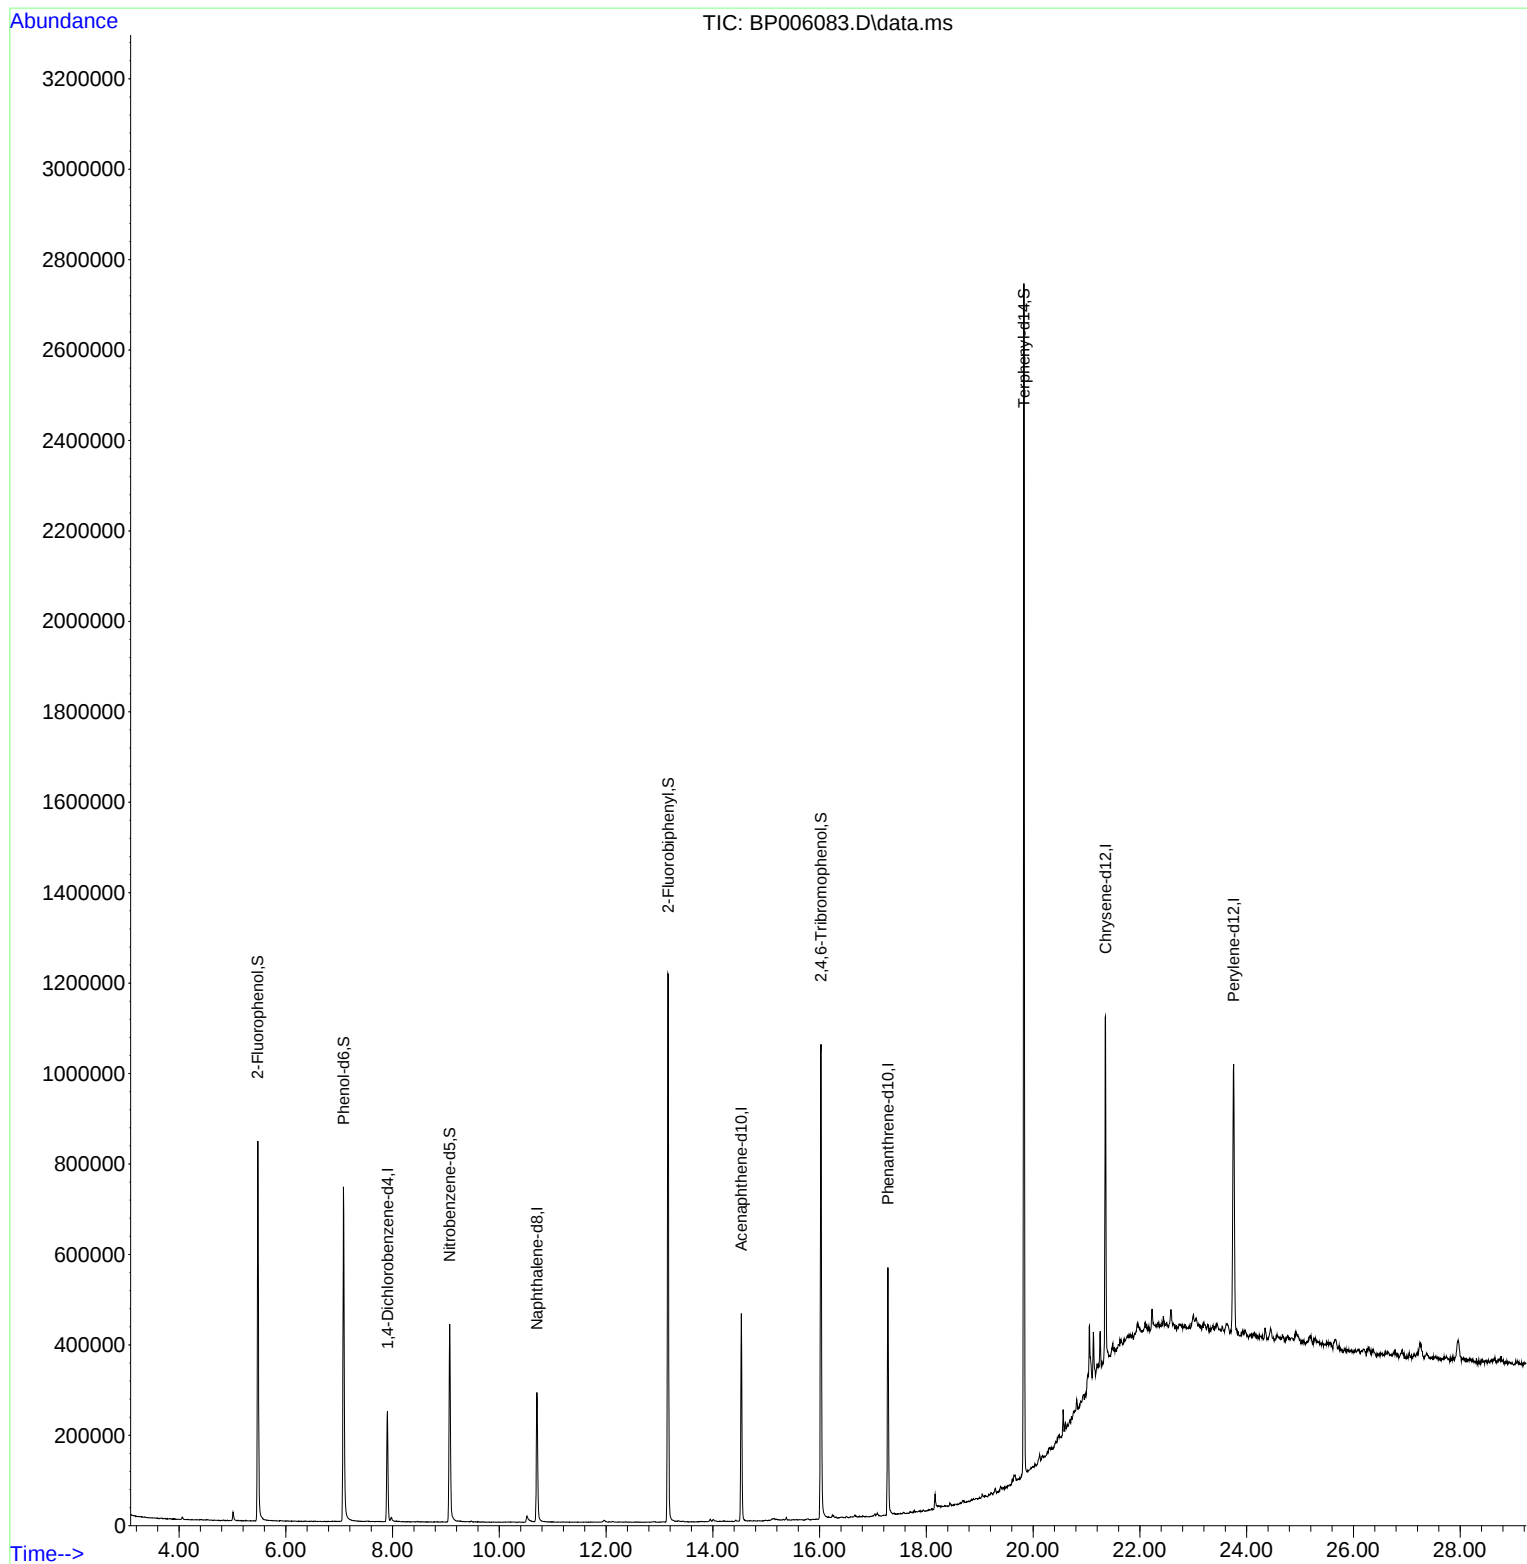


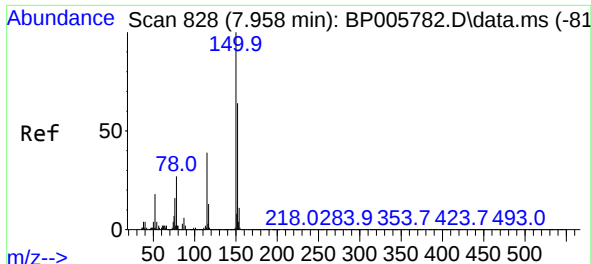

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.905 min Scan# 819
Delta R.T. -0.000 min
Lab File: BP006083.D
Acq: 28 Jun 2021 18:24




Instrument :
BNA_P
ClientSampleId :
SB-14-COMP


Tgt Ion:152 Resp: 68929
Ion Ratio Lower Upper
152 100
150 164.9 125.6 188.4
115 60.4 48.5 72.7

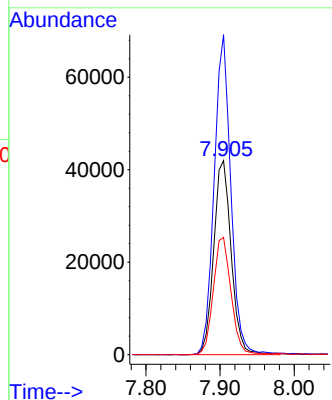

#5
2-Fluorophenol
Concen: 92.681 ng
RT: 5.475 min Scan# 406
Delta R.T. 0.000 min
Lab File: BP006083.D
Acq: 28 Jun 2021 18:24

Tgt Ion:112 Resp: 398122
Ion Ratio Lower Upper
112 100
64 51.7 41.4 62.2
63 27.9 23.8 35.8

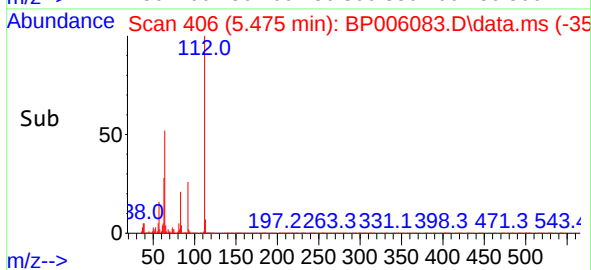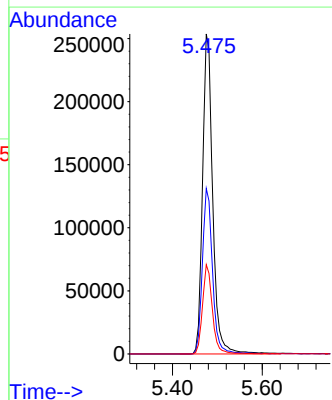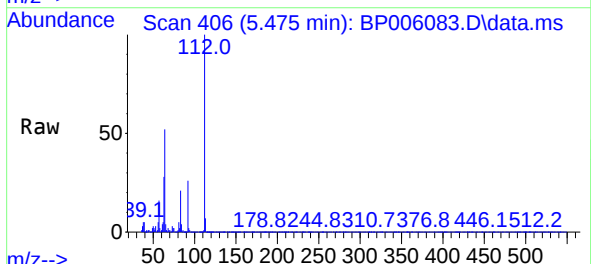




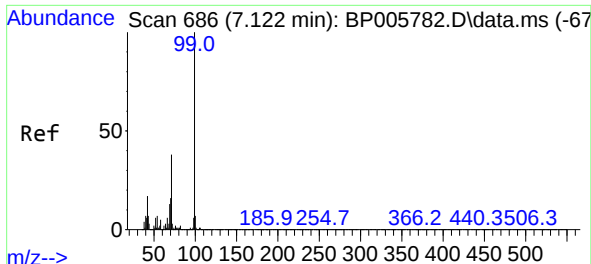


#7
Phenol-d6
Concen: 85.583 ng
RT: 7.081 min Scan# 679
Delta R.T. 0.000 min
Lab File: BP006083.D
Acq: 28 Jun 2021 18:24

Instrument :
BNA_P
ClientSampleId :
SB-14-COMP

Tgt Ion: 99 Resp: 476505




Ion	Ratio	Lower	Upper
99	100		
42	15.4	13.4	20.0
71	36.8	30.6	46.0

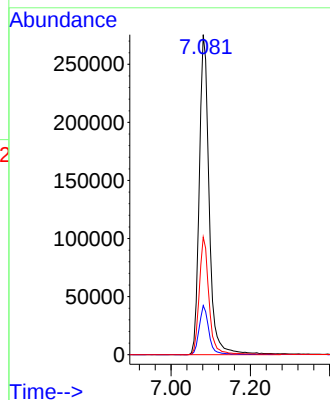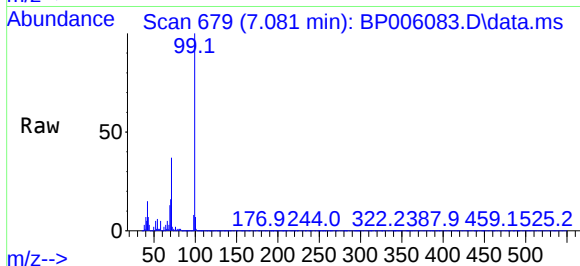


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.704 min Scan# 1295
Delta R.T. -0.006 min
Lab File: BP006083.D
Acq: 28 Jun 2021 18:24

Tgt Ion: 136 Resp: 260956

Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.6	12.8
54	5.6	4.6	6.8
68	4.9	3.6	5.4


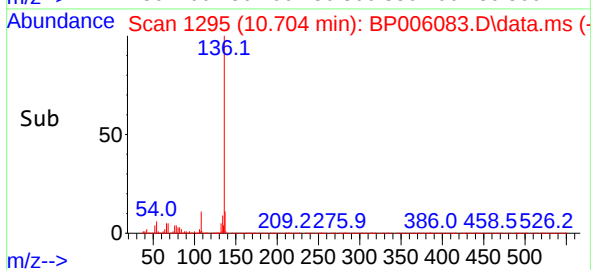
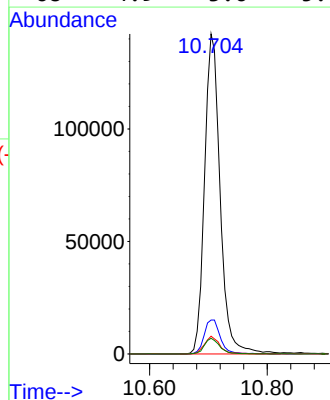
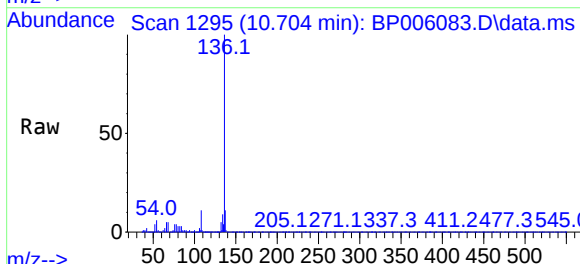


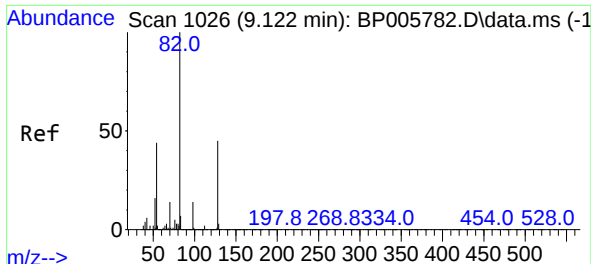

#23
Nitrobenzene-d5
Concen: 53.492 ng
RT: 9.069 min Scan# 1017
Delta R.T. -0.006 min
Lab File: BP006083.D
Acq: 28 Jun 2021 18:24




Instrument :
BNA_P
ClientSampleId :
SB-14-COMP

Tgt Ion: 82 Resp: 284719
Ion Ratio Lower Upper
82 100
128 45.1 35.7 53.5
54 40.9 35.0 52.4

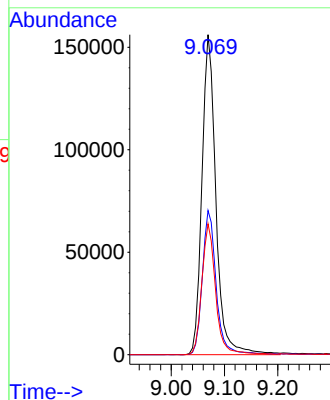

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.534 min Scan# 1946
Delta R.T. 0.000 min
Lab File: BP006083.D
Acq: 28 Jun 2021 18:24

Tgt Ion: 164 Resp: 159554
Ion Ratio Lower Upper
164 100
162 99.8 80.2 120.2
160 44.4 34.5 51.7


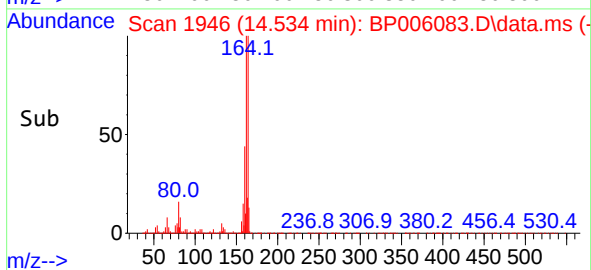
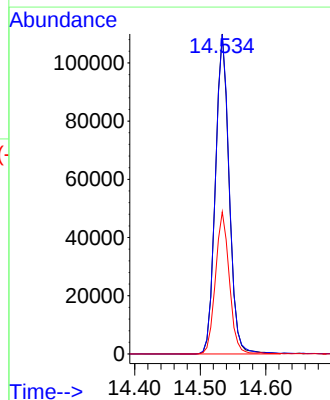
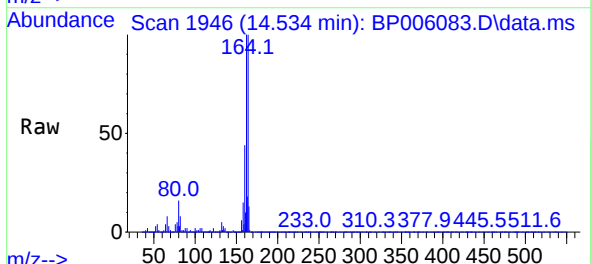




#42
2,4,6-Tribromophenol
Concen: 86.483 ng
RT: 16.028 min Scan# 2200
Delta R.T. 0.000 min
Lab File: BP006083.D
Acq: 28 Jun 2021 18:24




Instrument :
BNA_P
ClientSampleId :
SB-14-COMP


Tgt Ion:330 Resp: 236797
Ion Ratio Lower Upper
330 100
332 97.4 77.8 116.8
141 29.4 25.4 38.2

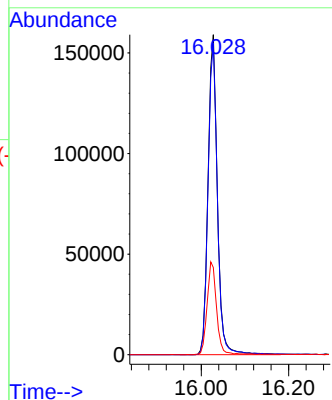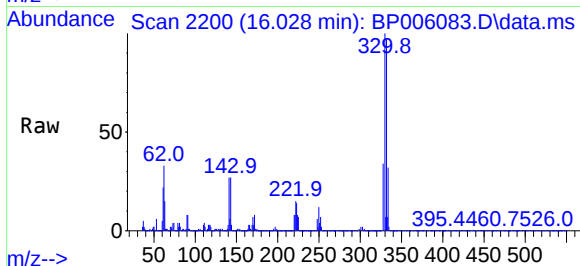

#45
2-Fluorobiphenyl
Concen: 54.482 ng
RT: 13.163 min Scan# 1713
Delta R.T. 0.000 min
Lab File: BP006083.D
Acq: 28 Jun 2021 18:24

Tgt Ion:172 Resp: 661986
Ion Ratio Lower Upper
172 100
171 35.5 27.9 41.9
170 22.7 18.6 27.8


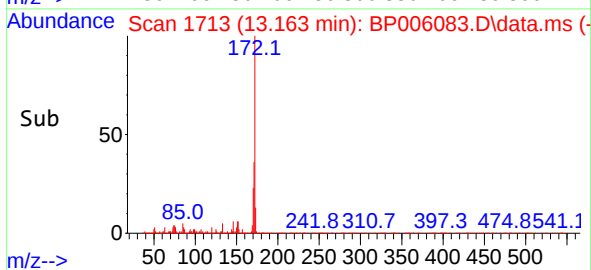
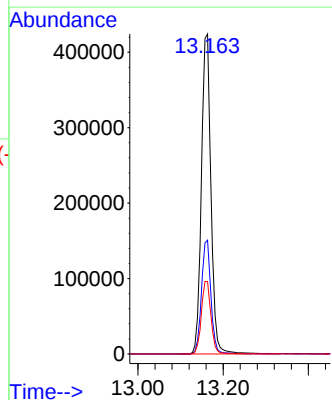
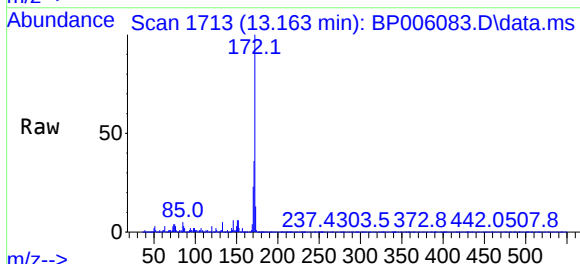




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.281 min Scan# 2413
Delta R.T. 0.000 min
Lab File: BP006083.D
Acq: 28 Jun 2021 18:24




Instrument :
BNA_P
ClientSampleId :
SB-14-COMP


Tgt Ion:188 Resp: 331126
Ion Ratio Lower Upper
188 100
94 8.2 5.6 8.4
80 8.8 6.3 9.5

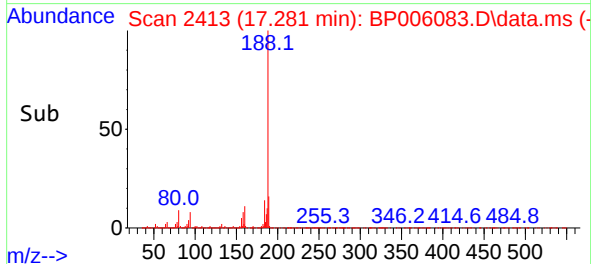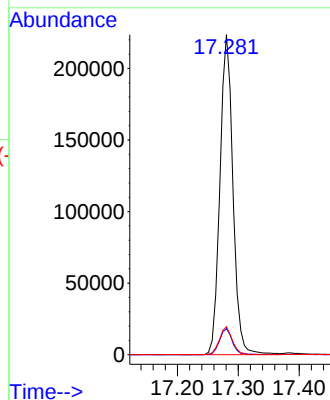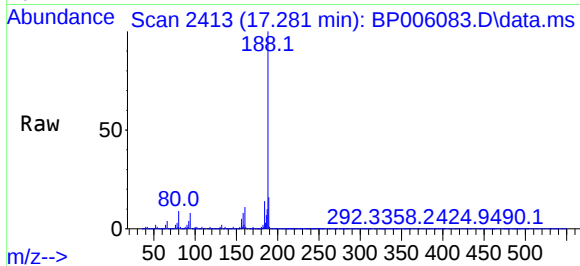

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.357 min Scan# 3106
Delta R.T. 0.000 min
Lab File: BP006083.D
Acq: 28 Jun 2021 18:24

Tgt Ion:240 Resp: 401630
Ion Ratio Lower Upper
240 100
120 8.9 6.5 9.7
236 25.3 20.6 31.0


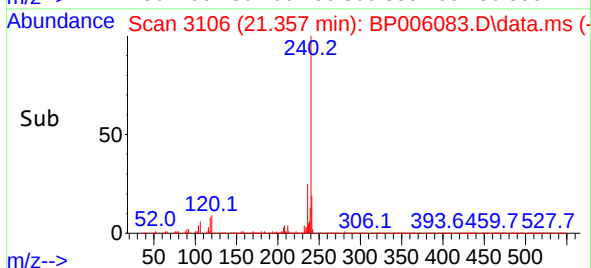
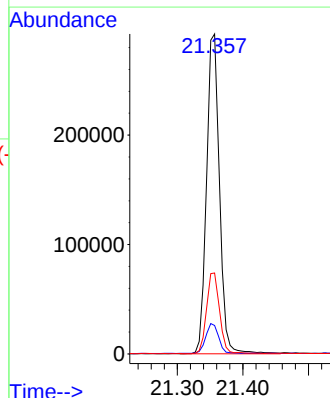
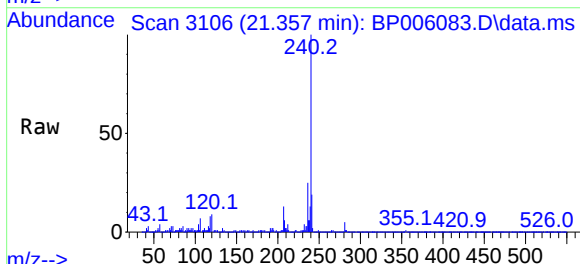




#79
Terphenyl-d14
Concen: 53.811 ng
RT: 19.827 min Scan# 2846
Delta R.T. -0.006 min
Lab File: BP006083.D
Acq: 28 Jun 2021 18:24

Instrument :
BNA_P
ClientSampleId :
SB-14-COMP

Tgt Ion:244 Resp: 1154185
Ion Ratio Lower Upper
244 100
212 7.4 6.0 9.0
122 9.3 7.1 10.7

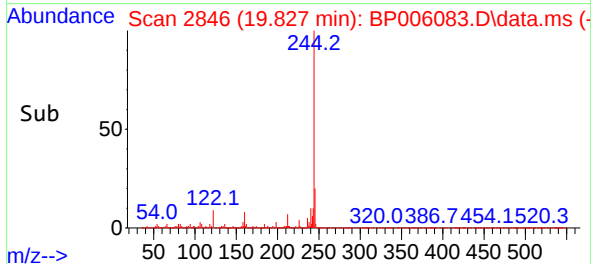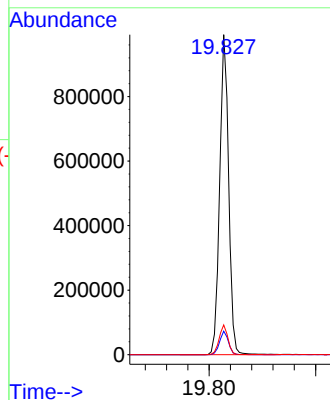

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.757 min Scan# 3514
Delta R.T. 0.000 min
Lab File: BP006083.D
Acq: 28 Jun 2021 18:24

Tgt Ion:264 Resp: 470030
Ion Ratio Lower Upper
264 100
260 24.5 18.6 28.0
265 22.6 17.6 26.4

