

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062821\
Data File : BP006070.D
Acq On : 28 Jun 2021 10:55
Operator : CG/JU
Sample : PB137356BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137356BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	400	406	419	rBV	1424198	2136796	47.95%	10.900%
2	7.087	673	680	696	rBV	1218970	2075512	46.58%	10.587%
3	7.904	810	819	833	rBV	253929	410911	9.22%	2.096%
4	9.069	1010	1017	1041	rBV	727477	1309573	29.39%	6.680%
5	10.710	1286	1296	1316	rBV	261794	524245	11.76%	2.674%
6	13.163	1705	1713	1732	rBV	2005423	3041547	68.25%	15.515%
7	14.533	1940	1946	1965	rBV	414993	667050	14.97%	3.403%
8	16.027	2193	2200	2223	rBV	1559967	2443192	54.83%	12.462%
9	17.280	2407	2413	2431	rBV	458448	756551	16.98%	3.859%
10	19.827	2841	2846	2858	rBV	3458415	4456174	100.00%	22.730%
11	21.356	3101	3106	3115	rBV	610708	887995	19.93%	4.530%
12	23.756	3508	3514	3525	rVB2	425845	894885	20.08%	4.565%




Sum of corrected areas: 19604431

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062821\
Data File : BP006070.D
Acq On : 28 Jun 2021 10:55
Operator : CG/JU
Sample : PB137356BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137356BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

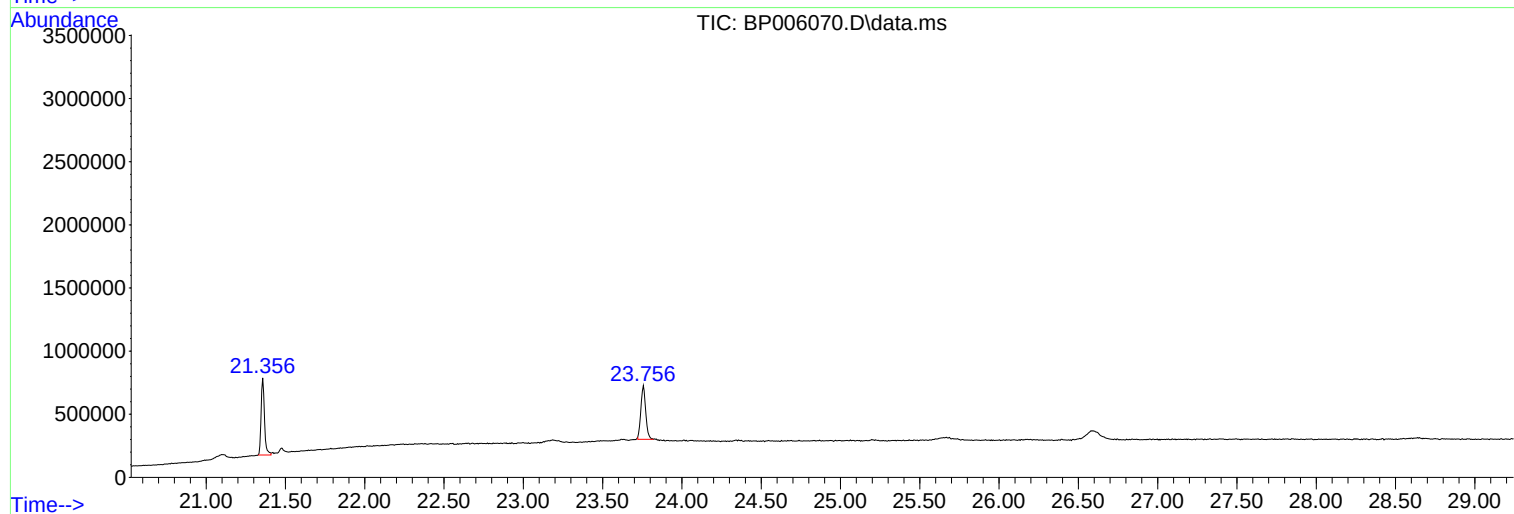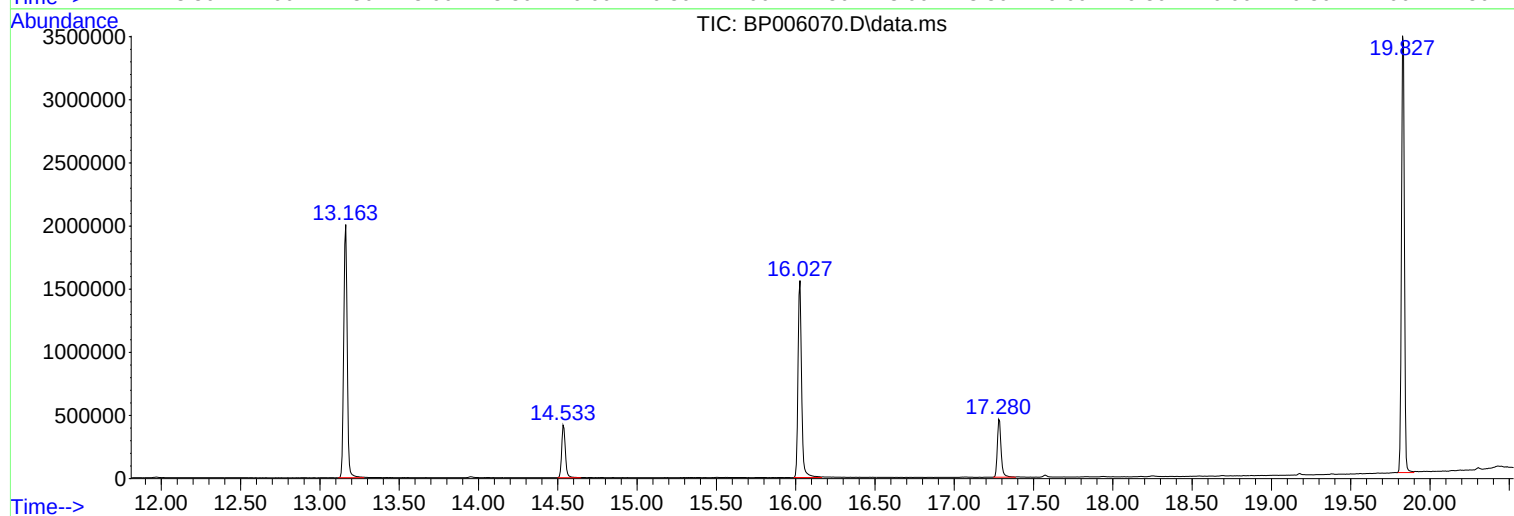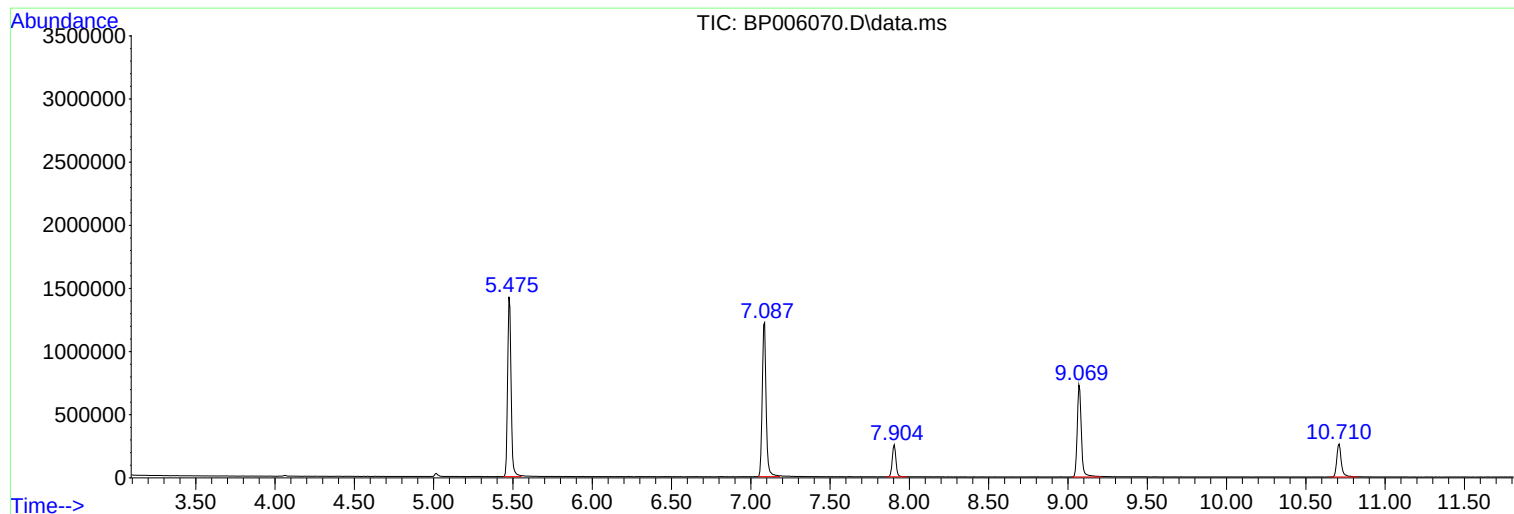

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062821\
Data File : BP006070.D
Acq On : 28 Jun 2021 10:55
Operator : CG/JU
Sample : PB137356BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137356BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062821\
Data File : BP006070.D
Acq On : 28 Jun 2021 10:55
Operator : CG/JU
Sample : PB137356BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137356BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------