
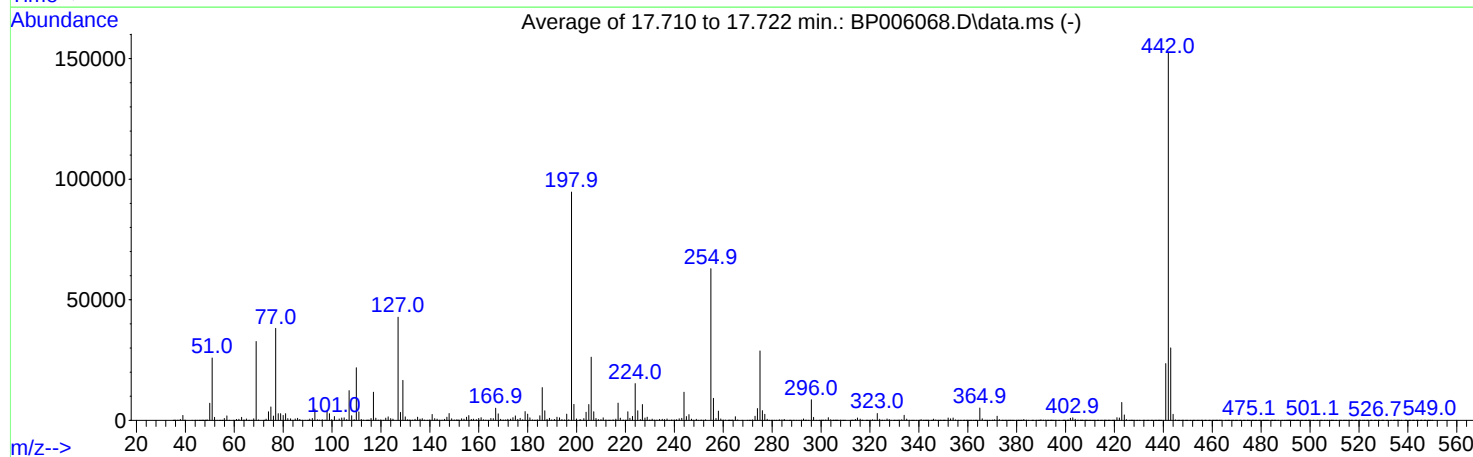


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062821\
 Data File : BP006068.D
 Acq On : 28 Jun 2021 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 28 11:34:30 2021

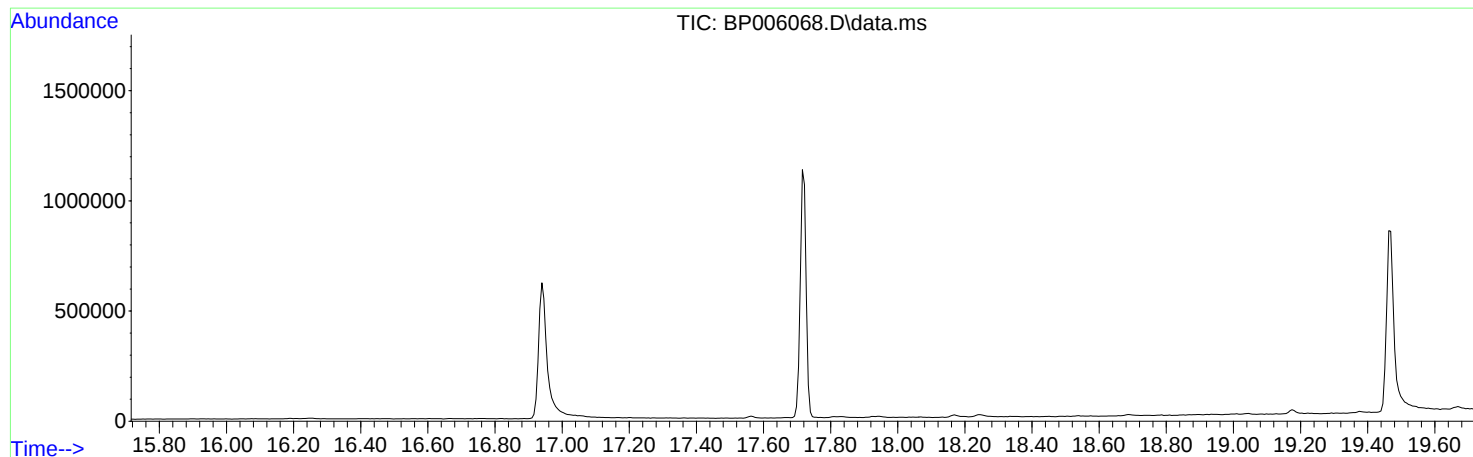




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	25914	PASS
68	69	0.00	2	2.0	652	PASS
69	198	0.00	100	34.6	32726	PASS
70	69	0.00	2	0.7	227	PASS
127	198	10	80	45.2	42769	PASS
197	198	0.00	2	0.3	277	PASS
198	198	100	100	100.0	94664	PASS
199	198	5	9	7.0	6639	PASS
275	198	10	60	30.5	28835	PASS
365	198	1	100	5.4	5114	PASS
441	198	0.01	100	24.9	23576	PASS
442	442	100	100	100.0	152549	PASS
443	442	15	24	19.7	30043	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062821\
 Data File : BP006068.D
 Acq On : 28 Jun 2021 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 28 11:28:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 22 17:52:38 2021
 Response via : Initial Calibration

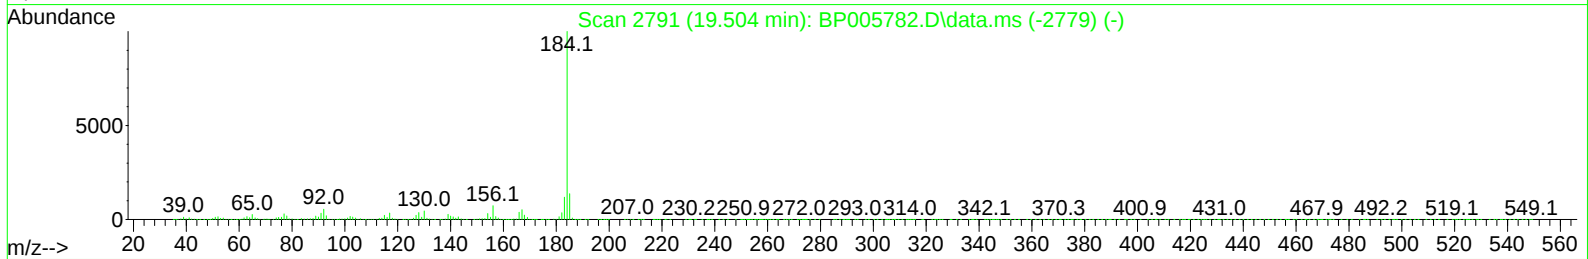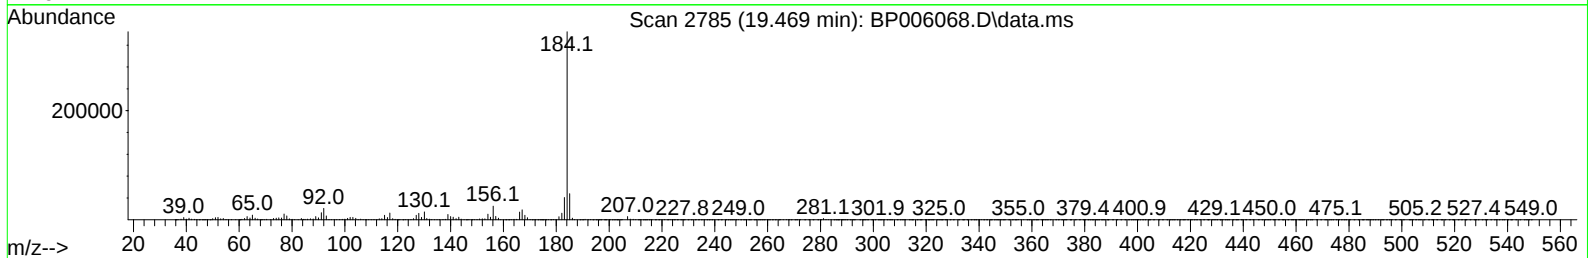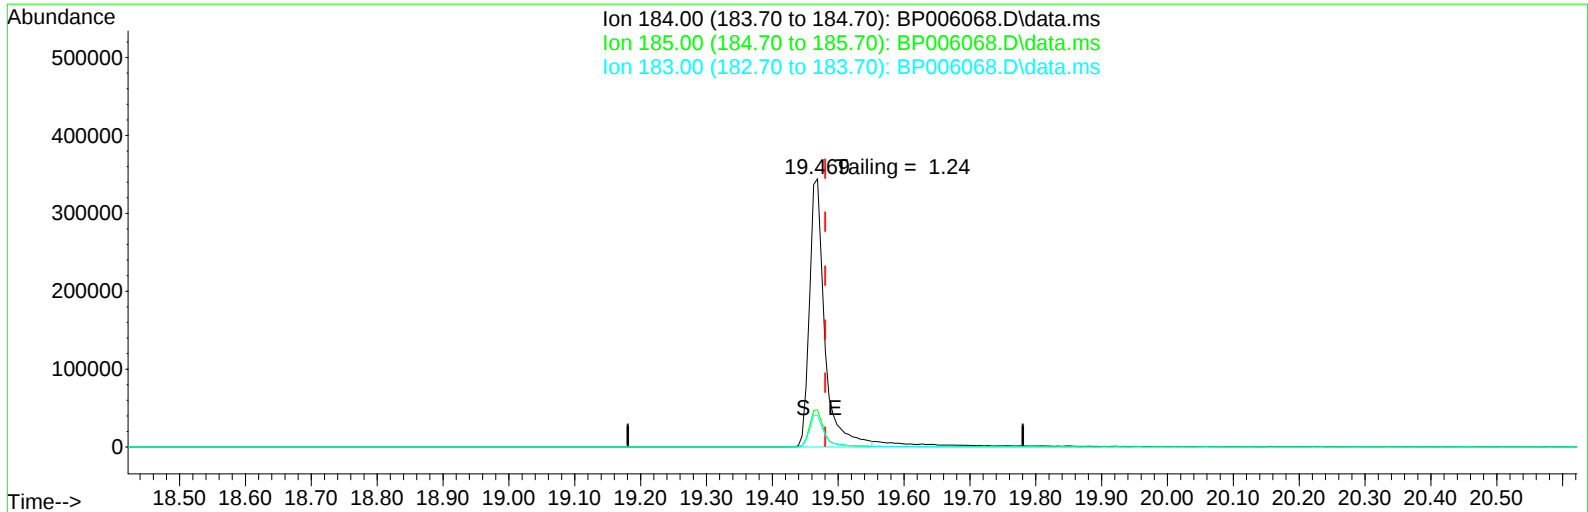

TIC: BP006068.D\data.ms

(77) Benzidine

19.469min (-0.012) 895322.45 ng




response 577526

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.89
183.00	11.90	11.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062821\
Data File : BP006068.D
Acq On : 28 Jun 2021 09:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 28 11:28:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 22 17:52:38 2021
Response via : Initial Calibration

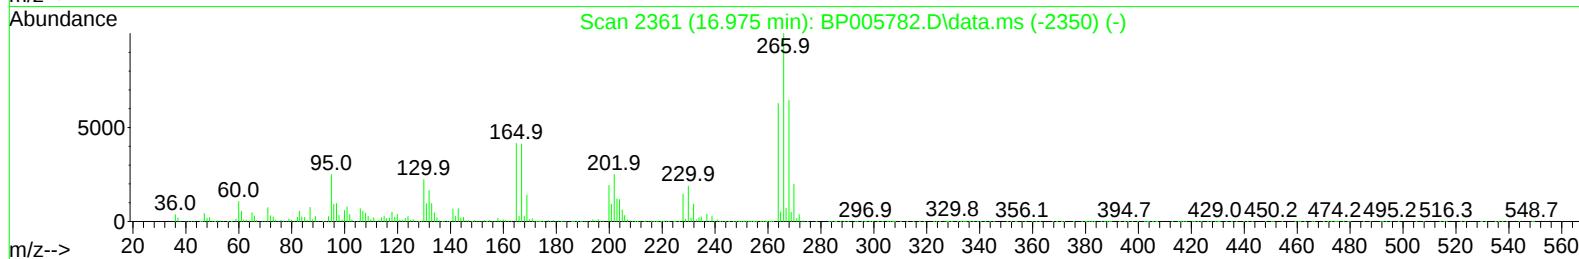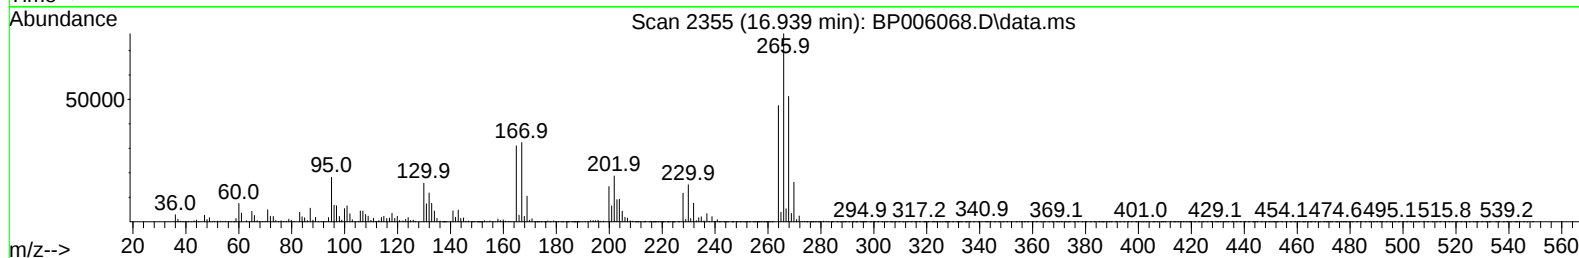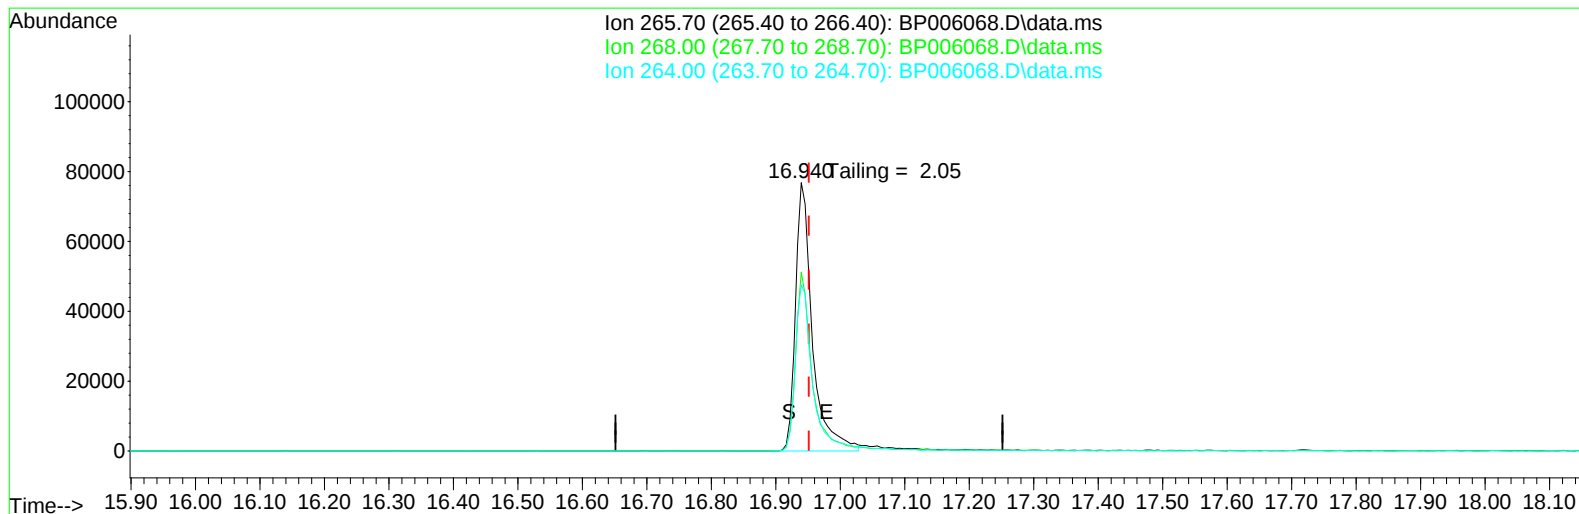

TIC: BP006068.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.012) 712898.25 ng

response 146362

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	66.66
264.00	62.90	61.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
28/6/2021	BNA_P	<u>BP006068.D</u>
Compound Name	Response	Retention Time
DDT	360281	20.65
DDD	1032	20.23
DDE	892	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1924	362205	0.53