

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
 Data File : BP010904.D
 Acq On : 28 Jun 2022 14:54
 Operator : CG/JU
 Sample : PB145854BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK854

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	27	rVB	122450	151084	2.01%	0.187%
2	3.611	85	89	106	rBV	1453570	2044549	27.26%	2.535%
3	3.928	138	143	149	rVB	140672	183018	2.44%	0.227%
4	6.887	638	646	658	rBV	1538631	2364256	31.52%	2.932%
5	7.046	664	673	682	rBV	1269771	1975324	26.33%	2.449%
6	7.240	699	706	719	rBV	1637655	2480213	33.07%	3.075%
7	7.705	776	785	793	rBV	1707453	2617922	34.90%	3.246%
8	8.422	900	907	918	rBV	1888882	2879931	38.39%	3.571%
9	8.869	974	983	991	rBV	1366243	2199537	29.32%	2.727%
10	9.587	1096	1105	1116	rBV	1017845	1626229	21.68%	2.017%
11	10.122	1188	1196	1214	rBV	1581592	2632875	35.10%	3.265%
12	10.498	1251	1260	1268	rBV	2200553	3625109	48.33%	4.495%
13	10.646	1277	1285	1296	rBV	1748841	2842082	37.89%	3.524%
14	11.457	1418	1423	1426	rBV6	4246	8293	0.11%	0.010%
15	12.093	1525	1531	1538	rVB2	31642	53120	0.71%	0.066%
16	12.304	1562	1567	1572	rBV8	6998	13599	0.18%	0.017%
17	13.269	1724	1731	1736	rBV3	17956	31429	0.42%	0.039%
18	13.781	1811	1818	1828	rBV	2462173	3367599	44.90%	4.176%
19	14.051	1857	1864	1884	rBV	2854741	4171585	55.61%	5.173%
20	14.363	1910	1917	1931	rBV	2801413	4047907	53.97%	5.019%
21	14.581	1946	1954	1969	rBV	1059080	1656074	22.08%	2.054%
22	15.363	2080	2087	2101	rBV	3675971	5132810	68.43%	6.365%
23	15.481	2101	2107	2116	rBV	657828	913689	12.18%	1.133%
24	15.604	2123	2128	2132	rVB	40900	59184	0.79%	0.073%
25	16.151	2217	2221	2229	rVB9	12888	19884	0.27%	0.025%
26	16.798	2329	2331	2337	rVB7	7262	10378	0.14%	0.013%
27	16.910	2346	2350	2355	rBV5	6815	13352	0.18%	0.017%
28	17.128	2380	2387	2397	rBV	2955680	4205193	56.06%	5.214%
29	17.228	2398	2404	2420	rVV	3809650	5320016	70.93%	6.597%
30	17.392	2428	2432	2436	rVB6	6040	8571	0.11%	0.011%
31	19.051	2711	2714	2719	rBV3	45800	63527	0.85%	0.079%
32	19.122	2723	2726	2730	rVB	44912	51674	0.69%	0.064%
33	19.480	2781	2787	2793	rBV	4812891	6212359	82.82%	7.703%
34	21.239	3081	3086	3092	rBV2	3881990	4910924	65.47%	6.090%
35	23.457	3456	3463	3472	rVB2	3847137	7500841	100.00%	9.301%
36	23.610	3482	3489	3501	rVB2	2674102	5251301	70.01%	6.512%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
Data File : BP010904.D
Acq On : 28 Jun 2022 14:54
Operator : CG/JU
Sample : PB145854BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK854

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION




Sum of corrected areas: 80645438

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
Data File : BP010904.D
Acq On : 28 Jun 2022 14:54
Operator : CG/JU
Sample : PB145854BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK854

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

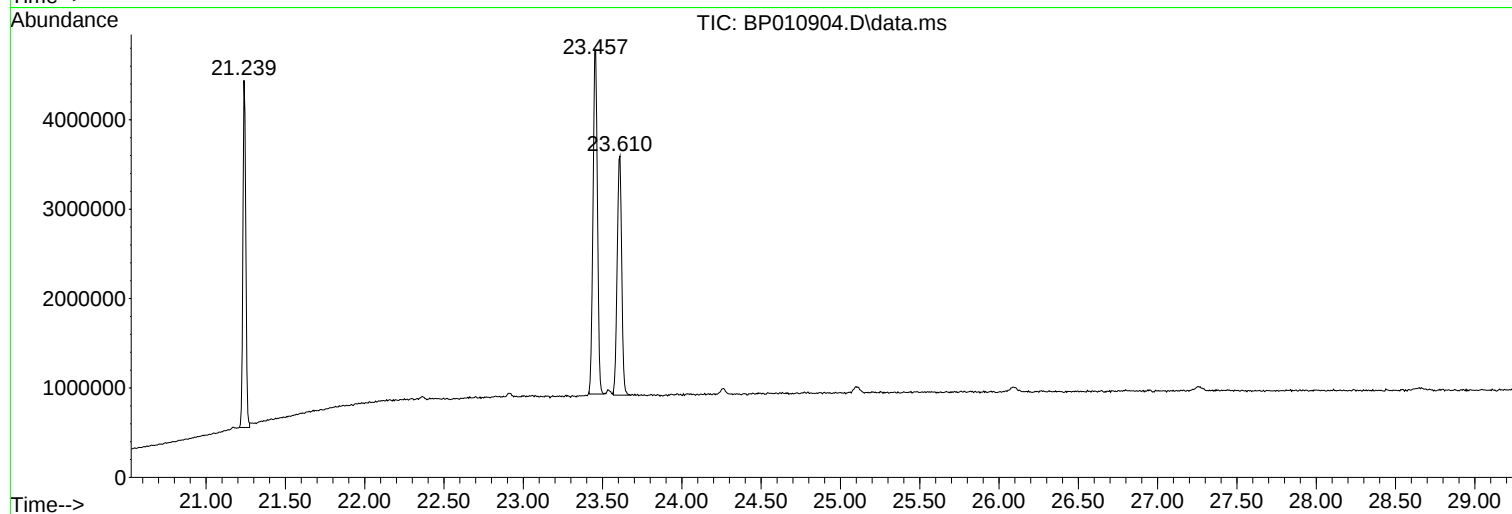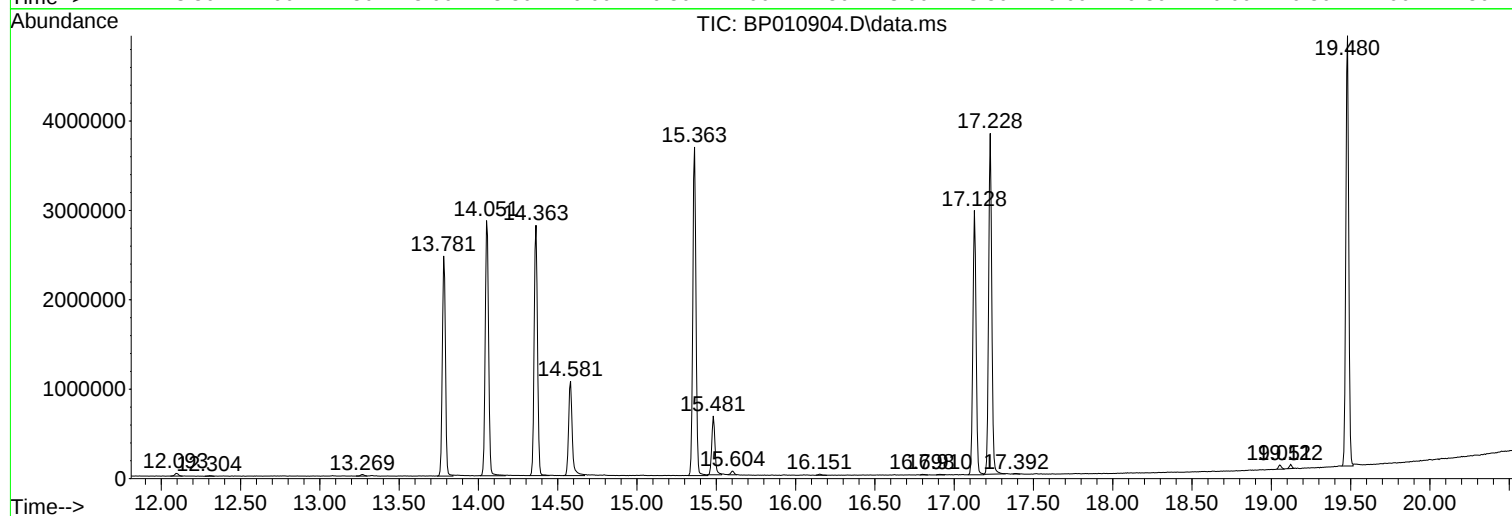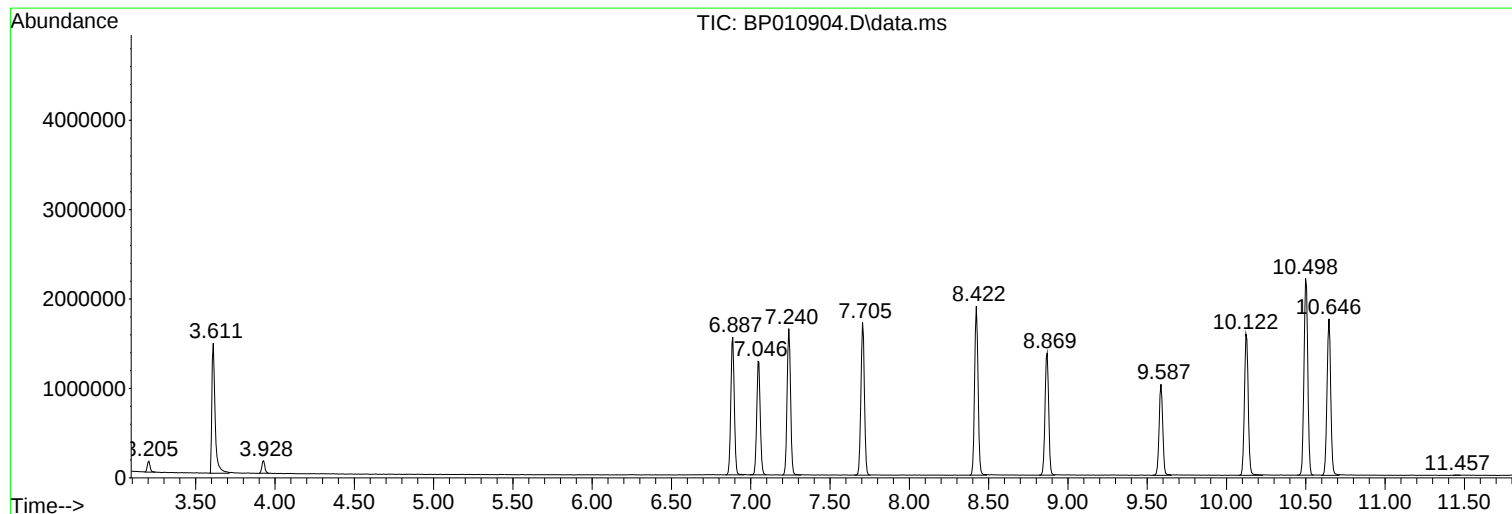

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
Data File : BP010904.D
Acq On : 28 Jun 2022 14:54
Operator : CG/JU
Sample : PB145854BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK854

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
Data File : BP010904.D
Acq On : 28 Jun 2022 14:54
Operator : CG/JU
Sample : PB145854BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK854

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc