

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
 Data File : BP010906.D
 Acq On : 28 Jun 2022 16:01
 Operator : CG/JU
 Sample : N3474-01DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010906.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.475	63	66	75	rBV	26887	40373	0.54%	0.069%
2	3.622	88	91	101	rBV	139170	211325	2.80%	0.360%
3	3.928	138	143	151	rVB	37589	52956	0.70%	0.090%
4	6.199	525	529	537	rVB	35239	50177	0.67%	0.086%
5	6.881	637	645	653	rBV	103337	175292	2.33%	0.299%
6	7.046	666	673	681	rBV	361475	556966	7.39%	0.950%
7	7.240	699	706	713	rBV	352959	534893	7.10%	0.912%
8	7.705	777	785	794	rVV	1880221	2895644	38.41%	4.940%
9	8.422	899	907	915	rVB	300214	474351	6.29%	0.809%
10	8.869	976	983	991	rVB	361236	614138	8.15%	1.048%
11	9.063	1008	1016	1020	rBV4	18643	32486	0.43%	0.055%
12	9.169	1026	1034	1039	rBV2	23312	45951	0.61%	0.078%
13	9.587	1098	1105	1113	rBV	232718	386366	5.13%	0.659%
14	9.910	1153	1160	1170	rBV7	38235	90079	1.19%	0.154%
15	9.999	1170	1175	1179	rBV2	20069	36054	0.48%	0.062%
16	10.122	1187	1196	1205	rBV	422666	709568	9.41%	1.210%
17	10.499	1253	1260	1267	rVV	2381069	3991421	52.95%	6.809%
18	10.552	1267	1269	1276	rVB4	20323	35848	0.48%	0.061%
19	10.646	1276	1285	1299	rBV2	308809	673747	8.94%	1.149%
20	10.804	1306	1312	1318	rVV10	14220	33723	0.45%	0.058%
21	10.887	1320	1326	1329	rVV5	15302	37713	0.50%	0.064%
22	10.922	1329	1332	1338	rVB2	21918	33340	0.44%	0.057%
23	11.099	1356	1362	1370	rVB	99324	169883	2.25%	0.290%
24	11.540	1429	1437	1443	rBV	75718	127685	1.69%	0.218%
25	11.616	1443	1450	1460	rVB	100670	201418	2.67%	0.344%
26	11.928	1497	1503	1508	rVB	35827	59366	0.79%	0.101%
27	12.063	1520	1526	1533	rVV3	99286	162157	2.15%	0.277%
28	12.228	1549	1554	1558	rBV2	22654	42349	0.56%	0.072%
29	12.351	1570	1575	1588	rVB3	90123	221473	2.94%	0.378%
30	12.534	1593	1606	1610	rBV3	56836	138470	1.84%	0.236%
31	12.604	1615	1618	1624	rVB4	24710	46452	0.62%	0.079%
32	12.781	1643	1648	1654	rBV3	30366	54232	0.72%	0.093%
33	12.881	1661	1665	1670	rVB5	39914	61443	0.82%	0.105%
34	13.151	1706	1711	1714	rBV3	35599	58135	0.77%	0.099%
35	13.193	1714	1718	1725	rVV7	40346	89106	1.18%	0.152%
36	13.363	1741	1747	1751	rBV8	18251	33430	0.44%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
 Data File : BP010906.D
 Acq On : 28 Jun 2022 16:01
 Operator : CG/JU
 Sample : N3474-01DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	13.416	1751	1756	1765	rVB2	190771	301640	4.00%	0.515%
38	13.504	1765	1771	1773	rBV5	36761	66480	0.88%	0.113%
39	13.551	1774	1779	1785	rVB5	57037	113270	1.50%	0.193%
40	13.693	1798	1803	1806	rBV4	37153	64755	0.86%	0.110%
41	13.781	1811	1818	1828	rVB	775756	1107260	14.69%	1.889%
42	13.916	1836	1841	1844	rBV	117041	171864	2.28%	0.293%
43	13.951	1844	1847	1853	rVB	91613	130412	1.73%	0.222%
44	14.051	1858	1864	1868	rBV	847998	1274198	16.90%	2.174%
45	14.169	1880	1884	1895	rVB6	37838	75239	1.00%	0.128%
46	14.363	1910	1917	1922	rBV	3086884	4388967	58.22%	7.487%
47	14.428	1922	1928	1936	rVV	5193207	7538363	100.00%	12.859%
48	14.492	1936	1939	1944	rVV2	47244	78497	1.04%	0.134%
49	14.581	1948	1954	1961	rVB4	57778	113391	1.50%	0.193%
50	14.675	1965	1970	1974	rVV	112143	147939	1.96%	0.252%
51	14.763	1982	1985	1992	rVB2	41187	66029	0.88%	0.113%
52	14.840	1994	1998	2002	rVV3	24440	32561	0.43%	0.056%
53	14.987	2016	2023	2028	rBV4	51606	100792	1.34%	0.172%
54	15.228	2061	2064	2074	rVB2	70671	123159	1.63%	0.210%
55	15.357	2074	2086	2091	rBV	1098367	1655050	21.96%	2.823%
56	15.416	2091	2096	2103	rVB	1690155	2315087	30.71%	3.949%
57	15.481	2103	2107	2110	rBV	112263	156234	2.07%	0.267%
58	15.539	2114	2117	2121	rVV2	134479	193126	2.56%	0.329%
59	15.575	2121	2123	2127	rVV	57775	63409	0.84%	0.108%
60	15.628	2128	2132	2135	rVB2	49502	67292	0.89%	0.115%
61	15.716	2143	2147	2148	rBV3	22652	32164	0.43%	0.055%
62	15.810	2159	2163	2164	rBV	22674	32309	0.43%	0.055%
63	15.863	2166	2172	2180	rVV2	170194	365644	4.85%	0.624%
64	15.951	2184	2187	2192	rVB	29855	41019	0.54%	0.070%
65	16.098	2206	2212	2219	rVB3	151522	257499	3.42%	0.439%
66	16.216	2227	2232	2240	rBV	97698	154882	2.05%	0.264%
67	16.286	2240	2244	2251	rBV3	73053	114729	1.52%	0.196%
68	16.386	2256	2261	2263	rBV5	35782	57022	0.76%	0.097%
69	16.428	2265	2268	2272	rVV	67946	100524	1.33%	0.171%
70	16.475	2273	2276	2289	rVB5	32412	63167	0.84%	0.108%
71	16.575	2290	2293	2297	rBV	29841	38029	0.50%	0.065%
72	16.863	2336	2342	2345	rBV8	23093	49401	0.66%	0.084%
73	16.910	2346	2350	2351	rVV	68304	89626	1.19%	0.153%
74	16.939	2351	2355	2364	rVB2	124998	212740	2.82%	0.363%
75	17.045	2369	2373	2378	rVB3	39998	60493	0.80%	0.103%
76	17.128	2378	2387	2392	rBV	3057497	4379279	58.09%	7.470%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
 Data File : BP010906.D
 Acq On : 28 Jun 2022 16:01
 Operator : CG/JU
 Sample : N3474-01DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

77	17.222	2398	2403	2407	rBV2	1031450	1524383	20.22%	2.600%
78	17.257	2407	2409	2416	rVV	229481	300688	3.99%	0.513%
79	17.322	2416	2420	2430	rVB3	63384	131676	1.75%	0.225%
80	17.510	2446	2452	2453	rBV3	79069	120060	1.59%	0.205%
81	17.539	2453	2457	2464	rVB	493820	706627	9.37%	1.205%
82	17.881	2512	2515	2521	rVB4	39101	61095	0.81%	0.104%
83	17.969	2526	2530	2534	rBV	85351	106038	1.41%	0.181%
84	18.045	2539	2543	2548	rBV	134677	184731	2.45%	0.315%
85	18.122	2549	2556	2561	rVB4	154995	270924	3.59%	0.462%
86	18.192	2562	2568	2573	rBV2	221925	340604	4.52%	0.581%
87	18.281	2580	2583	2585	rBV	22053	32007	0.42%	0.055%
88	18.339	2590	2593	2597	rVB3	43196	52153	0.69%	0.089%
89	18.380	2597	2600	2604	rVB4	36241	45059	0.60%	0.077%
90	18.433	2604	2609	2615	rBV3	75559	120153	1.59%	0.205%
91	18.486	2615	2618	2622	rBV2	50850	65346	0.87%	0.111%
92	18.528	2622	2625	2630	rBV3	22679	39398	0.52%	0.067%
93	19.151	2727	2731	2737	rVB	467154	602956	8.00%	1.029%
94	19.475	2781	2786	2790	rBV	1334565	1832883	24.31%	3.127%
95	19.875	2850	2854	2859	rBV2	115477	179117	2.38%	0.306%
96	19.939	2861	2865	2871	rBV	275292	401095	5.32%	0.684%
97	20.569	2969	2972	2979	rVB	181844	251756	3.34%	0.429%
98	21.239	3081	3086	3094	rBV	3761634	4640517	61.56%	7.916%
99	23.445	3456	3461	3470	rVB2	998851	1875311	24.88%	3.199%
100	23.604	3481	3488	3498	rVB2	2502294	5165851	68.53%	8.812%




Sum of corrected areas: 58621979

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
Data File : BP010906.D
Acq On : 28 Jun 2022 16:01
Operator : CG/JU
Sample : N3474-01DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

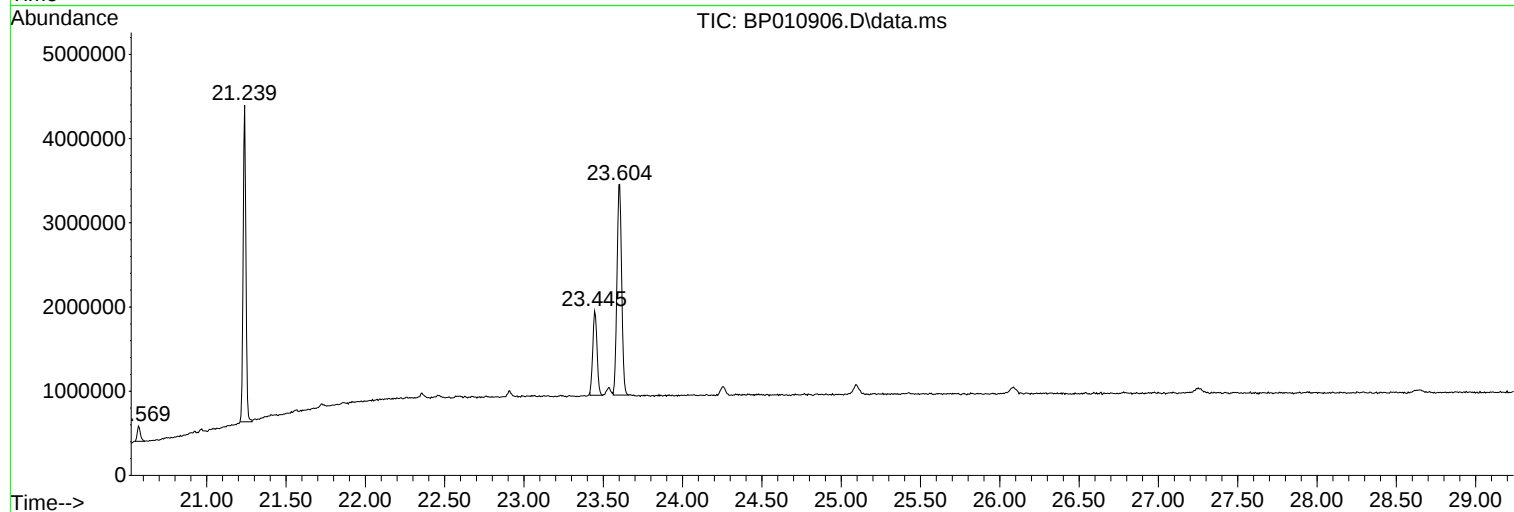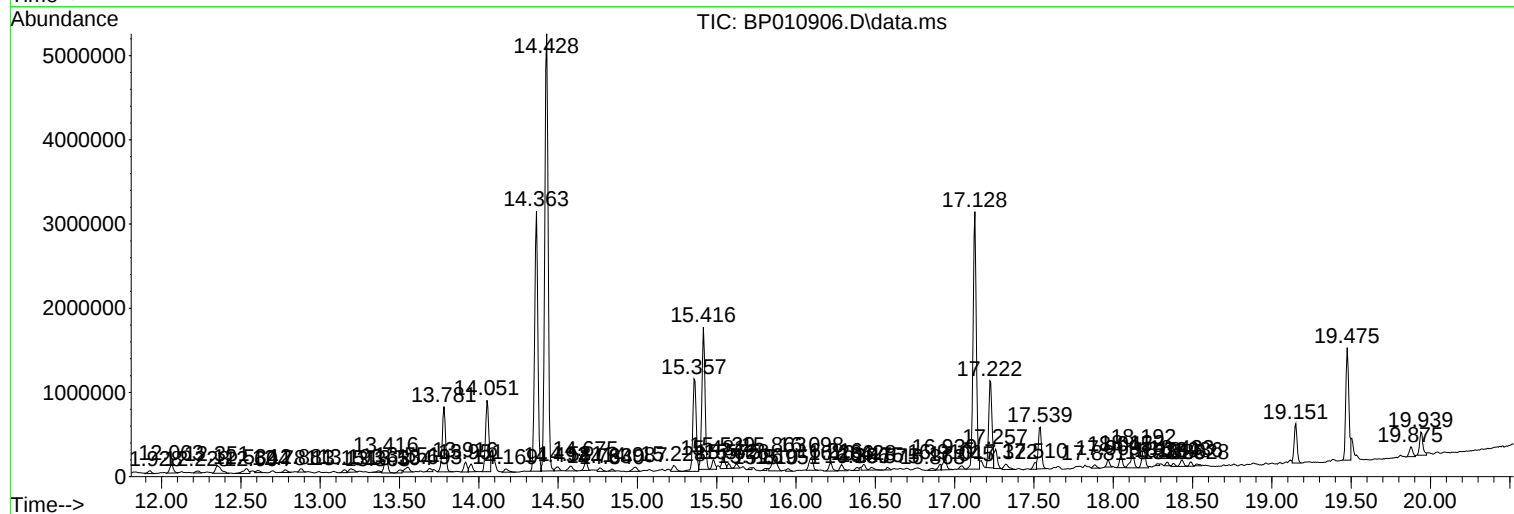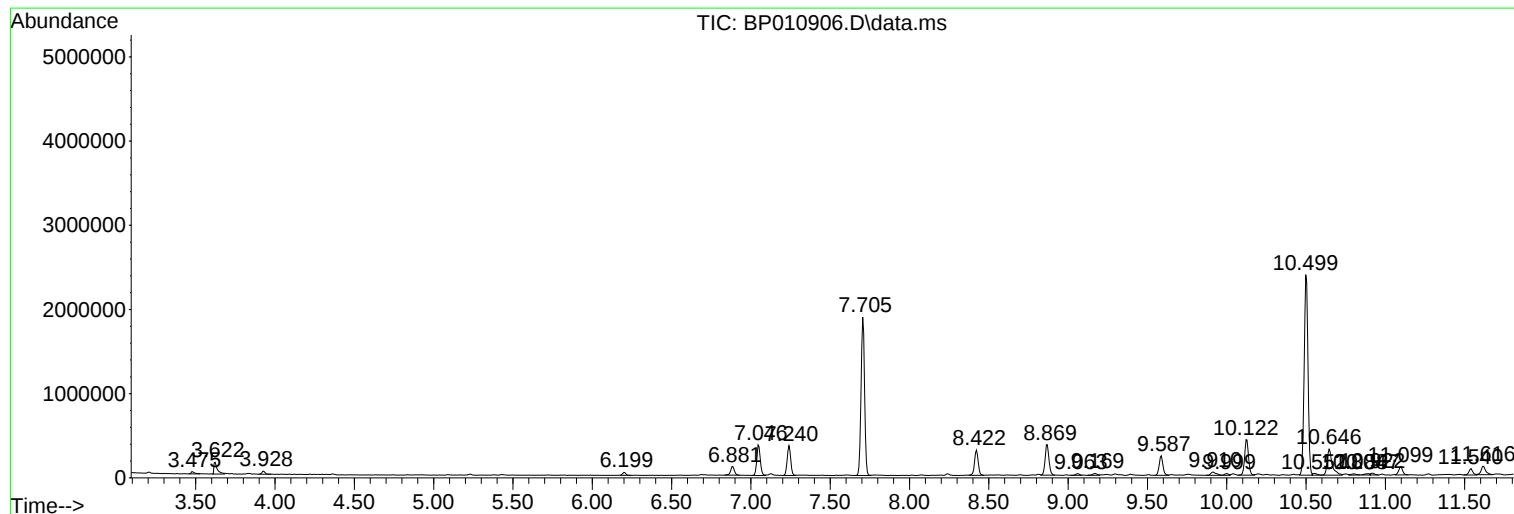

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
Data File : BP010906.D
Acq On : 28 Jun 2022 16:01
Operator : CG/JU
Sample : N3474-01DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
Data File : BP010906.D
Acq On : 28 Jun 2022 16:01
Operator : CG/JU
Sample : N3474-01DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc