

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
 Data File : BP010907.D
 Acq On : 28 Jun 2022 16:35
 Operator : CG/JU
 Sample : N3425-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	15	20	26	rBV	103775	131025	2.19%	0.169%
2	3.475	62	66	77	rBV	78252	113769	1.90%	0.147%
3	3.611	85	89	113	rBV	1256033	1777279	29.70%	2.295%
4	3.834	123	127	131	rVB2	15446	20338	0.34%	0.026%
5	3.928	138	143	147	rBV	42538	58107	0.97%	0.075%
6	4.834	292	297	301	rBV2	8535	15382	0.26%	0.020%
7	4.881	302	305	309	rVV	8438	11657	0.19%	0.015%
8	5.428	394	398	401	rBV4	7611	8940	0.15%	0.012%
9	6.711	613	616	620	rBV4	6749	8879	0.15%	0.011%
10	6.881	638	645	656	rBV	1446389	2241774	37.46%	2.895%
11	7.046	667	673	683	rVV	1242462	1910390	31.92%	2.467%
12	7.122	683	686	692	rVB2	13550	21418	0.36%	0.028%
13	7.240	699	706	718	rBV	1552271	2334770	39.01%	3.015%
14	7.705	777	785	794	rBV	1824874	2721726	45.48%	3.514%
15	8.422	900	907	921	rBV	1864216	2858330	47.76%	3.691%
16	8.869	974	983	992	rBV	1346715	2195730	36.69%	2.835%
17	8.993	1000	1004	1008	rVV7	5929	7783	0.13%	0.010%
18	9.040	1008	1012	1017	rVB8	5865	9073	0.15%	0.012%
19	9.587	1097	1105	1116	rBV	1011755	1584733	26.48%	2.046%
20	9.822	1140	1145	1150	rBV8	4245	7856	0.13%	0.010%
21	10.122	1187	1196	1208	rBV	1581479	2582556	43.15%	3.335%
22	10.299	1222	1226	1231	rBV5	7774	11955	0.20%	0.015%
23	10.499	1253	1260	1268	rBV	2281841	3800116	63.50%	4.907%
24	10.646	1275	1285	1303	rBV	1732276	2873807	48.02%	3.711%
25	11.310	1394	1398	1403	rBV7	6564	9831	0.16%	0.013%
26	11.475	1422	1426	1434	rVV7	3970	10429	0.17%	0.013%
27	11.857	1488	1491	1498	rVB9	2870	6225	0.10%	0.008%
28	12.010	1514	1517	1523	rBV7	4075	8026	0.13%	0.010%
29	12.093	1526	1531	1542	rVB2	33497	61786	1.03%	0.080%
30	12.722	1635	1638	1643	rVB6	5062	7030	0.12%	0.009%
31	12.975	1677	1681	1685	rBV5	7294	11543	0.19%	0.015%
32	13.081	1696	1699	1703	rVB6	4724	6291	0.11%	0.008%
33	13.269	1728	1731	1735	rVB6	4785	7283	0.12%	0.009%
34	13.781	1809	1818	1828	rBV	2608405	3521067	58.83%	4.547%
35	14.051	1855	1864	1879	rBV	3065206	4391815	73.38%	5.671%
36	14.363	1909	1917	1929	rBV	2893272	4253160	71.07%	5.492%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
 Data File : BP010907.D
 Acq On : 28 Jun 2022 16:35
 Operator : CG/JU
 Sample : N3425-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	14.575	1947	1953	1969	rBV	832095	1289384	21.54%	1.665%
38	14.792	1986	1990	1997	rVB9	15679	22773	0.38%	0.029%
39	15.175	2052	2055	2058	rBV3	7178	10020	0.17%	0.013%
40	15.363	2080	2087	2099	rBV	3670896	5326429	89.00%	6.878%
41	15.481	2102	2107	2120	rVV	503361	741809	12.40%	0.958%
42	15.598	2123	2127	2138	rVB2	43004	73388	1.23%	0.095%
43	16.034	2196	2201	2202	rBV5	4232	6156	0.10%	0.008%
44	16.151	2217	2221	2228	rVB7	14827	25640	0.43%	0.033%
45	16.798	2328	2331	2336	rVB7	6346	9889	0.17%	0.013%
46	16.910	2343	2350	2353	rBV6	10379	22161	0.37%	0.029%
47	17.128	2380	2387	2397	rVV	3026678	4198404	70.15%	5.421%
48	17.228	2397	2404	2418	rVV	3497016	5062722	84.60%	6.537%
49	17.328	2418	2421	2427	rVB7	30276	46236	0.77%	0.060%
50	17.822	2500	2505	2509	rVB2	34721	46045	0.77%	0.059%
51	19.051	2711	2714	2719	rBV3	42003	49754	0.83%	0.064%
52	19.116	2722	2725	2733	rVV	36184	55973	0.94%	0.072%
53	19.475	2781	2786	2793	rBV	4221122	5361077	89.58%	6.923%
54	20.963	3036	3039	3046	rBV	391380	532137	8.89%	0.687%
55	21.239	3081	3086	3094	rBV	3459799	4277948	71.48%	5.524%
56	23.451	3455	3462	3471	rVB2	3096263	5984651	100.00%	7.728%
57	23.604	3481	3488	3499	rVB2	2346928	4699690	78.53%	6.068%




Sum of corrected areas: 77444165

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
Data File : BP010907.D
Acq On : 28 Jun 2022 16:35
Operator : CG/JU
Sample : N3425-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

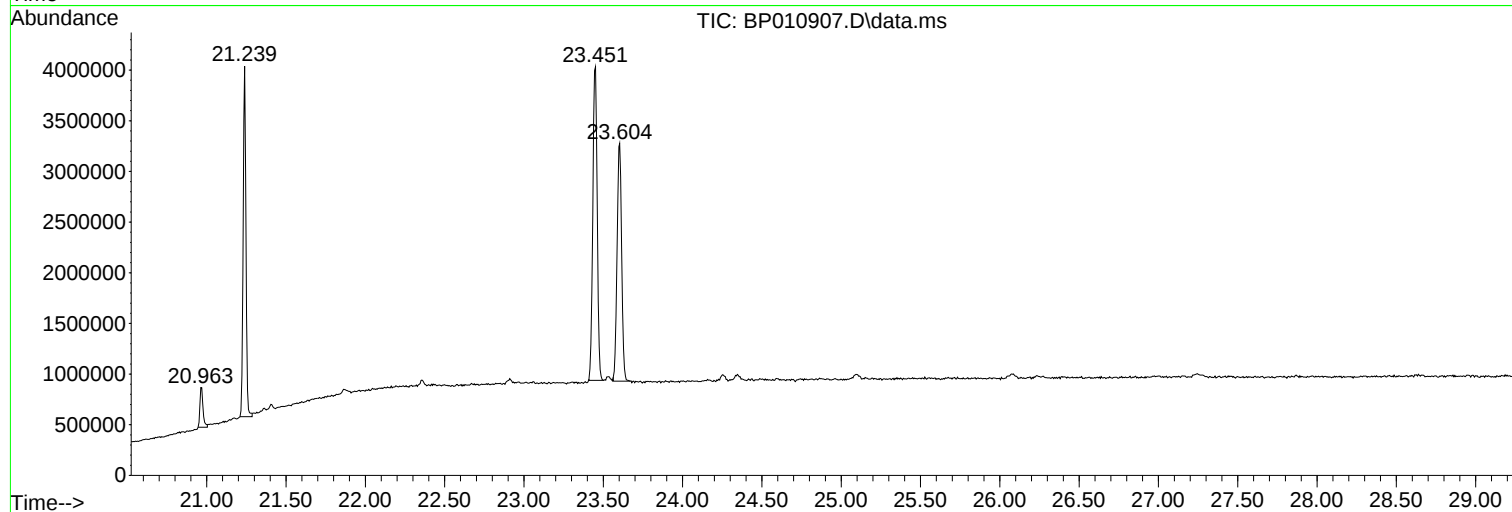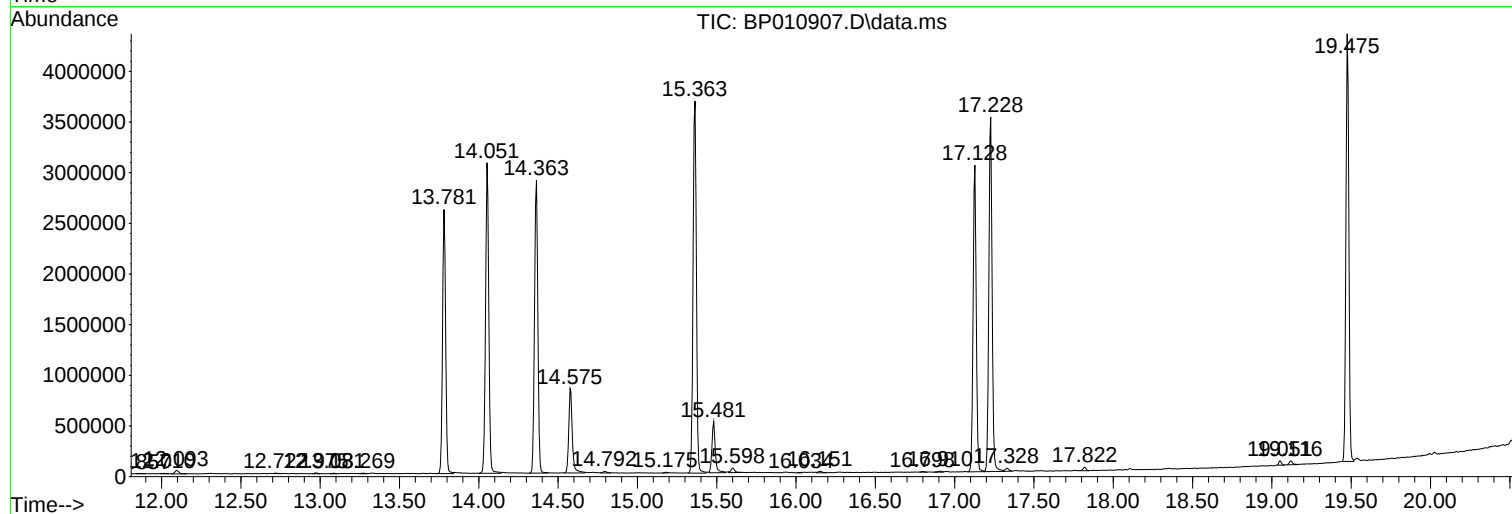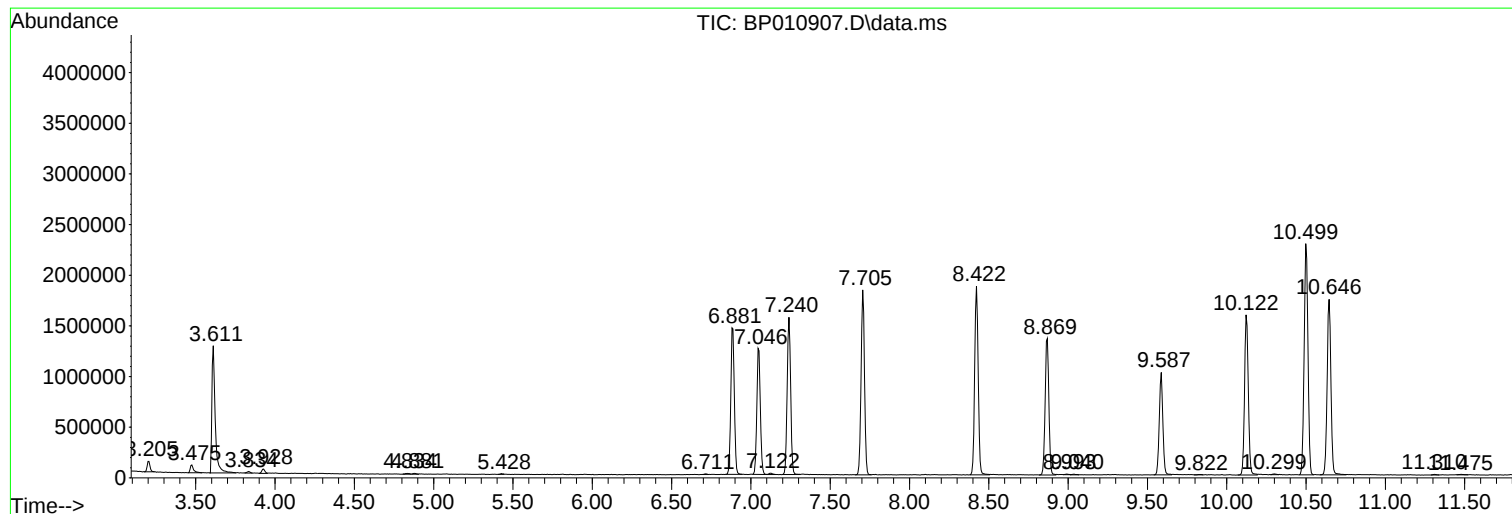

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
Data File : BP010907.D
Acq On : 28 Jun 2022 16:35
Operator : CG/JU
Sample : N3425-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.963	2.49 ng/ul	532137	Chrysene-d12	21.239

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	5-Eicosene, (E)-		280	C20H40	074685-30-6	98
2	1-Nonadecene		266	C19H38	018435-45-5	97
3	1-Nonadecene		266	C19H38	018435-45-5	96
4	Cyclotetracosane		336	C24H48	000297-03-0	94
5	Trifluoroacetoxy hexadecane		338	C18H33F3O2	006222-03-3	94

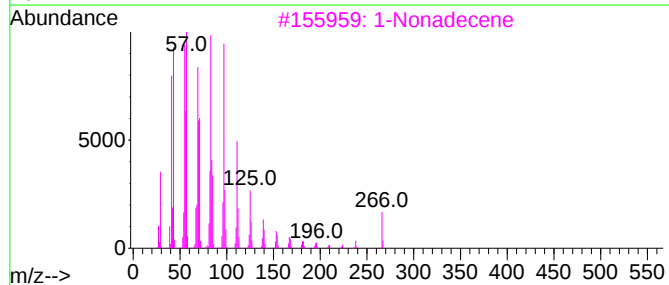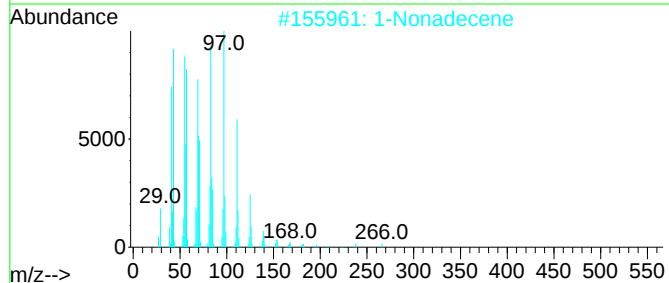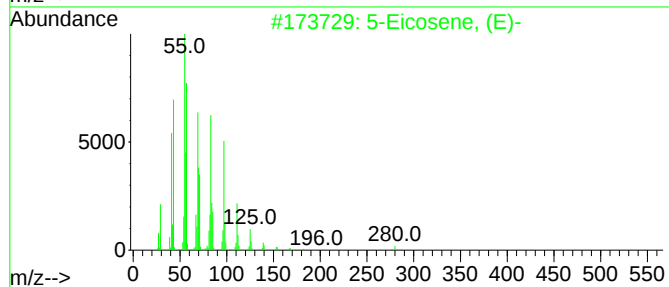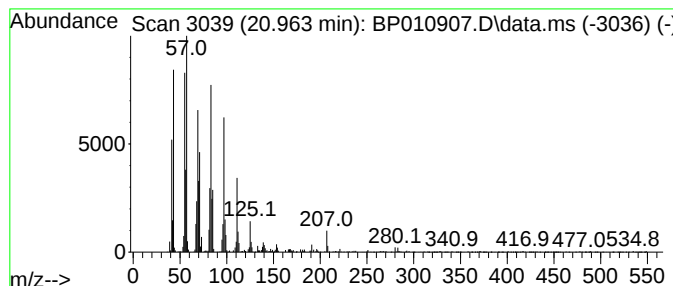

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062822\
Data File : BP010907.D
Acq On : 28 Jun 2022 16:35
Operator : CG/JU
Sample : N3425-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.963	2.5	ng/u1	532137	5	21.239	4277950	20.0