

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
 Data File : BP006091.D
 Acq On : 29 Jun 2021 14:41
 Operator : CG/JU
 Sample : PB137373BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB137373BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	400	406	428	rBV	1324443	2029831	49.36%	11.053%
2	7.087	673	680	701	rBV	1127082	1959649	47.66%	10.670%
3	7.905	811	819	832	rBV	243427	403539	9.81%	2.197%
4	9.069	1008	1017	1035	rBV	703990	1227226	29.84%	6.682%
5	10.704	1288	1295	1315	rBV	265686	506788	12.32%	2.759%
6	13.163	1705	1713	1728	rBV	1781179	2795470	67.98%	15.222%
7	14.534	1939	1946	1959	rBV	400934	625570	15.21%	3.406%
8	16.028	2193	2200	2230	rBV	1395318	2221496	54.02%	12.096%
9	17.286	2406	2414	2430	rBV	451512	709707	17.26%	3.864%
10	19.833	2841	2847	2860	rBV	3487168	4112081	100.00%	22.391%
11	21.363	3102	3107	3116	rBV	618543	847014	20.60%	4.612%
12	23.768	3510	3516	3528	rVB2	446679	926881	22.54%	5.047%




Sum of corrected areas: 18365252

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
Data File : BP006091.D
Acq On : 29 Jun 2021 14:41
Operator : CG/JU
Sample : PB137373BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137373BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

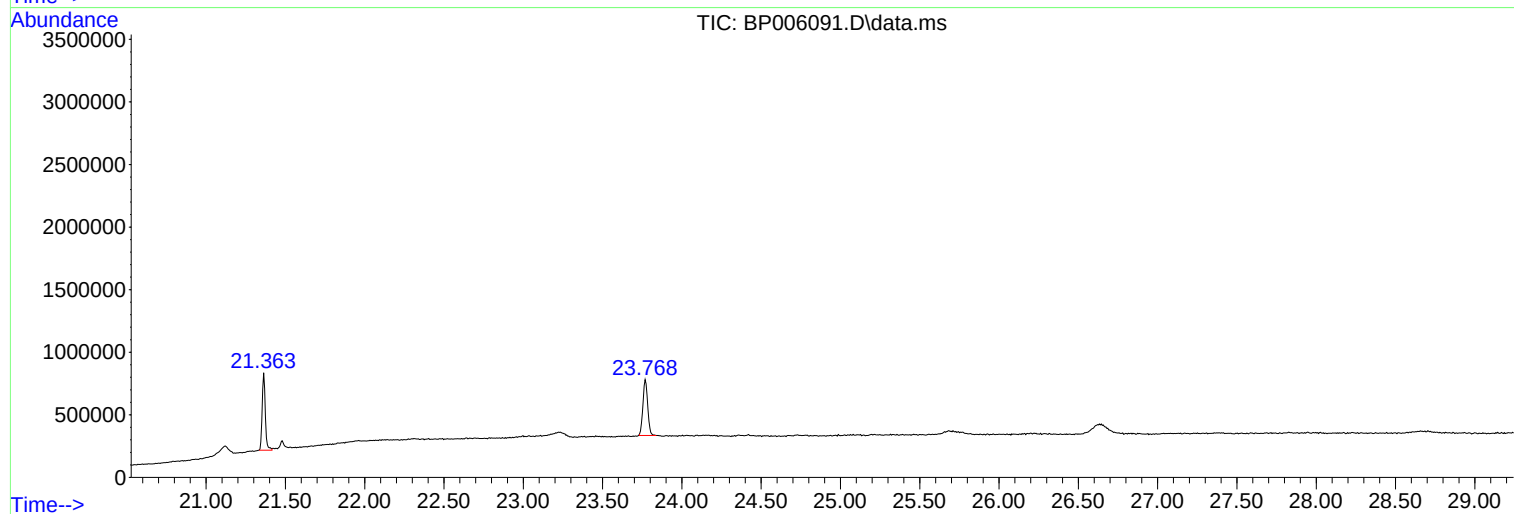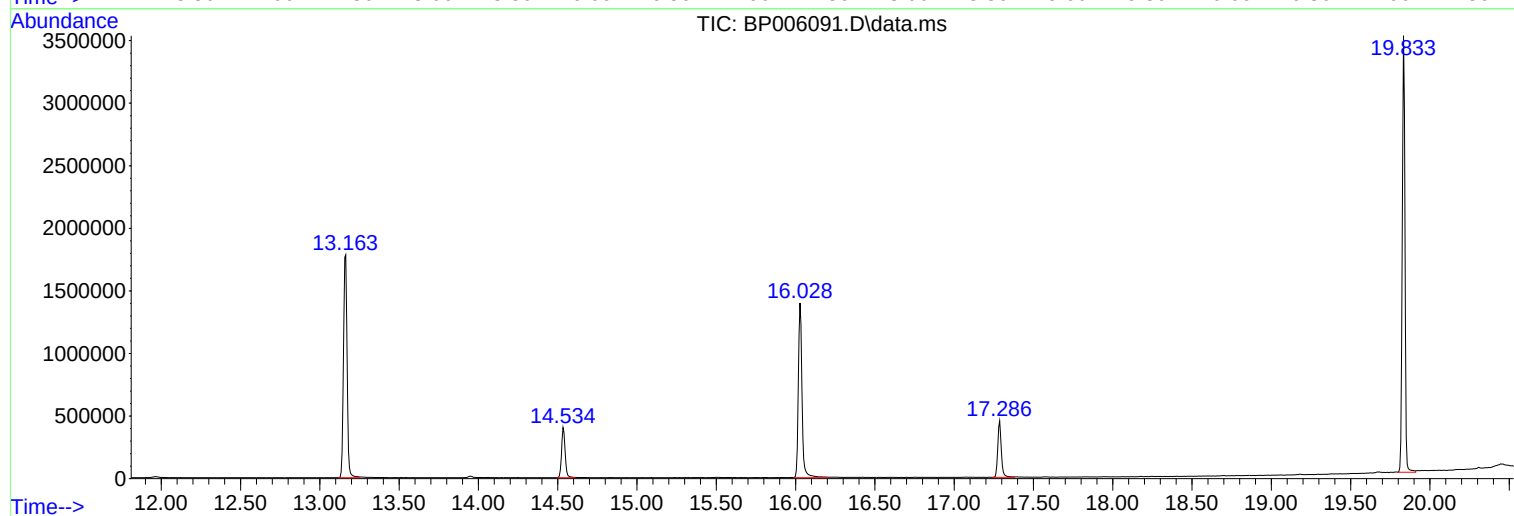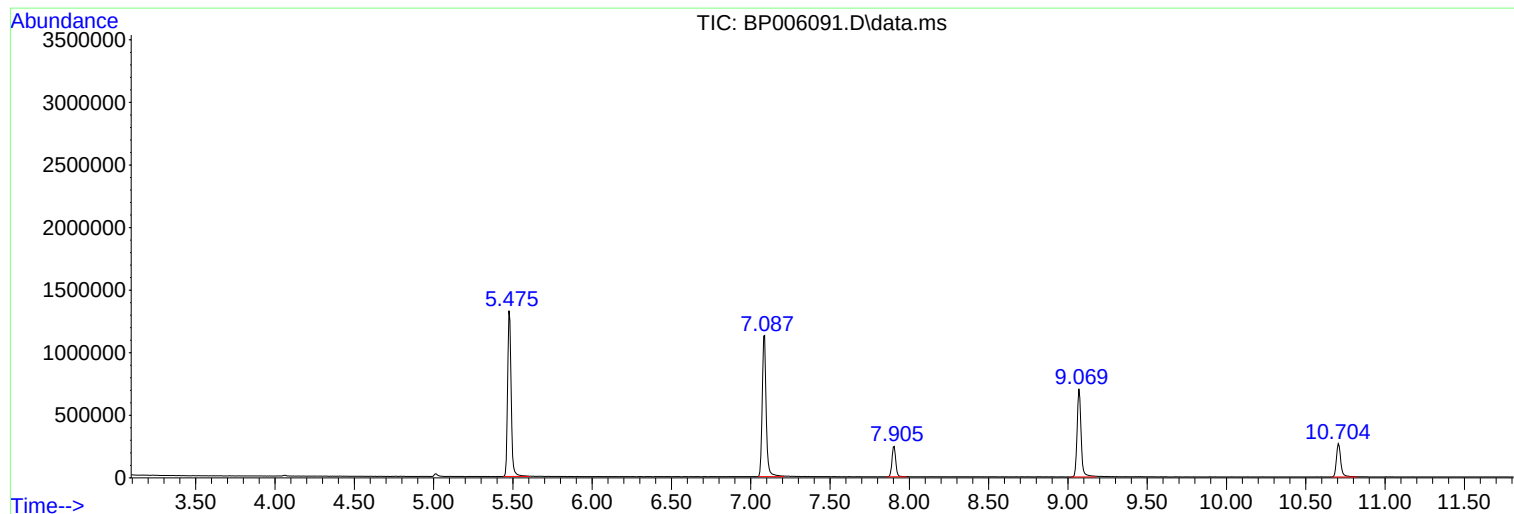

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
Data File : BP006091.D
Acq On : 29 Jun 2021 14:41
Operator : CG/JU
Sample : PB137373BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137373BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
Data File : BP006091.D
Acq On : 29 Jun 2021 14:41
Operator : CG/JU
Sample : PB137373BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137373BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------