

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
 Data File : BP006094.D
 Acq On : 29 Jun 2021 16:24
 Operator : CG/JU
 Sample : PB137375BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB137375BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	400	406	422	rBV	1340989	2028013	48.78%	10.979%
2	7.081	672	679	711	rBV	1144995	1956834	47.07%	10.594%
3	7.899	811	818	832	rBV	238882	399299	9.61%	2.162%
4	9.069	1009	1017	1038	rBV	688495	1228105	29.54%	6.649%
5	10.704	1286	1295	1316	rBV	263856	509949	12.27%	2.761%
6	13.157	1703	1712	1729	rBV	1838595	2820892	67.86%	15.272%
7	14.534	1939	1946	1963	rBV	385579	624358	15.02%	3.380%
8	16.028	2193	2200	2222	rBV	1426901	2207430	53.10%	11.951%
9	17.281	2407	2413	2429	rBV	422483	702149	16.89%	3.801%
10	19.833	2841	2847	2857	rBV	3426562	4157081	100.00%	22.506%
11	21.363	3102	3107	3116	rBV	594671	865183	20.81%	4.684%
12	23.763	3509	3515	3527	rVB	450303	972021	23.38%	5.262%




Sum of corrected areas: 18471314

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
Data File : BP006094.D
Acq On : 29 Jun 2021 16:24
Operator : CG/JU
Sample : PB137375BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137375BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

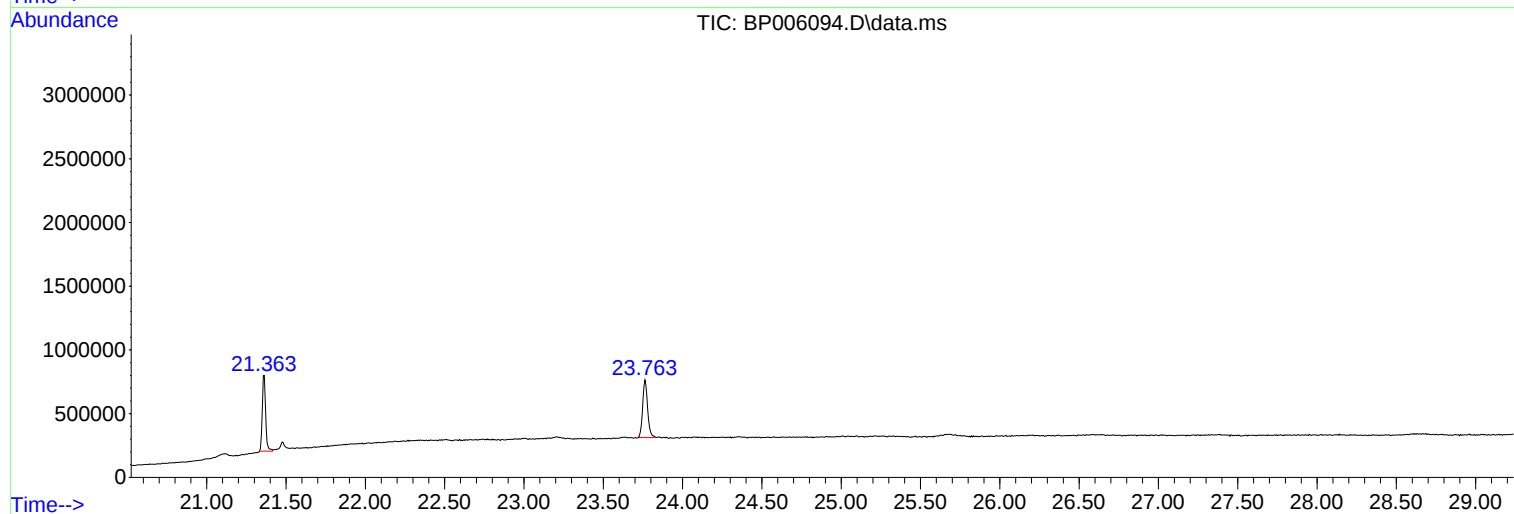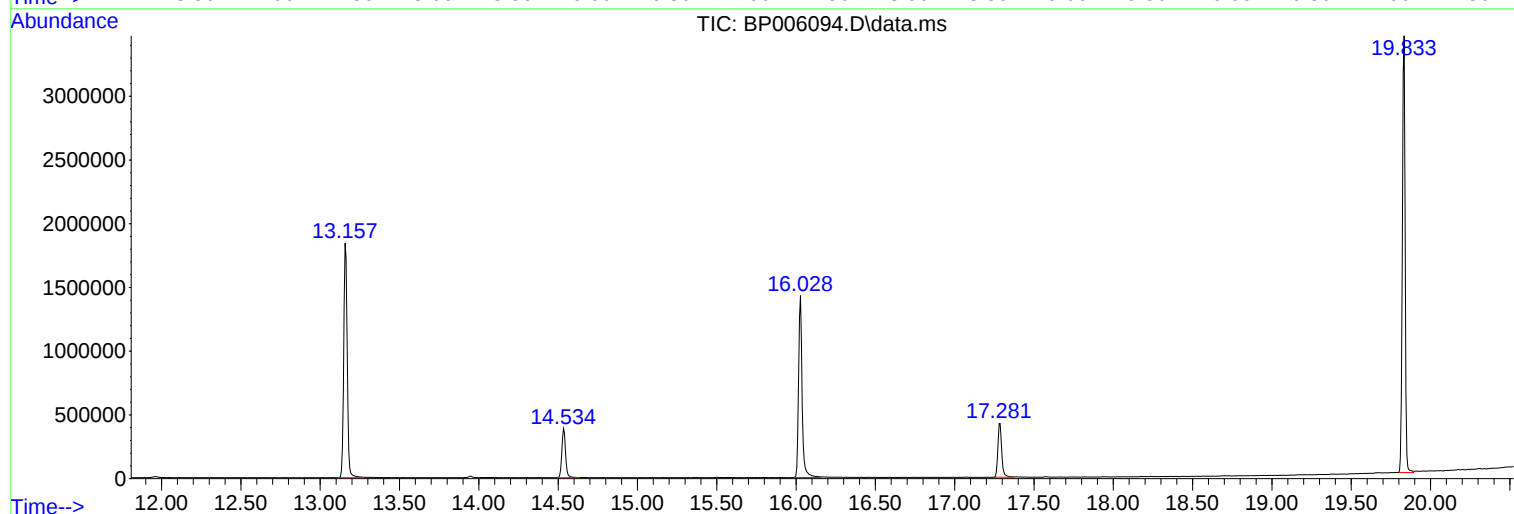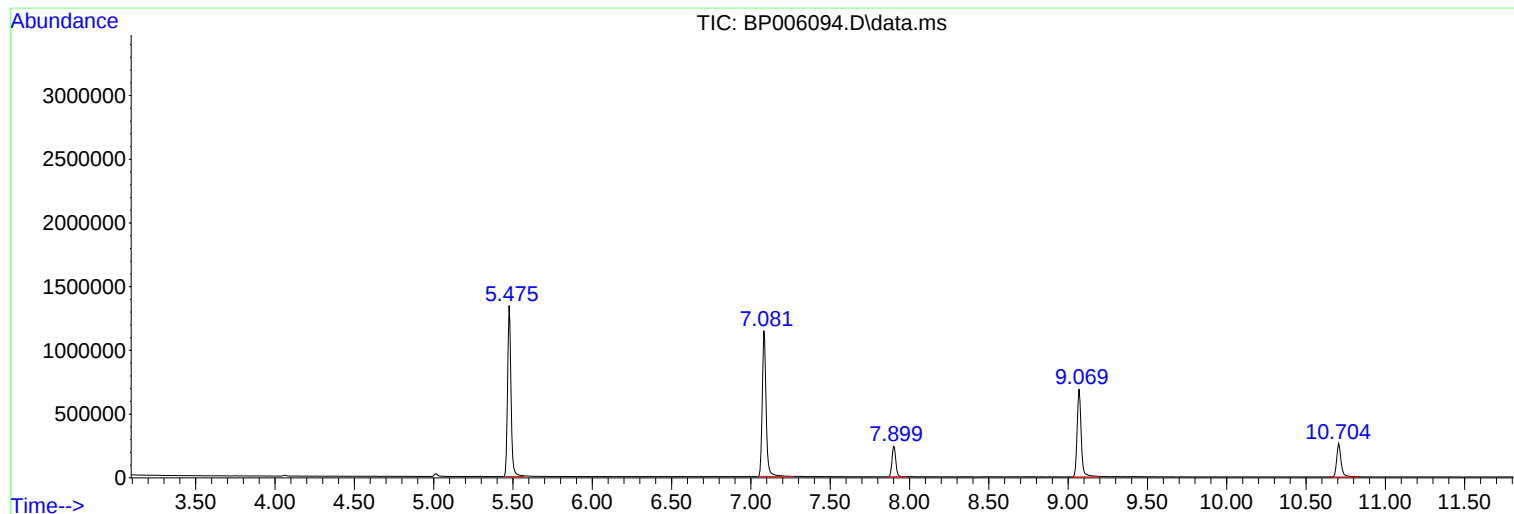

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
Data File : BP006094.D
Acq On : 29 Jun 2021 16:24
Operator : CG/JU
Sample : PB137375BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137375BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
Data File : BP006094.D
Acq On : 29 Jun 2021 16:24
Operator : CG/JU
Sample : PB137375BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137375BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------