

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
 Data File : BP006104.D
 Acq On : 29 Jun 2021 22:36
 Operator : CG/JU
 Sample : M2884-01 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OK-03-062821

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.011	321	327	333	rBV	12371	21506	1.03%	0.121%
2	5.481	399	407	421	rBV	675832	1083139	52.10%	6.073%
3	7.087	673	680	697	rBV	597510	1065780	51.27%	5.976%
4	7.899	811	818	826	rBV	502677	808003	38.87%	4.530%
5	9.069	1009	1017	1031	rBV	372031	682869	32.85%	3.829%
6	10.510	1257	1262	1268	rBV4	9954	23270	1.12%	0.130%
7	10.705	1286	1295	1309	rBV	610860	1070415	51.49%	6.002%
8	13.157	1704	1712	1724	rBV	1091266	1633619	78.58%	9.160%
9	14.422	1920	1927	1935	rBV4	20332	54653	2.63%	0.306%
10	14.534	1939	1946	1953	rVV	886323	1334154	64.18%	7.481%
11	14.593	1953	1956	1964	rVB2	15924	30086	1.45%	0.169%
12	16.022	2193	2199	2215	rBV	790194	1241418	59.72%	6.961%
13	16.234	2232	2235	2237	rBV3	17383	21801	1.05%	0.122%
14	17.028	2367	2370	2374	rBV3	20438	20981	1.01%	0.118%
15	17.281	2407	2413	2417	rBV	1033915	1475995	71.00%	8.276%
16	17.322	2417	2420	2427	rVB	236501	319676	15.38%	1.792%
17	17.410	2432	2435	2441	rVB	38798	59283	2.85%	0.332%
18	17.692	2479	2483	2491	rVB	30887	48904	2.35%	0.274%
19	18.157	2556	2562	2565	rBV2	58596	108362	5.21%	0.608%
20	18.192	2565	2568	2573	rVB	44259	66000	3.17%	0.370%
21	18.334	2588	2592	2596	rBV2	53170	74194	3.57%	0.416%
22	18.439	2607	2610	2613	rBV3	22546	27135	1.31%	0.152%
23	18.628	2639	2642	2646	rBV	23557	26467	1.27%	0.148%
24	18.675	2647	2650	2655	rVV2	42102	48506	2.33%	0.272%
25	19.281	2749	2753	2759	rBV	601010	799082	38.44%	4.480%
26	19.604	2804	2808	2810	rBV2	116266	162652	7.82%	0.912%
27	19.633	2810	2813	2822	rVB	465362	627824	30.20%	3.520%
28	19.828	2841	2846	2851	rBV	1736151	2078842	100.00%	11.656%
29	21.351	3100	3105	3109	rBV2	1154427	1592688	76.61%	8.930%
30	23.757	3509	3514	3520	rVB2	648428	1227747	59.06%	6.884%




Sum of corrected areas: 17835051

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
Data File : BP006104.D
Acq On : 29 Jun 2021 22:36
Operator : CG/JU
Sample : M2884-01 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-03-062821

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

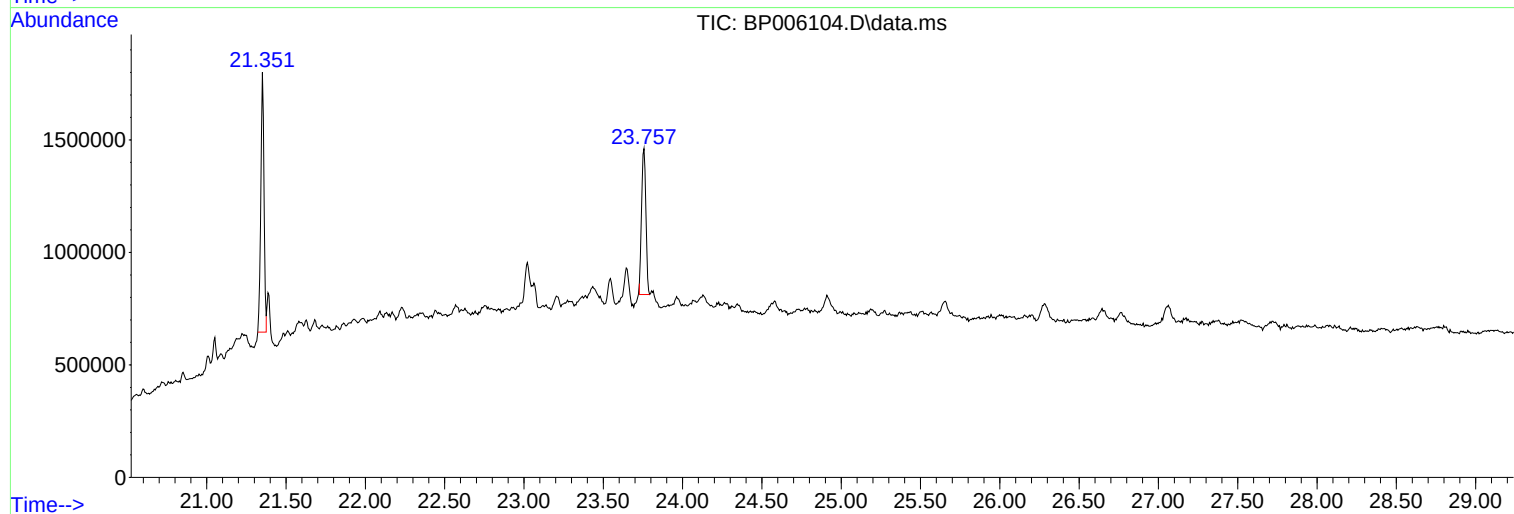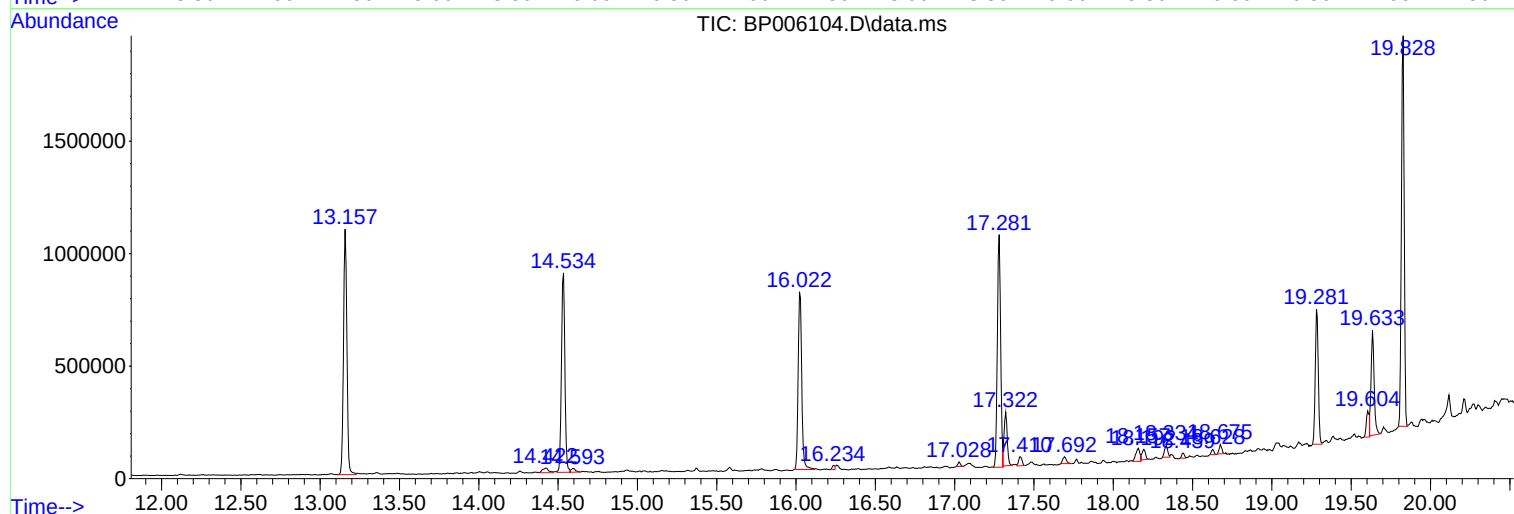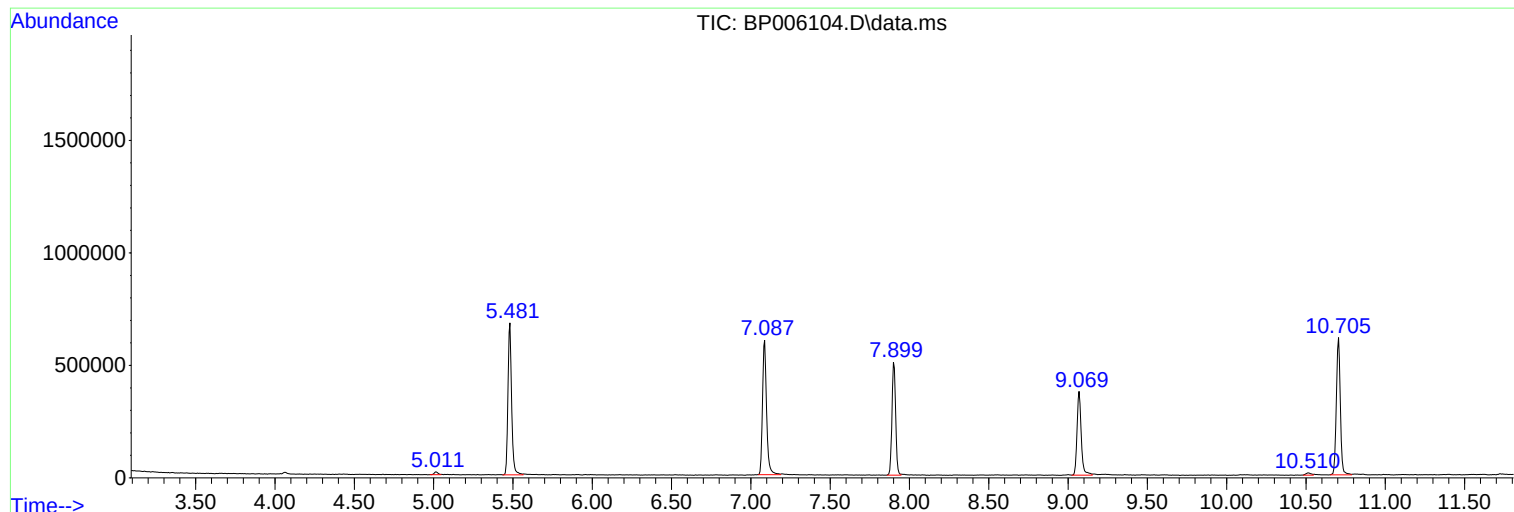

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
Data File : BP006104.D
Acq On : 29 Jun 2021 22:36
Operator : CG/JU
Sample : M2884-01 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-03-062821

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
Data File : BP006104.D
Acq On : 29 Jun 2021 22:36
Operator : CG/JU
Sample : M2884-01 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-03-062821

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
