
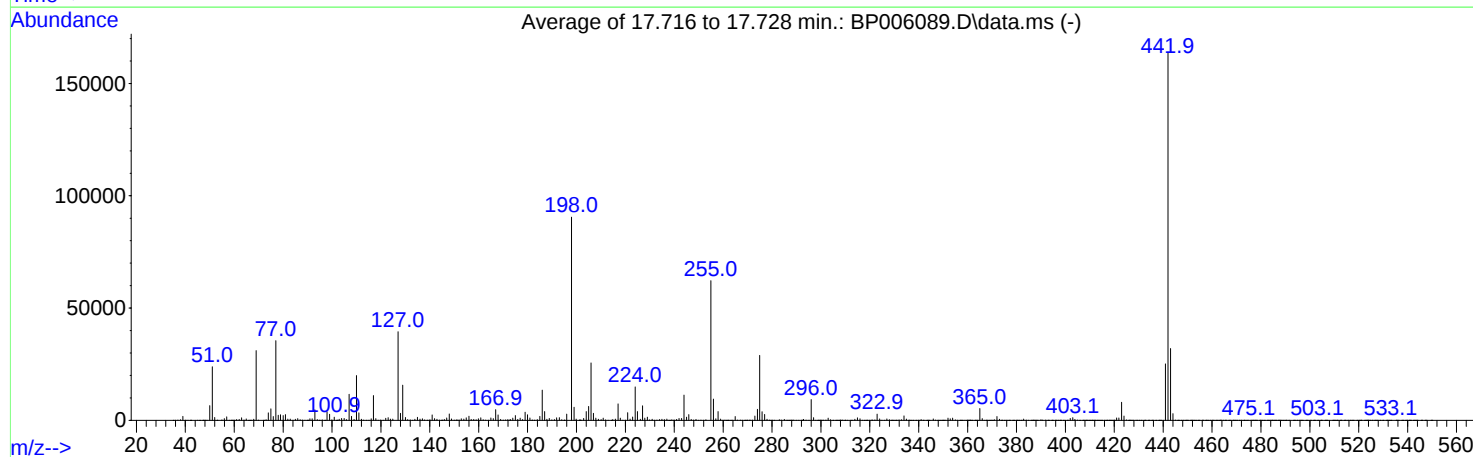


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
 Data File : BP006089.D
 Acq On : 29 Jun 2021 12:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 28 11:34:30 2021

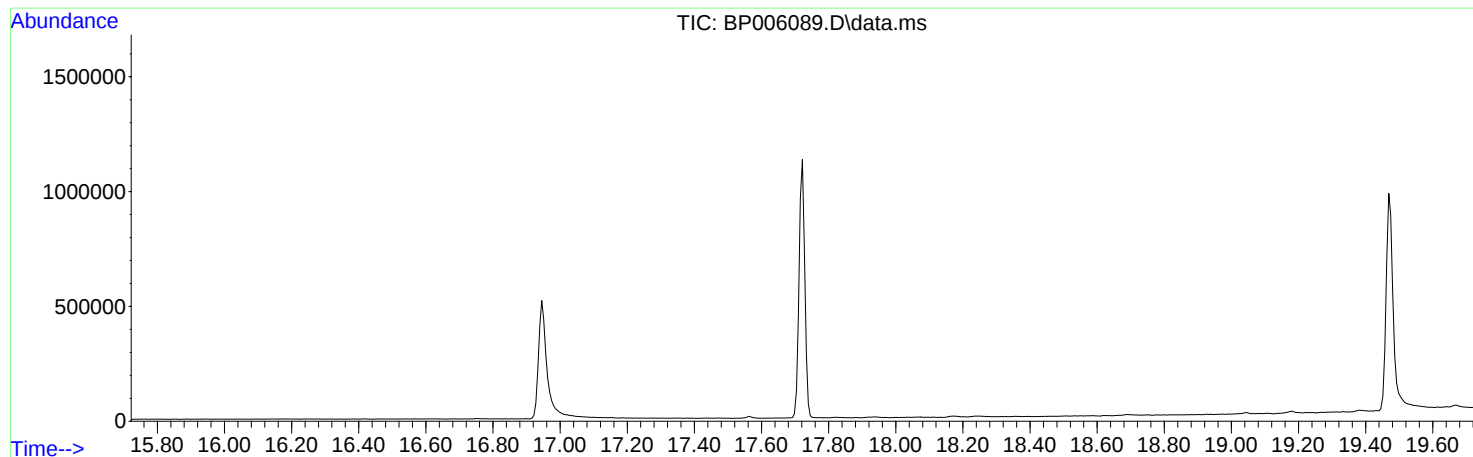




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	23893	PASS
68	69	0.00	2	1.7	525	PASS
69	198	0.00	100	34.3	31036	PASS
70	69	0.00	2	0.5	170	PASS
127	198	10	80	43.6	39451	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90514	PASS
199	198	5	9	6.5	5839	PASS
275	198	10	60	32.0	28920	PASS
365	198	1	100	5.9	5296	PASS
441	198	0.01	100	27.8	25143	PASS
442	442	100	100	100.0	163796	PASS
443	442	15	24	19.5	31968	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
 Data File : BP006089.D
 Acq On : 29 Jun 2021 12:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 29 13:45:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 11:34:30 2021
 Response via : Initial Calibration

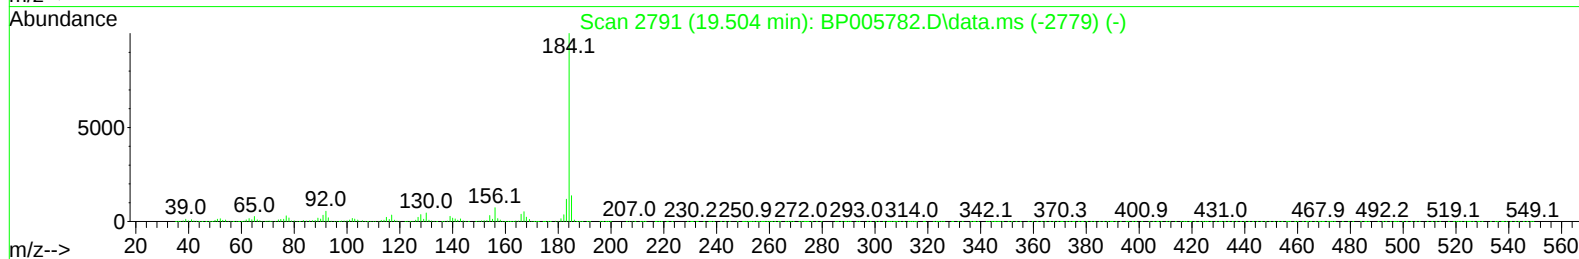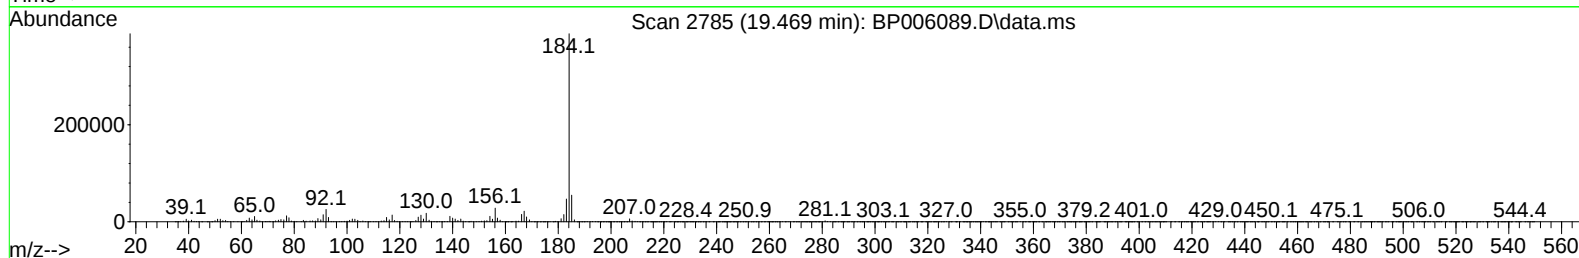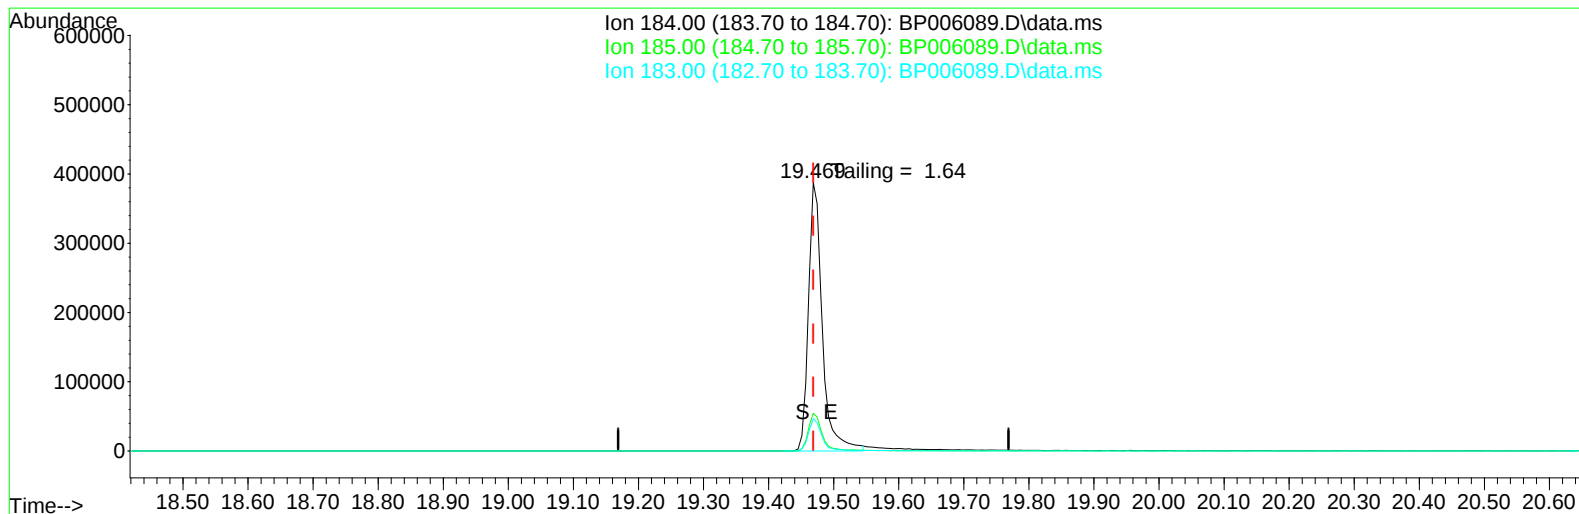

TIC: BP006089.D\data.ms

(77) Benzidine

19.469min (+ 0.000) 477462.16 ng




response 596102

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.11
183.00	11.90	12.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062921\
Data File : BP006089.D
Acq On : 29 Jun 2021 12:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 29 13:45:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 28 11:34:30 2021
Response via : Initial Calibration

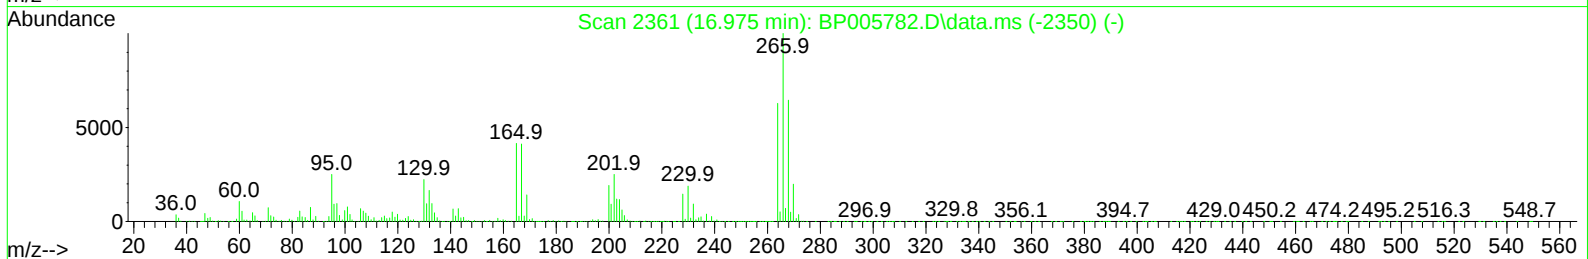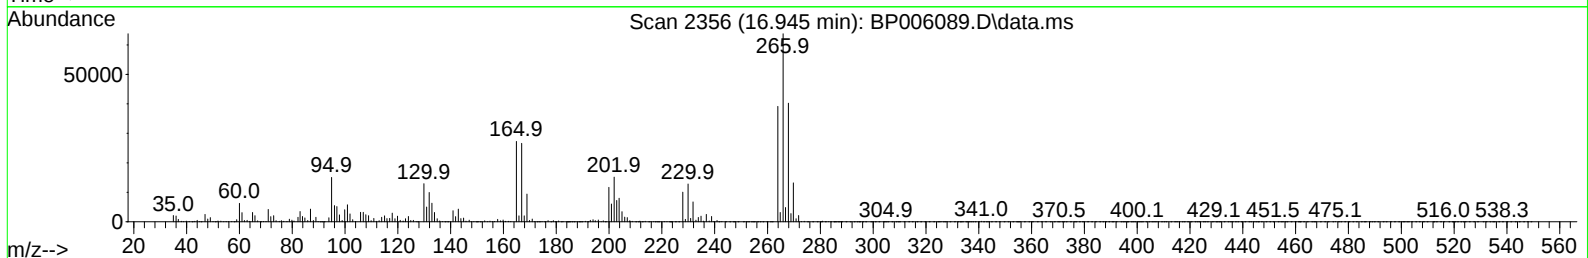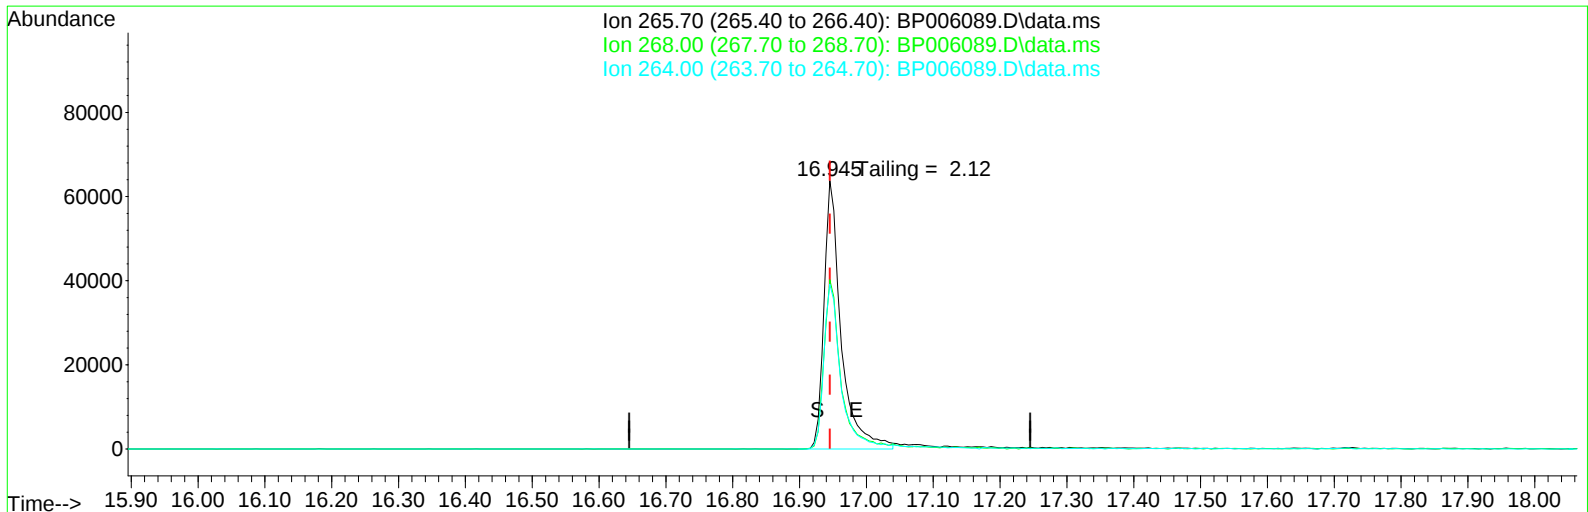

TIC: BP006089.D\data.ms

(70) Pentachlorophenol (C)

16.945min (+ 0.000) 964624.73 ng

response 115525

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.09
264.00	62.90	61.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/29/2021	BNA_P	<u>BP006089.D</u>
Compound Name	Response	Retention Time
DDT	345412	20.66
DDD	2843	20.23
DDE	1126	19.74
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3969	349381	1.14