
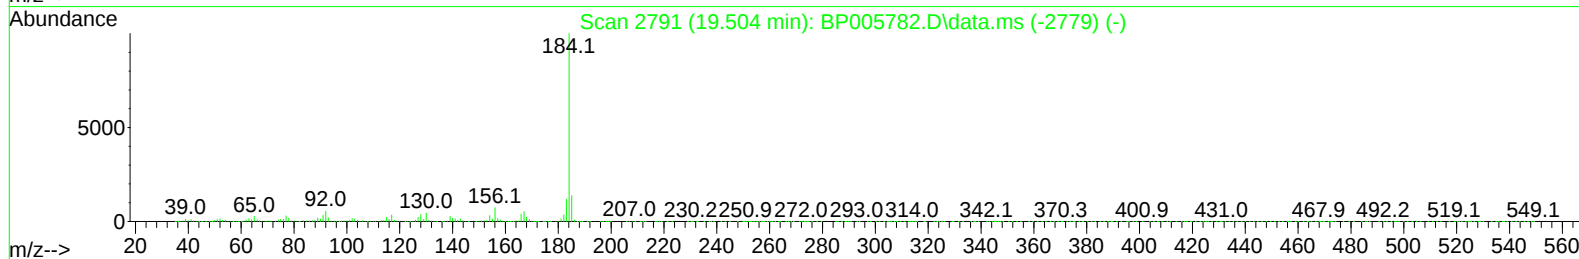
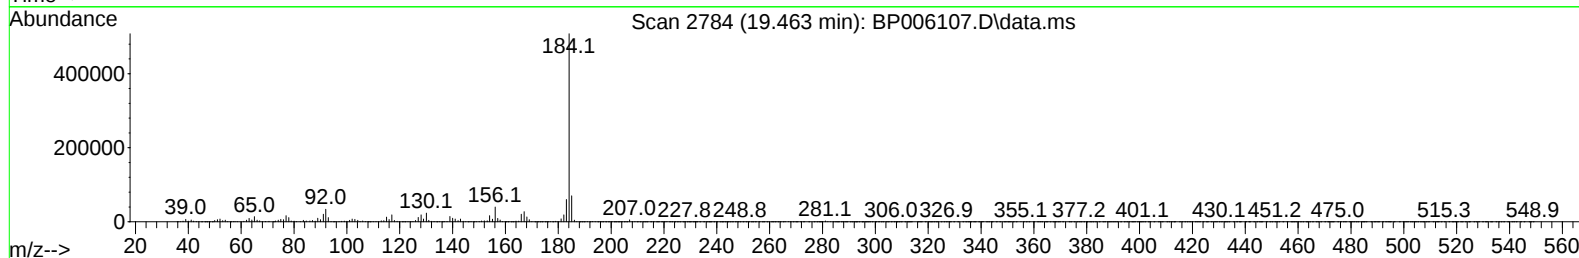


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063021\
 Data File : BP006107.D
 Acq On : 30 Jun 2021 14:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 14:56:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 11:34:30 2021
 Response via : Initial Calibration

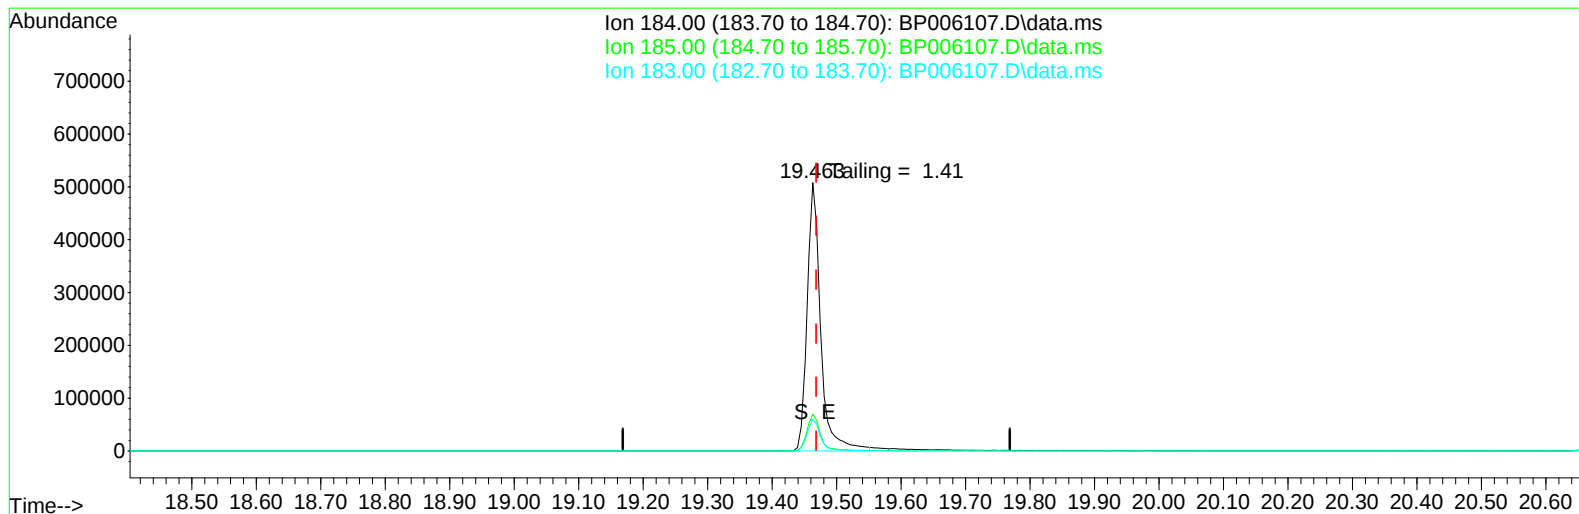




TIC: BP006107.D\data.ms

(77) Benzidine**19.463min (-0.006) 964551.77 ng****response 762675**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.77
183.00	11.90	11.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063021\
 Data File : BP006107.D
 Acq On : 30 Jun 2021 14:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 14:56:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 11:34:30 2021
 Response via : Initial Calibration

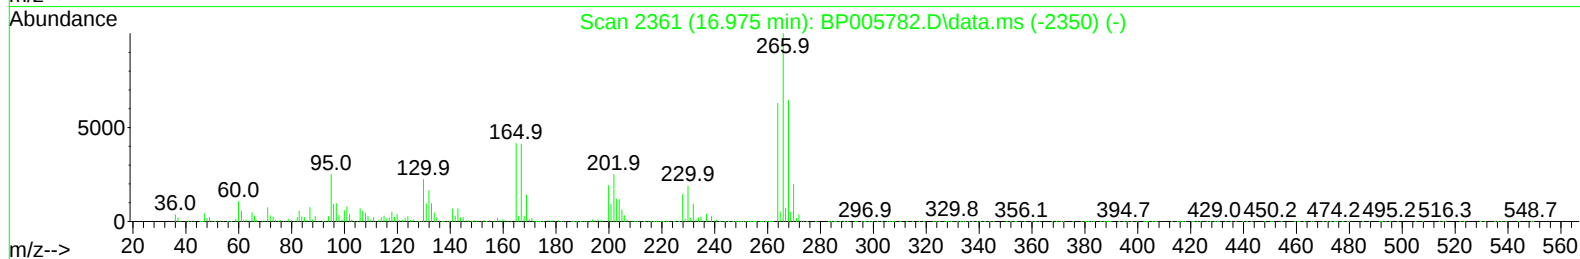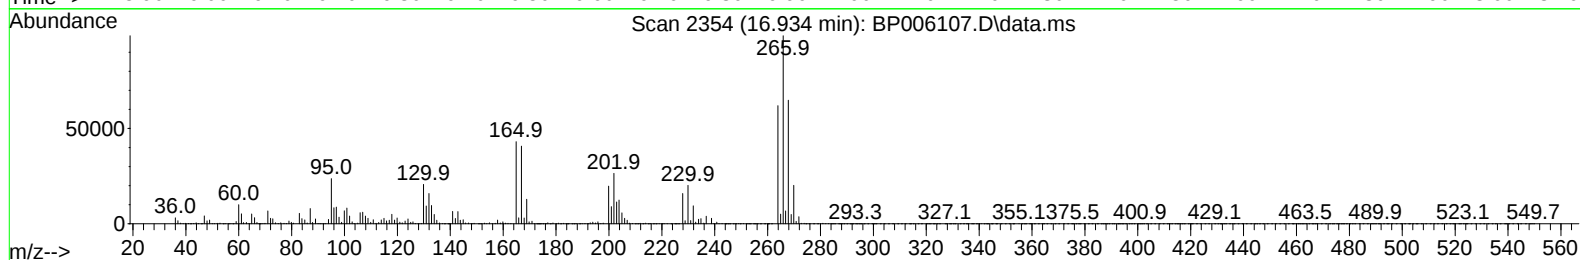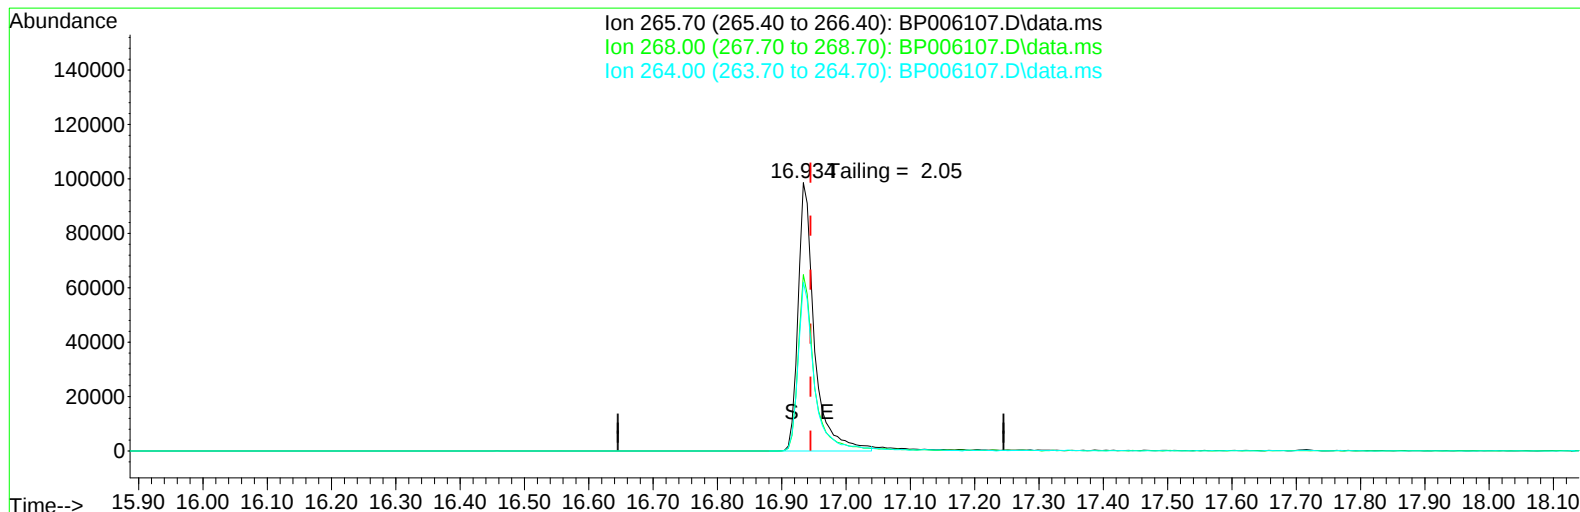

TIC: BP006107.D\data.ms

(70) Pentachlorophenol (C)

16.934min (-0.012) 388392.29 ng

response 179413

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	65.68
264.00	62.90	62.83
0.00	0.00	0.00