

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063021\
 Data File : BP006124.D
 Acq On : 01 Jul 2021 00:30
 Operator : CG/JU
 Sample : M2896-01 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FS-01

Manual Integrations
 APPROVED

mohammad
 7/1/2021 2:53:01 PM

Quant Time: Jul 01 03:09:51 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 30 16:39:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	120889	20.000	ng	0.00
21) Naphthalene-d8	10.693	136	412728	20.000	ng	0.00
39) Acenaphthene-d10	14.522	164	231997	20.000	ng	0.00
64) Phenanthrene-d10	17.275	188	411609	20.000	ng	# 0.00
76) Chrysene-d12	21.357	240	509816	20.000	ng	0.00
86) Perylene-d12	23.763	264	613287	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.469	112	67302	8.933	ng	0.00
7) Phenol-d6	7.081	99	73957	7.574	ng	0.00
23) Nitrobenzene-d5	9.057	82	48208	5.727	ng	0.00
42) 2,4,6-Tribromophenol	16.022	330	30794	7.735	ng	0.00
45) 2-Fluorobiphenyl	13.145	172	100992	5.716	ng	0.00
79) Terphenyl-d14	19.822	244	153985	5.656	ng	0.00
Target Compounds						
						Qvalue
17) 2-Methylphenol	8.357	107	27758	4.176	ng	98
20) 3+4-Methylphenols	8.693	107	53876	6.001	ng	92
27) 2,4-Dimethylphenol	9.881	122	66207m	10.655	ng	
37) 2-Methylnaphthalene	12.351	142	37882	2.228	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063021\
Data File : BP006124.D
Acq On : 01 Jul 2021 00:30
Operator : CG/JU
Sample : M2896-01 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
FS-01

Manual Integrations
APPROVED

mohammad
7/1/2021 2:53:01 PM

Quant Time: Jul 01 03:09:51 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 30 16:39:37 2021
Response via : Initial Calibration

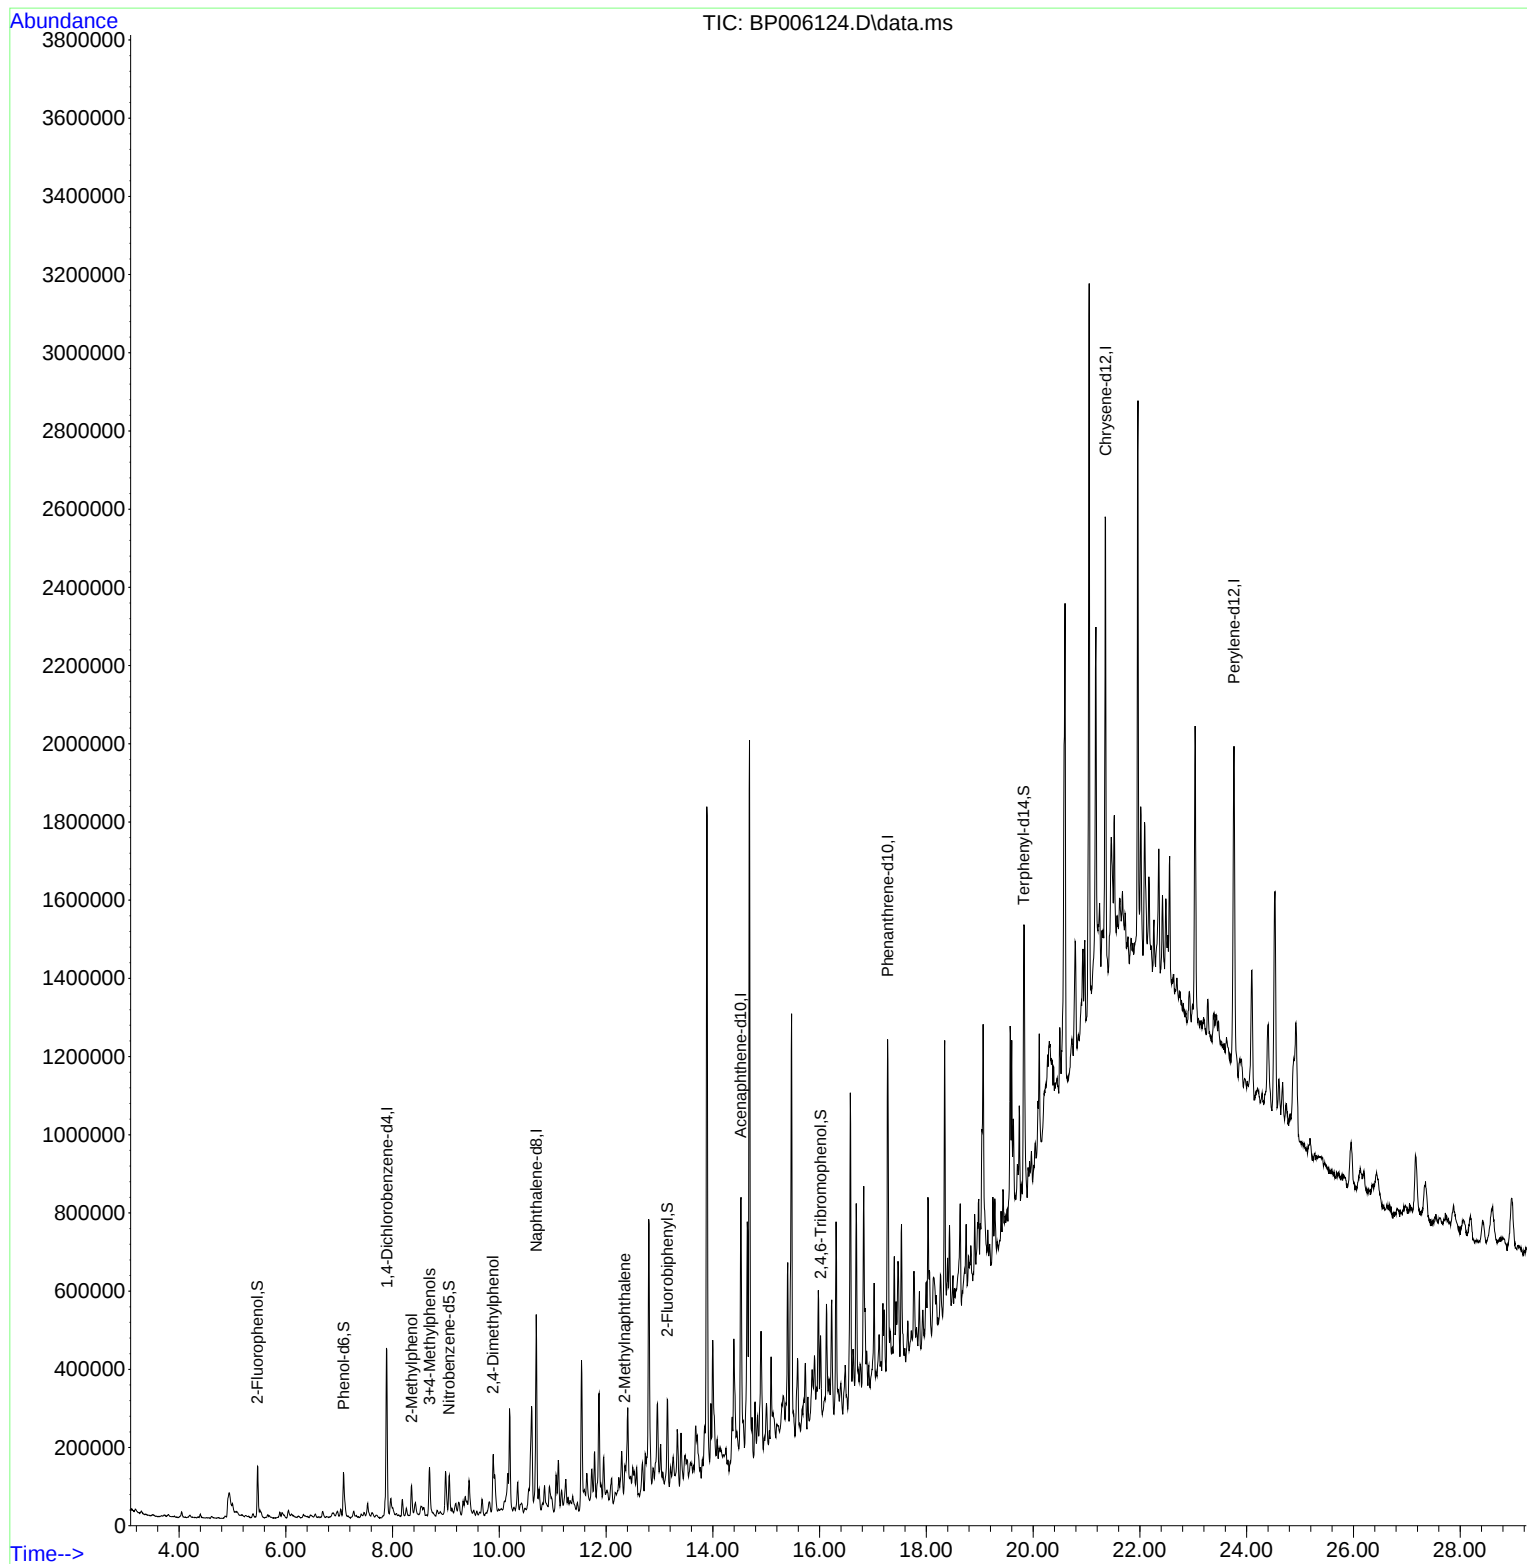

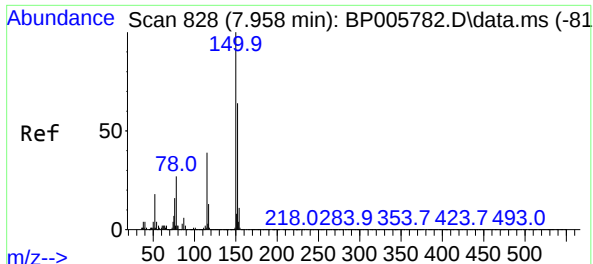





#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.893 min Scan# 817
Delta R.T. -0.000 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30

Tgt Ion:152 Resp: 120889
Ion Ratio Lower Upper
152 100
150 154.7 125.6 188.4
115 59.8 48.5 72.7

Instrument :
BNA_P
ClientSampled :
FS-01




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:01 PM

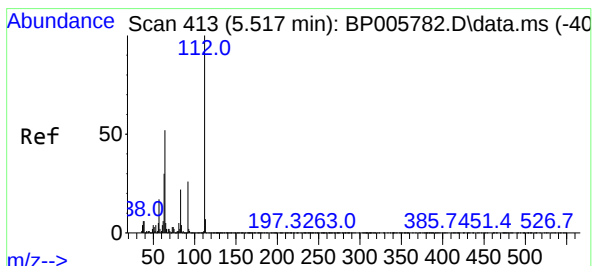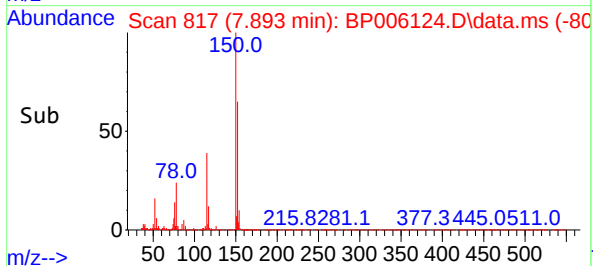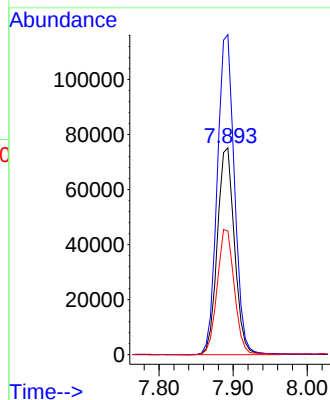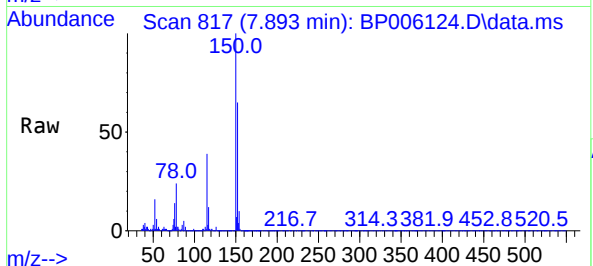

#5
2-Fluorophenol
Concen: 8.933 ng
RT: 5.469 min Scan# 405
Delta R.T. 0.000 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30


Tgt Ion:112 Resp: 67302
Ion Ratio Lower Upper
112 100
64 52.2 41.4 62.2
63 28.5 23.8 35.8

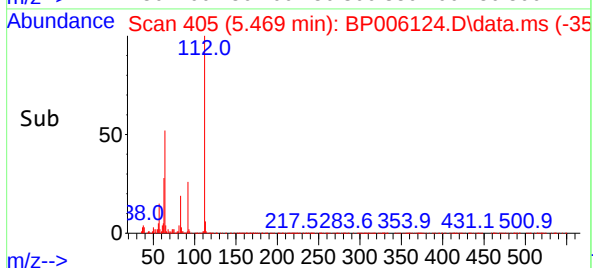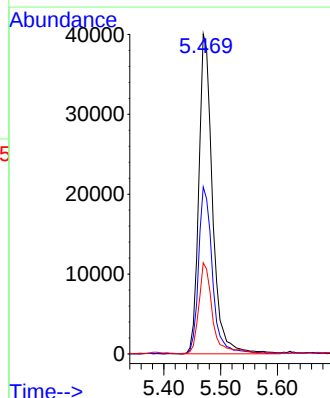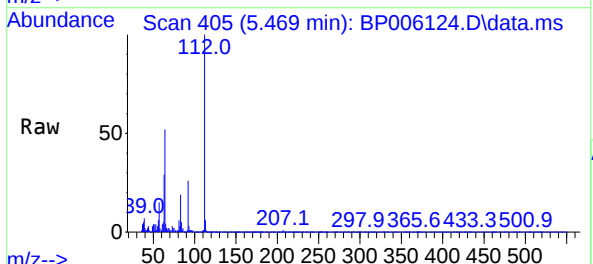



#7
Phenol-d6
Concen: 7.574 ng
RT: 7.081 min Scan# 679
Delta R.T. 0.006 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30




Instrument :
BNA_P
ClientSampled :
FS-01

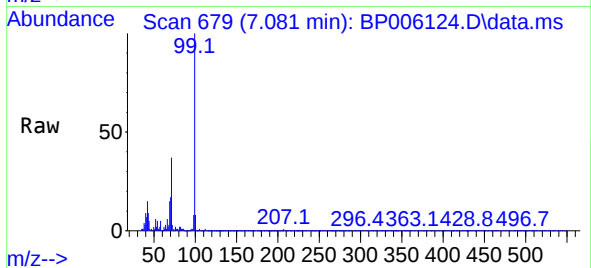


Tgt Ion: 99 Resp: 73957
Ion Ratio Lower Upper
99 100
42 14.8 13.4 20.0
71 37.3 30.6 46.0

Manual Integrations
APPROVED



mohammad
7/1/2021 2:53:01 PM

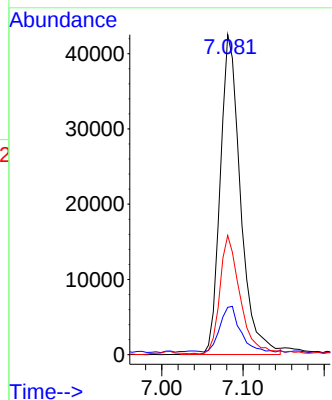


#17
2-Methylphenol
Concen: 4.176 ng
RT: 8.357 min Scan# 896
Delta R.T. 0.006 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30

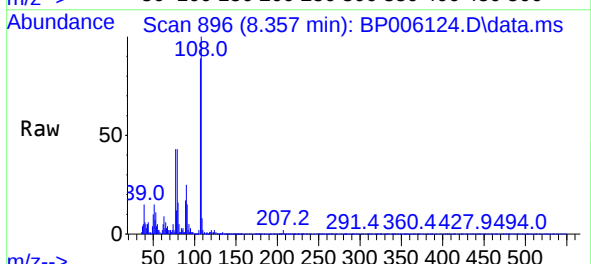


Tgt Ion: 107 Resp: 27758
Ion Ratio Lower Upper
107 100
108 112.2 87.7 131.5
77 48.3 40.2 60.2
79 48.4 39.0 58.4

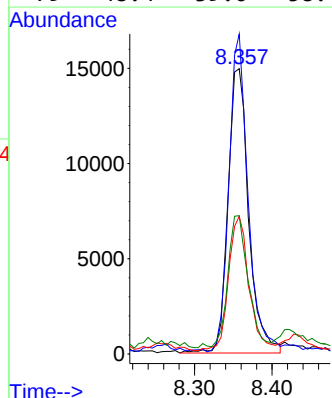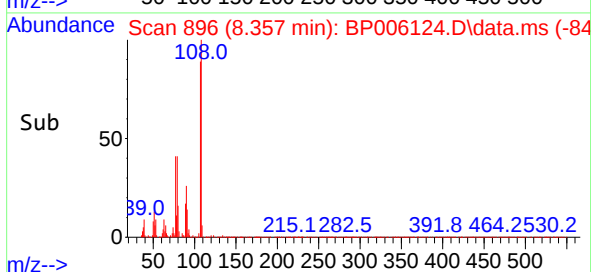

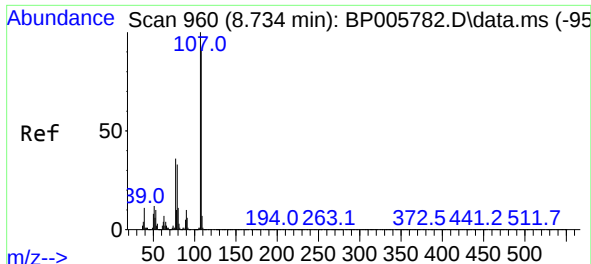

#20
3+4-Methylphenols
Concen: 6.001 ng
RT: 8.693 min Scan# 953
Delta R.T. 0.012 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30




Instrument :
BNA_P
ClientSampled :
FS-01




Tgt Ion:	107	Resp:	53876
Ion	Ratio	Lower	Upper
107	100		
108	99.7	71.0	111.0
77	38.1	16.6	56.6
79	38.8	12.7	52.7

Manual Integrations
APPROVED



mohammad
7/1/2021 2:53:01 PM

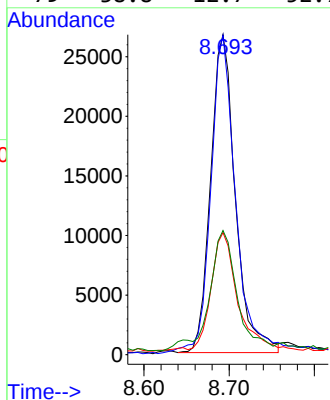


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.693 min Scan# 1293
Delta R.T. 0.000 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30

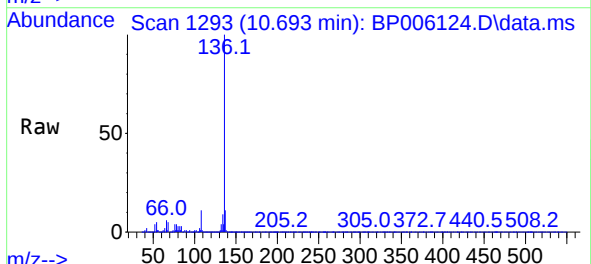

Tgt Ion:	136	Resp:	412728
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.6	12.8
54	5.4	4.6	6.8
68	5.3	3.6	5.4

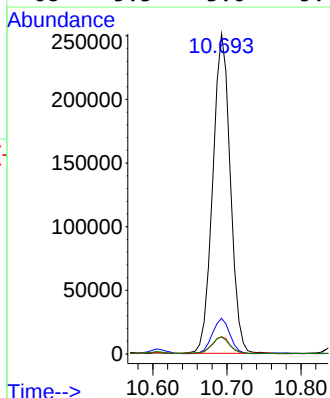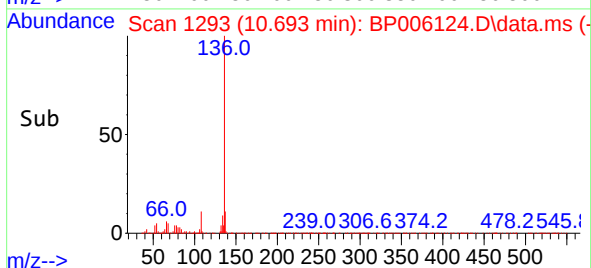

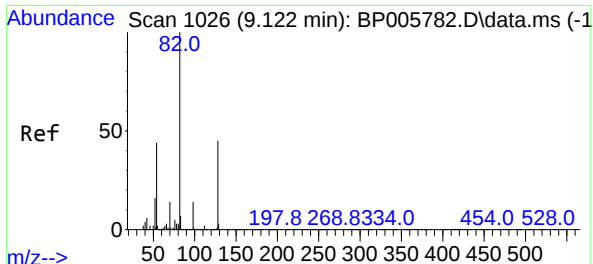





#23
Nitrobenzene-d5
Concen: 5.727 ng
RT: 9.057 min Scan# 1015
Delta R.T. 0.000 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30

Instrument :
BNA_P
ClientSampled :
FS-01

Tgt Ion: 82 Resp: 48208
Ion Ratio Lower Upper
82 100
128 44.7 35.7 53.5
54 40.7 35.0 52.4




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:01 PM

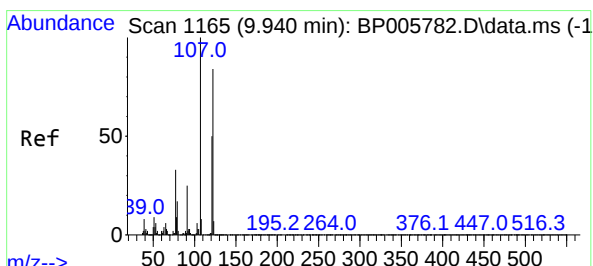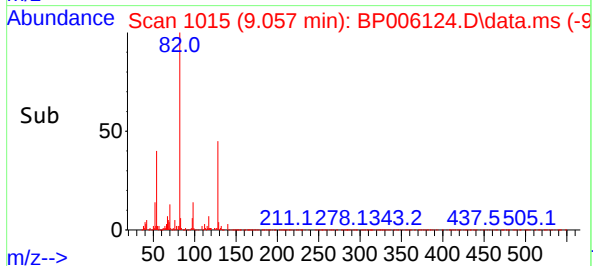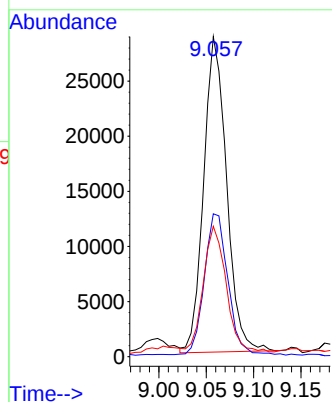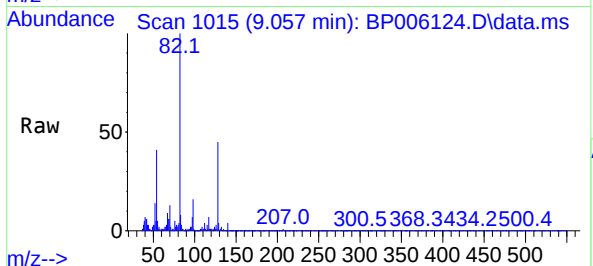

#27
2,4-Dimethylphenol
Concen: 10.655 ng m
RT: 9.881 min Scan# 1155
Delta R.T. 0.000 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30

Tgt Ion: 122 Resp: 66207
Ion Ratio Lower Upper
122 100
107 117.6 94.5 141.7
121 55.9 47.4 71.2

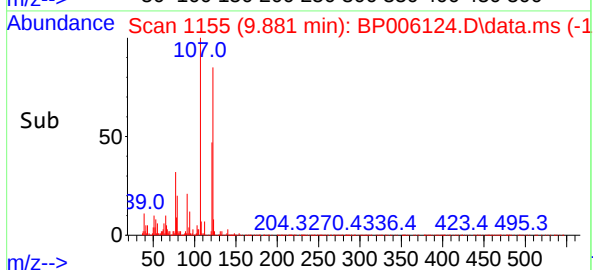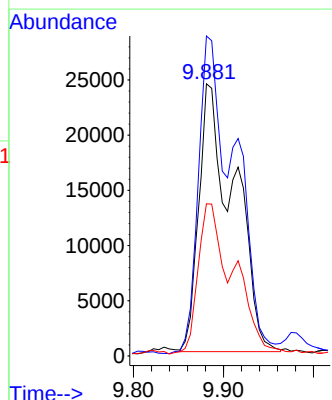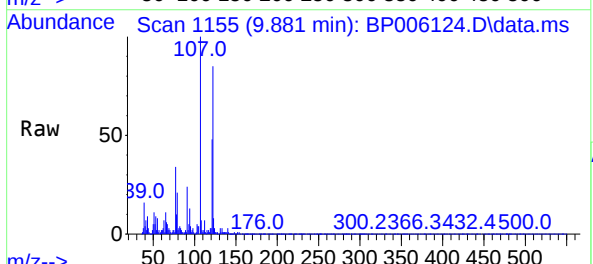







#37
2-Methylnaphthalene
Concen: 2.228 ng
RT: 12.351 min Scan# 1575
Delta R.T. -0.006 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30

Tgt Ion:	142	Resp:	37882
Ion	Ratio	Lower	Upper
142	100		
141	89.9	71.8	107.6
115	39.5	31.6	47.4

Instrument :
BNA_P
ClientSampled :
FS-01




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:01 PM

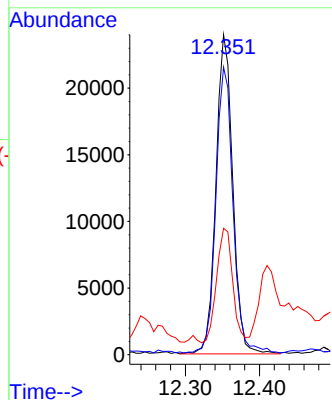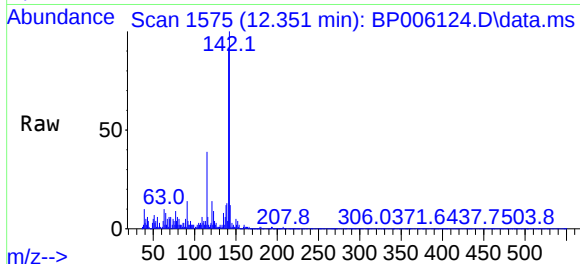

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.522 min Scan# 1944
Delta R.T. -0.006 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30


Tgt Ion:	164	Resp:	231997
Ion	Ratio	Lower	Upper
164	100		
162	102.8	80.2	120.2
160	44.8	34.5	51.7

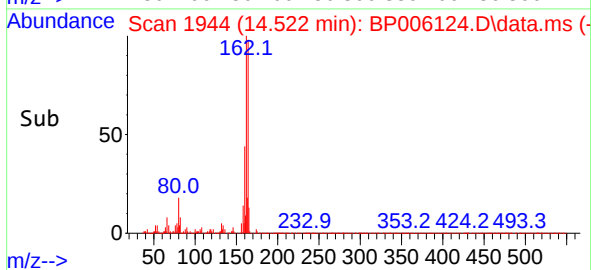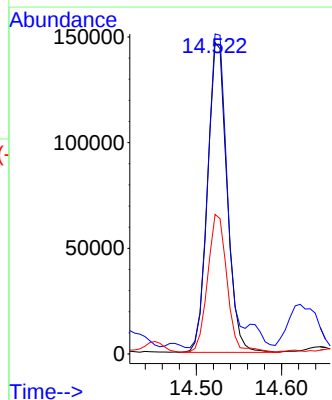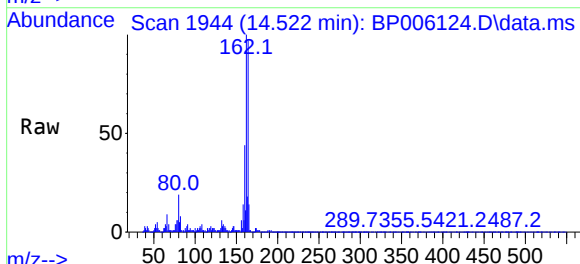

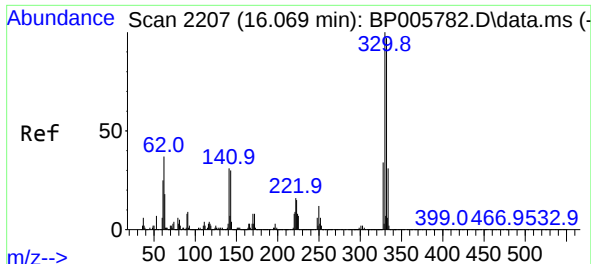

#42
2,4,6-Tribromophenol
Concen: 7.735 ng
RT: 16.022 min Scan# 2199
Delta R.T. 0.000 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30




Instrument :
BNA_P
ClientSampled :
FS-01




Tgt Ion:330 Resp: 30794
Ion Ratio Lower Upper
330 100
332 97.7 77.8 116.8
141 33.1 25.4 38.2

Manual Integrations
APPROVED



mohammad
7/1/2021 2:53:01 PM

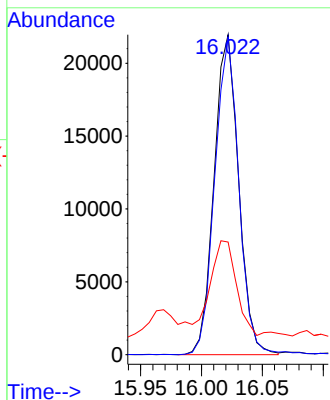


#45
2-Fluorobiphenyl
Concen: 5.716 ng
RT: 13.145 min Scan# 1710
Delta R.T. -0.006 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30

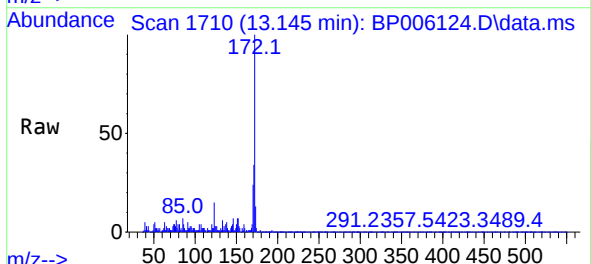


Tgt Ion:172 Resp: 100992
Ion Ratio Lower Upper
172 100
171 34.4 27.9 41.9
170 23.6 18.6 27.8

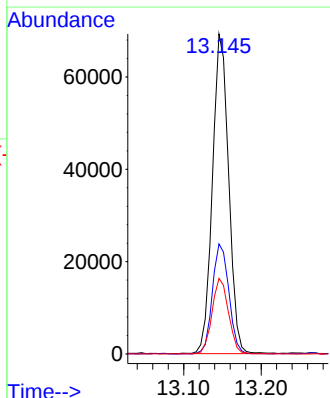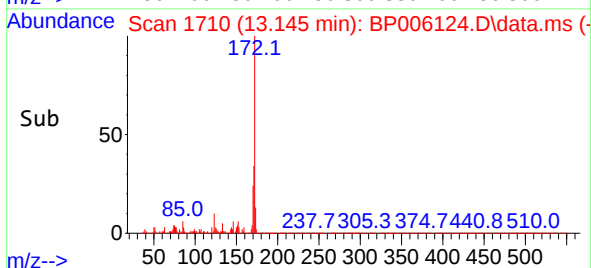



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.275 min Scan# 2412
Delta R.T. 0.000 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30




Instrument :
BNA_P
ClientSampled :
FS-01



Tgt Ion:188 Resp: 411609
Ion Ratio Lower Upper
188 100
94 8.5 5.6 8.4#
80 9.2 6.3 9.5




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:01 PM

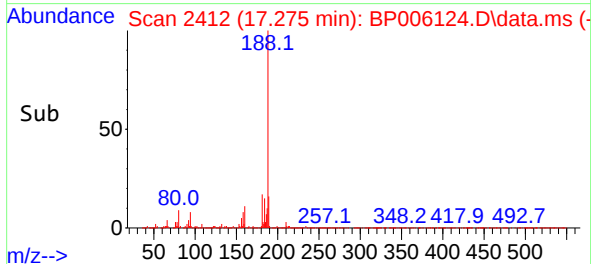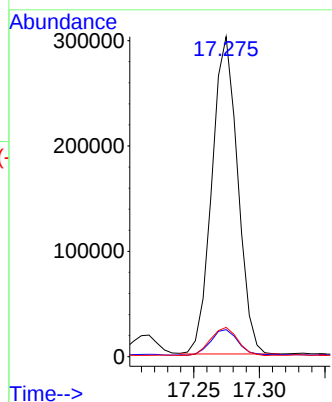

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.357 min Scan# 3106
Delta R.T. 0.000 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30


Tgt Ion:240 Resp: 509816
Ion Ratio Lower Upper
240 100
120 9.2 6.5 9.7
236 26.0 20.6 31.0

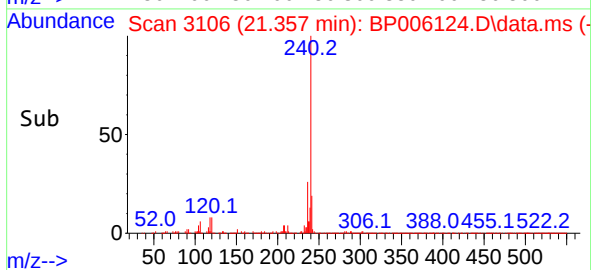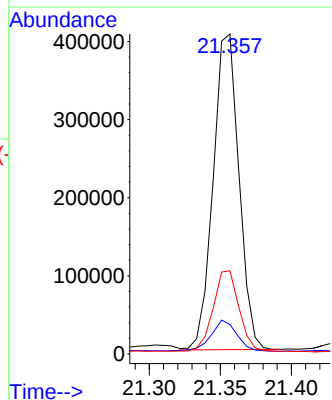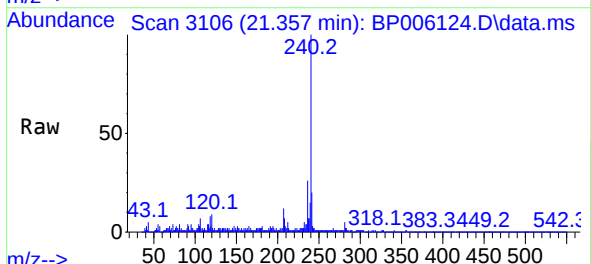



#79
Terphenyl-d14
Concen: 5.656 ng
RT: 19.822 min Scan# 2845
Delta R.T. -0.006 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30




Instrument :
BNA_P
ClientSampled :
FS-01



Tgt Ion:244 Resp: 153985
Ion Ratio Lower Upper
244 100
212 8.9 6.0 9.0
122 12.3 7.1 10.7#

Manual Integrations
APPROVED

mohammad
7/1/2021 2:53:01 PM

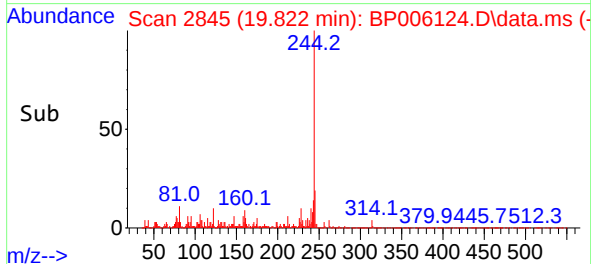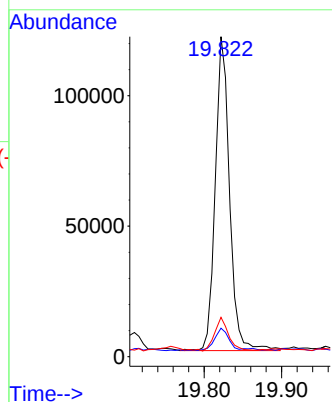

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.763 min Scan# 3515
Delta R.T. 0.006 min
Lab File: BP006124.D
Acq: 01 Jul 2021 00:30

Tgt Ion:264 Resp: 613287
Ion Ratio Lower Upper
264 100
260 23.7 18.6 28.0
265 23.1 17.6 26.4

