
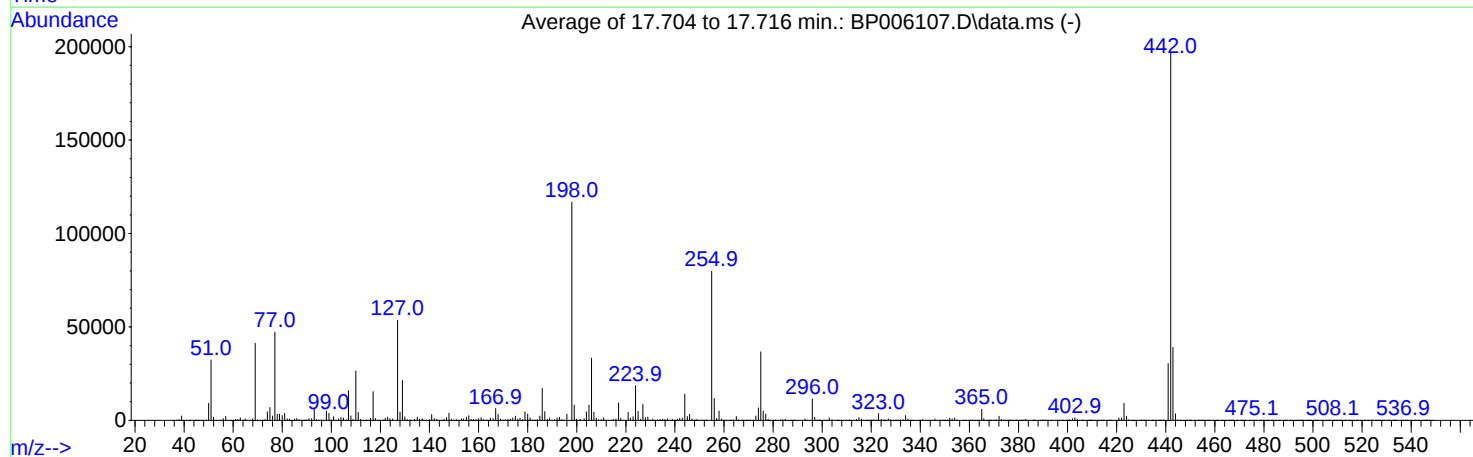


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063021\
 Data File : BP006107.D
 Acq On : 30 Jun 2021 14:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 30 16:39:37 2021

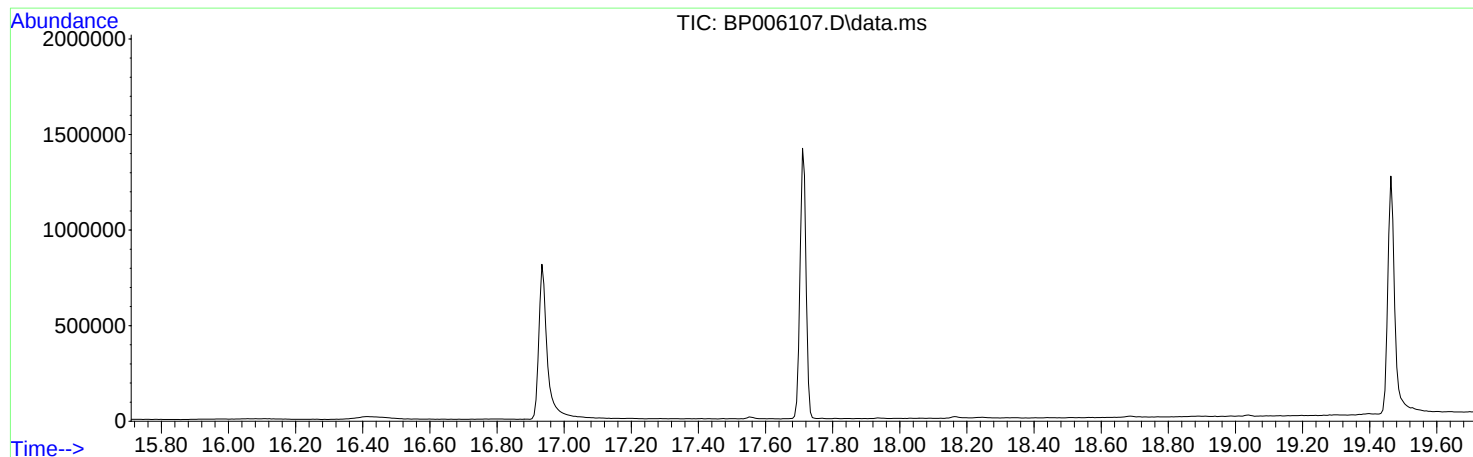




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	32351	PASS
68	69	0.00	2	1.9	771	PASS
69	198	0.00	100	35.4	41307	PASS
70	69	0.00	2	0.7	278	PASS
127	198	10	80	45.8	53533	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	116840	PASS
199	198	5	9	7.0	8169	PASS
275	198	10	60	31.4	36640	PASS
365	198	1	100	5.1	5941	PASS
441	198	0.01	100	26.0	30391	PASS
442	442	100	100	100.0	196888	PASS
443	442	15	24	19.8	39046	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063021\
 Data File : BP006107.D
 Acq On : 30 Jun 2021 14:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 30 14:56:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 11:34:30 2021
 Response via : Initial Calibration

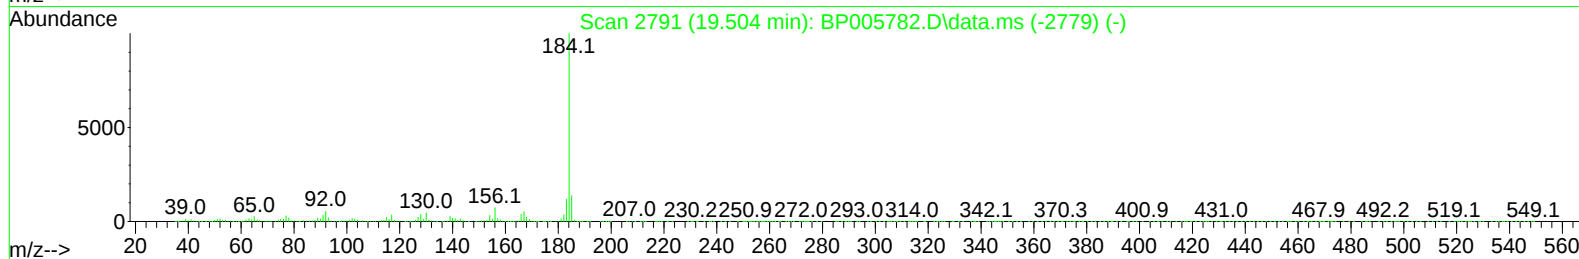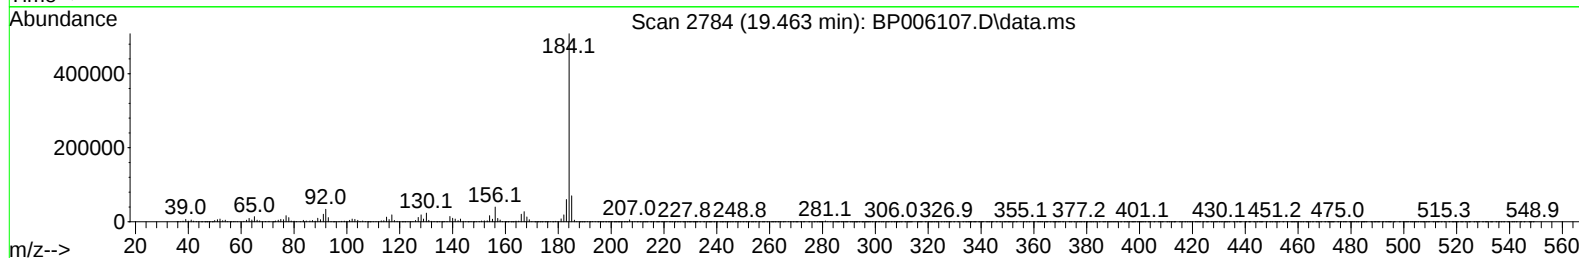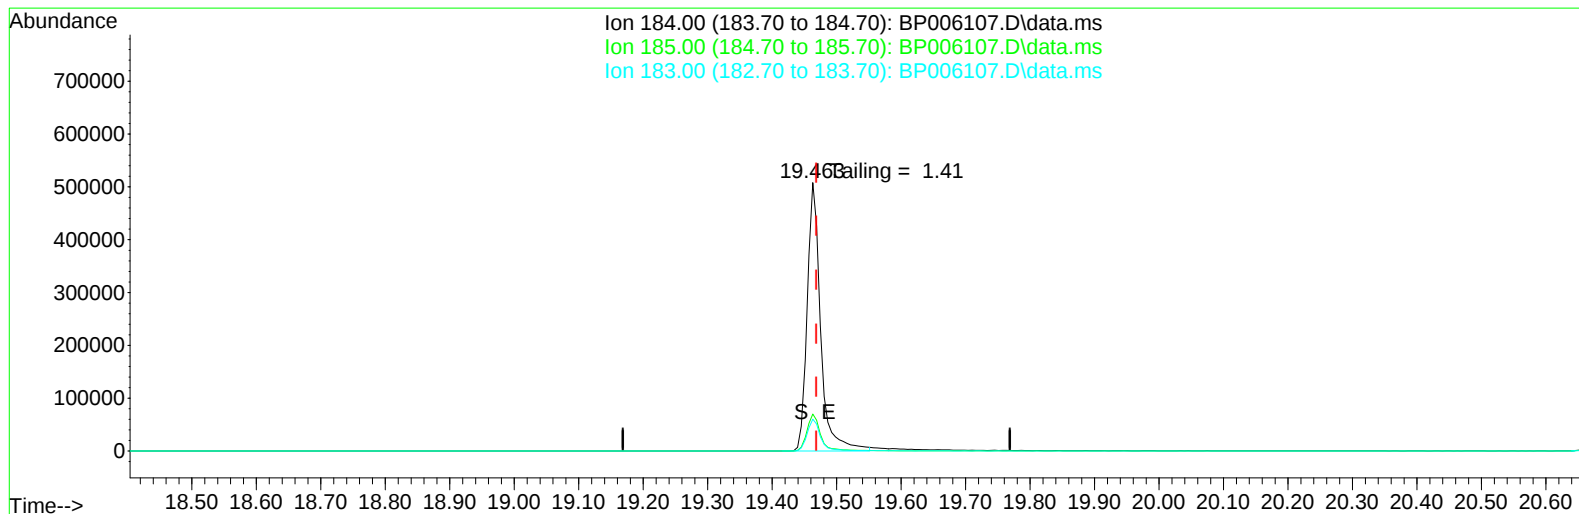

TIC: BP006107.D\data.ms

(77) Benzidine

19.463min (-0.006) 964551.77 ng




response 762675

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.77
183.00	11.90	11.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063021\
 Data File : BP006107.D
 Acq On : 30 Jun 2021 14:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 30 14:56:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 11:34:30 2021
 Response via : Initial Calibration

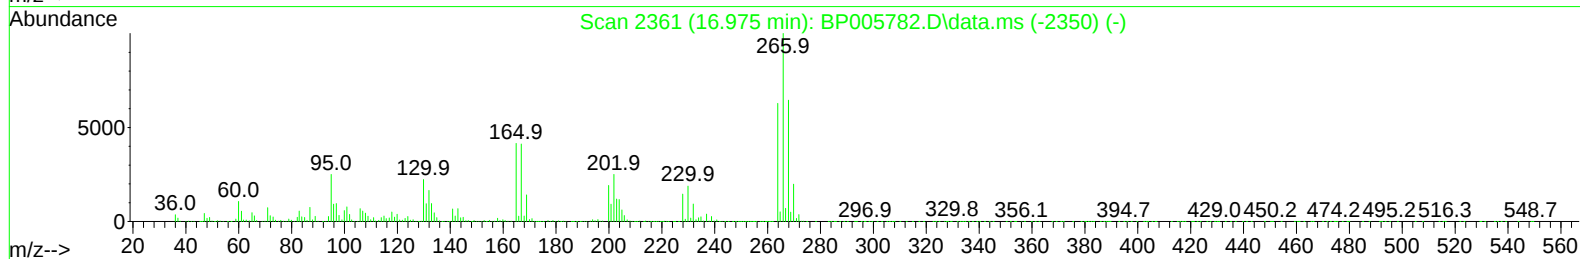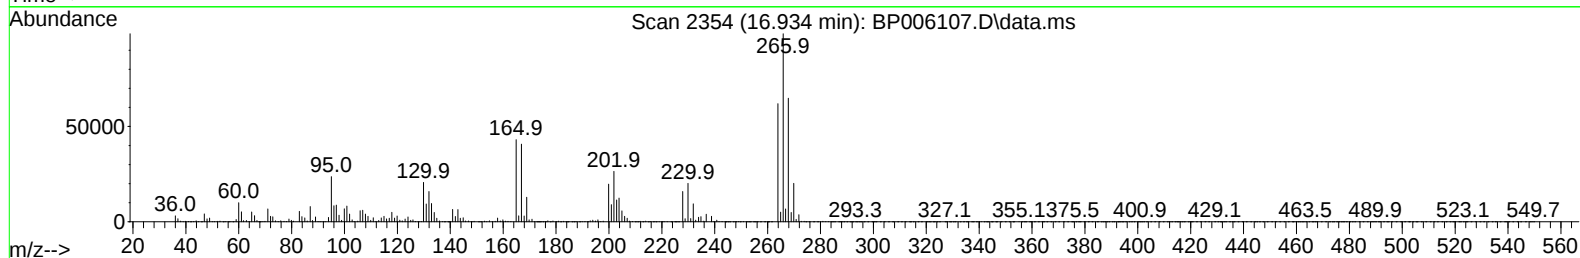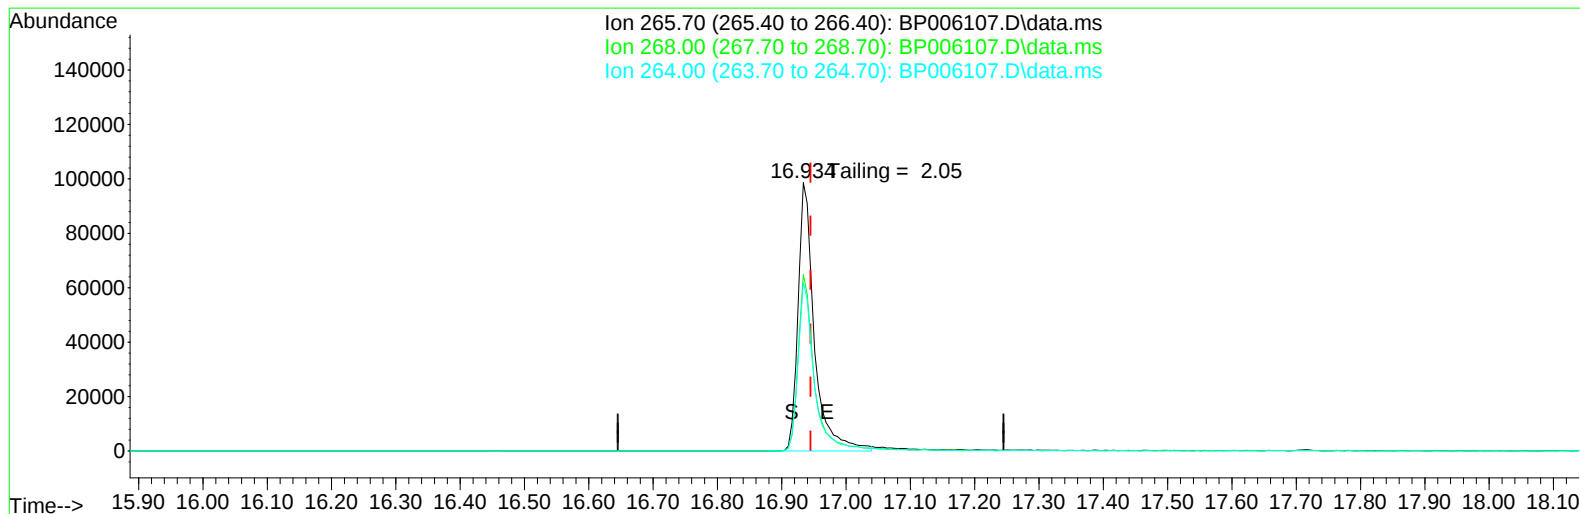

TIC: BP006107.D\data.ms

(70) Pentachlorophenol (C)

16.934min (-0.012) 388392.29 ng

response 179413

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	65.68
264.00	62.90	62.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/30/2021	BNA_P	<u>BP006107.D</u>
Compound Name	Response	Retention Time
DDT	446170	20.65
DDD	1141	20.23
DDE	1326	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2467	448637	0.55