

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
 Data File : BP010912.D
 Acq On : 30 Jun 2022 10:22
 Operator : CG/JU
 Sample : PB145923BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK923

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	15	20	25	rBV	146217	182287	2.31%	0.207%
2	3.611	86	89	111	rBV	1755074	2540801	32.22%	2.884%
3	3.923	138	142	149	rVB	42304	59953	0.76%	0.068%
4	6.881	638	645	660	rBV	1831319	2800440	35.51%	3.179%
5	7.046	666	673	684	rVB	1595175	2375448	30.12%	2.696%
6	7.240	699	706	715	rBV	1942379	2955173	37.48%	3.355%
7	7.705	778	785	796	rVB	1810734	2759174	34.99%	3.132%
8	8.422	896	907	918	rBV	2167660	3402251	43.15%	3.862%
9	8.863	975	982	999	rBV	1609125	2613037	33.14%	2.966%
10	9.587	1098	1105	1117	rBV	1160202	1865275	23.65%	2.117%
11	10.122	1187	1196	1210	rBV	1896172	3060286	38.81%	3.474%
12	10.499	1252	1260	1273	rBV	2363894	3806345	48.27%	4.321%
13	10.646	1275	1285	1299	rBV	1981940	3318860	42.09%	3.767%
14	11.446	1418	1421	1427	rBV8	4848	9023	0.11%	0.010%
15	12.099	1526	1532	1540	rVB	36263	58920	0.75%	0.067%
16	12.304	1565	1567	1574	rVB8	6519	10094	0.13%	0.011%
17	13.087	1695	1700	1705	rVB5	5210	9987	0.13%	0.011%
18	13.263	1727	1730	1735	rVB6	7282	11447	0.15%	0.013%
19	13.781	1810	1818	1827	rBV	2850342	3803395	48.23%	4.317%
20	14.051	1857	1864	1879	rBV	3390049	4721386	59.87%	5.359%
21	14.363	1909	1917	1926	rBV	2827637	4176842	52.97%	4.741%
22	14.575	1945	1953	1971	rBV	1189865	1816860	23.04%	2.062%
23	14.787	1987	1989	1995	rVB7	6005	8068	0.10%	0.009%
24	15.357	2080	2086	2100	rBV	4007928	5656266	71.73%	6.421%
25	15.481	2100	2107	2117	rBV	687047	978625	12.41%	1.111%
26	15.598	2123	2127	2135	rVB	50165	76468	0.97%	0.087%
27	16.145	2217	2220	2226	rVB5	13873	21775	0.28%	0.025%
28	16.910	2345	2350	2354	rBV6	6048	10155	0.13%	0.012%
29	17.122	2380	2386	2397	rBV	2977033	4266289	54.10%	4.843%
30	17.222	2397	2403	2418	rVV2	4160052	5904787	74.88%	6.703%
31	17.392	2427	2432	2438	rVB9	7973	16866	0.21%	0.019%
32	19.051	2710	2714	2719	rBV2	55547	78294	0.99%	0.089%
33	19.122	2722	2726	2729	rVV	43075	59944	0.76%	0.068%
34	19.475	2780	2786	2793	rBV	5203154	6735618	85.42%	7.646%
35	21.239	3081	3086	3091	rBV	3733463	4785643	60.69%	5.432%
36	23.445	3455	3461	3472	rVB2	4291498	7885405	100.00%	8.951%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010912.D
Acq On : 30 Jun 2022 10:22
Operator : CG/JU
Sample : PB145923BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK923

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION

37	23.598	3481	3487	3498	rVB2	2687245	5254205	66.63%	5.964%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 88095692

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010912.D
Acq On : 30 Jun 2022 10:22
Operator : CG/JU
Sample : PB145923BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK923

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

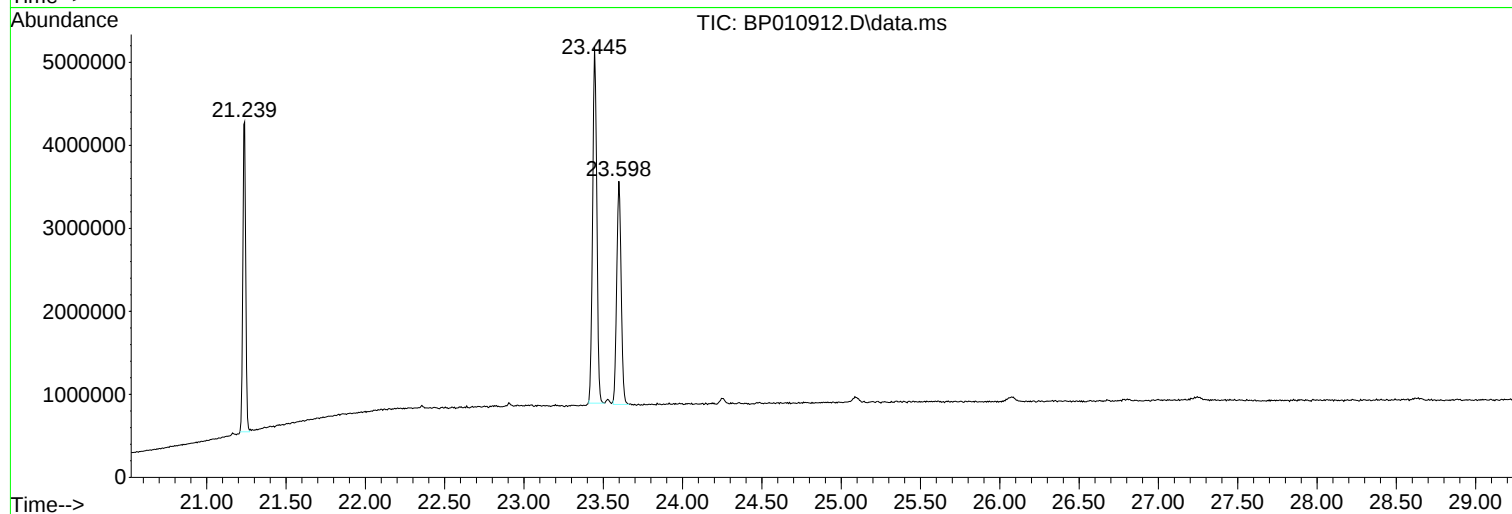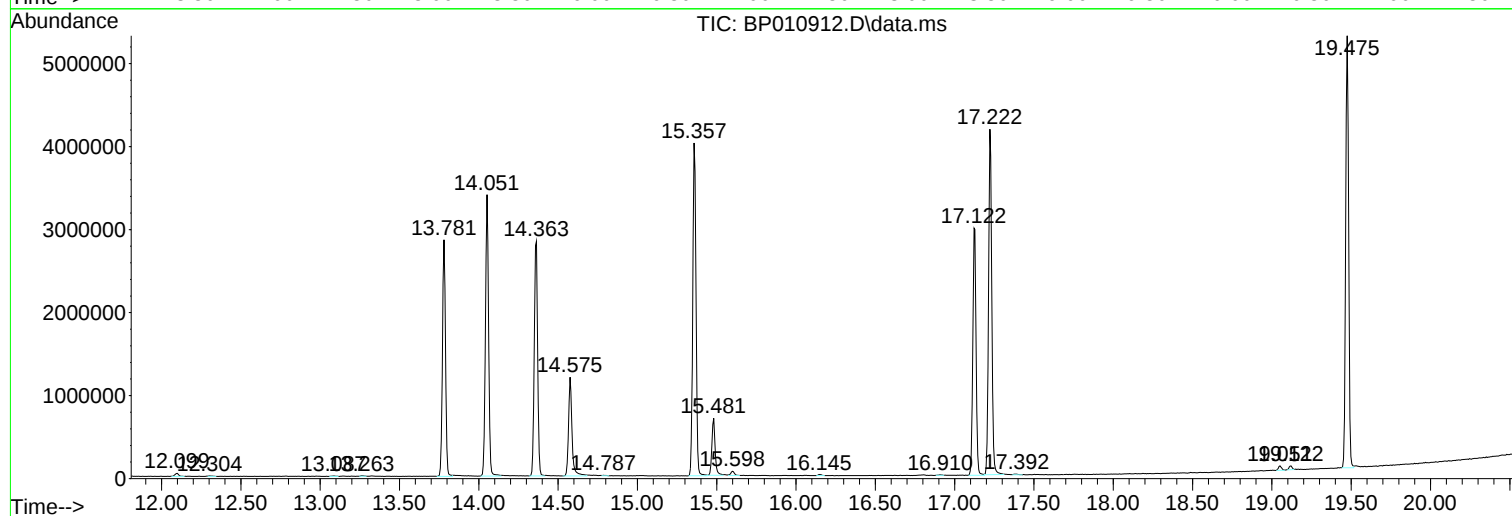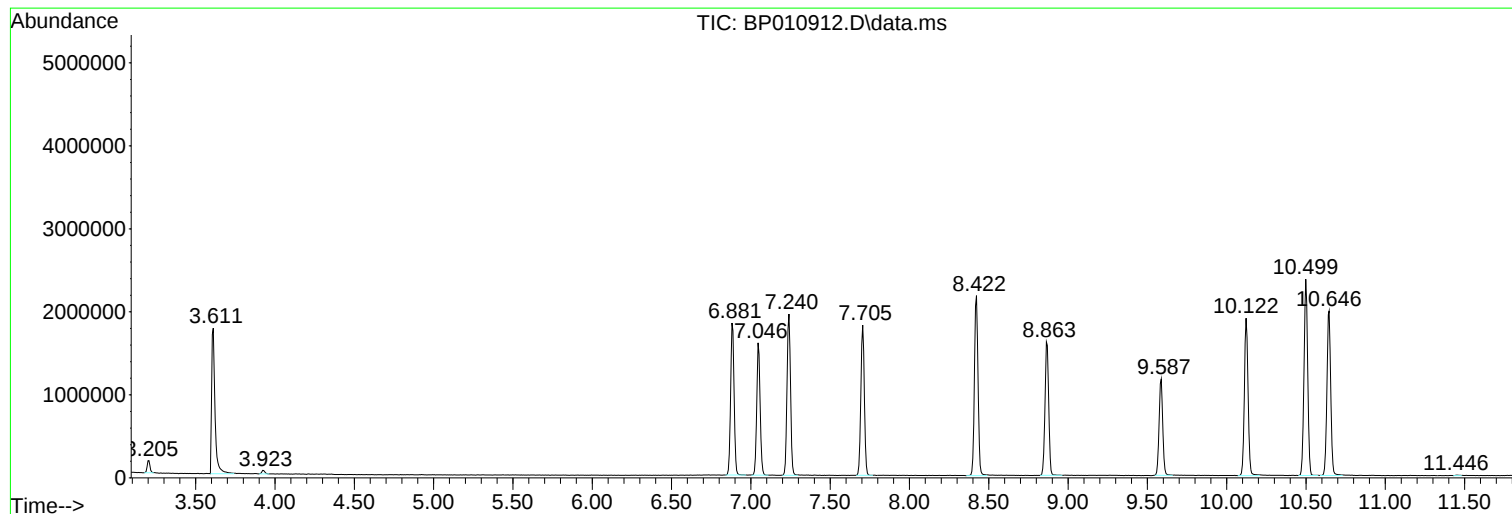

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010912.D
Acq On : 30 Jun 2022 10:22
Operator : CG/JU
Sample : PB145923BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK923

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063022\
Data File : BP010912.D
Acq On : 30 Jun 2022 10:22
Operator : CG/JU
Sample : PB145923BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK923

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------